

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/01/2022

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:09
INTERNAL STANDARD	VERIFIED	16:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:10
BLANK TEST	0.00	16:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:11
BLANK TEST	0.00	16:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:12
BLANK TEST	0.00	16:13

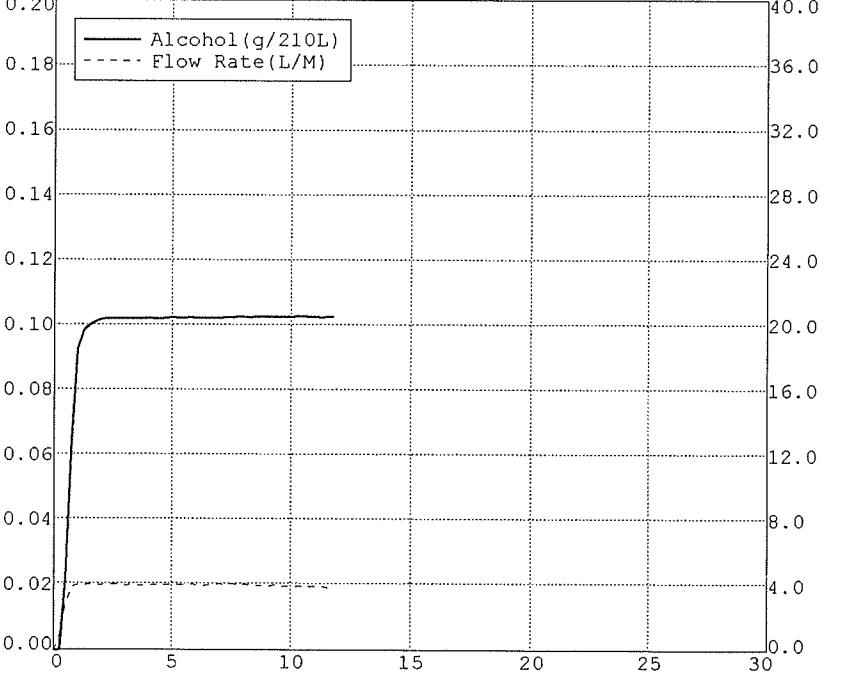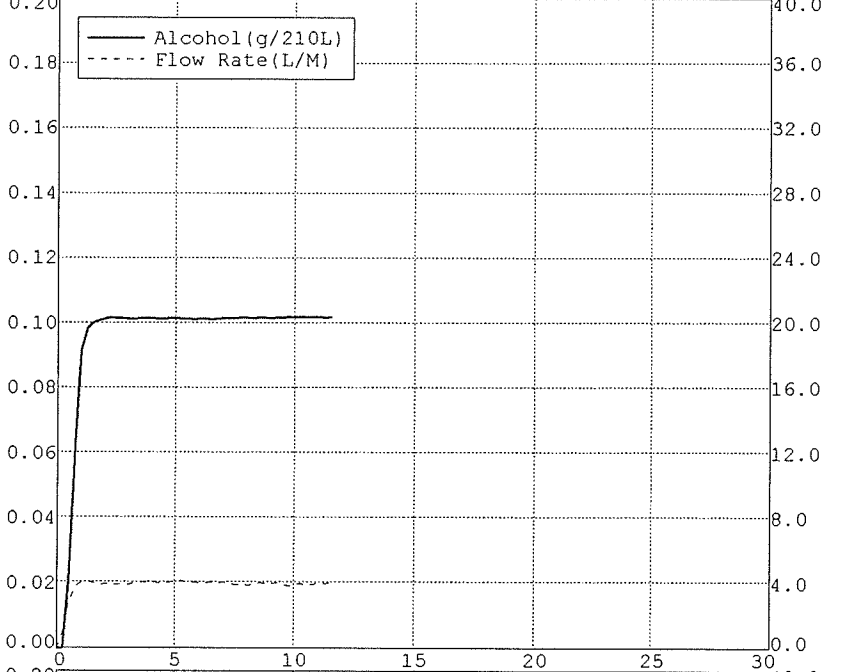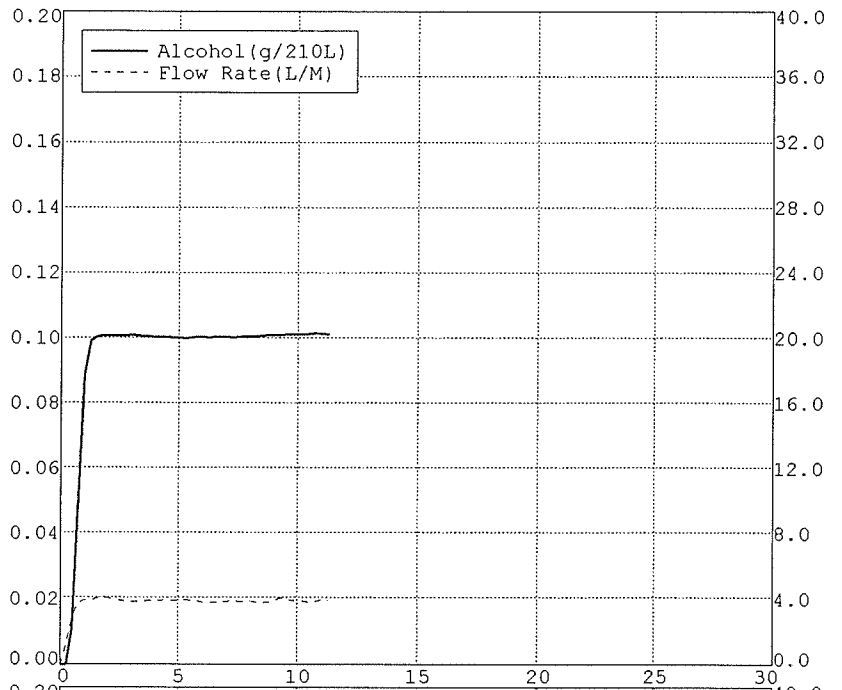

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/09/2022

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:04
INTERNAL STANDARD	VERIFIED	01:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:04
BLANK TEST	0.00	01:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:05
BLANK TEST	0.00	01:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:06
BLANK TEST	0.00	01:07

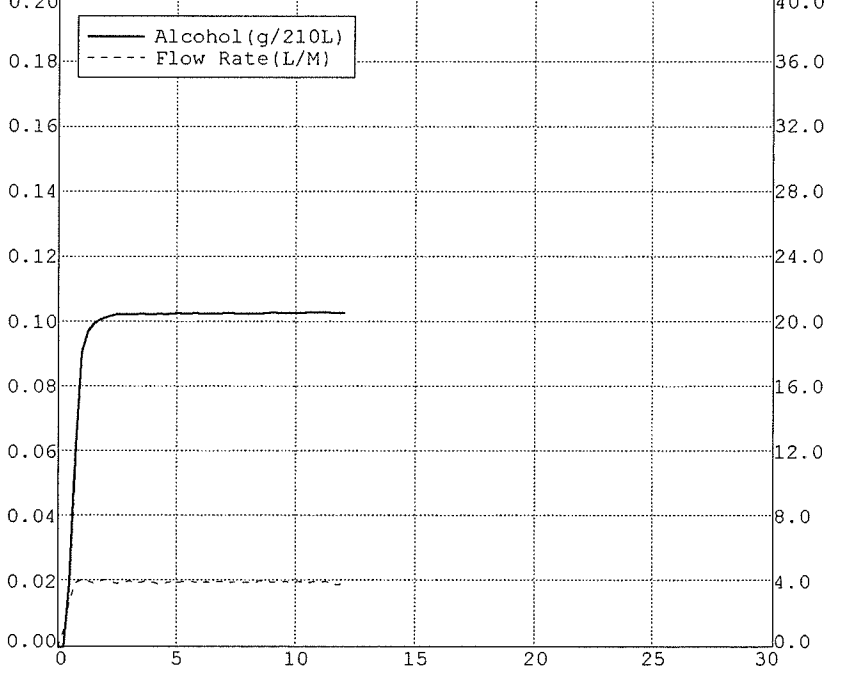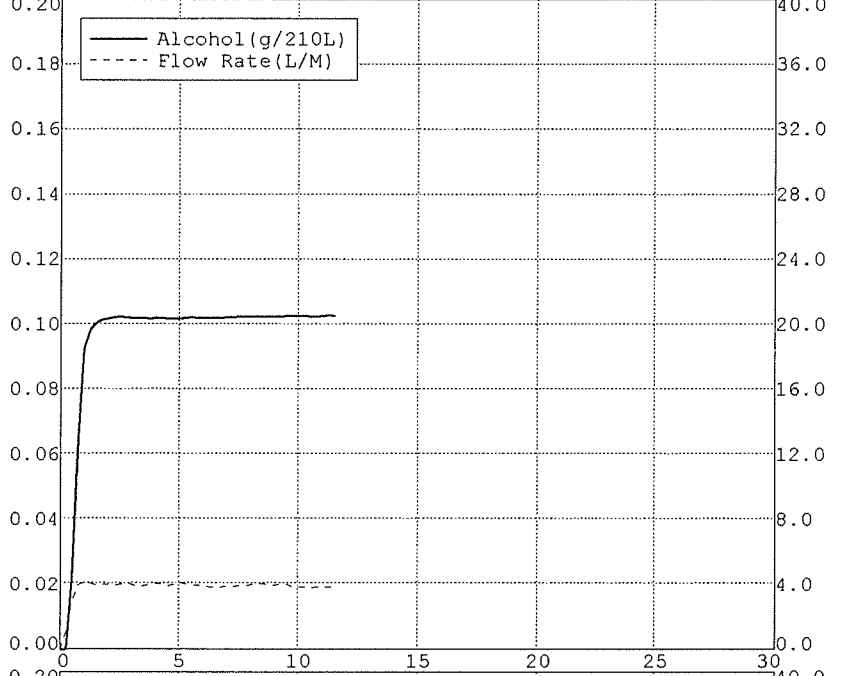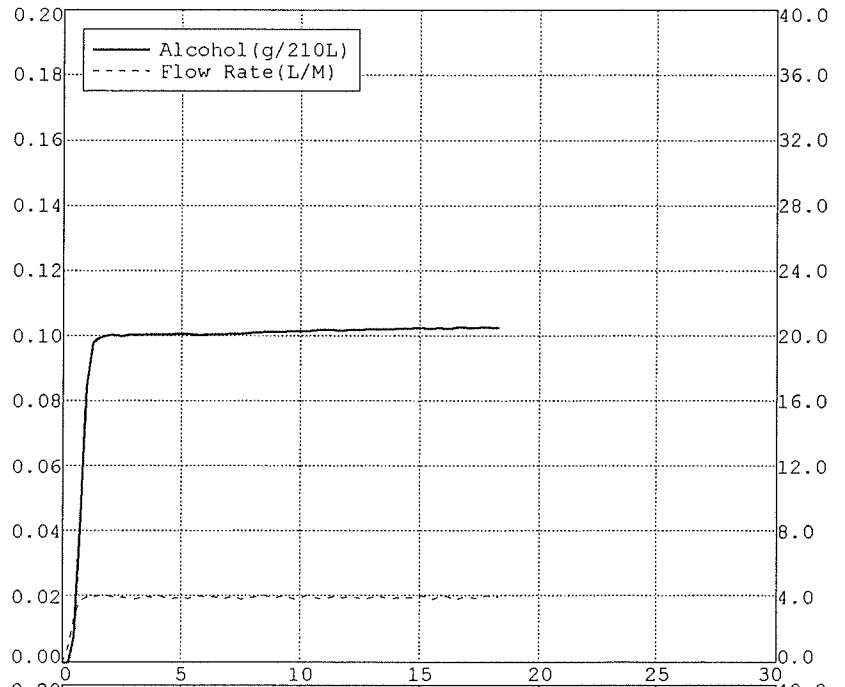

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/15/2022

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:48
INTERNAL STANDARD	VERIFIED	21:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:48
BLANK TEST	0.00	21:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:49
BLANK TEST	0.00	21:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:50
BLANK TEST	0.00	21:51

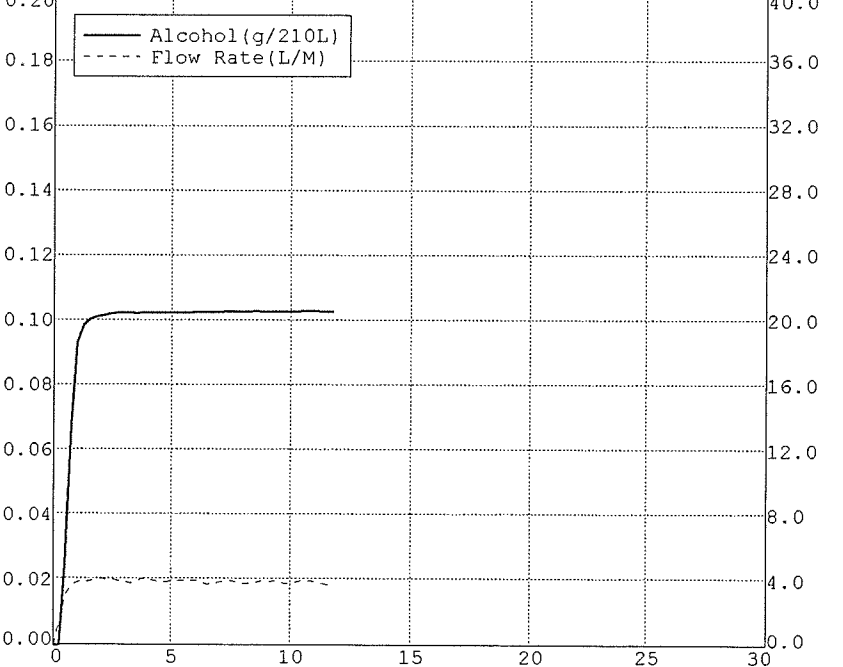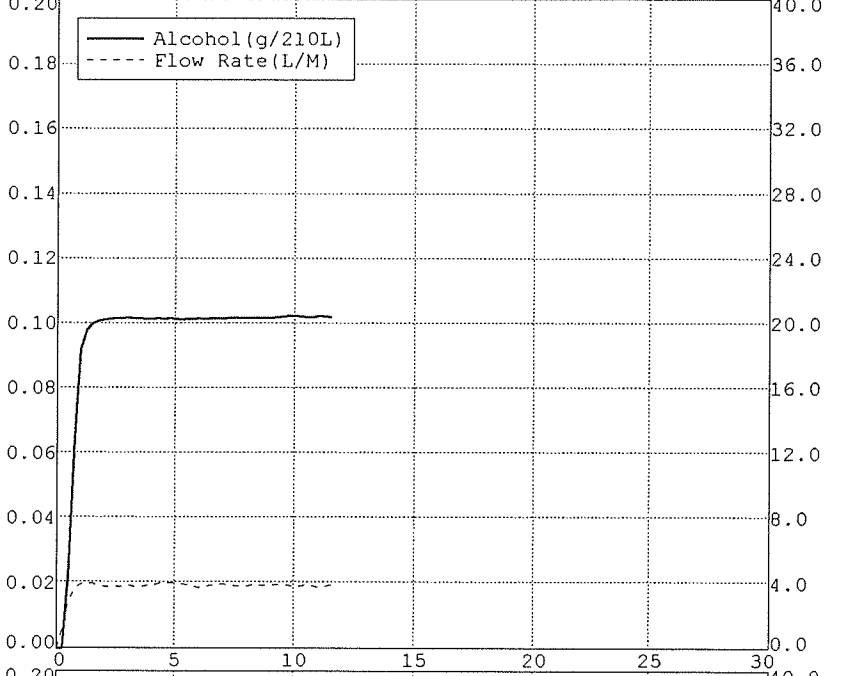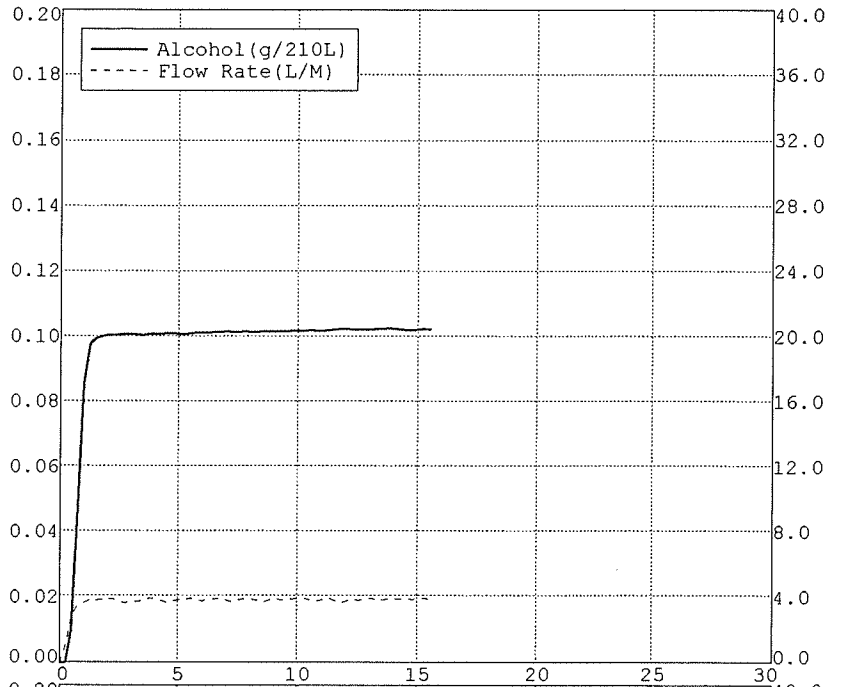

SUPERVISOR TEST



LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/23/2022

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:28
INTERNAL STANDARD	VERIFIED	03:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:28
BLANK TEST	0.00	03:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:30
BLANK TEST	0.00	03:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:31
BLANK TEST	0.00	03:31

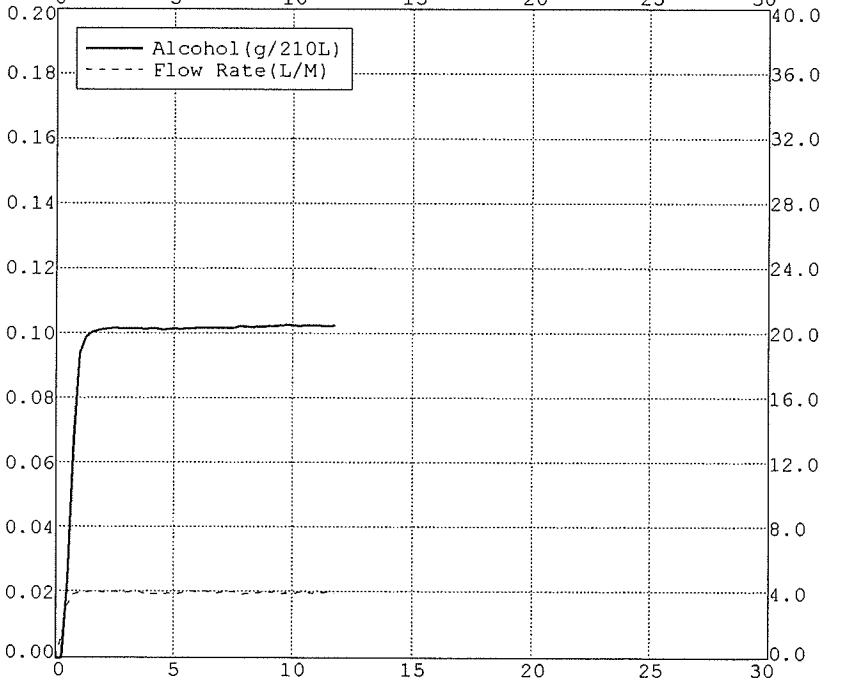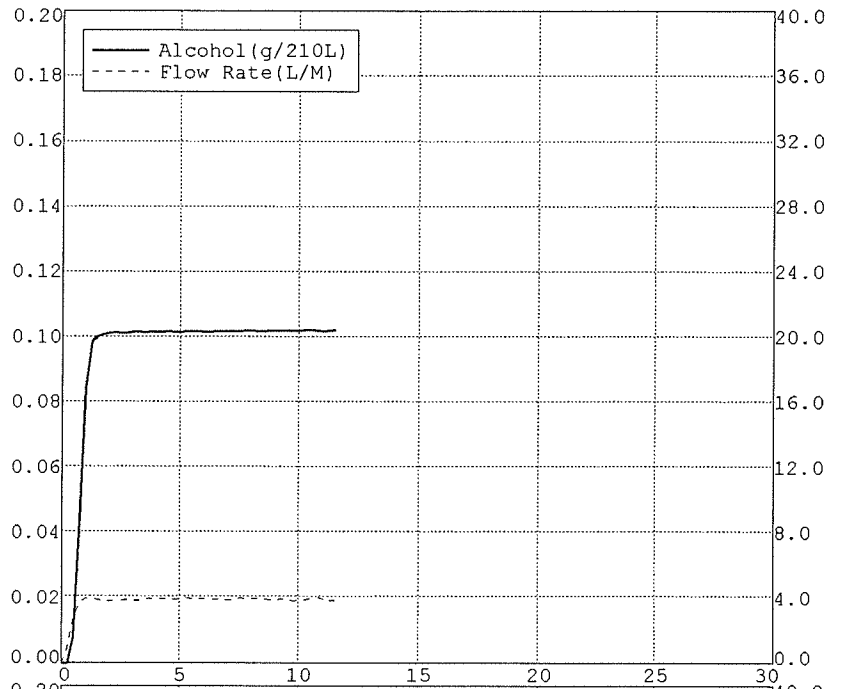

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/31/2022

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:21
INTERNAL STANDARD	VERIFIED	00:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:21
BLANK TEST	0.00	00:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:22
BLANK TEST	0.00	00:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:23
BLANK TEST	0.00	00:24

