

SUPERVISOR TEST



LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/03/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25250

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:49
INTERNAL STANDARD	VERIFIED	16:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:49
BLANK TEST	0.00	16:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:50
BLANK TEST	0.00	16:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:51
BLANK TEST	0.00	16:52

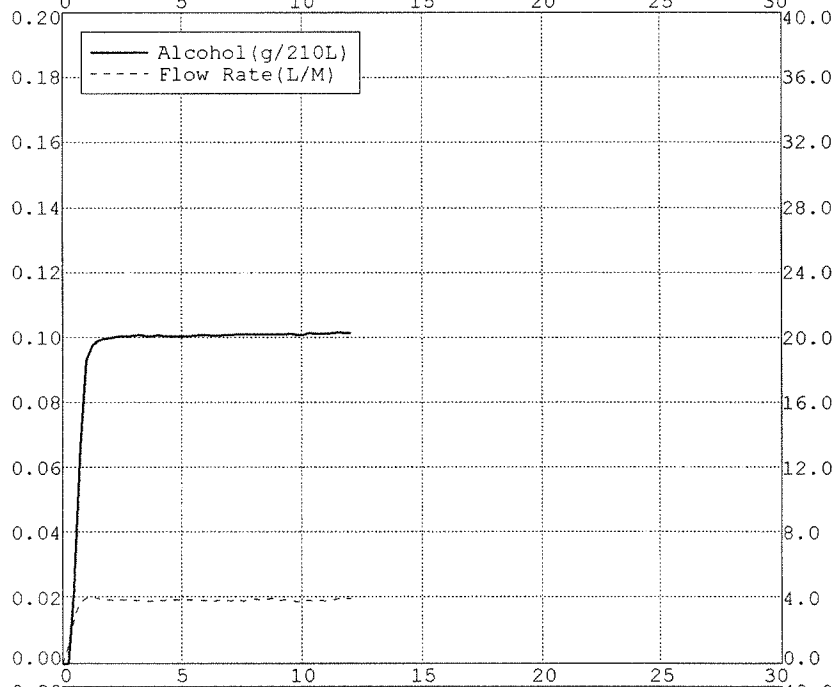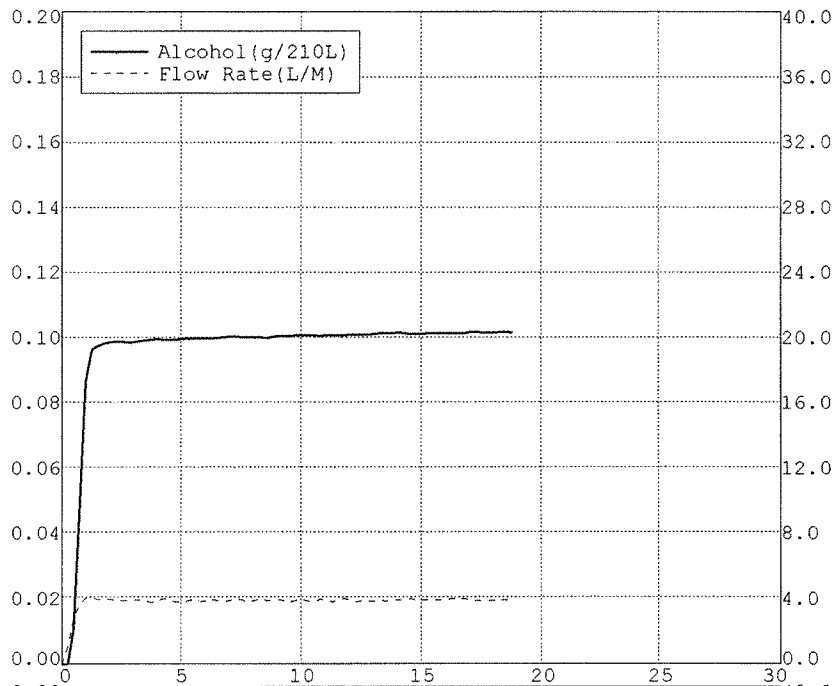

SUPERVISOR TEST


LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/09/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25250

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:15
INTERNAL STANDARD	VERIFIED	13:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:16
BLANK TEST	0.00	13:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:17
BLANK TEST	0.00	13:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:18
BLANK TEST	0.00	13:19

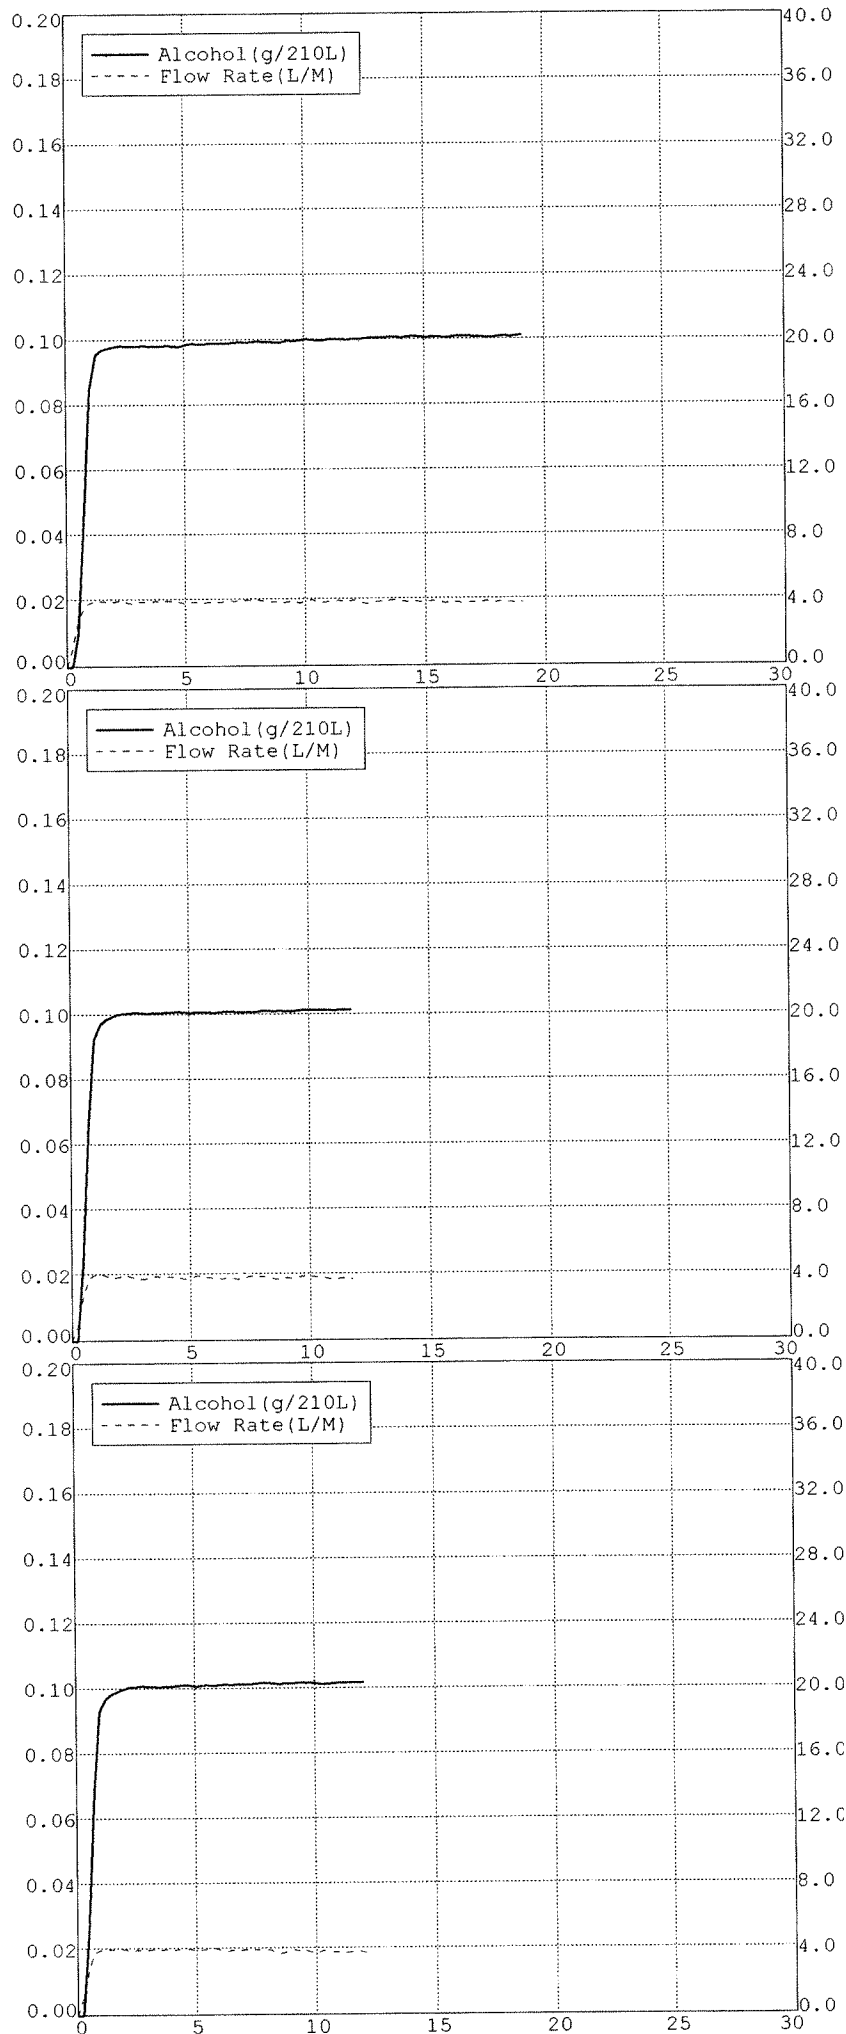

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/16/2025

OPERATOR NAME:
JULIA C ENNIS
Permit #: 55296
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25250

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:04
INTERNAL STANDARD	VERIFIED	18:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:05
BLANK TEST	0.00	18:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:06
BLANK TEST	0.00	18:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:07
BLANK TEST	0.00	18:08

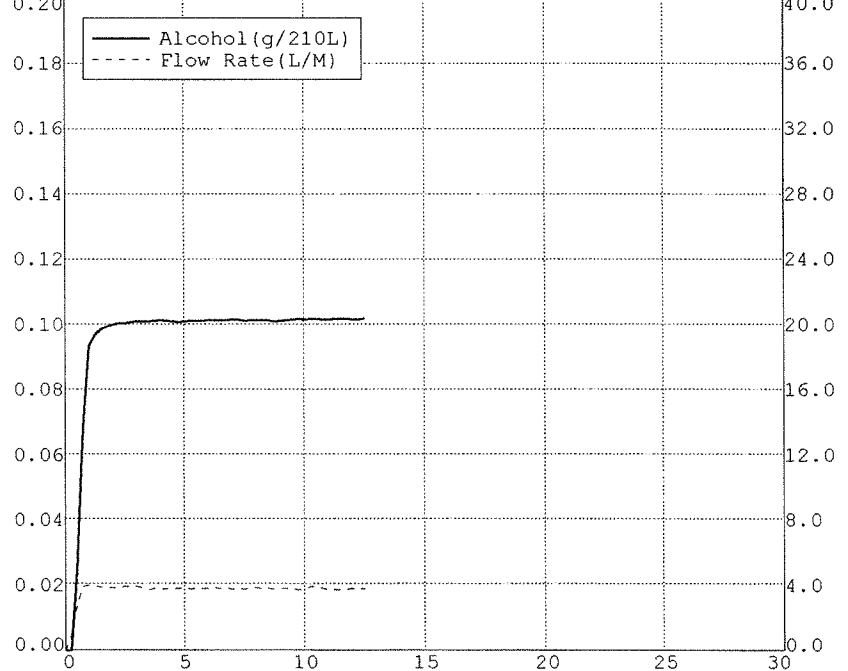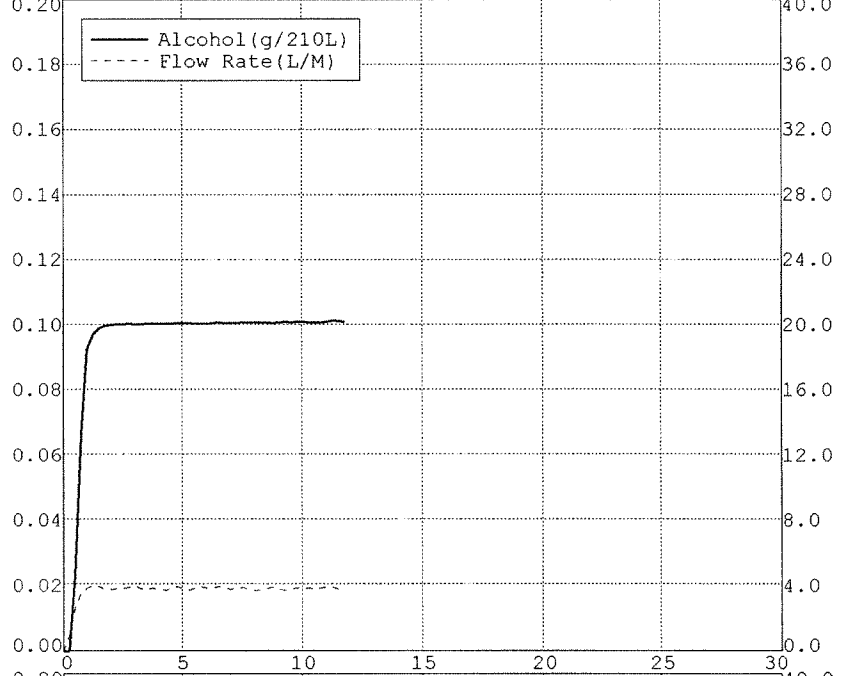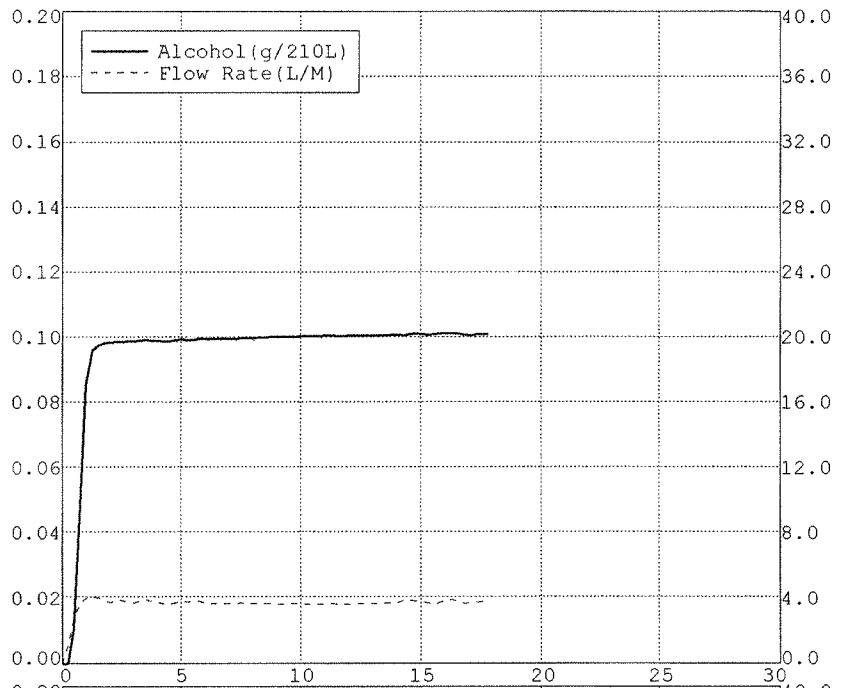

SUPERVISOR TEST


LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/23/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25250

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:16
INTERNAL STANDARD	VERIFIED	12:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:17
BLANK TEST	0.00	12:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:18
BLANK TEST	0.00	12:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:19
BLANK TEST	0.00	12:20

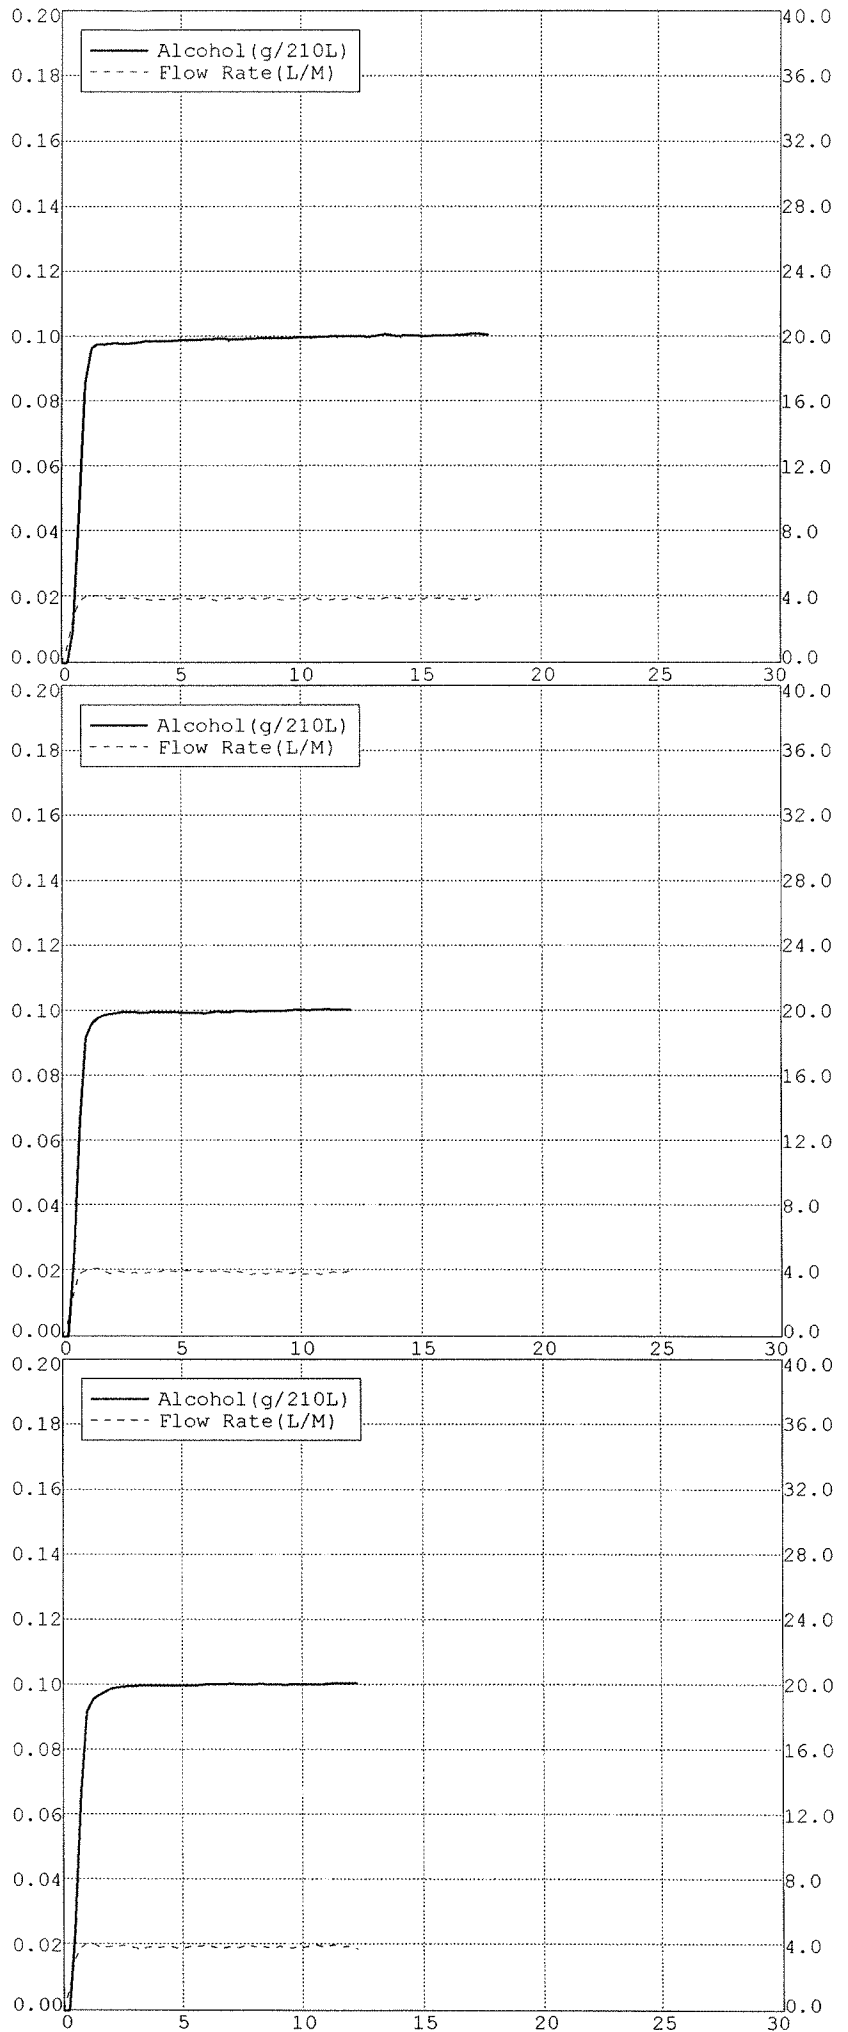

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/30/2025

OPERATOR NAME:
JULIA C ENNIS
Permit #: 55296
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25330

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:05
INTERNAL STANDARD	VERIFIED	19:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:06
BLANK TEST	0.00	19:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:07
BLANK TEST	0.00	19:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:08
BLANK TEST	0.00	19:09

