

SOLUTION CHANGE




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 12/02/2019

OPERATOR NAME:  
DORAN H SORRELL  
Permit #: 47507  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:33
INTERNAL STANDARD	VERIFIED	18:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:34
BLANK TEST	0.00	18:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:35
BLANK TEST	0.00	18:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:36
BLANK TEST	0.00	18:37

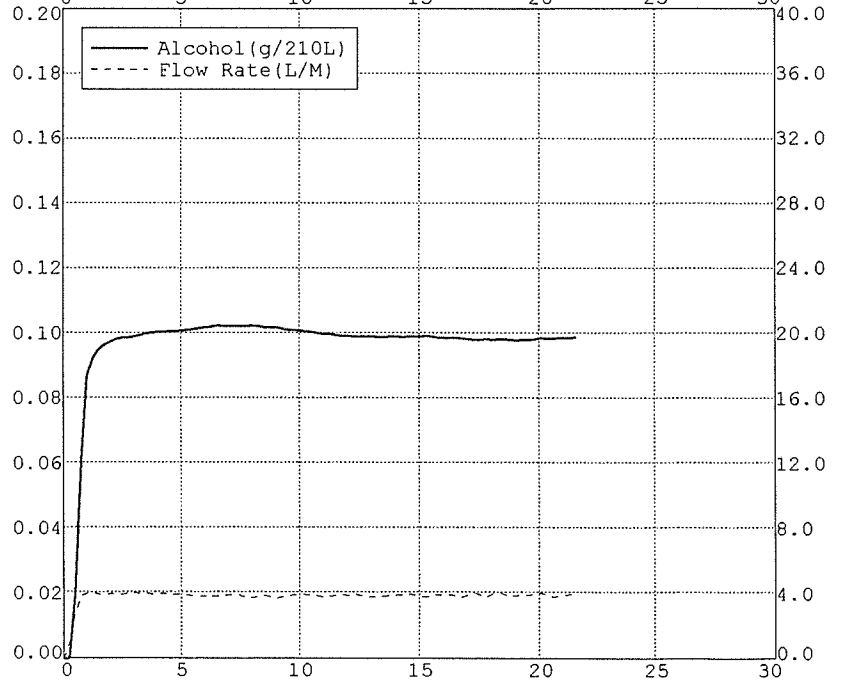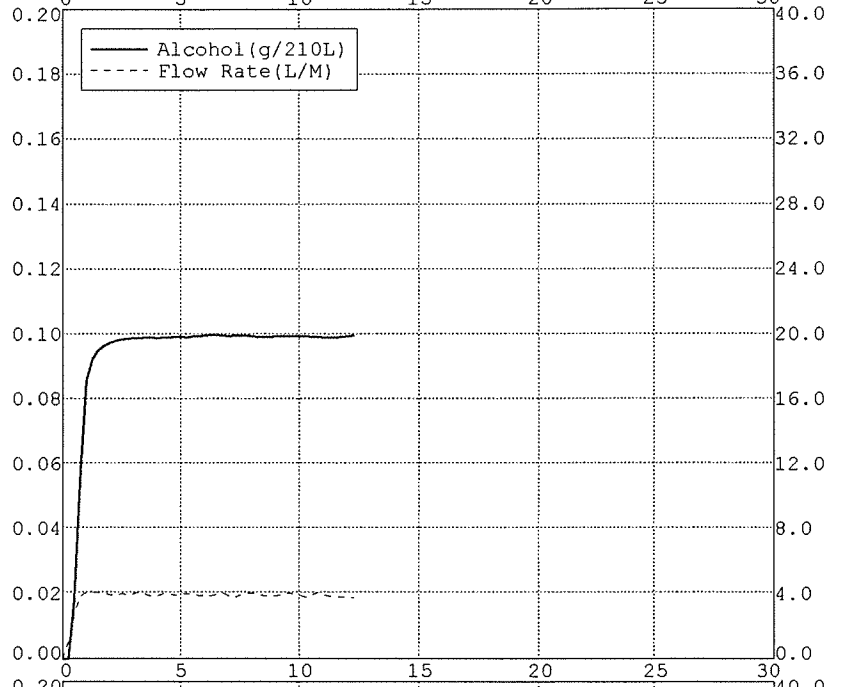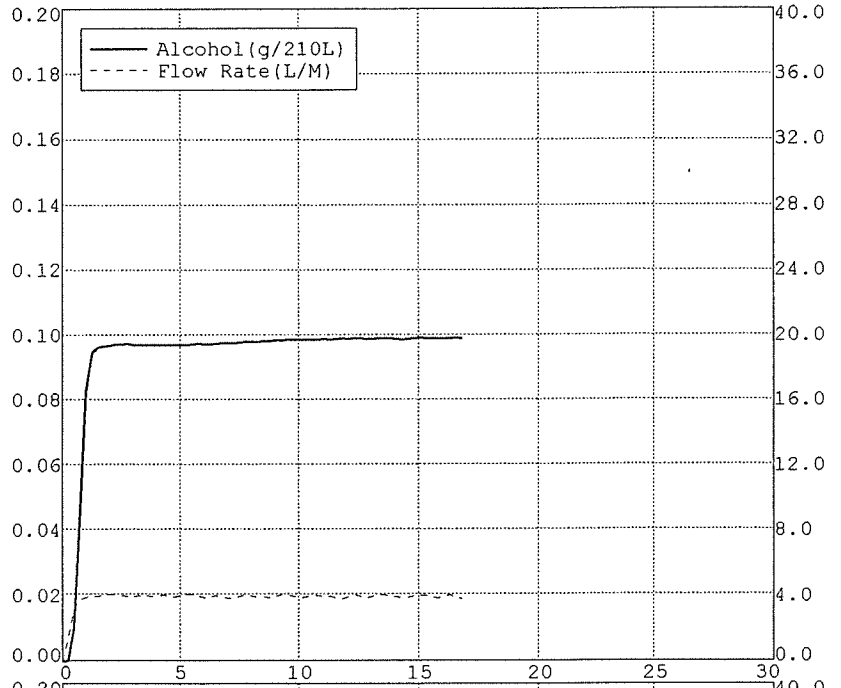

SUPERVISOR TEST




-----  
LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290  
-----

Date: 12/09/2019

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:32
INTERNAL STANDARD	VERIFIED	15:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:33
BLANK TEST	0.00	15:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:34
BLANK TEST	0.00	15:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:35
BLANK TEST	0.00	15:36

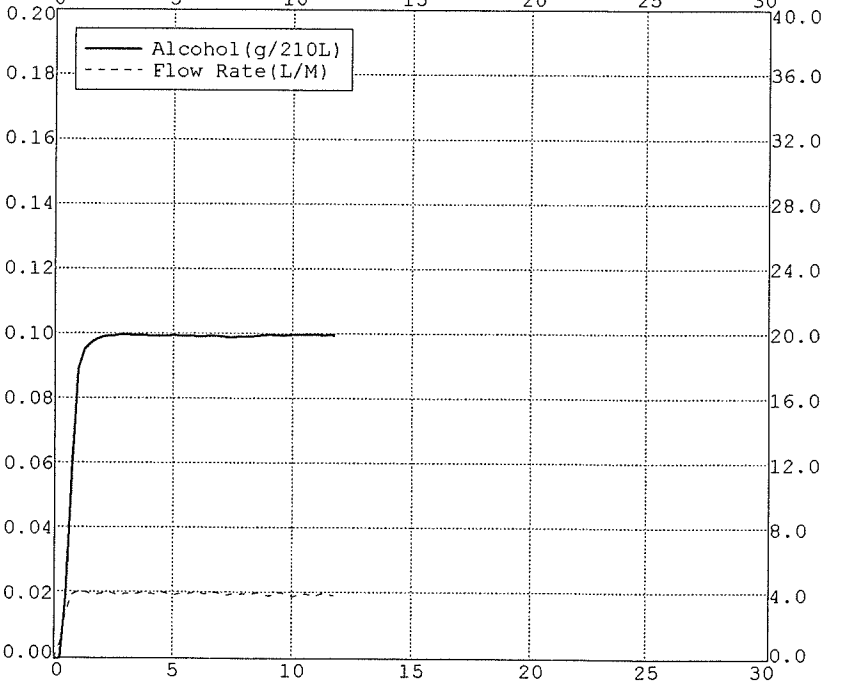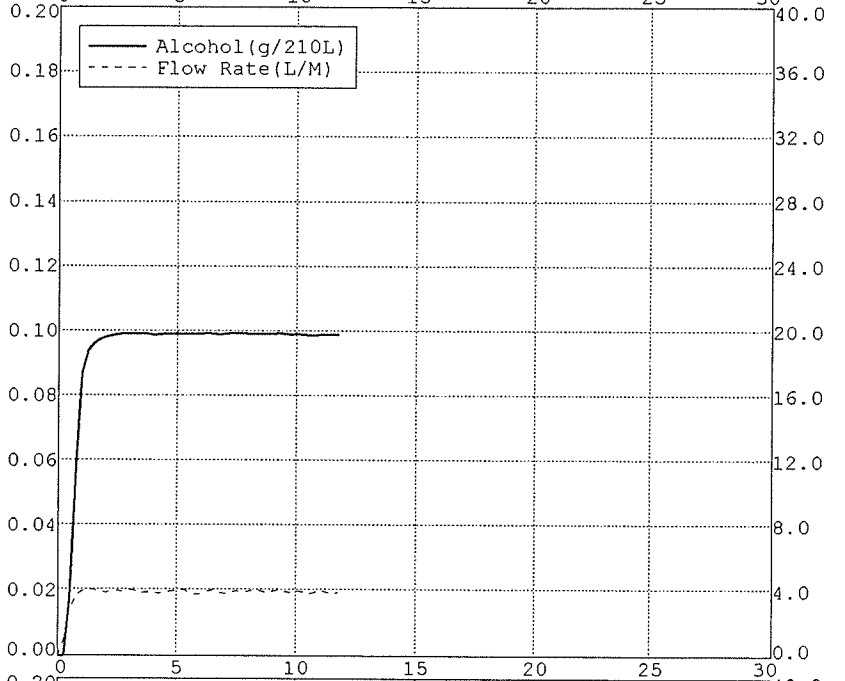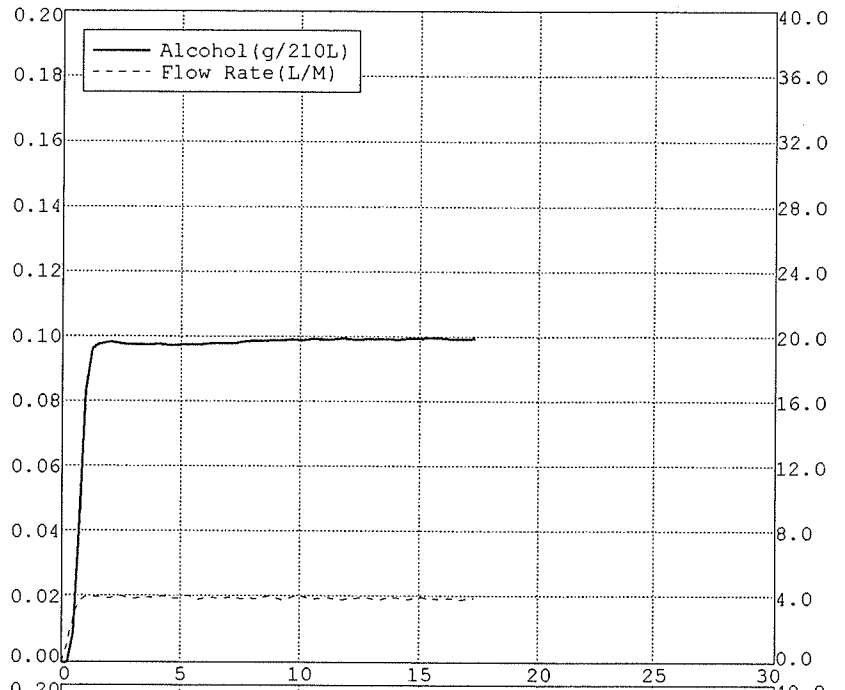

SUPERVISOR TEST



LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 12/15/2019

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:55
INTERNAL STANDARD	VERIFIED	11:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:56
BLANK TEST	0.00	11:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:57
BLANK TEST	0.00	11:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:58
BLANK TEST	0.00	11:59

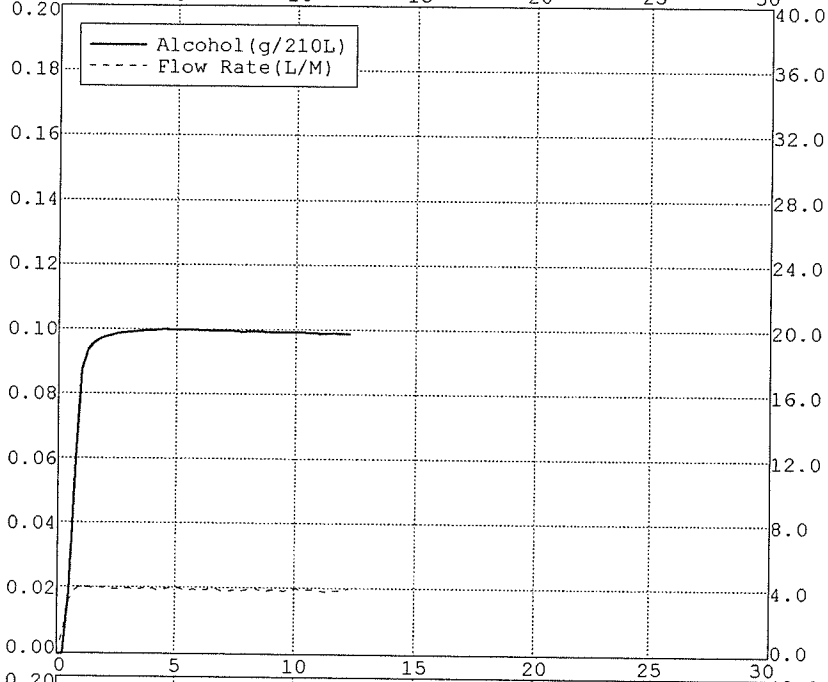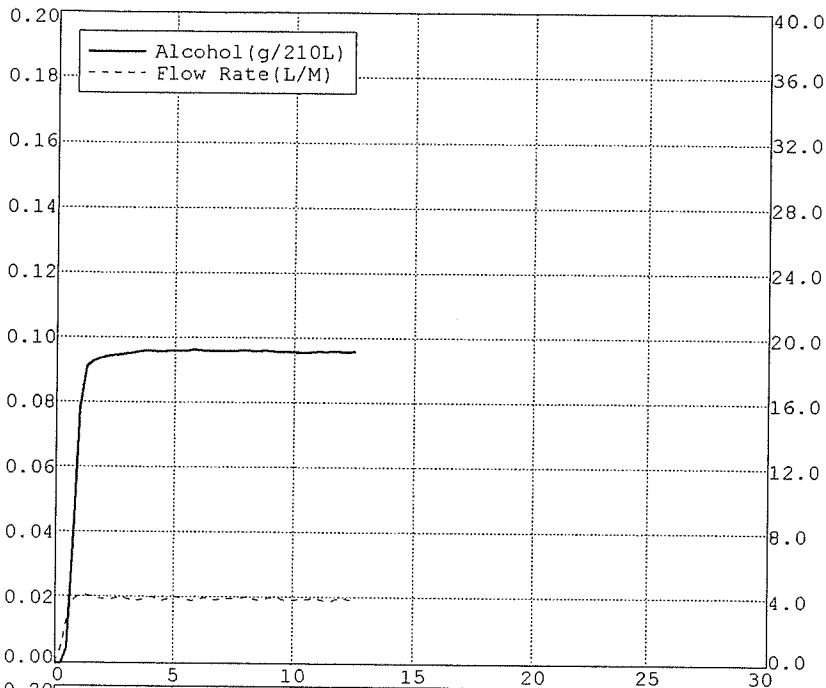

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 12/23/2019

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:34
INTERNAL STANDARD	VERIFIED	06:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:35
BLANK TEST	0.00	06:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:36
BLANK TEST	0.00	06:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:37
BLANK TEST	0.00	06:38

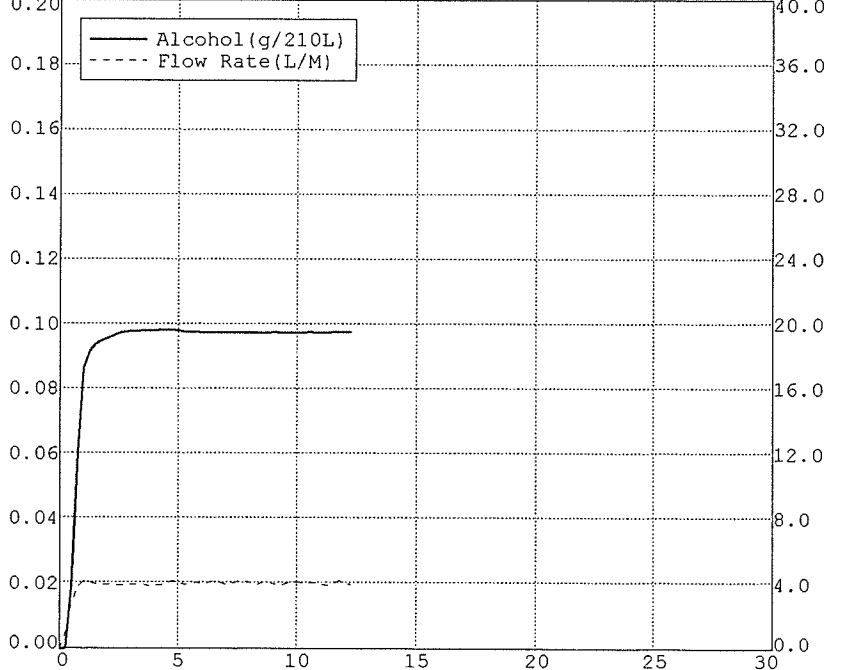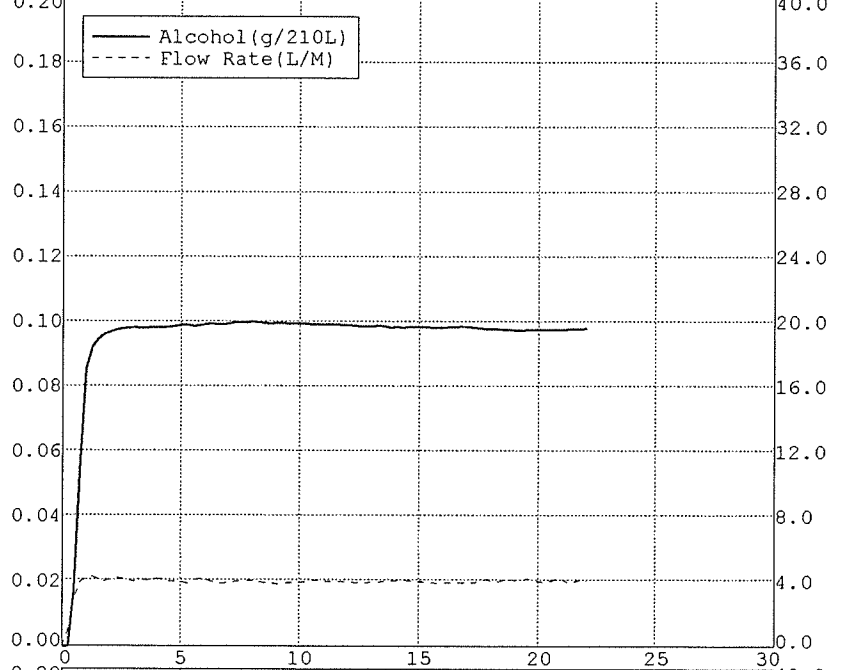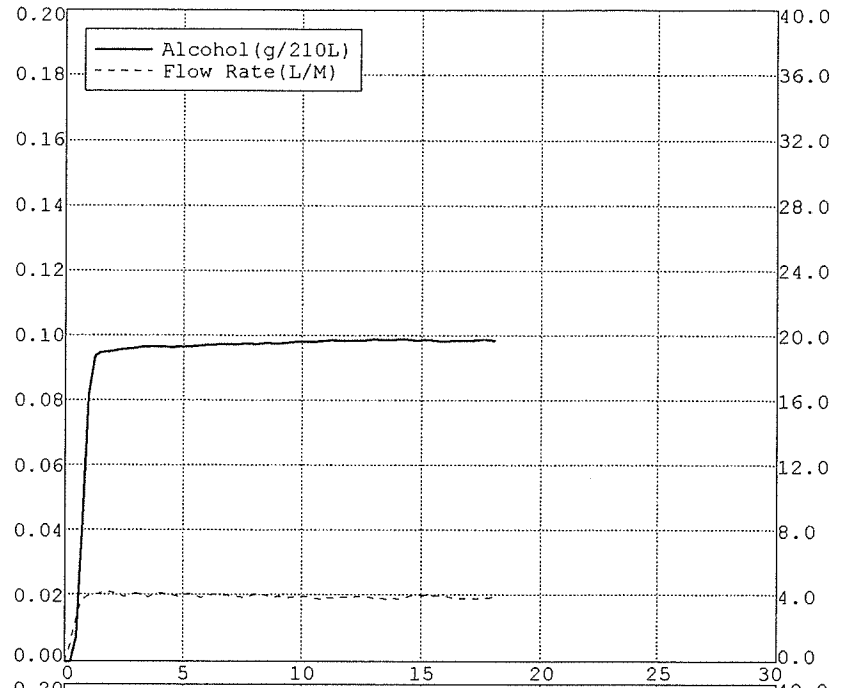

SUPERVISOR TEST

LAKE PLACID VILLAGE  
 POLICE DEPT.  
 DATAMASTER dmt: 100290

Date: 12/29/2019

OPERATOR NAME:  
 CHAD P BLINN  
 Permit #: 33034  
 Operator Agency/Dept: LAKE PLACID VILL. PD  
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:04
INTERNAL STANDARD	VERIFIED	09:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:05
BLANK TEST	0.00	09:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:06
BLANK TEST	0.00	09:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:07
BLANK TEST	0.00	09:08

