

SOLUTION CHANGE




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 12/01/2024

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24350

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:09
INTERNAL STANDARD	VERIFIED	07:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:09
BLANK TEST	0.00	07:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:11
BLANK TEST	0.00	07:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:12
BLANK TEST	0.00	07:13

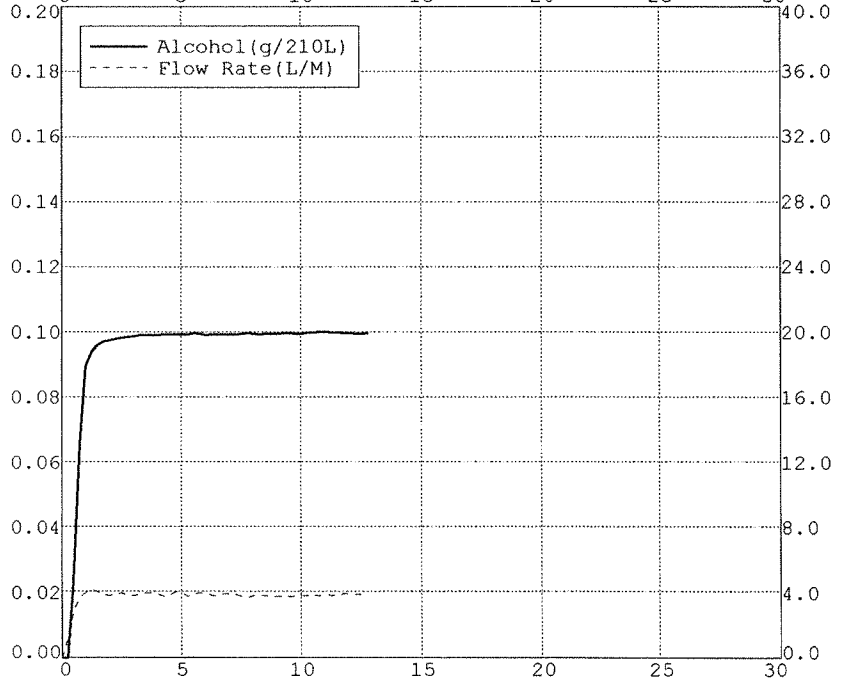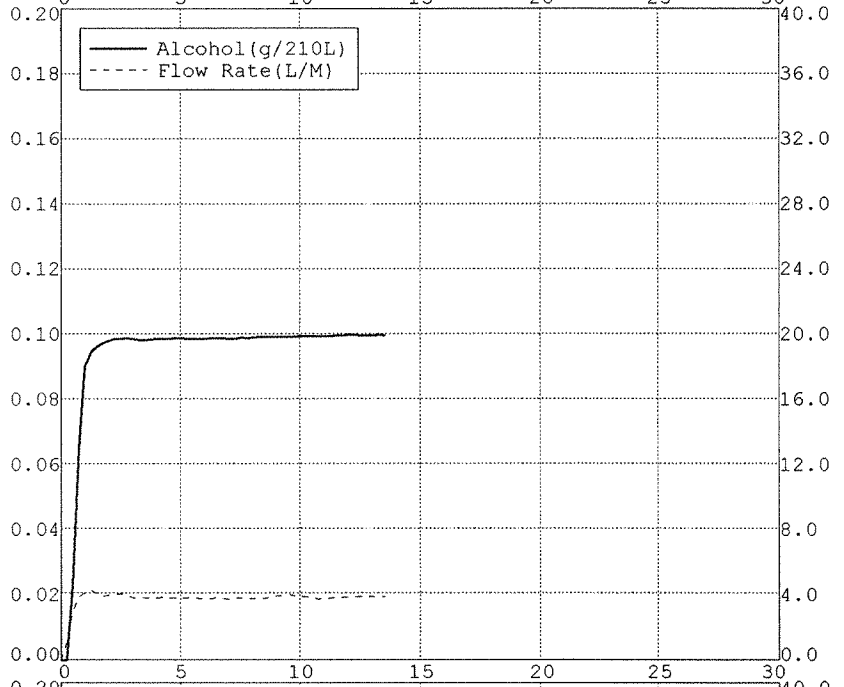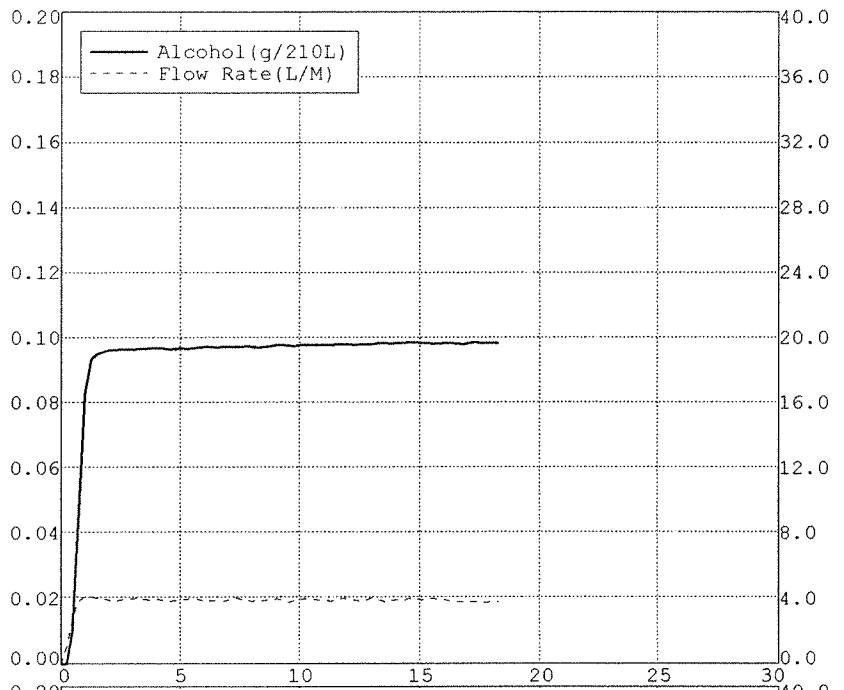

SUPERVISOR TEST




LAKE PLACID VILLAGE
 POLICE DEPT.
 DATAMASTER dmt: 100290

Date: 12/08/2024

OPERATOR NAME:
 CHAD P BLINN
 Permit #: 33034
 Operator Agency/Dept: LAKE PLACID VILL. PD
 Reference Standard #: 24350

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:10
INTERNAL STANDARD	VERIFIED	07:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:10
BLANK TEST	0.00	07:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:11
BLANK TEST	0.00	07:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:12
BLANK TEST	0.00	07:13

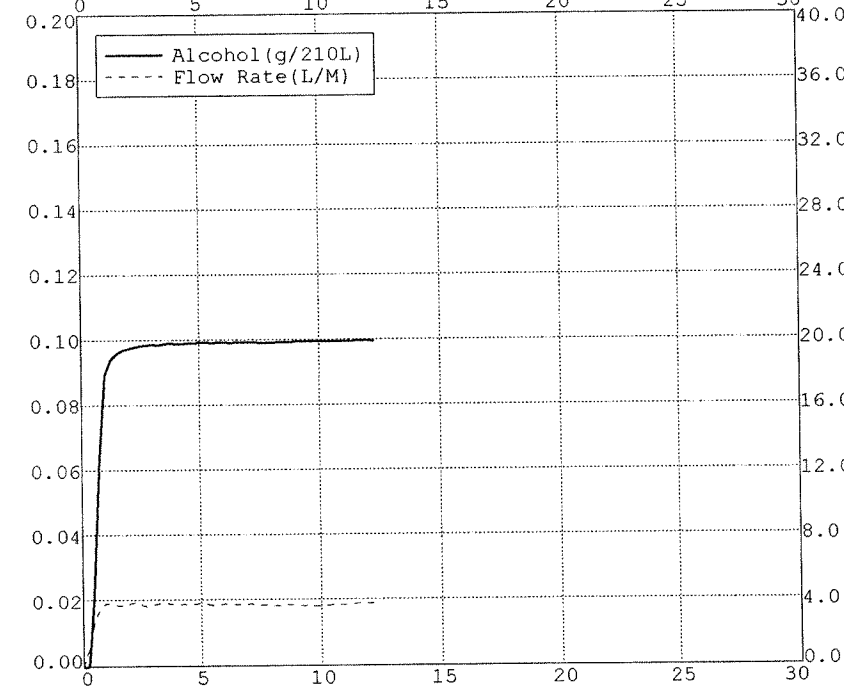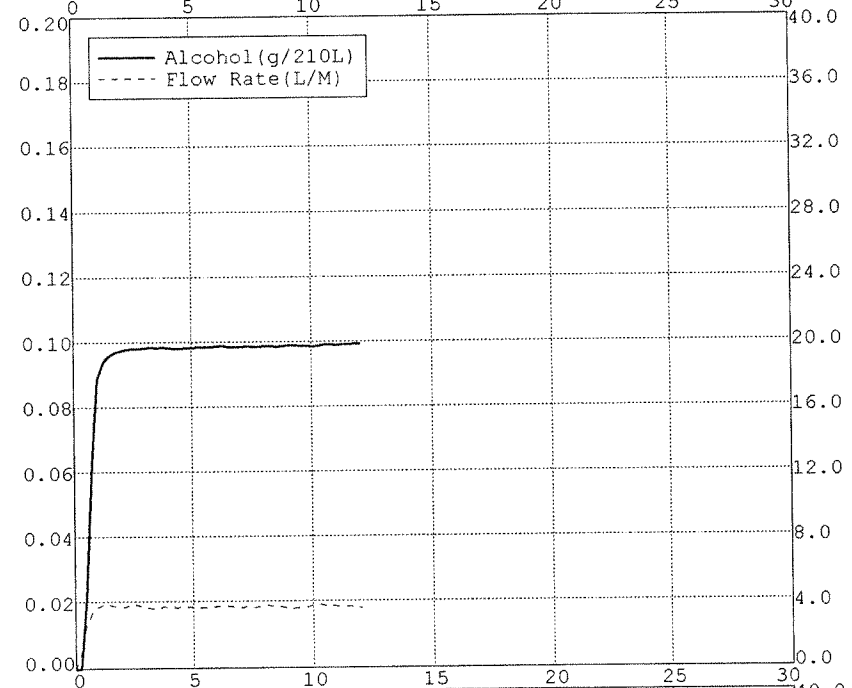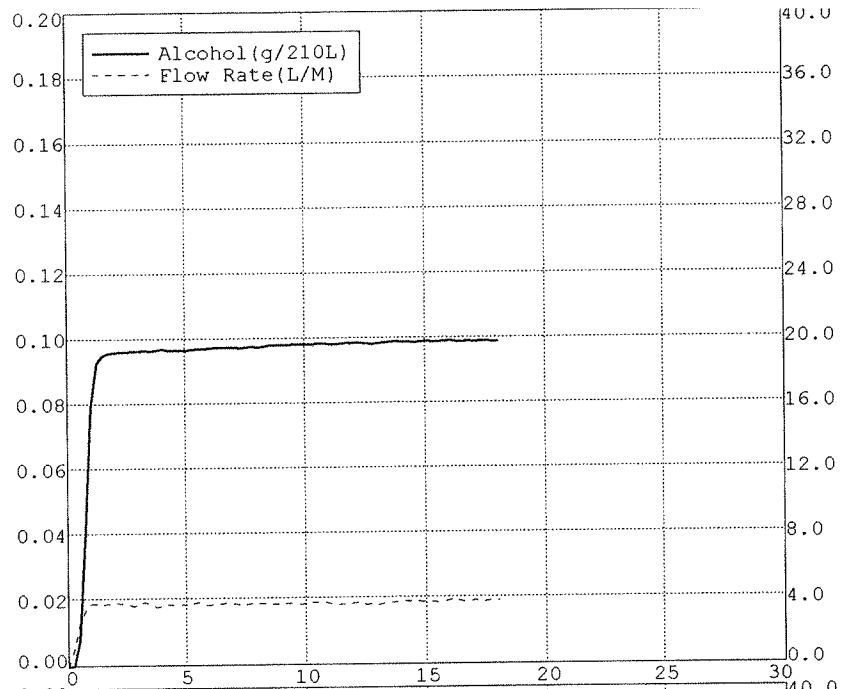

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 12/15/2024

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24350

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:00
INTERNAL STANDARD	VERIFIED	07:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:00
BLANK TEST	0.00	07:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:01
BLANK TEST	0.00	07:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:02
BLANK TEST	0.00	07:03

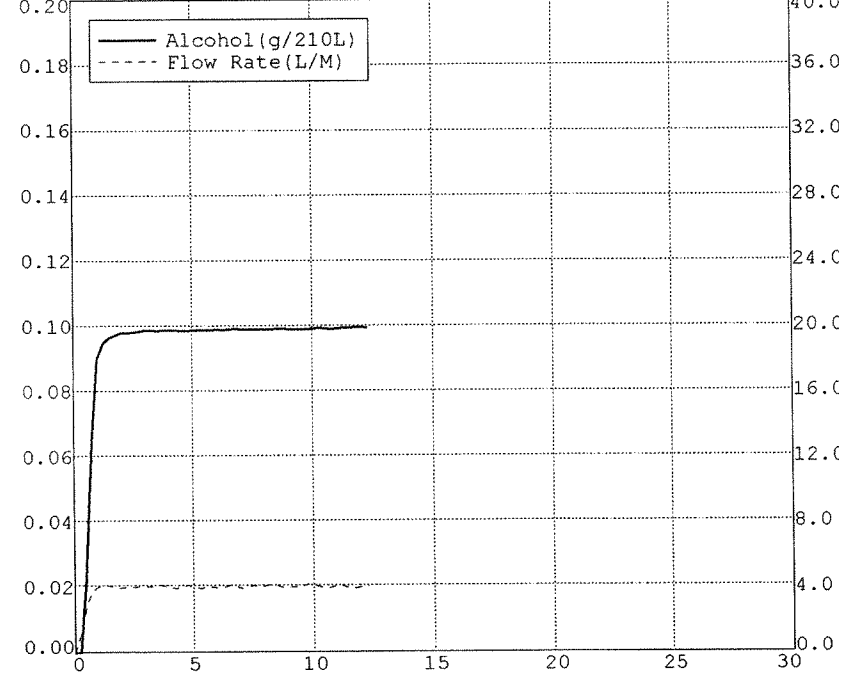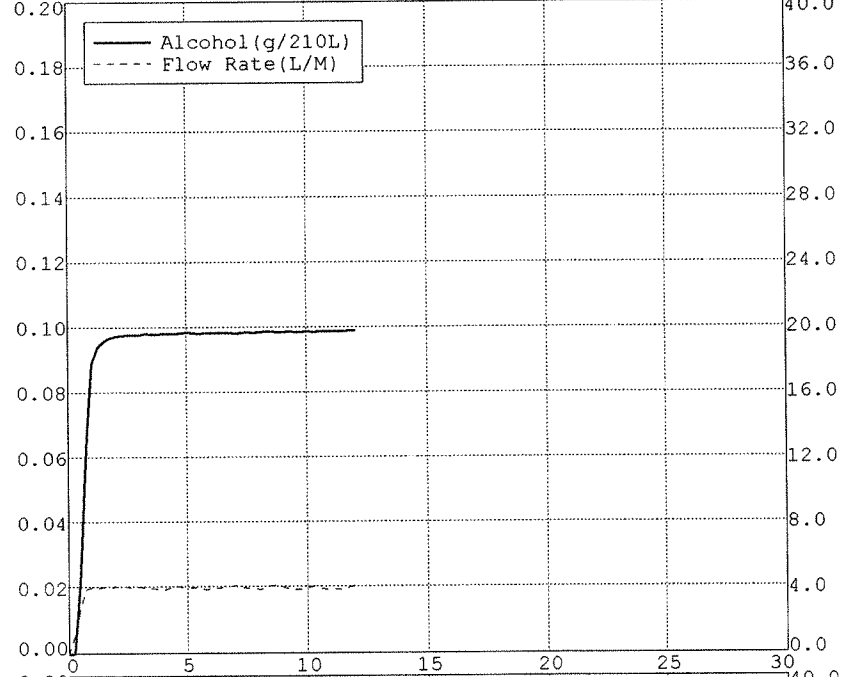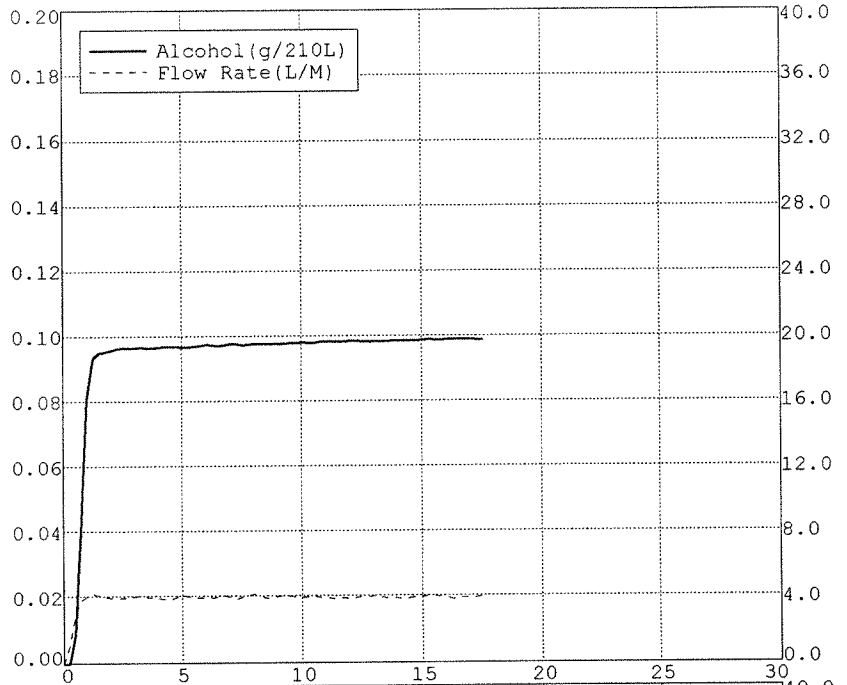

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 12/22/2024

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24350

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:00
INTERNAL STANDARD	VERIFIED	04:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:01
BLANK TEST	0.00	04:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:02
BLANK TEST	0.00	04:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:03
BLANK TEST	0.00	04:04

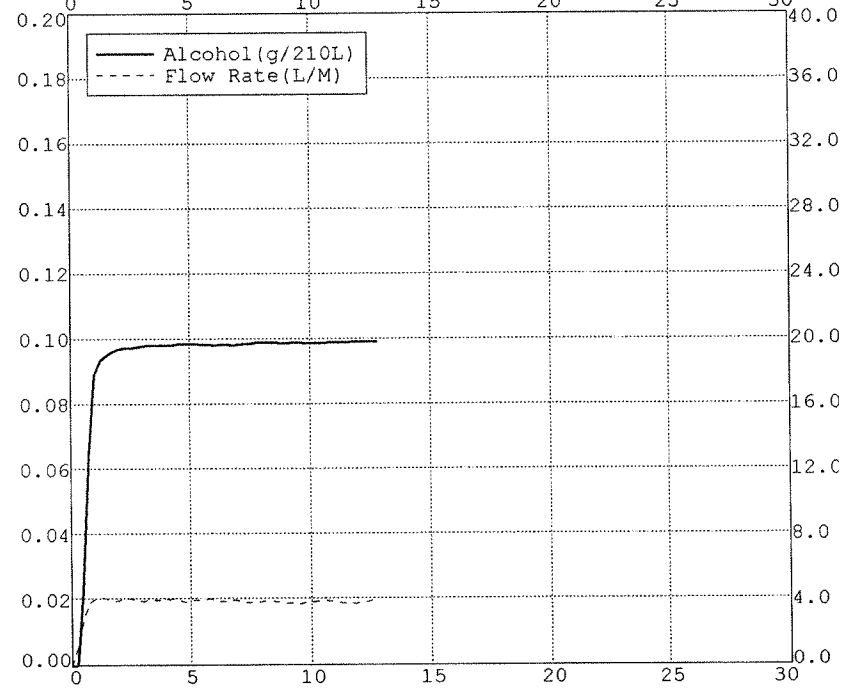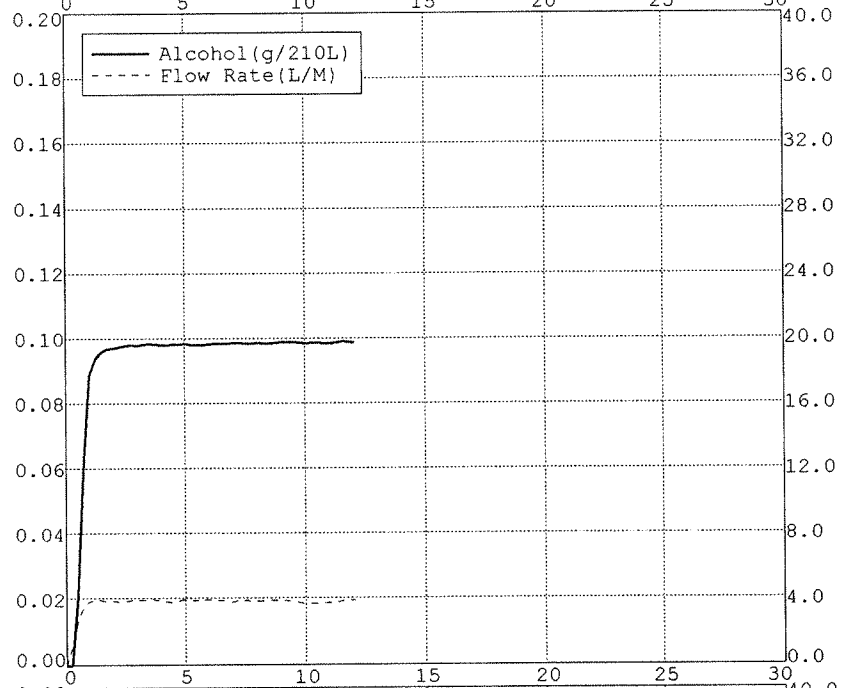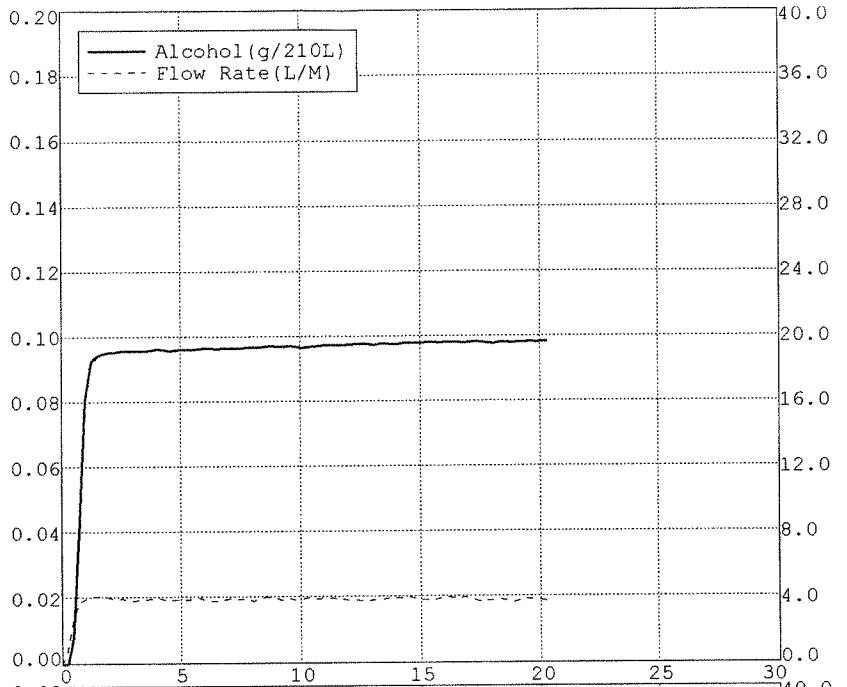

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290


Date: 12/29/2024

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24350

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:15
INTERNAL STANDARD	VERIFIED	17:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD INTERFERENCE		17:16

Interference Detected

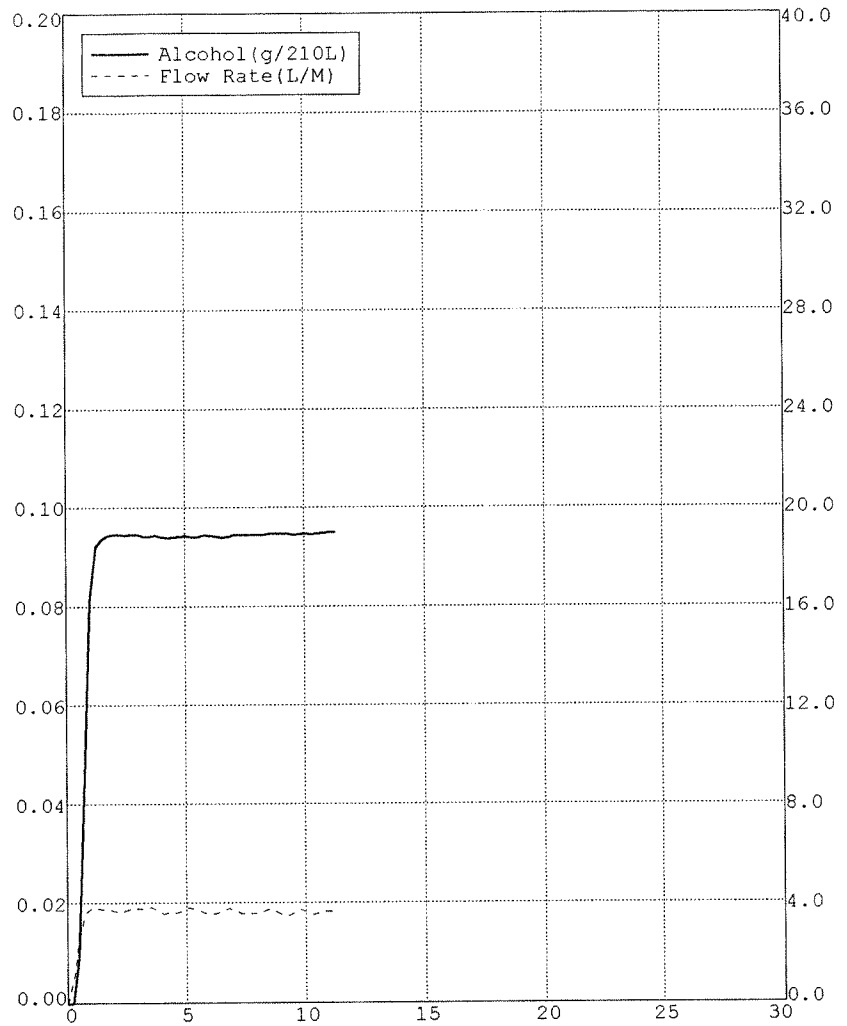

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 12/29/2024

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24350

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:18
INTERNAL STANDARD	VERIFIED	17:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:18
BLANK TEST	0.00	17:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:19
BLANK TEST	0.00	17:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:20
BLANK TEST	0.00	17:21

