

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/04/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:40
INTERNAL STANDARD	VERIFIED	11:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:40
BLANK TEST	0.00	11:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:41
BLANK TEST	0.00	11:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:42
BLANK TEST	0.00	11:43

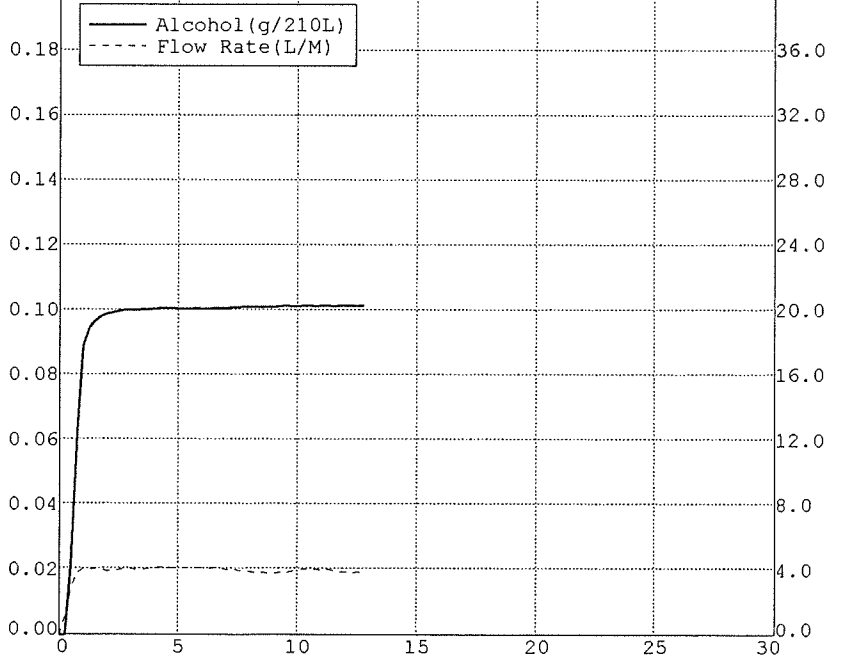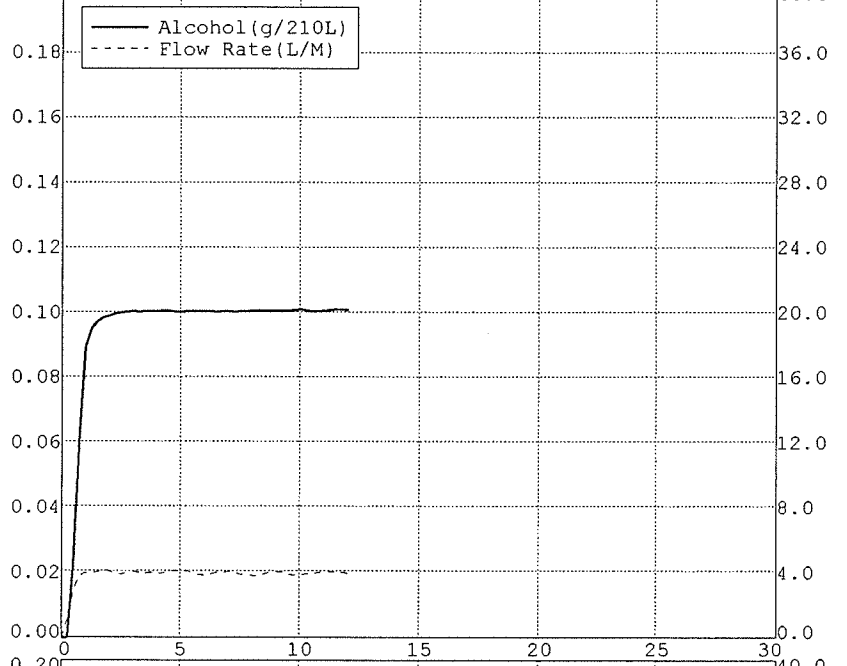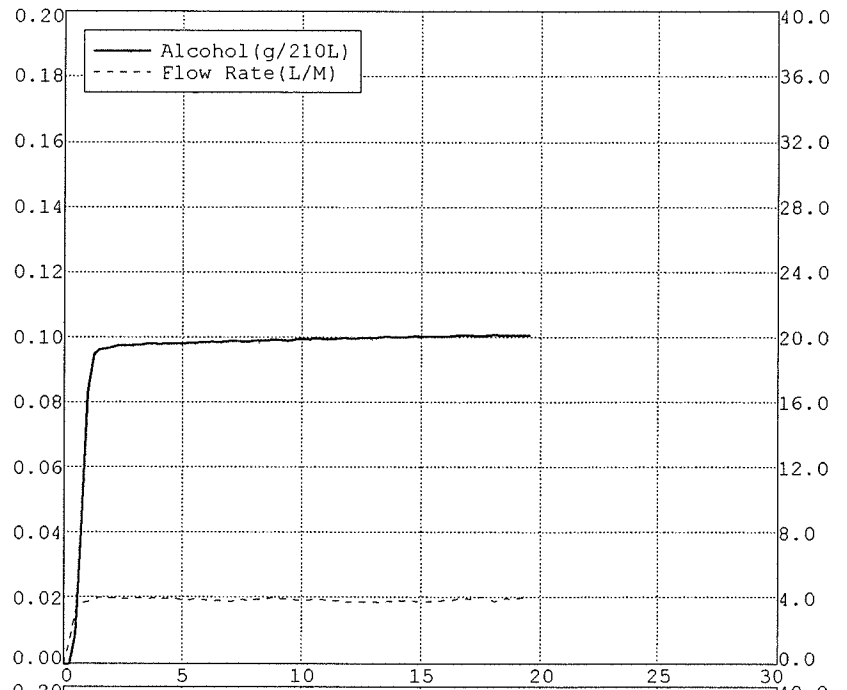

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/12/2021

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:02
INTERNAL STANDARD	VERIFIED	18:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:02
BLANK TEST	0.00	18:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:03
BLANK TEST	0.00	18:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:05
BLANK TEST	0.00	18:05

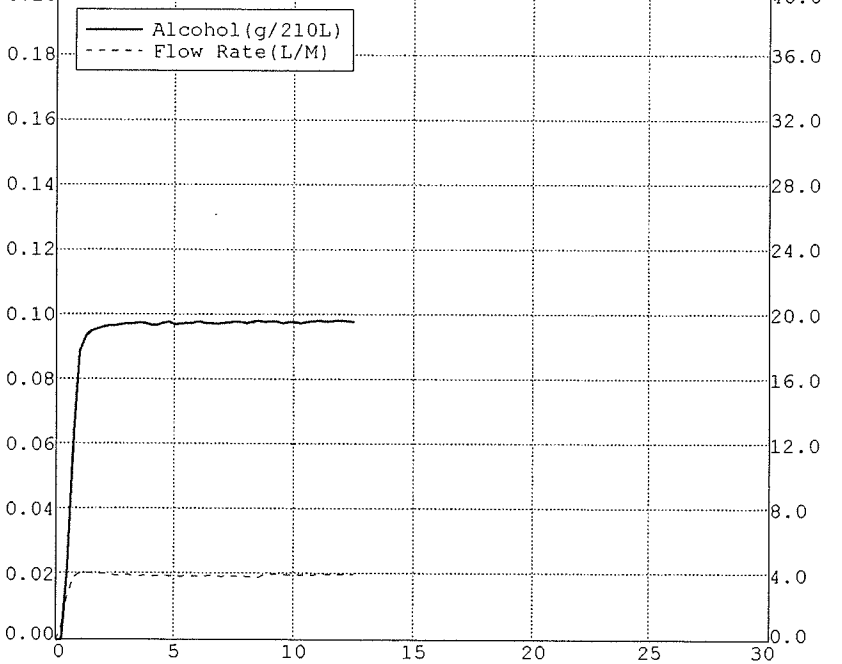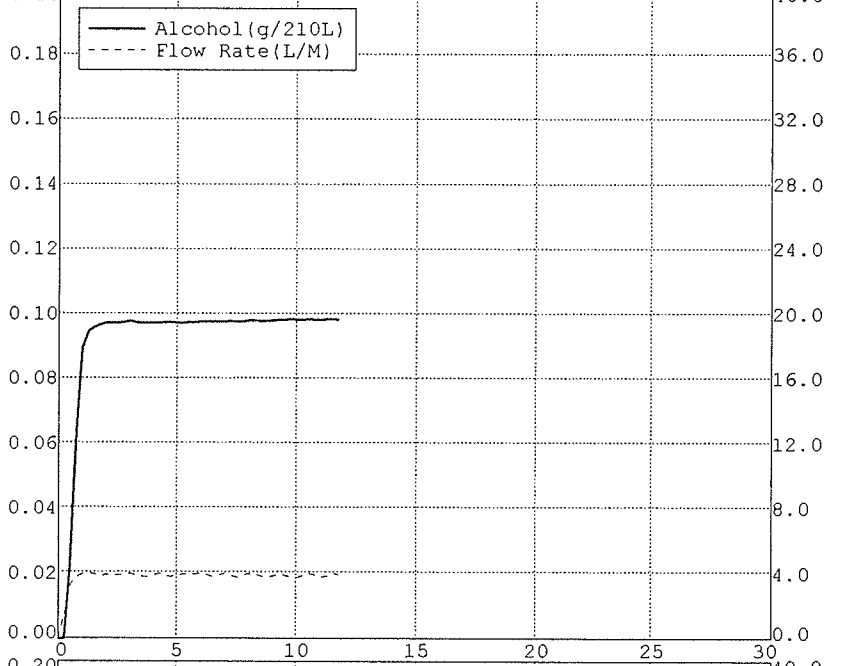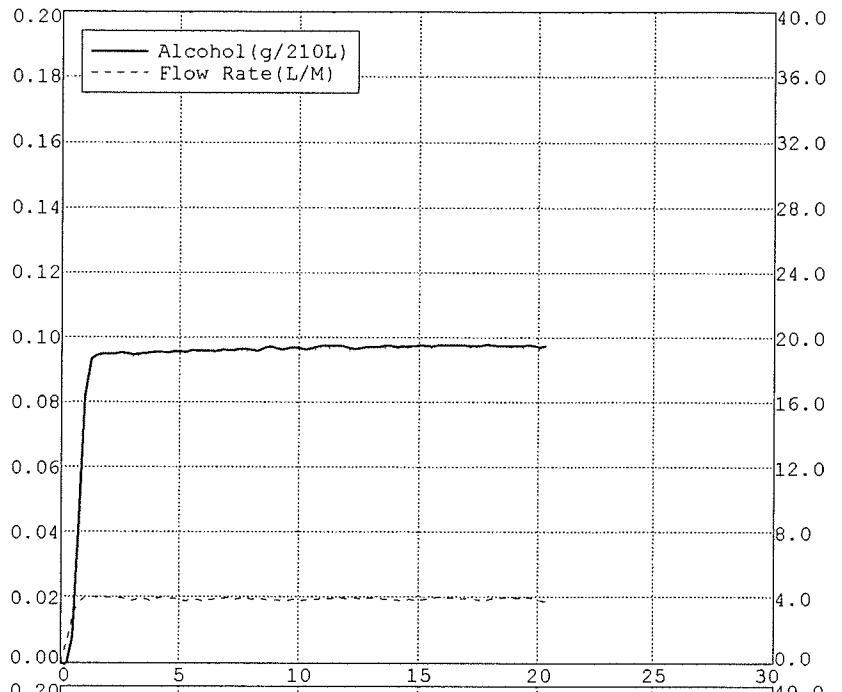

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/18/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:26
INTERNAL STANDARD	VERIFIED	09:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:26
BLANK TEST	0.00	09:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:27
BLANK TEST	0.00	09:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:28
BLANK TEST	0.00	09:29

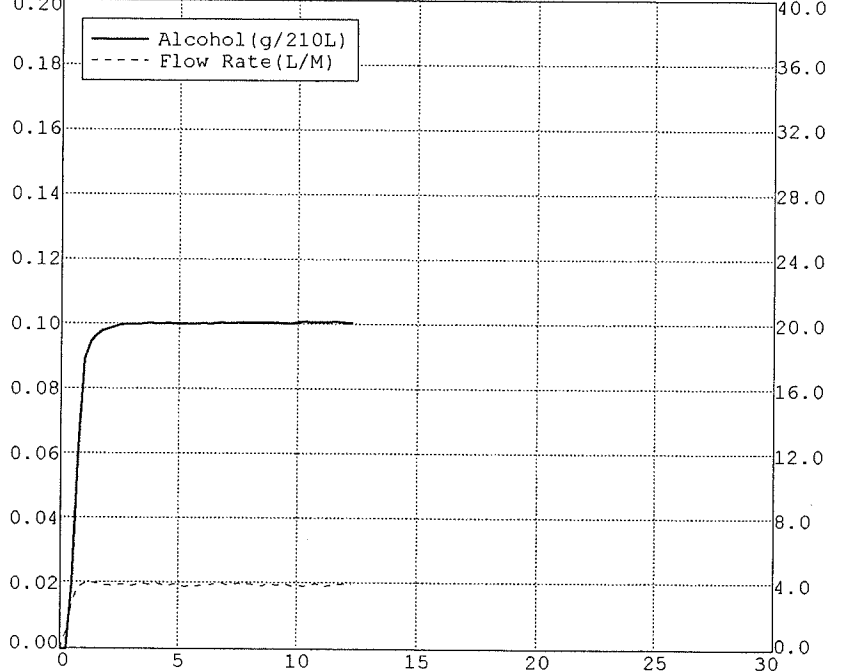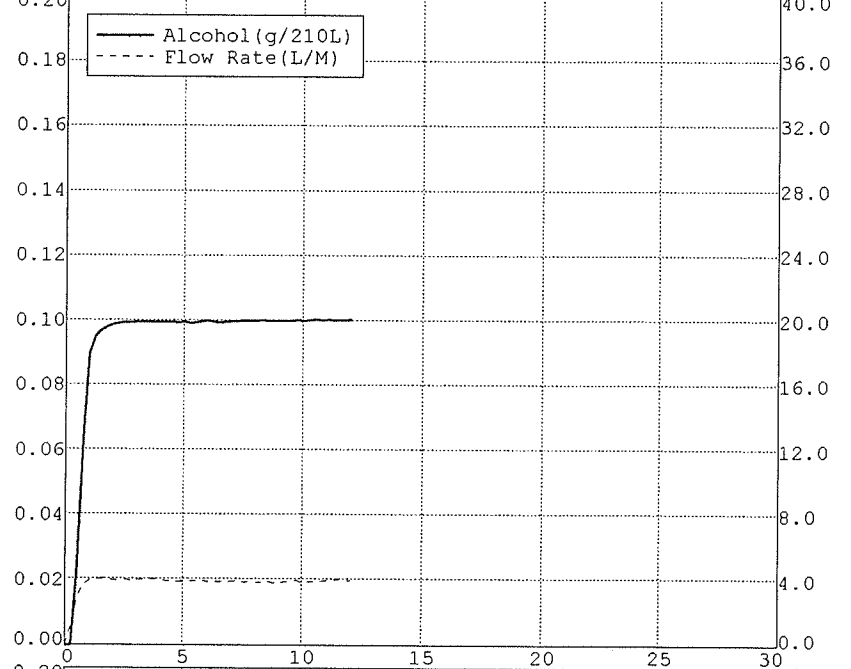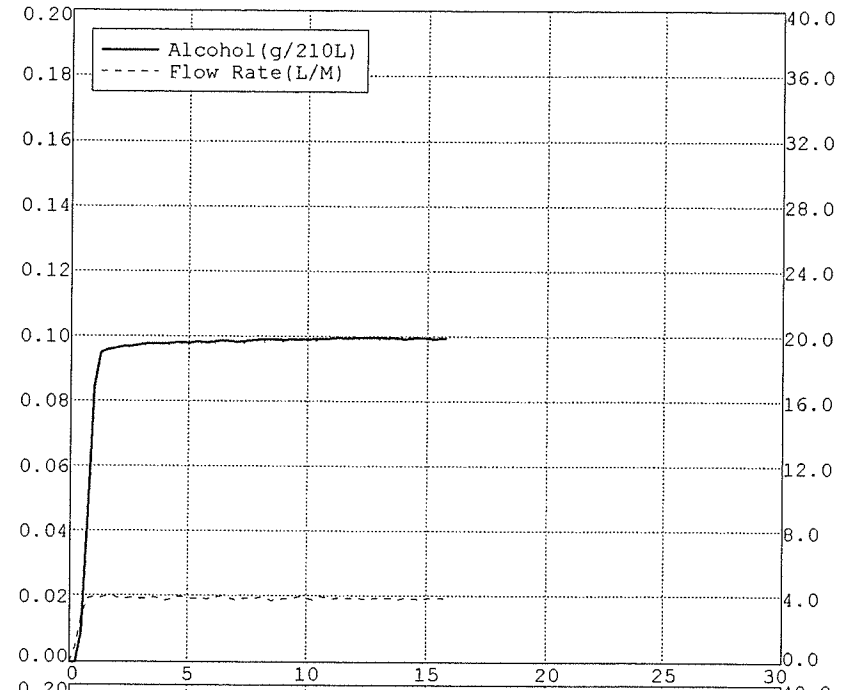

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/26/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:43
INTERNAL STANDARD	VERIFIED	17:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:43
BLANK TEST	0.00	17:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:44
BLANK TEST	0.00	17:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:46
BLANK TEST	0.00	17:46

