

SUPERVISOR TEST



LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 07/04/2021

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:05
INTERNAL STANDARD	VERIFIED	12:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:06
BLANK TEST	0.00	12:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:07
BLANK TEST	0.00	12:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:08
BLANK TEST	0.00	12:09

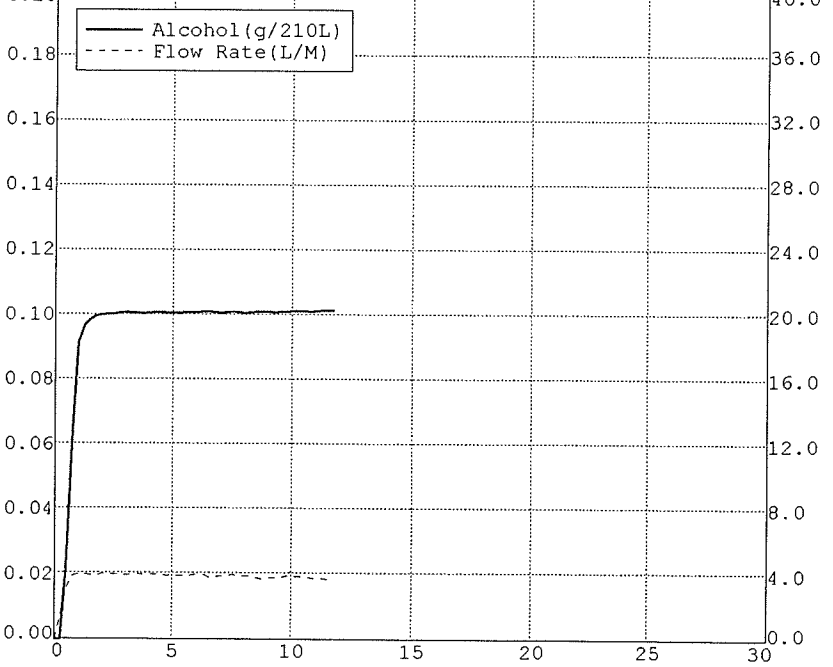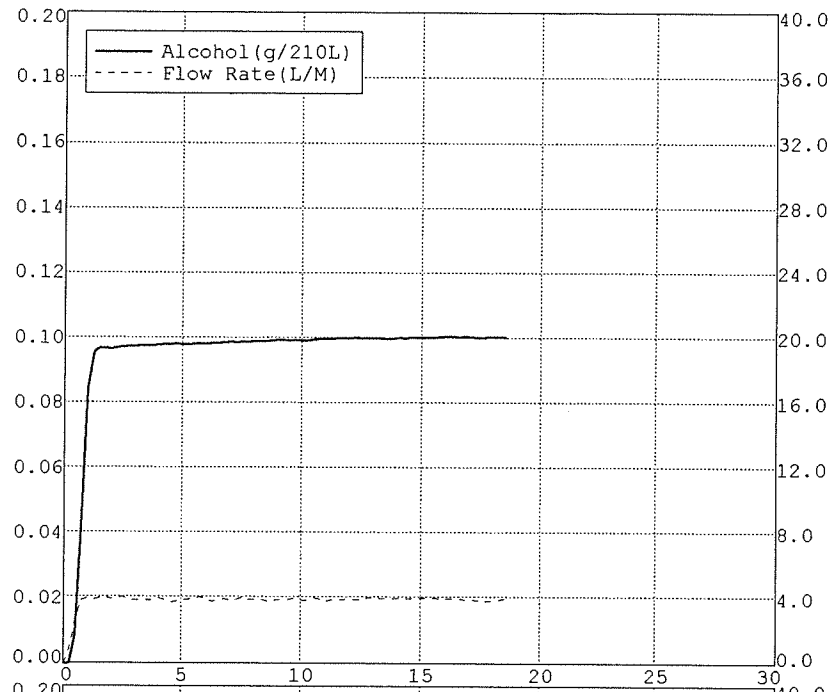

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 07/11/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:22
INTERNAL STANDARD	VERIFIED	07:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:23
BLANK TEST	0.00	07:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:24
BLANK TEST	0.00	07:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:25
BLANK TEST	0.00	07:26

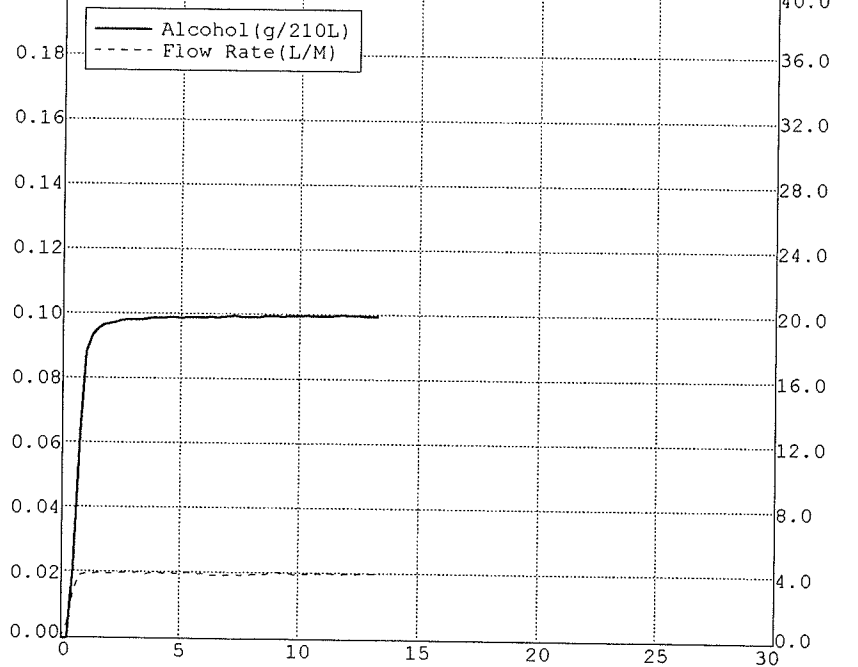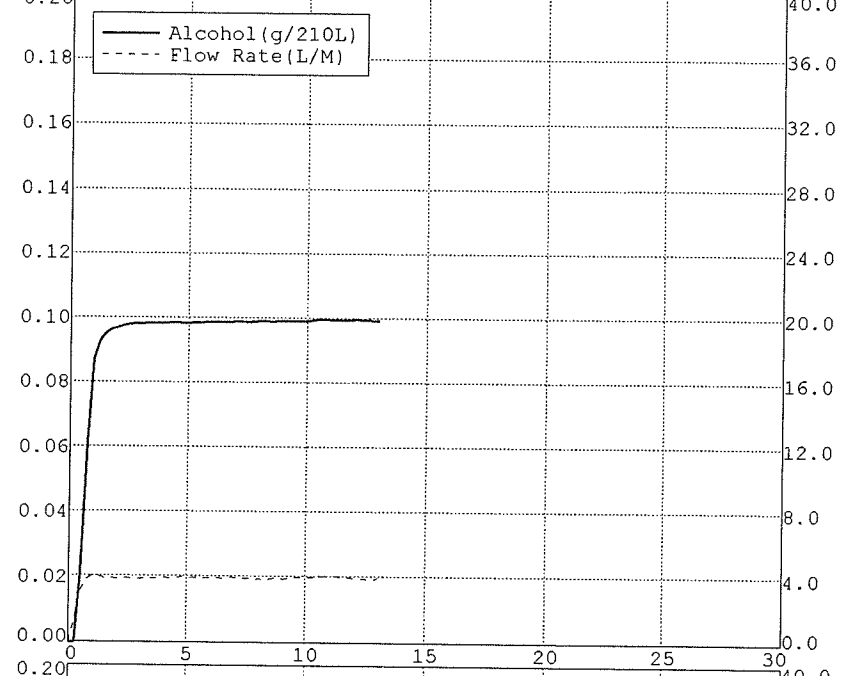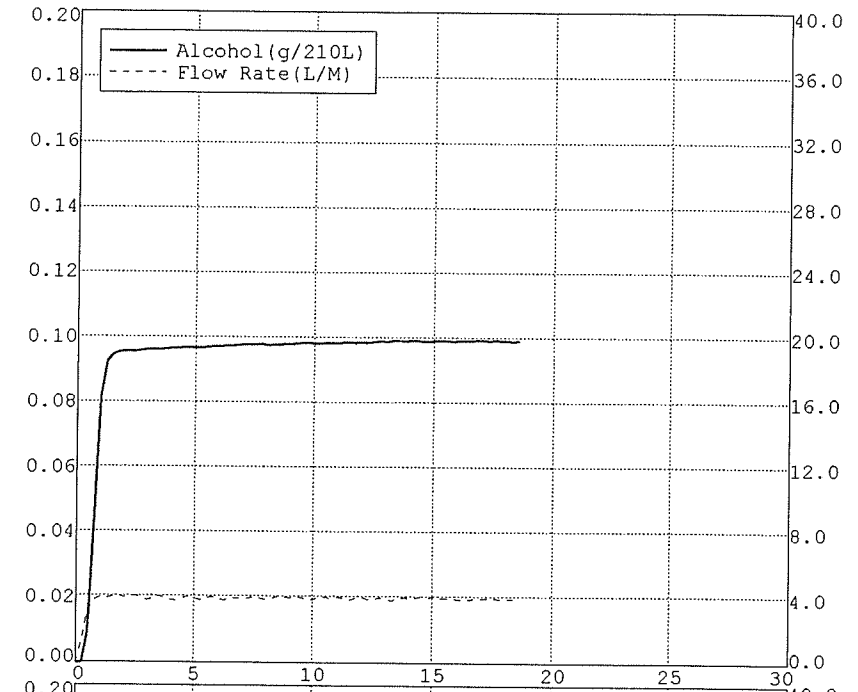

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 07/19/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:58
INTERNAL STANDARD	VERIFIED	06:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:58
BLANK TEST	0.00	06:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:00
BLANK TEST	0.00	07:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:01
BLANK TEST	0.00	07:02

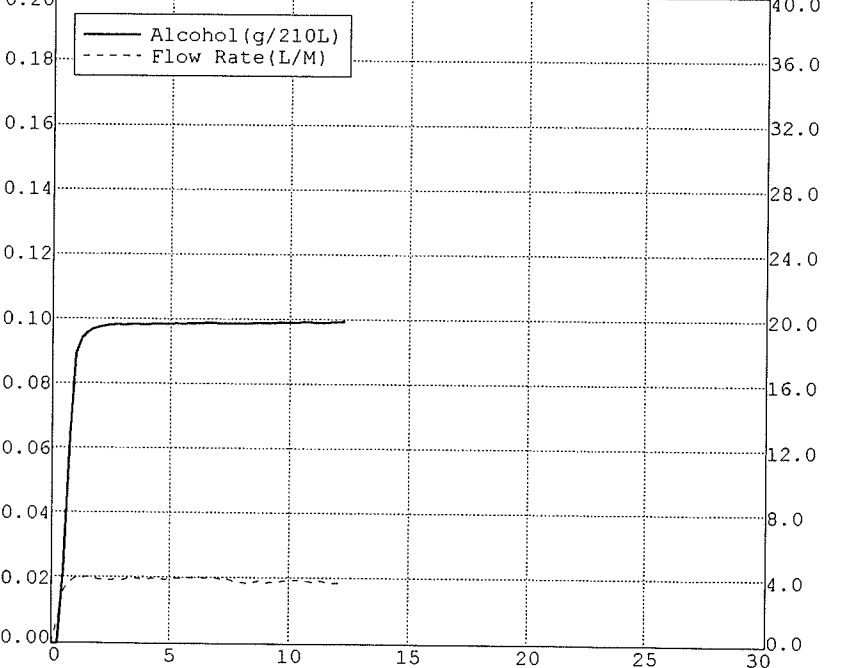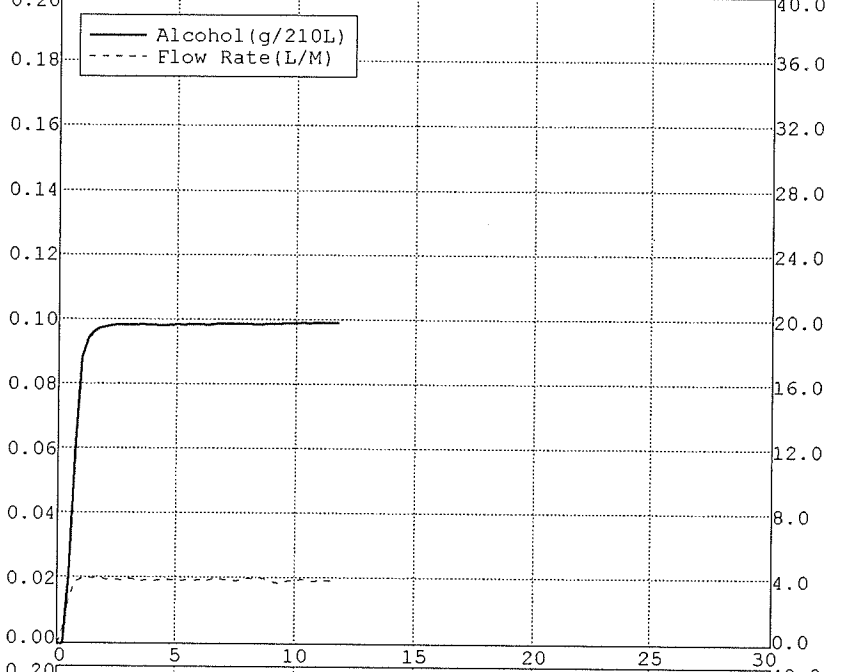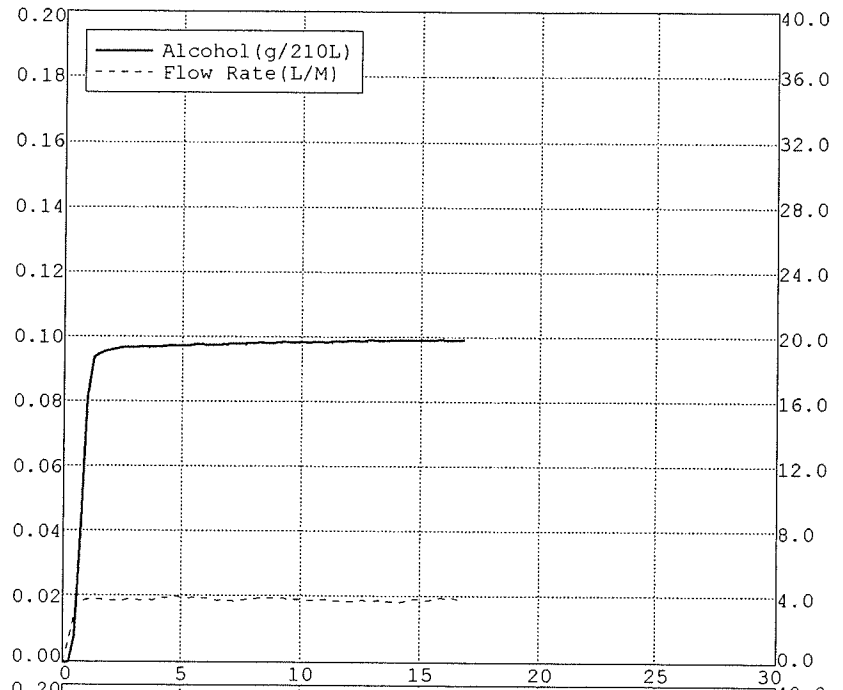

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 07/25/2021

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:23
INTERNAL STANDARD	VERIFIED	05:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:24
BLANK TEST	0.00	05:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:25
BLANK TEST	0.00	05:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:26
BLANK TEST	0.00	05:27

