

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 07/06/2020

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:49
INTERNAL STANDARD	VERIFIED	06:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:49
BLANK TEST	0.00	06:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:51
BLANK TEST	0.00	06:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:52
BLANK TEST	0.00	06:53

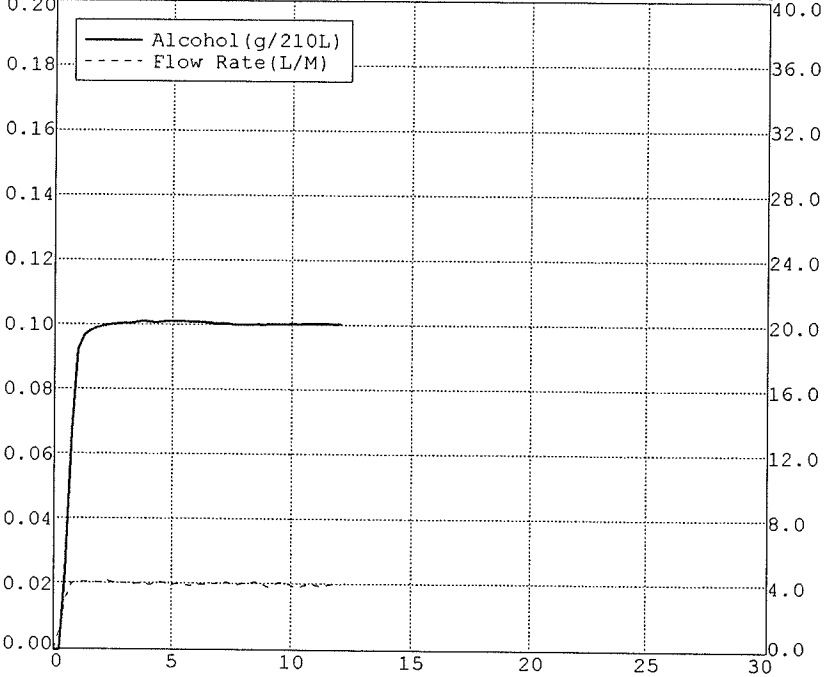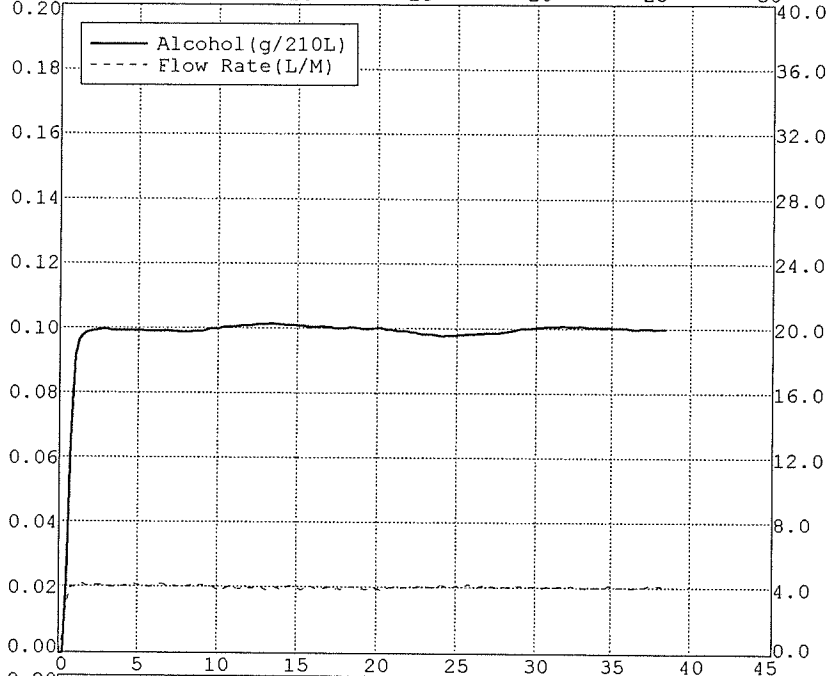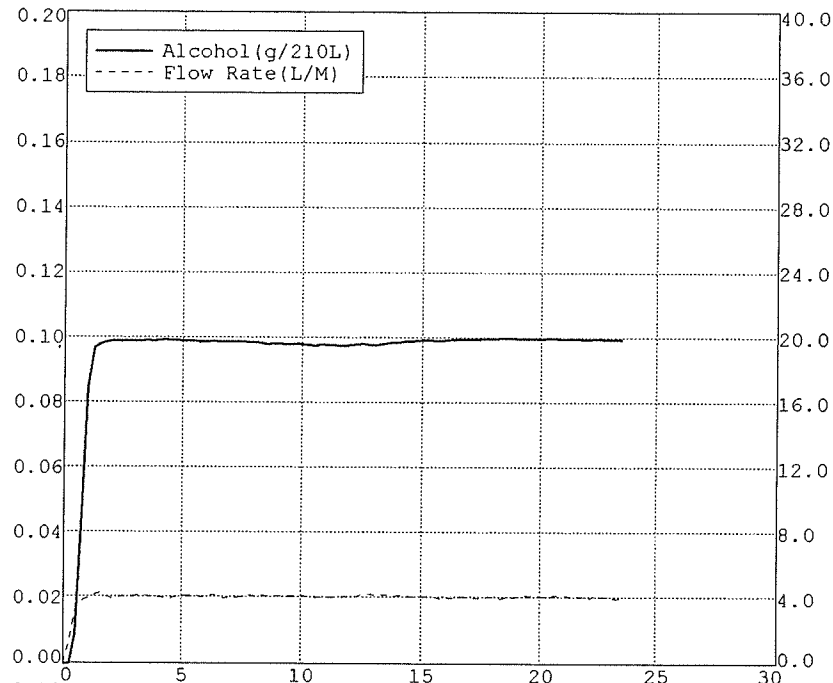

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 07/12/2020

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:19
INTERNAL STANDARD	VERIFIED	07:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:19
BLANK TEST	0.00	07:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:20
BLANK TEST	0.00	07:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:22
BLANK TEST	0.00	07:22

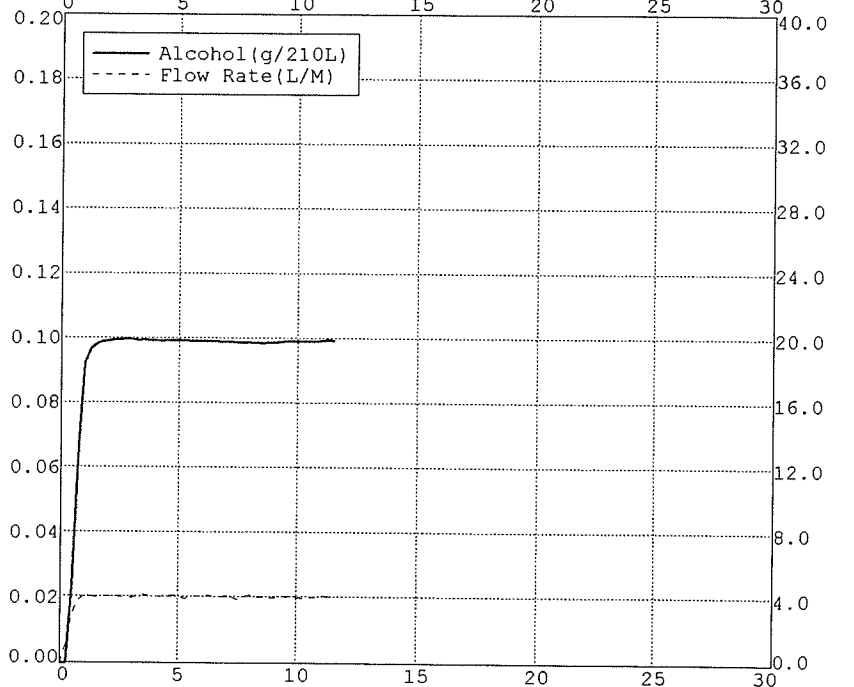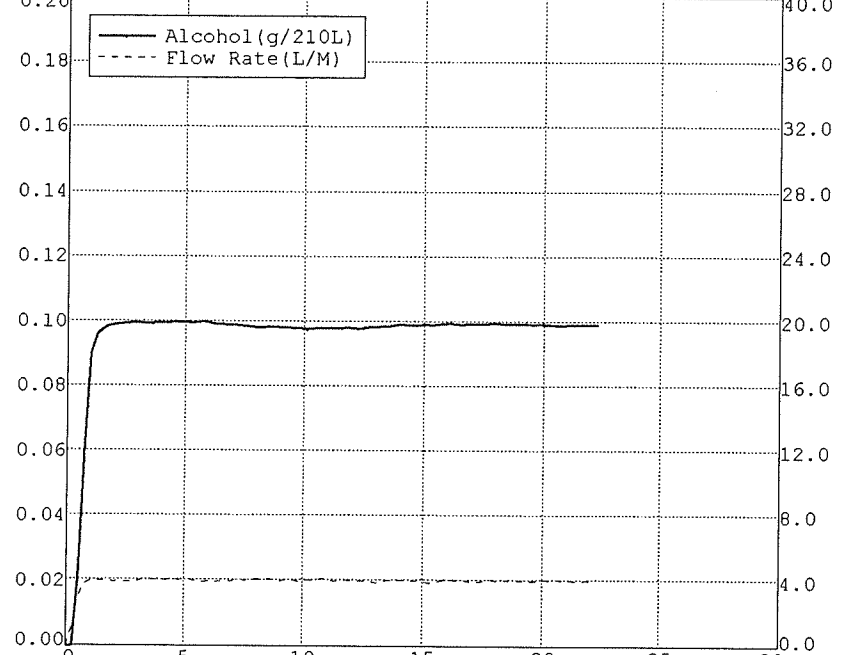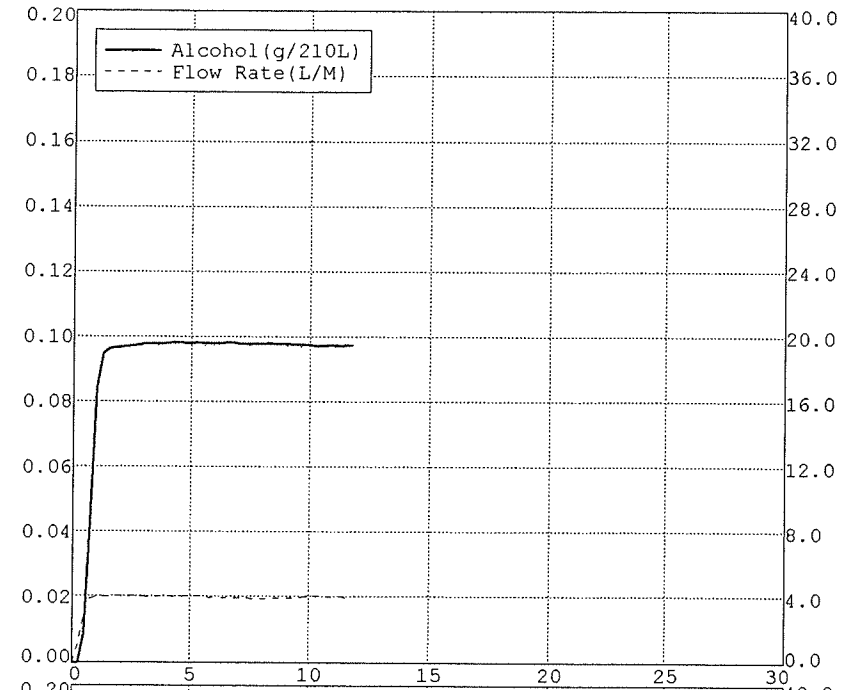

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 07/20/2020

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:43
INTERNAL STANDARD	VERIFIED	06:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:44
BLANK TEST	0.00	06:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:45
BLANK TEST	0.00	06:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:46
BLANK TEST	0.00	06:47

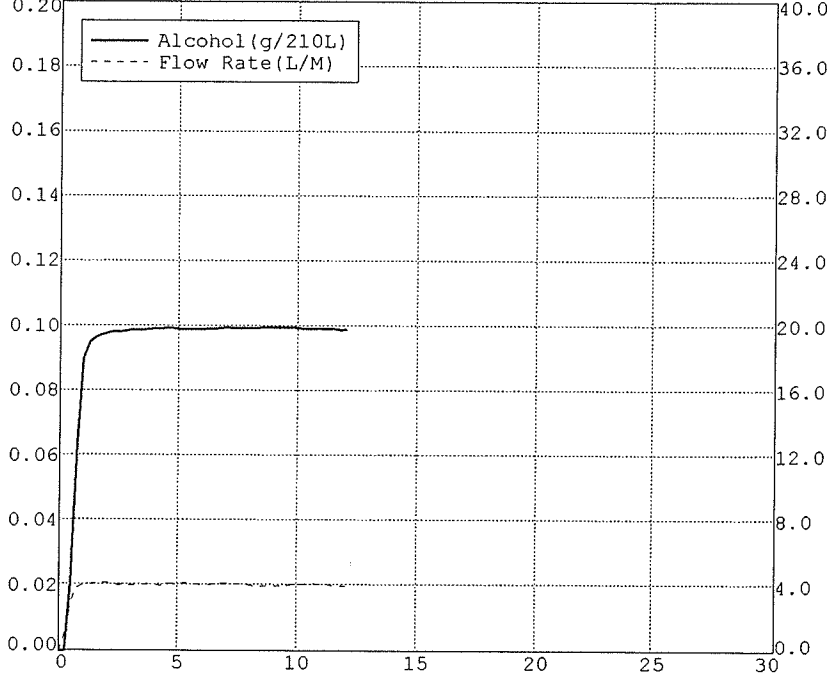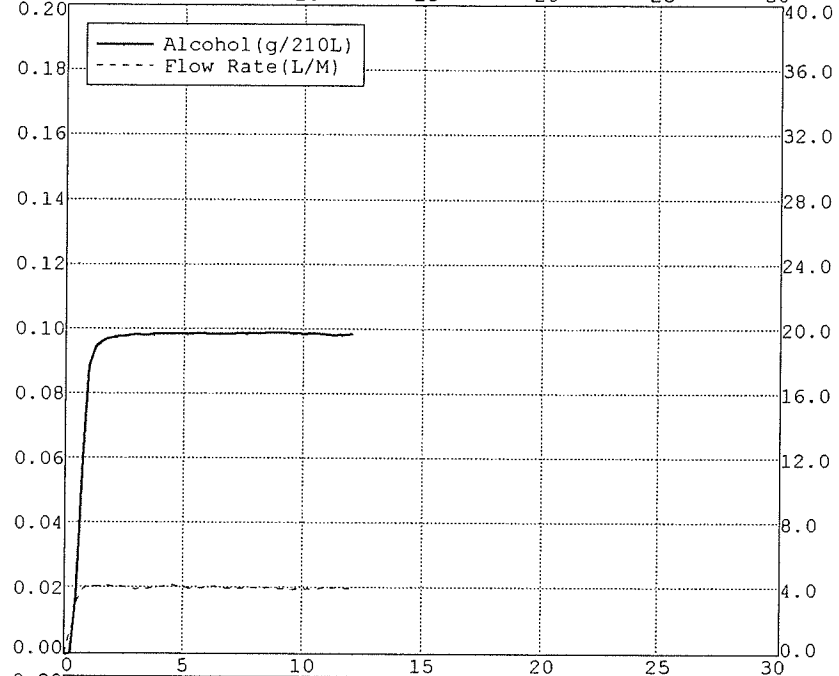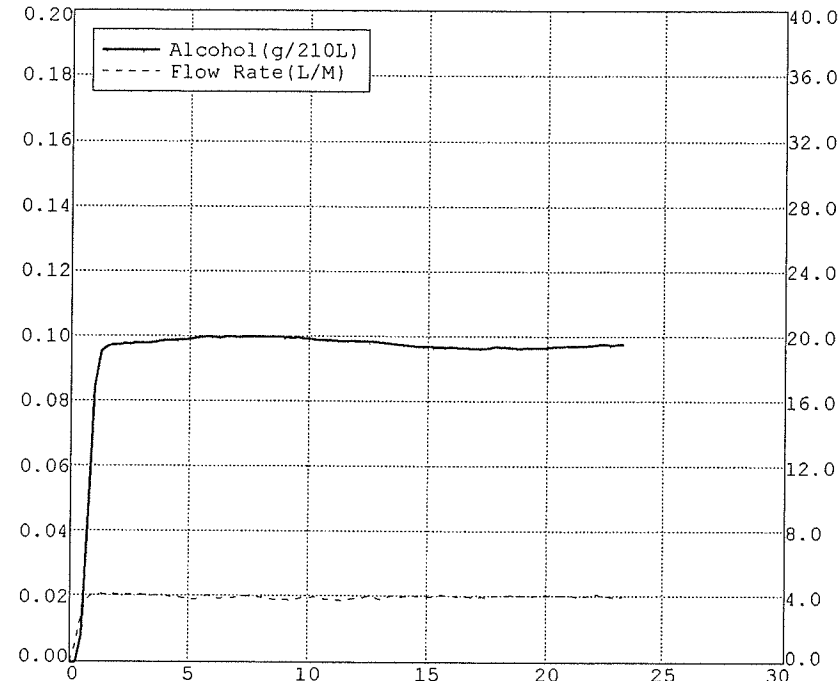

SOLUTION CHANGE

-----  
LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290  
-----

Date: 07/26/2020

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:55
INTERNAL STANDARD	ERROR	09:55

Internal Standard Error

SOLUTION CHANGE

LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 07/26/2020

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:58
INTERNAL STANDARD	VERIFIED	09:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:58
BLANK TEST	0.00	09:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:59
BLANK TEST	0.00	10:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:00
BLANK TEST	0.00	10:01

