

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/02/2020

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:27
INTERNAL STANDARD	VERIFIED	08:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:28
BLANK TEST	0.00	08:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:29
BLANK TEST	0.00	08:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:30
BLANK TEST	0.00	08:31

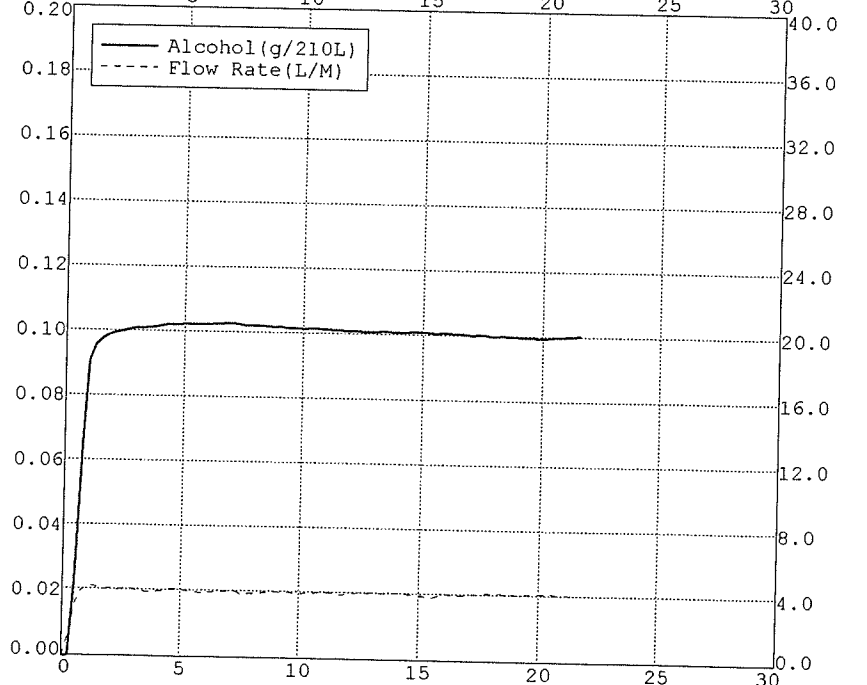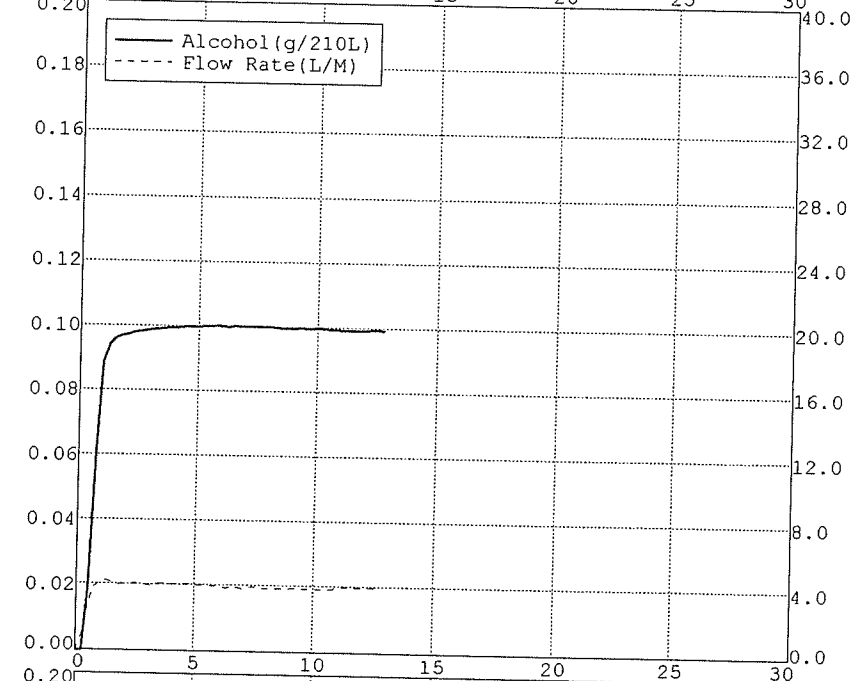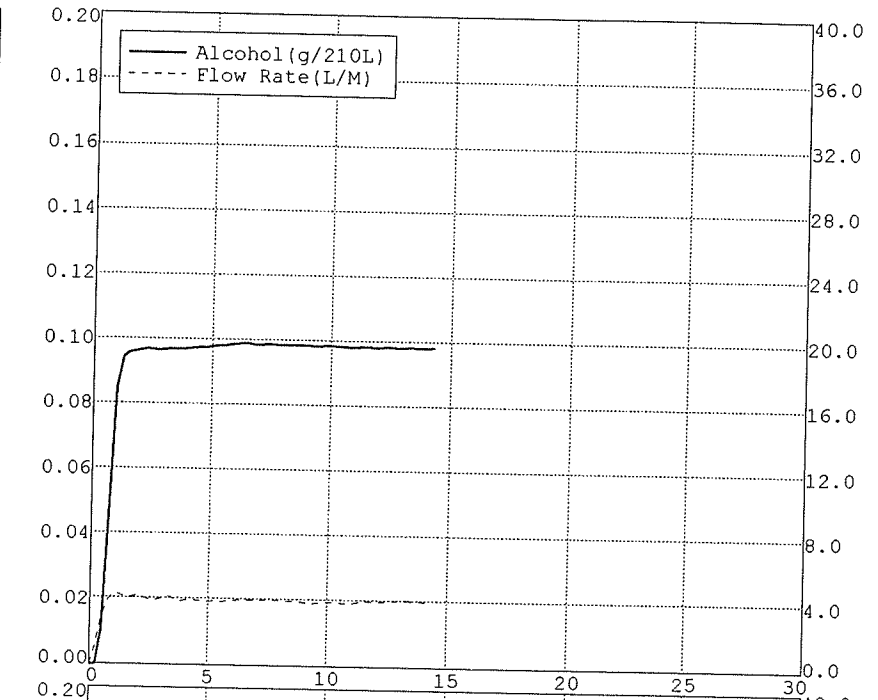

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/08/2020

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:09
INTERNAL STANDARD	VERIFIED	11:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:09
BLANK TEST	0.00	11:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:11
BLANK TEST	0.00	11:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:12
BLANK TEST	0.00	11:12

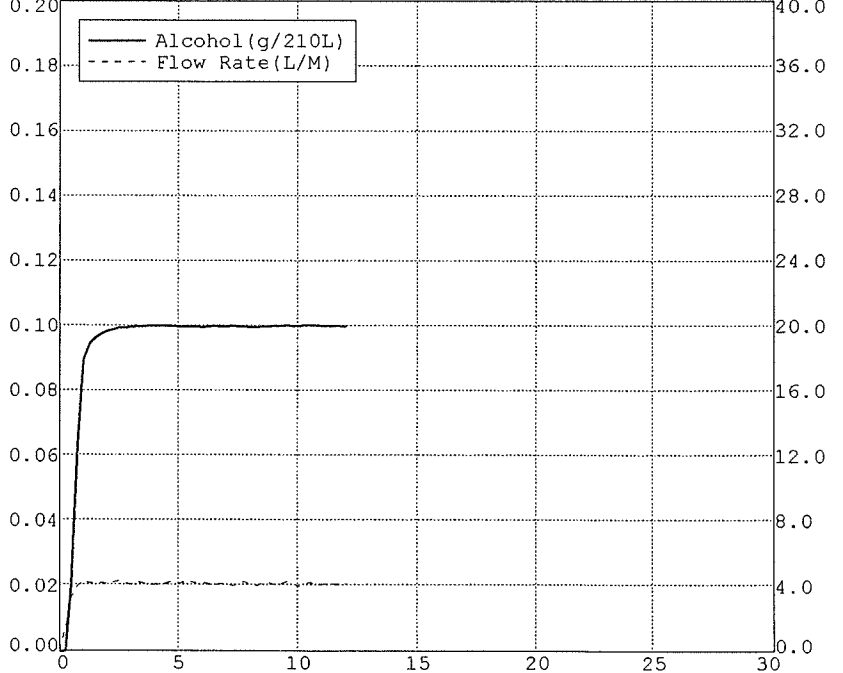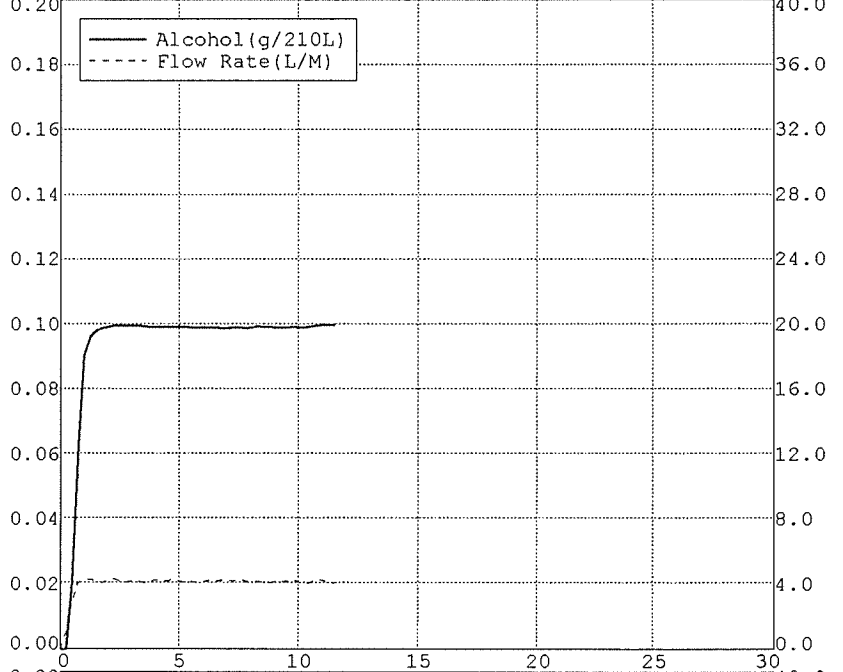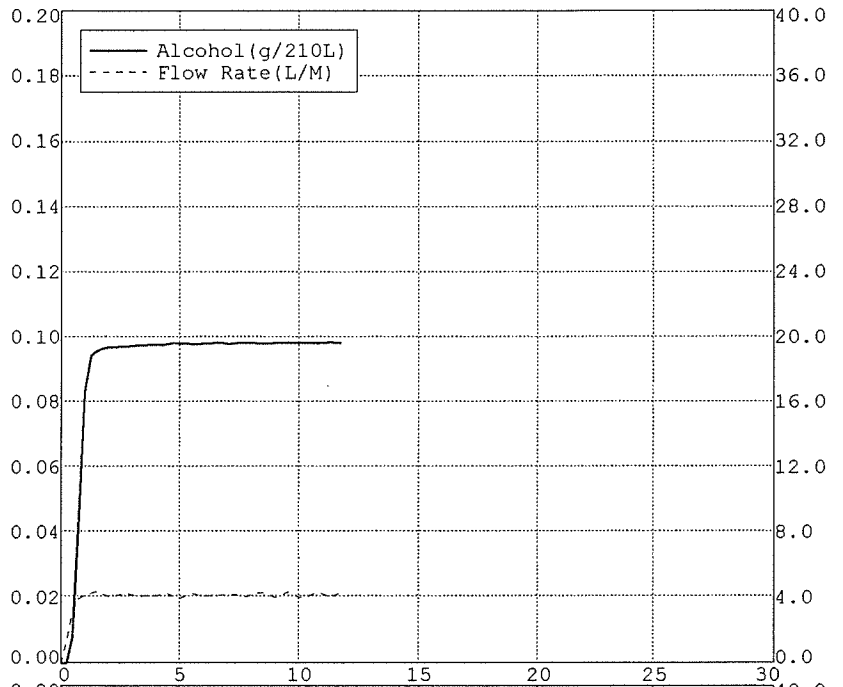

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/16/2020

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:30
INTERNAL STANDARD	VERIFIED	17:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:30
BLANK TEST	0.00	17:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:31
BLANK TEST	0.00	17:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:32
BLANK TEST	0.00	17:33

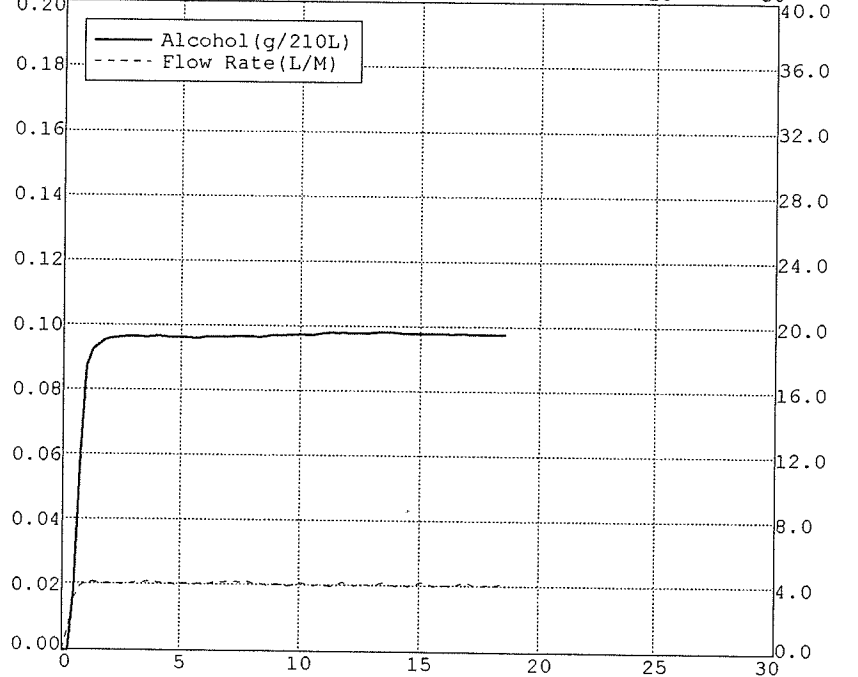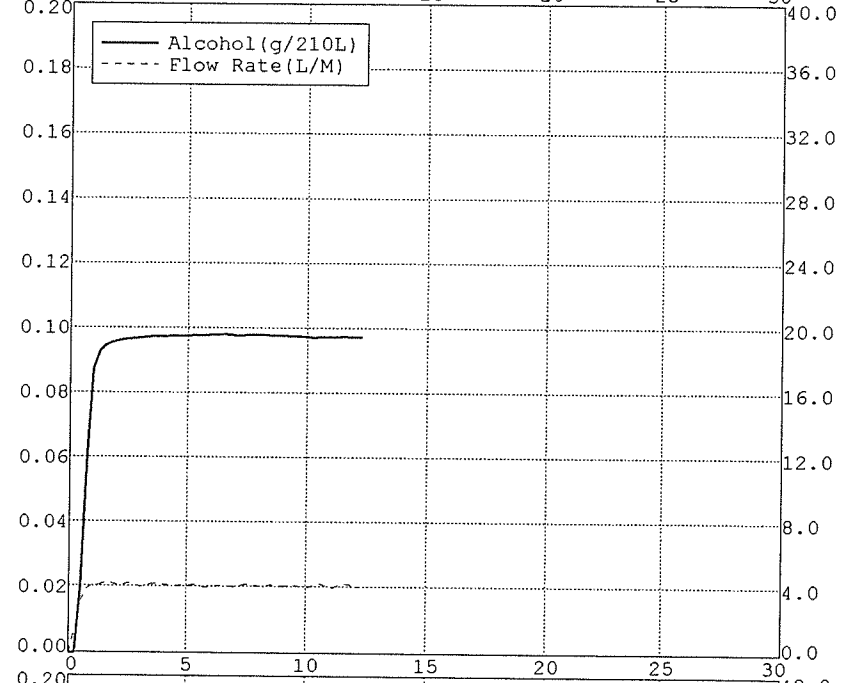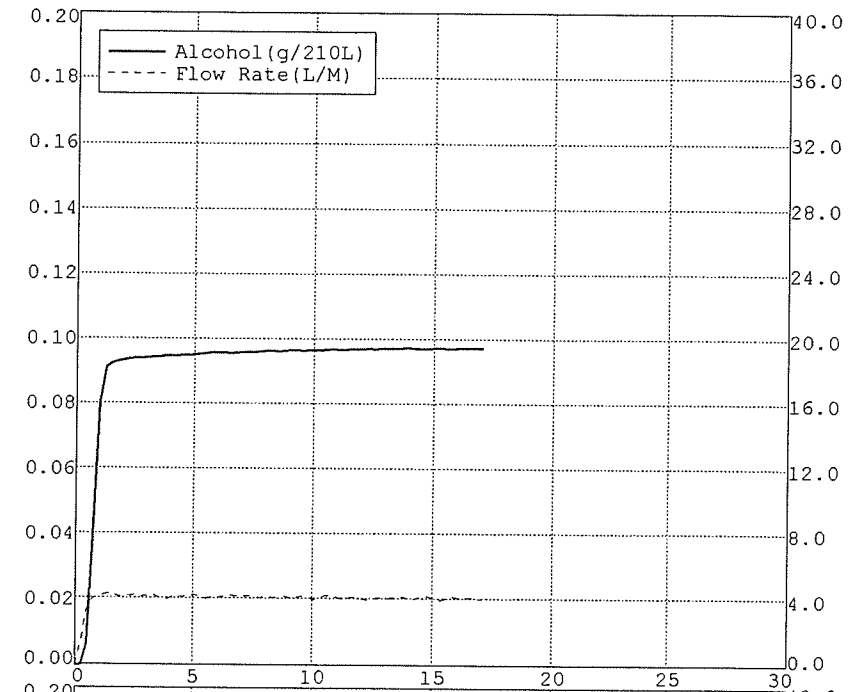

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/22/2020

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:33
INTERNAL STANDARD	VERIFIED	12:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:33
BLANK TEST	0.00	12:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:35
BLANK TEST	0.00	12:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:36
BLANK TEST	0.00	12:37

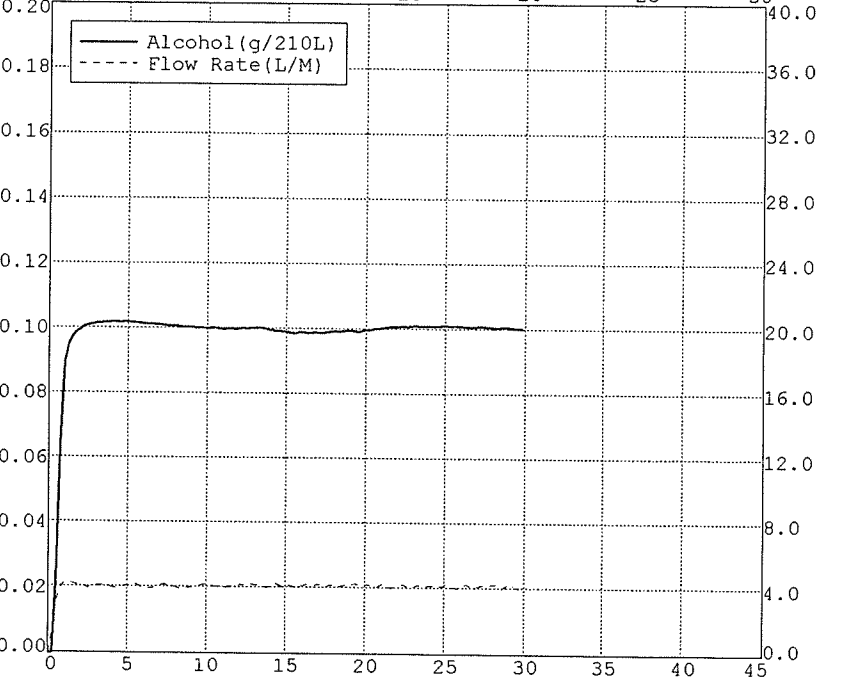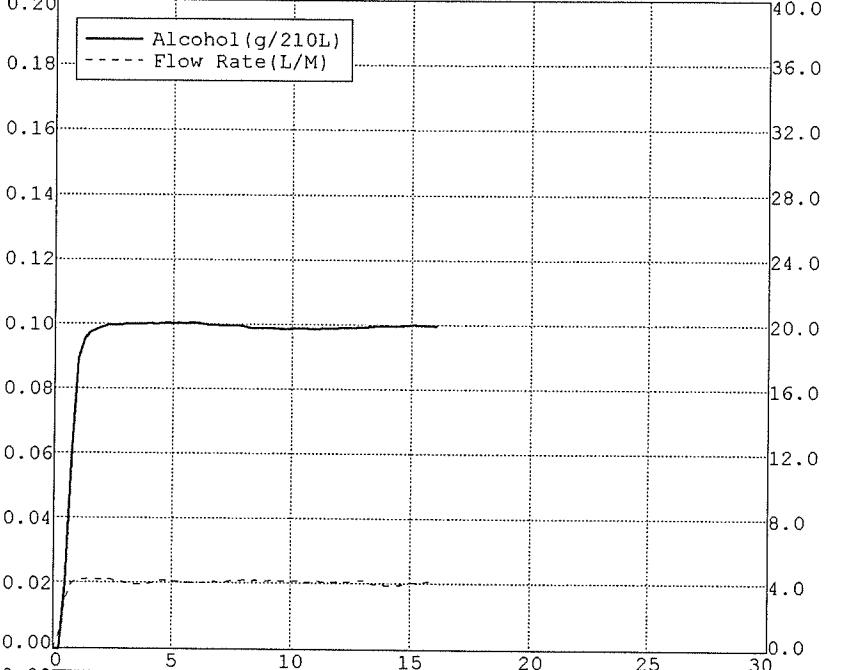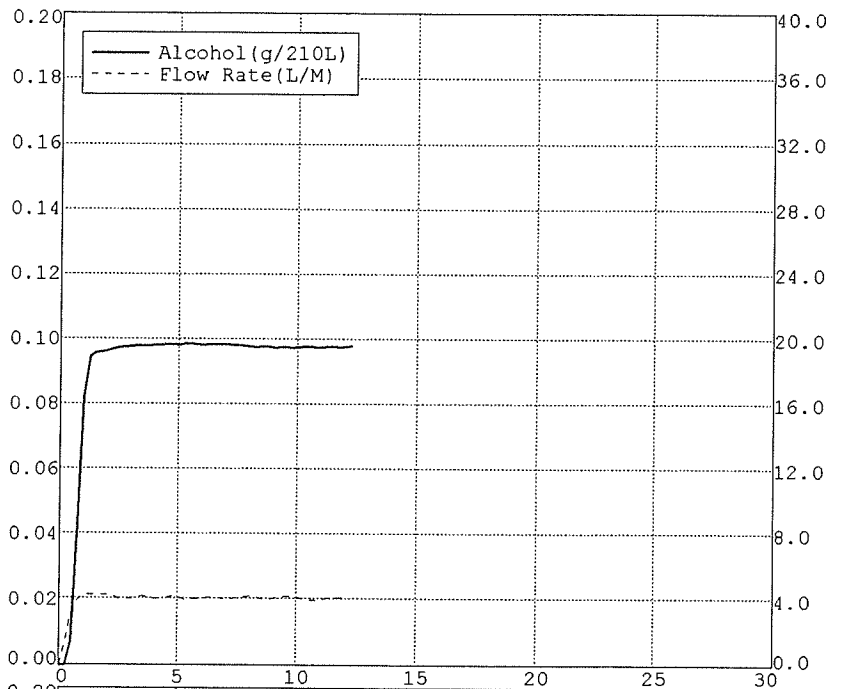

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/30/2020

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:59
INTERNAL STANDARD	VERIFIED	23:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:59
BLANK TEST	0.00	00:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:00
BLANK TEST	0.00	00:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:01
BLANK TEST	0.00	00:02

