

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/04/2019

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:46
INTERNAL STANDARD	VERIFIED	15:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:46
BLANK TEST	0.00	15:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:47
BLANK TEST	0.00	15:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:49
BLANK TEST	0.00	15:49

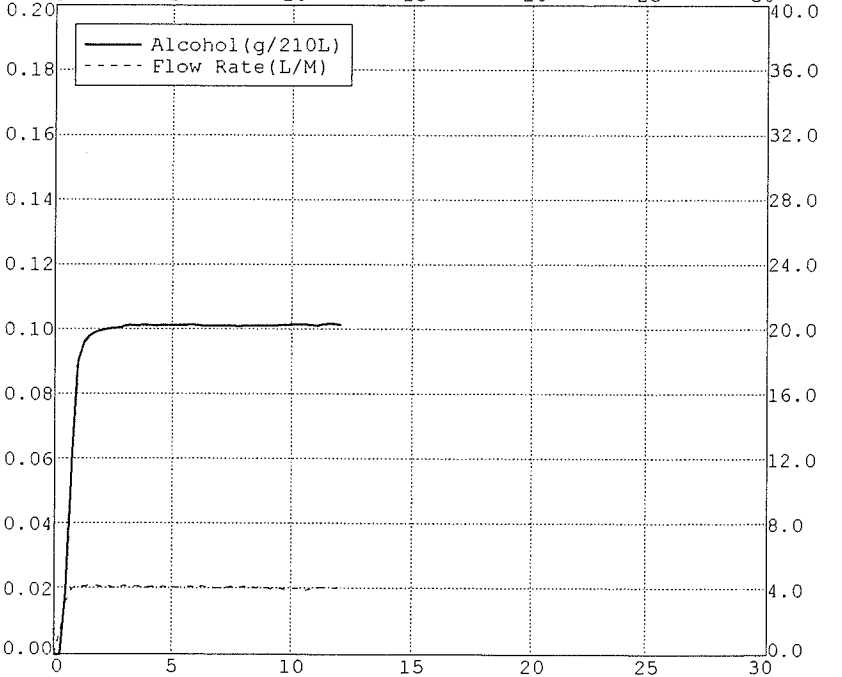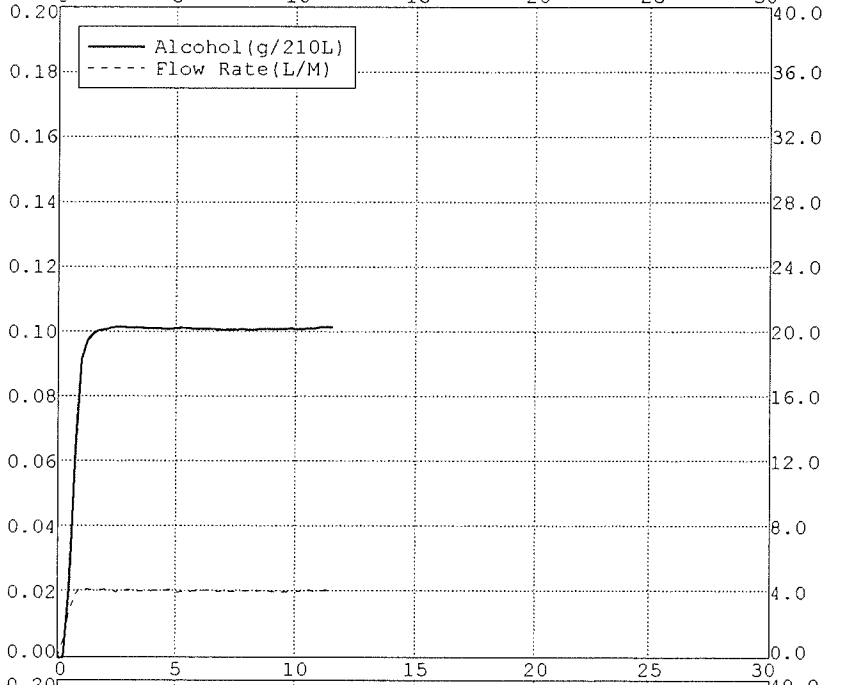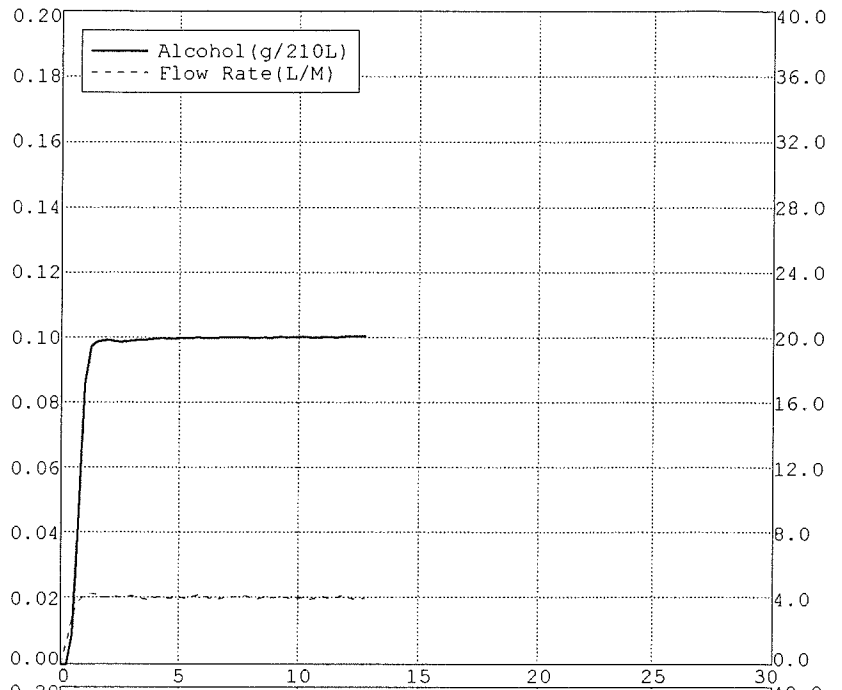

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/10/2019

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:15
INTERNAL STANDARD	VERIFIED	08:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:16
BLANK TEST	0.00	08:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:17
BLANK TEST	0.00	08:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:18
BLANK TEST	0.00	08:19

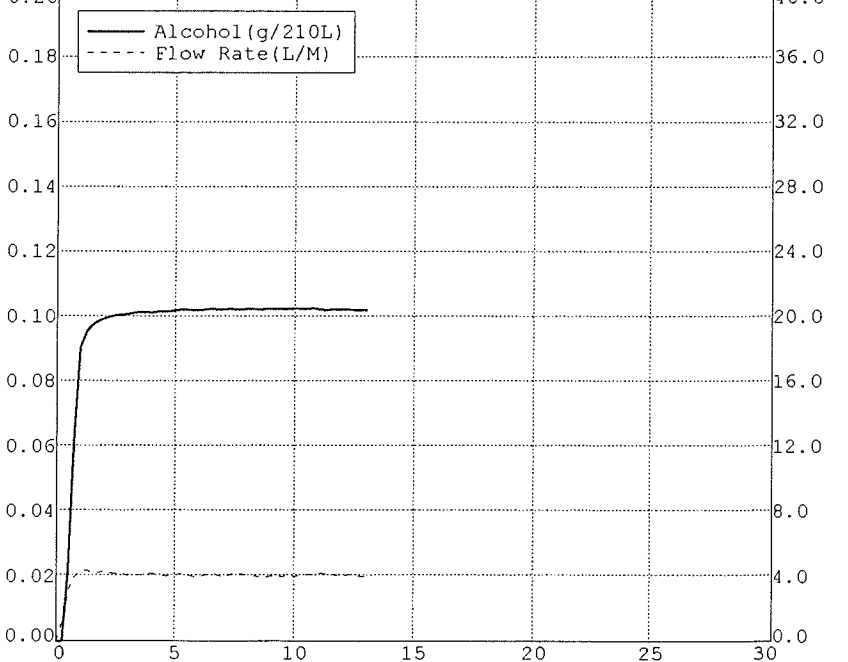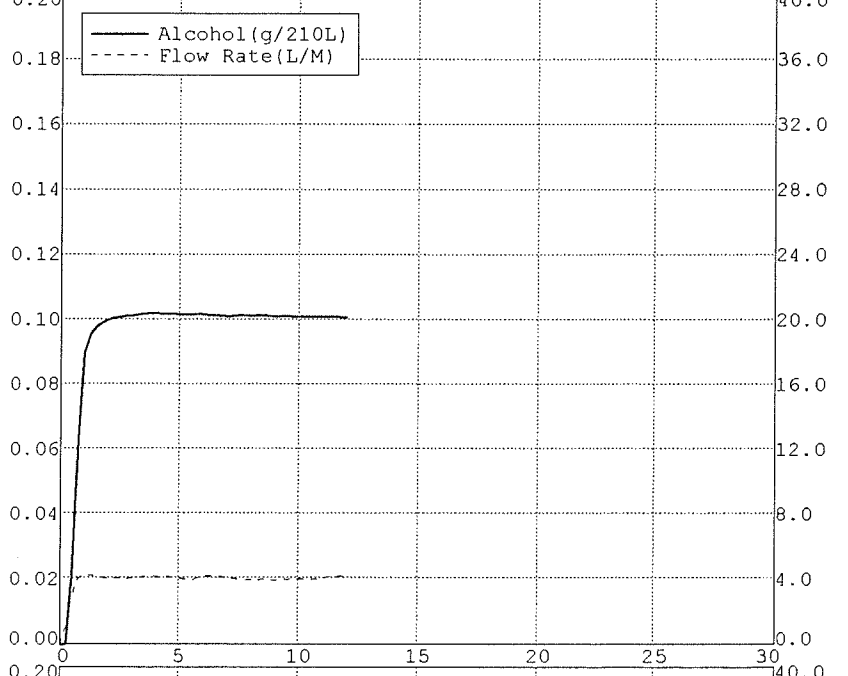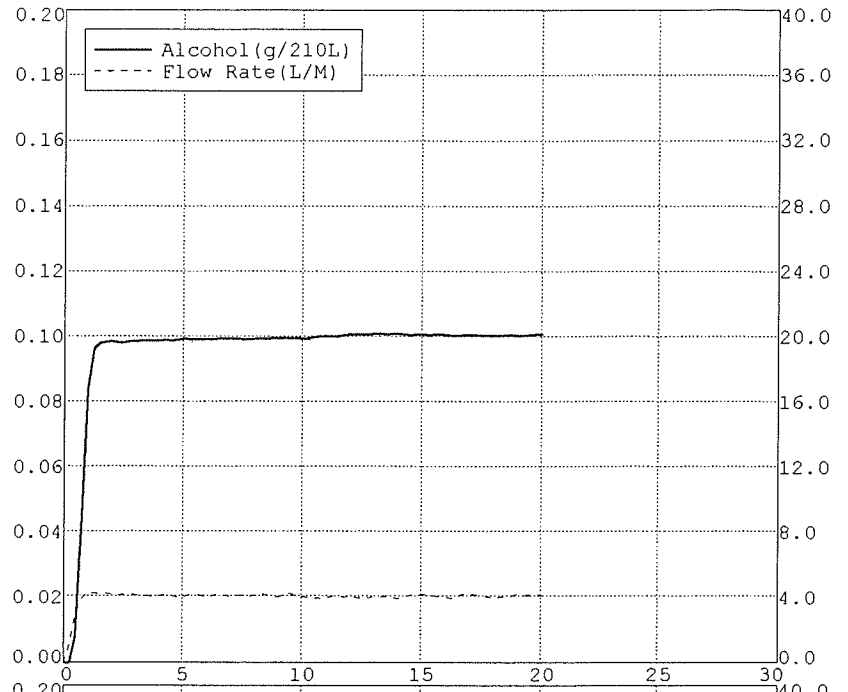

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/18/2019

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:29
INTERNAL STANDARD	VERIFIED	17:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:30
BLANK TEST	0.00	17:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:31
BLANK TEST	0.00	17:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:32
BLANK TEST	0.00	17:33

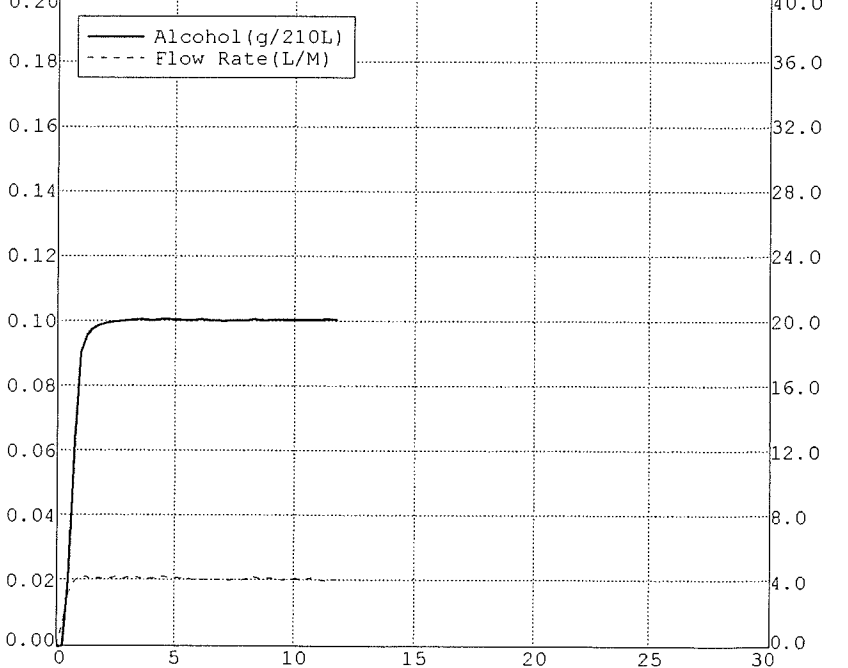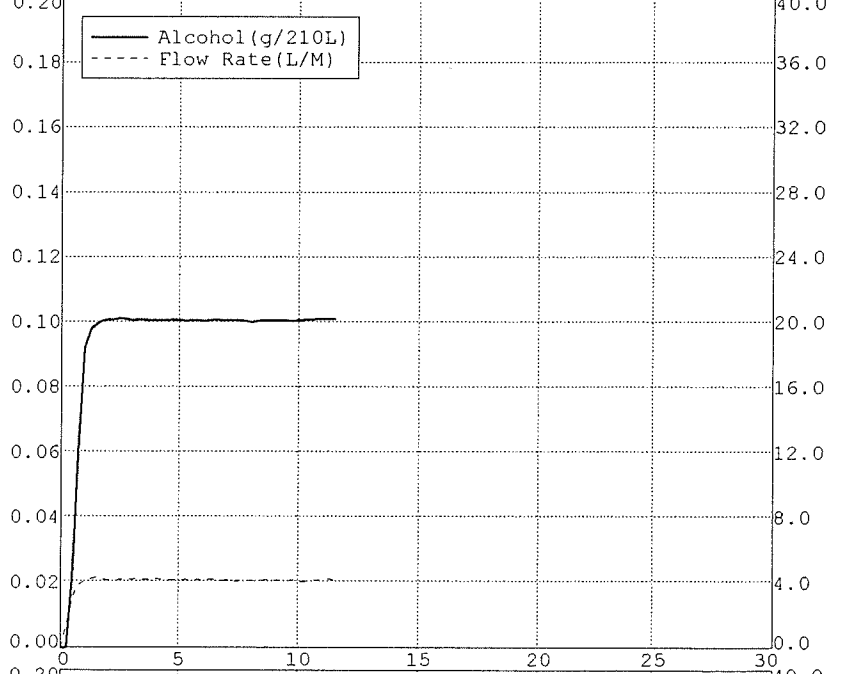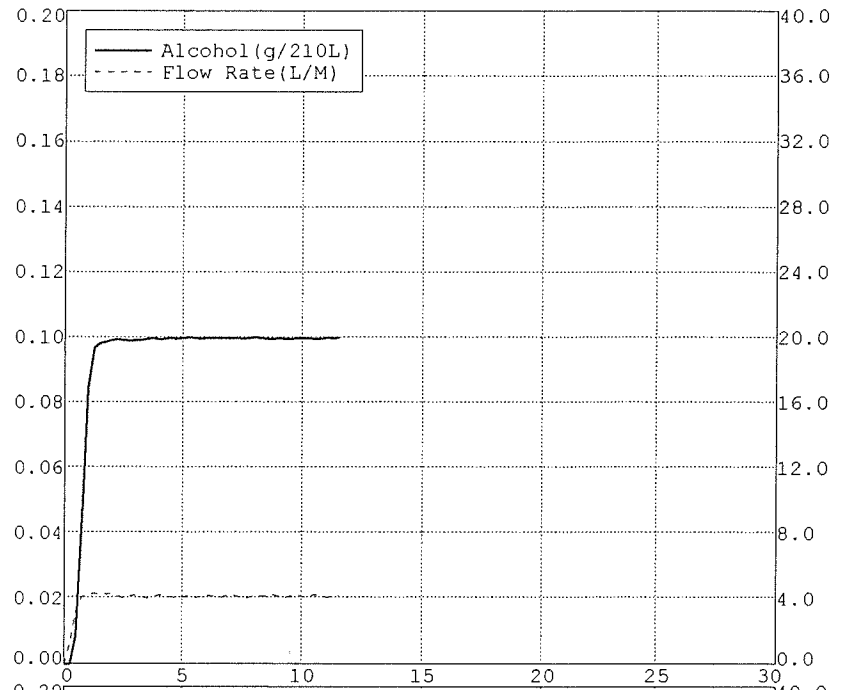

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/24/2019

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:32
INTERNAL STANDARD	VERIFIED	11:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:32
BLANK TEST	0.00	11:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:34
BLANK TEST	0.00	11:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:35
BLANK TEST	0.00	11:35

