

SUPERVISOR TEST



LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 06/04/2023

OPERATOR NAME:
PATRICK J KANE
Permit #: 48775
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:22
INTERNAL STANDARD	VERIFIED	17:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:22
BLANK TEST	0.00	17:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:24
BLANK TEST	0.00	17:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:25
BLANK TEST	0.00	17:26

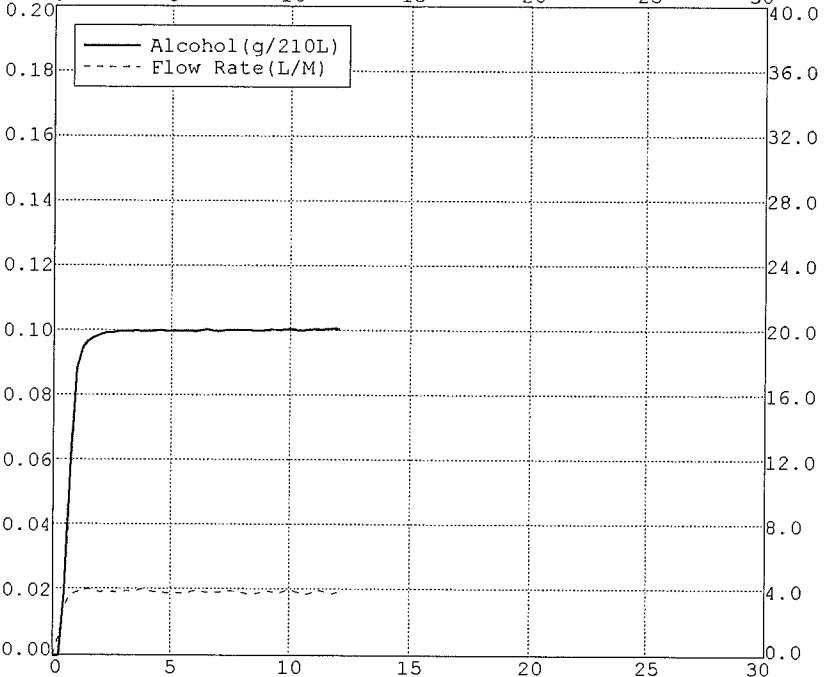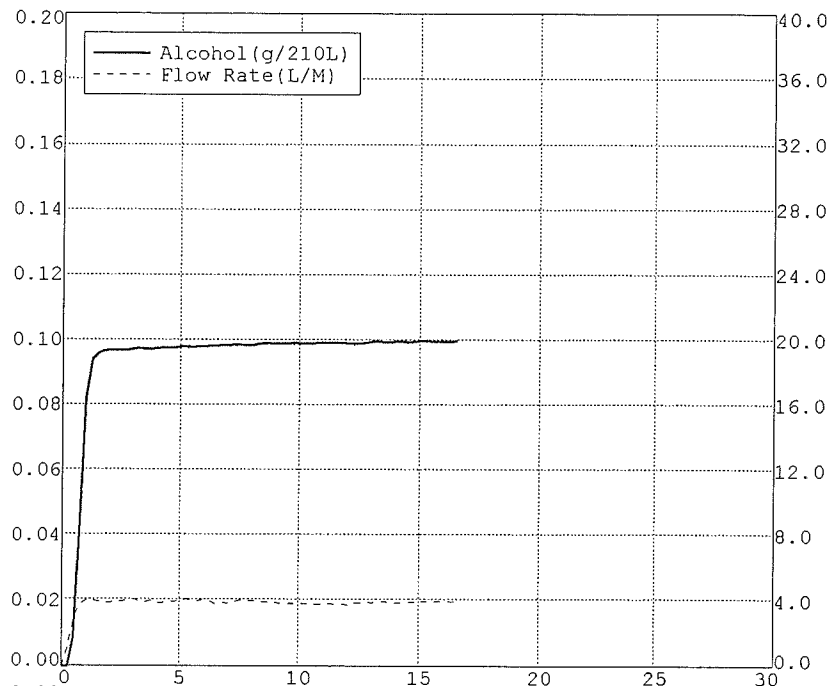

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 06/12/2023

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:11
INTERNAL STANDARD	VERIFIED	12:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:11
BLANK TEST	0.00	12:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:12
BLANK TEST	0.00	12:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:13
BLANK TEST	0.00	12:14

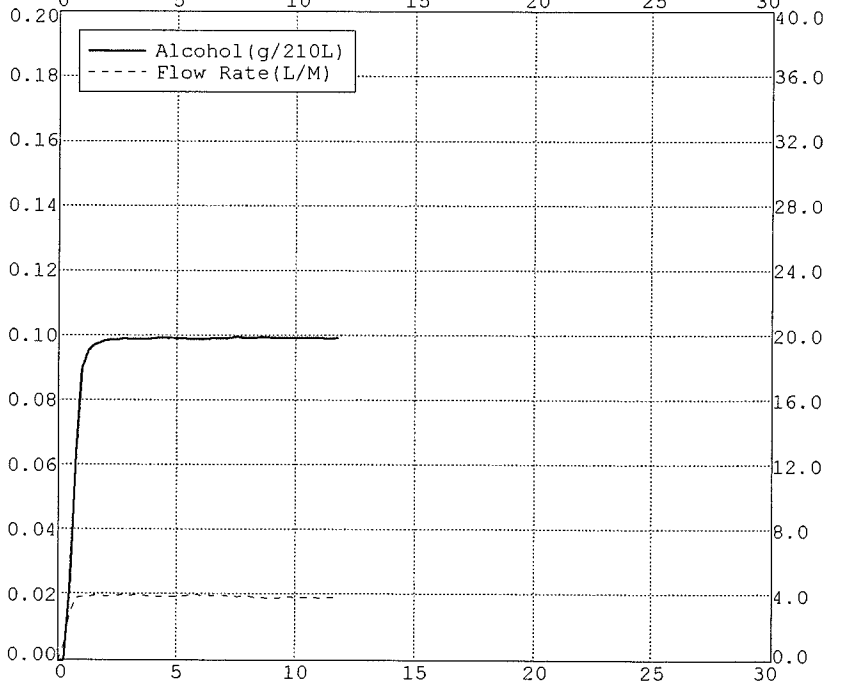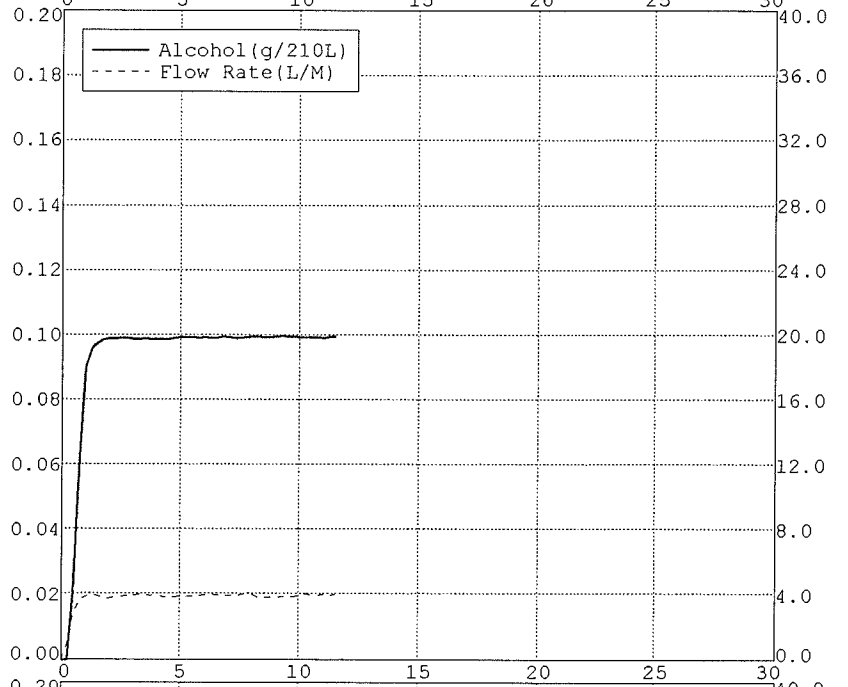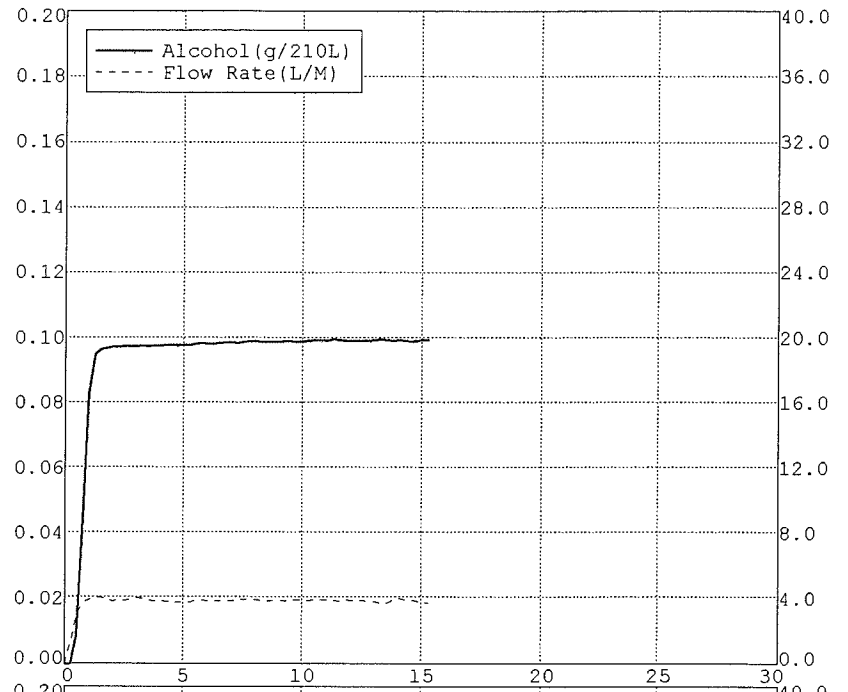

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 06/18/2023

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:31
INTERNAL STANDARD	VERIFIED	19:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:31
BLANK TEST	0.00	19:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:33
BLANK TEST	0.00	19:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:34
BLANK TEST	0.00	19:34

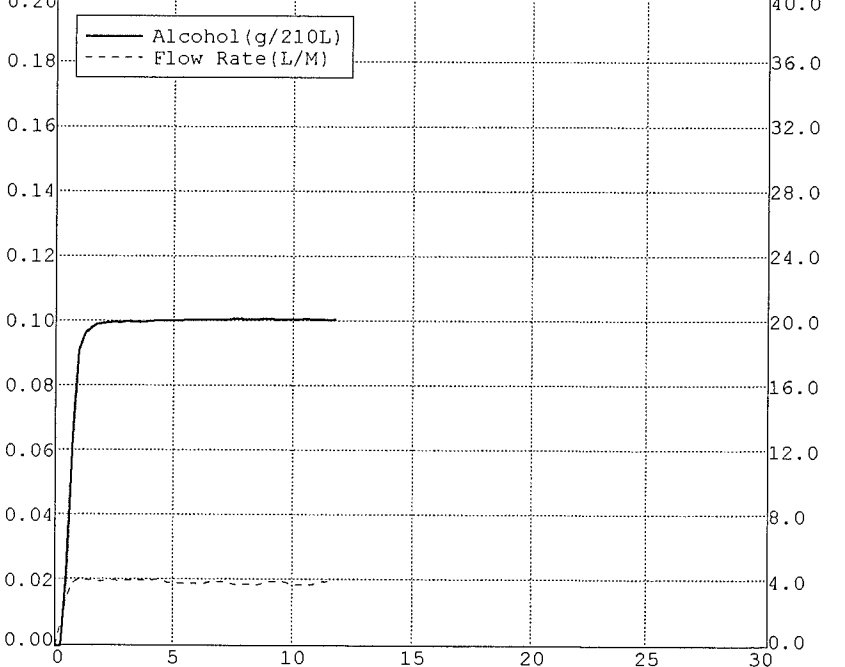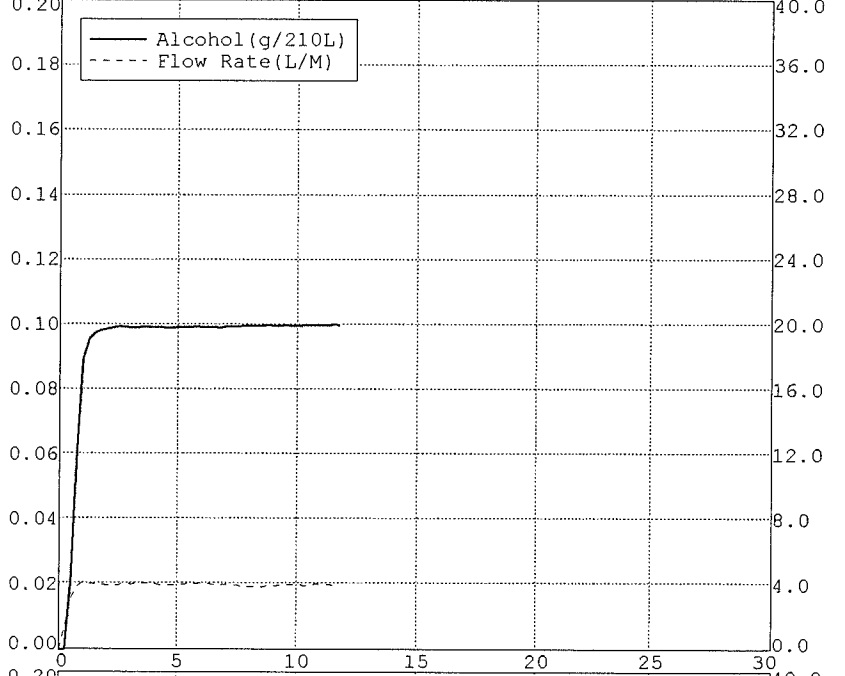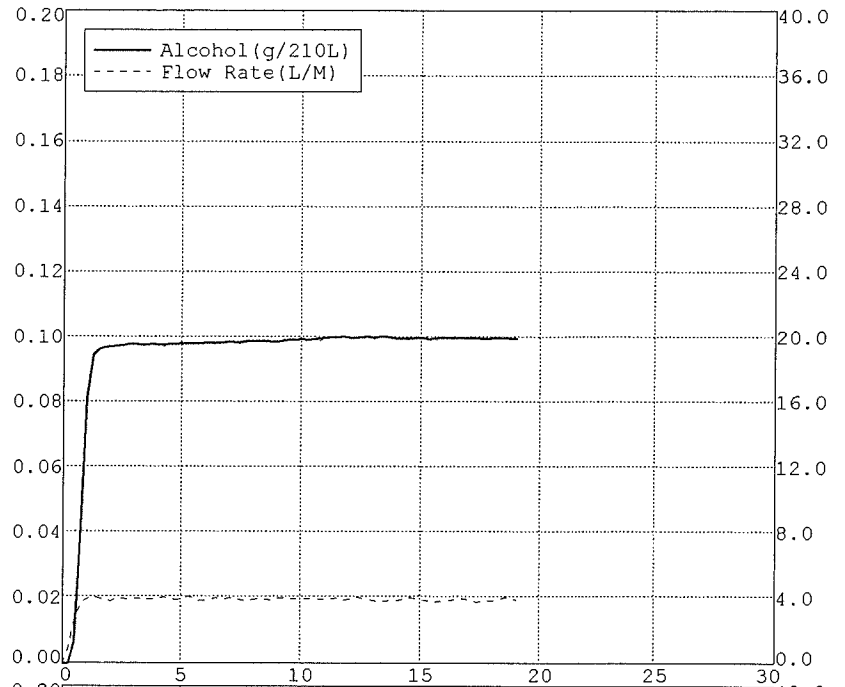

SUPERVISOR TEST

LAKE PLACID VILLAGE
 POLICE DEPT.
 DATAMASTER dmt: 100290

Date: 06/26/2023

OPERATOR NAME:
 CHAD P BLINN
 Permit #: 33034
 Operator Agency/Dept: LAKE PLACID VILL. PD
 Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:43
INTERNAL STANDARD	VERIFIED	18:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:44
BLANK TEST	0.00	18:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:45
BLANK TEST	0.00	18:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:46
BLANK TEST	0.00	18:47

