

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/05/2019

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:13
INTERNAL STANDARD	VERIFIED	10:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:14
BLANK TEST	0.00	10:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:15
BLANK TEST	0.00	10:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:16
BLANK TEST	0.00	10:17

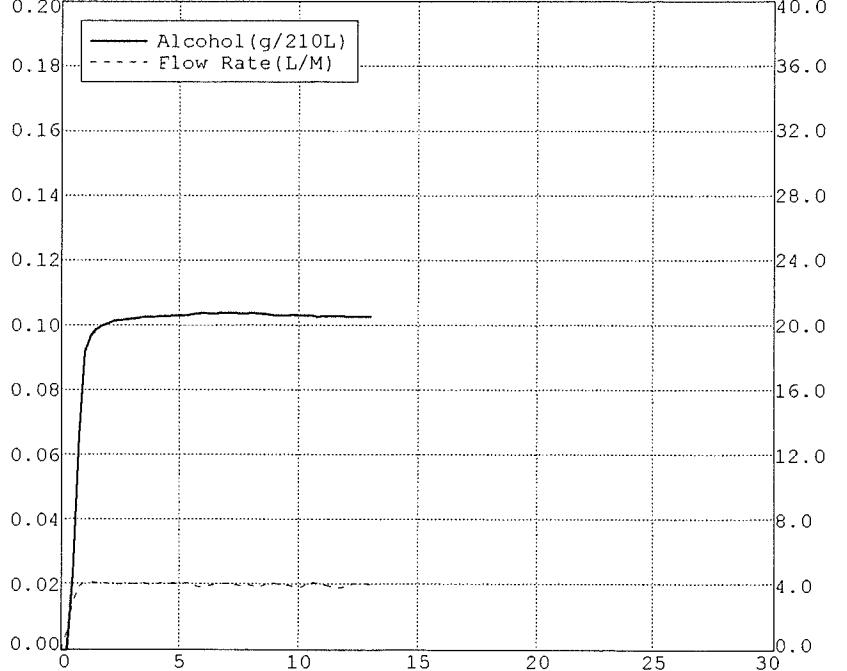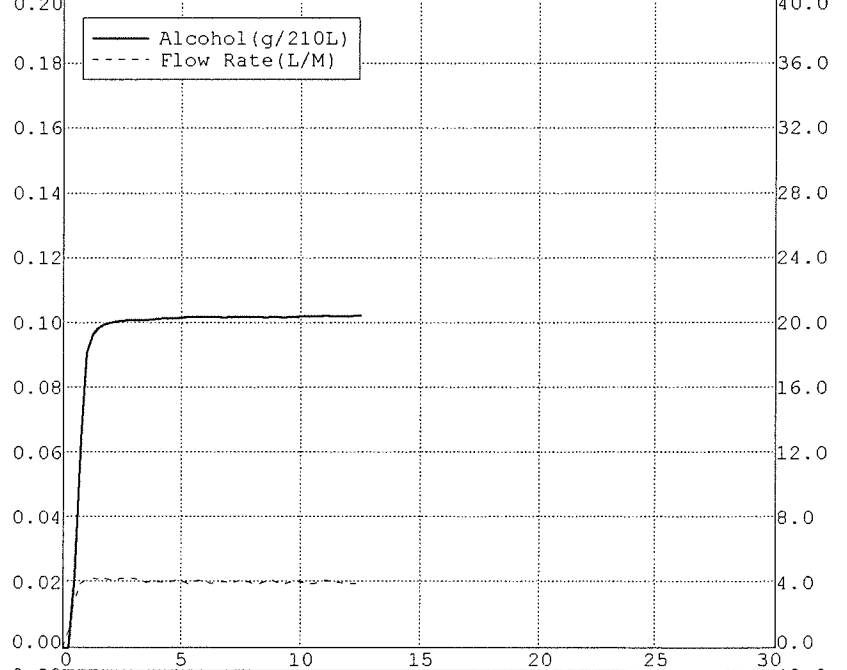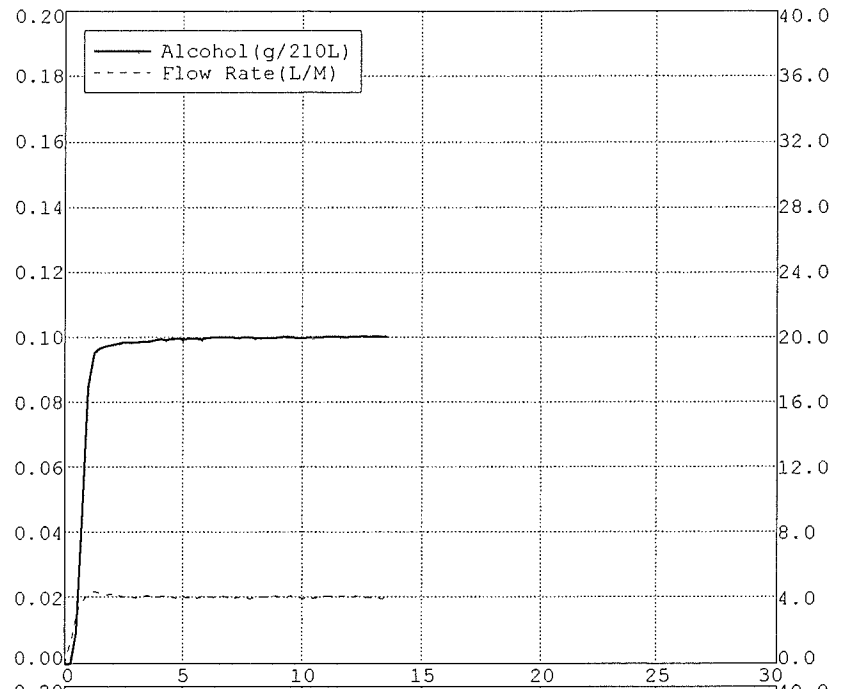

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/13/2019

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:45
INTERNAL STANDARD	VERIFIED	09:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:46
BLANK TEST	0.00	09:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:47
BLANK TEST	0.00	09:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:48
BLANK TEST	0.00	09:49

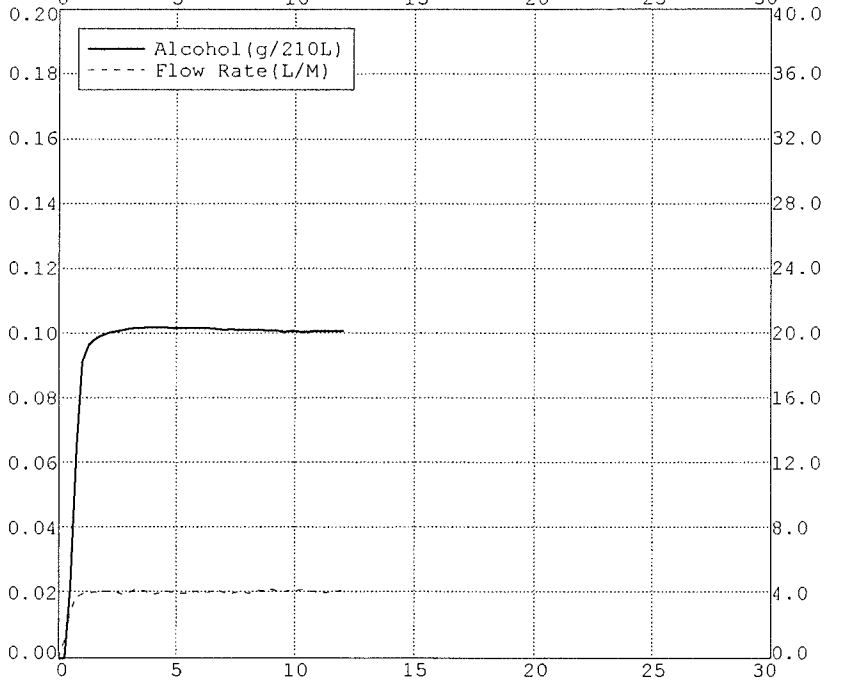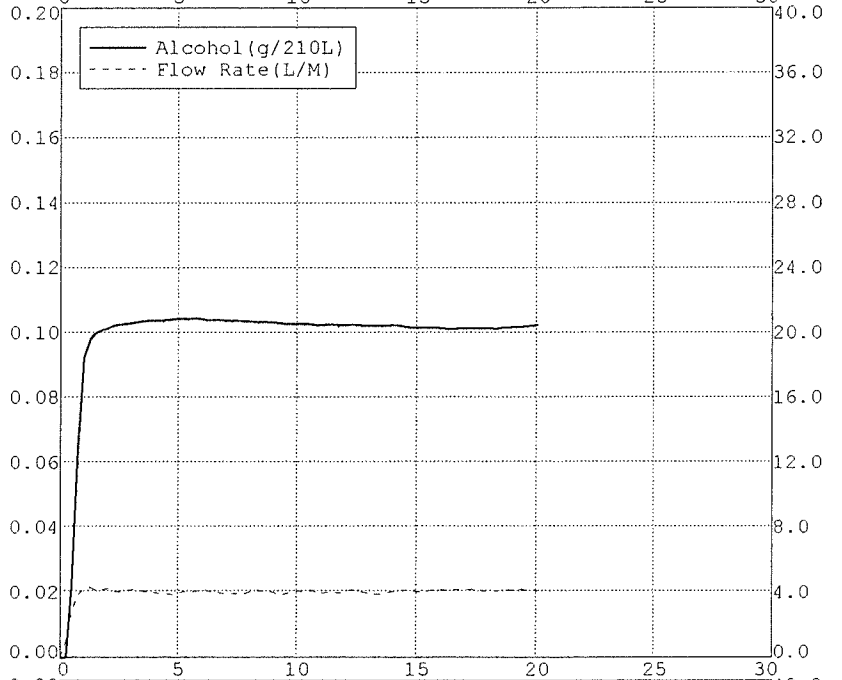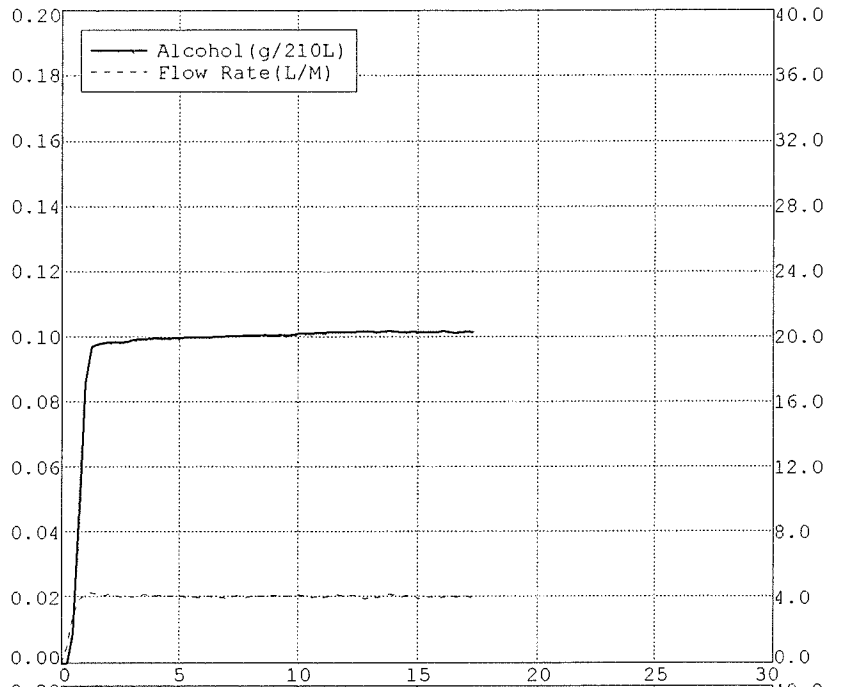

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/19/2019

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:27
INTERNAL STANDARD	VERIFIED	11:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:28
BLANK TEST	0.00	11:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:29
BLANK TEST	0.00	11:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:30
BLANK TEST	0.00	11:31

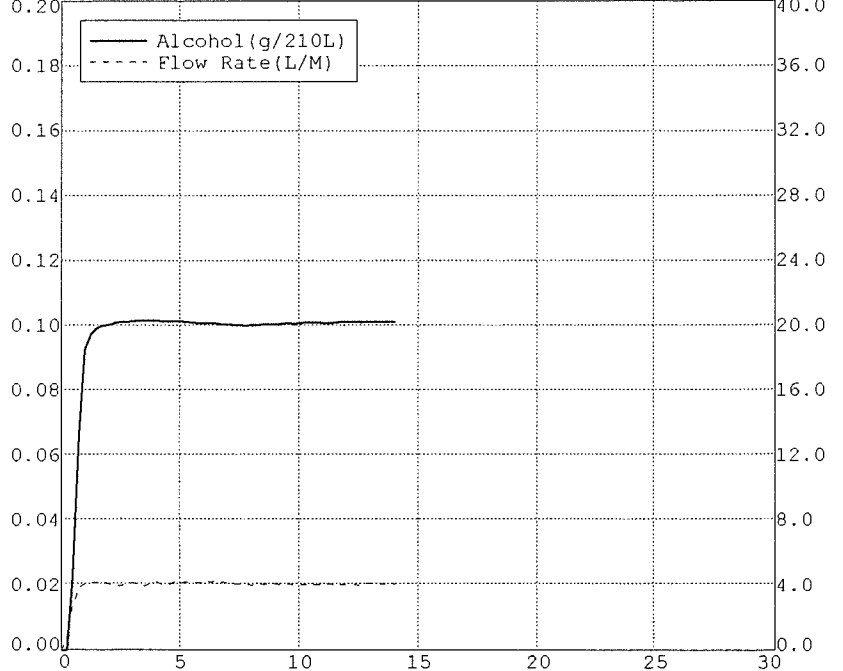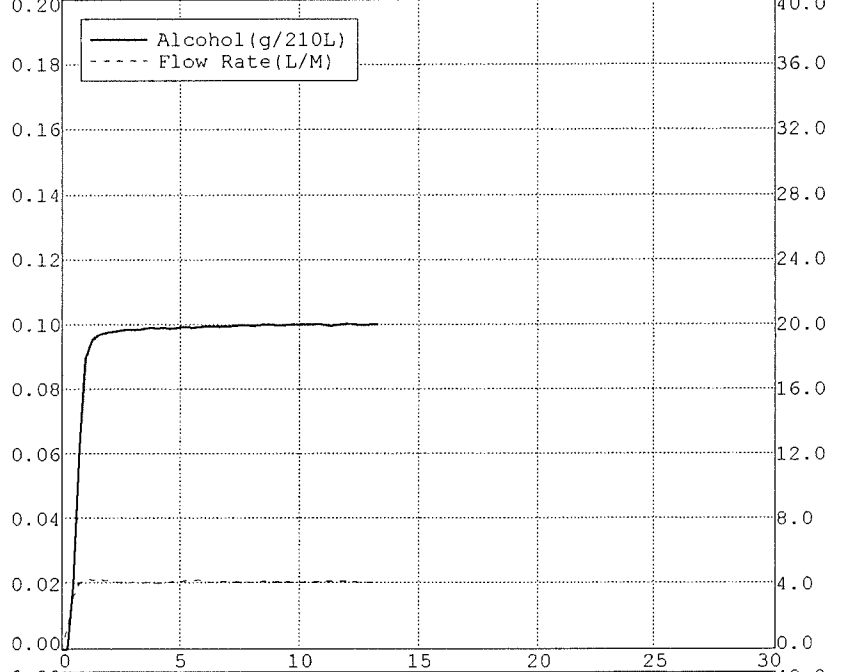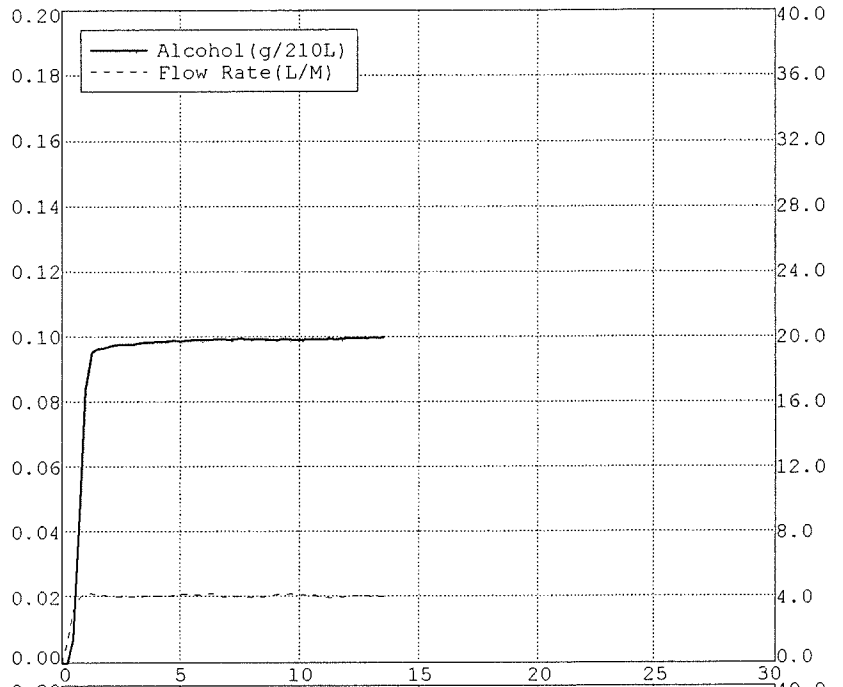

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/27/2019

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:29
INTERNAL STANDARD	VERIFIED	17:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:30
BLANK TEST	0.00	17:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:31
BLANK TEST	0.00	17:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:32
BLANK TEST	0.00	17:33

