

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 06/07/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:19
INTERNAL STANDARD	VERIFIED	06:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:20
BLANK TEST	0.00	06:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:21
BLANK TEST	0.00	06:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:22
BLANK TEST	0.00	06:23

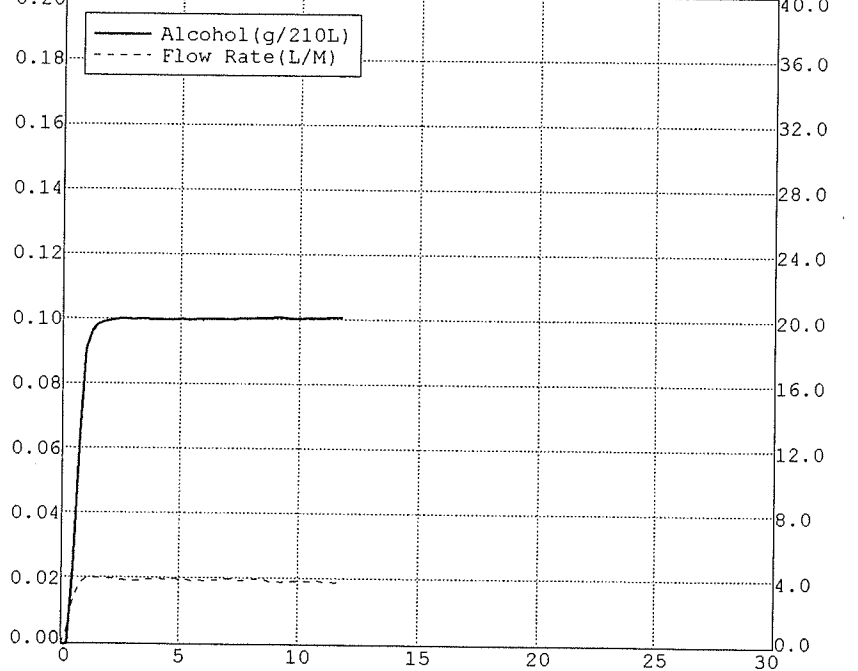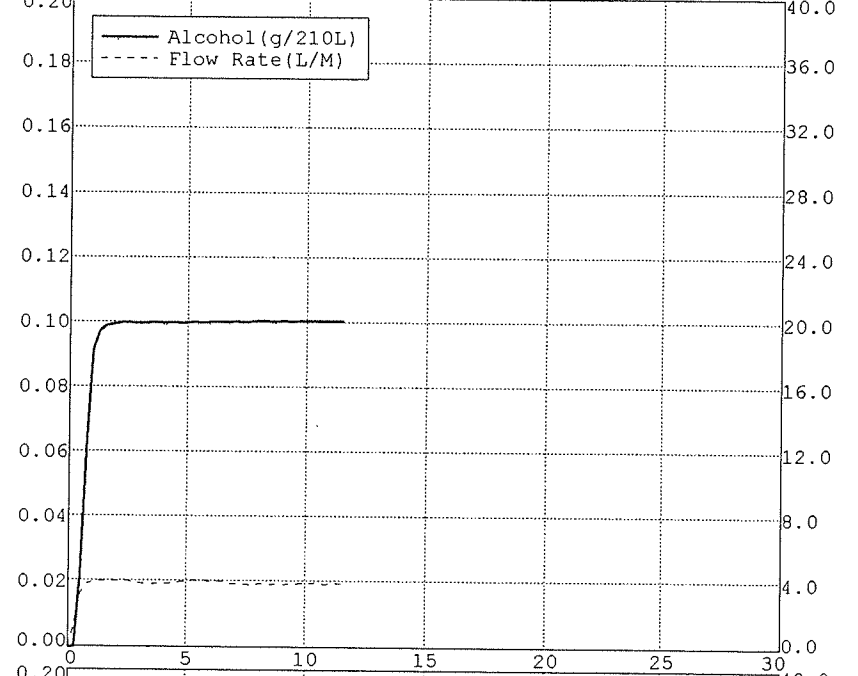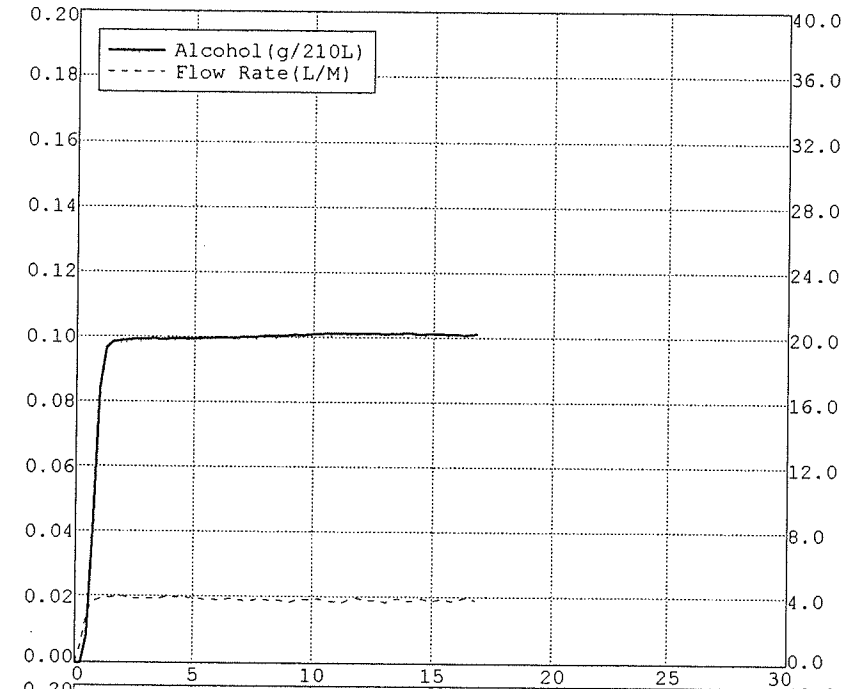

SUPERVISOR TEST




LAKE PLACID VILLAGE
 POLICE DEPT.
 DATAMASTER dmt: 100290

Date: 06/13/2021

OPERATOR NAME:
 CHAD P BLINN
 Permit #: 33034
 Operator Agency/Dept: LAKE PLACID VILL. PD
 Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:13
INTERNAL STANDARD	VERIFIED	17:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:13
BLANK TEST	0.00	17:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:15
BLANK TEST	0.00	17:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:16
BLANK TEST	0.00	17:17

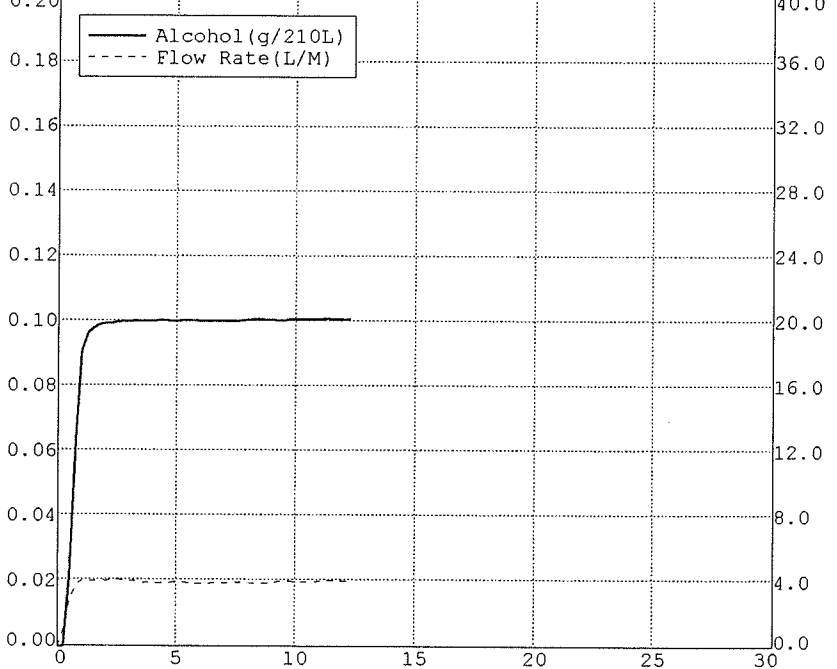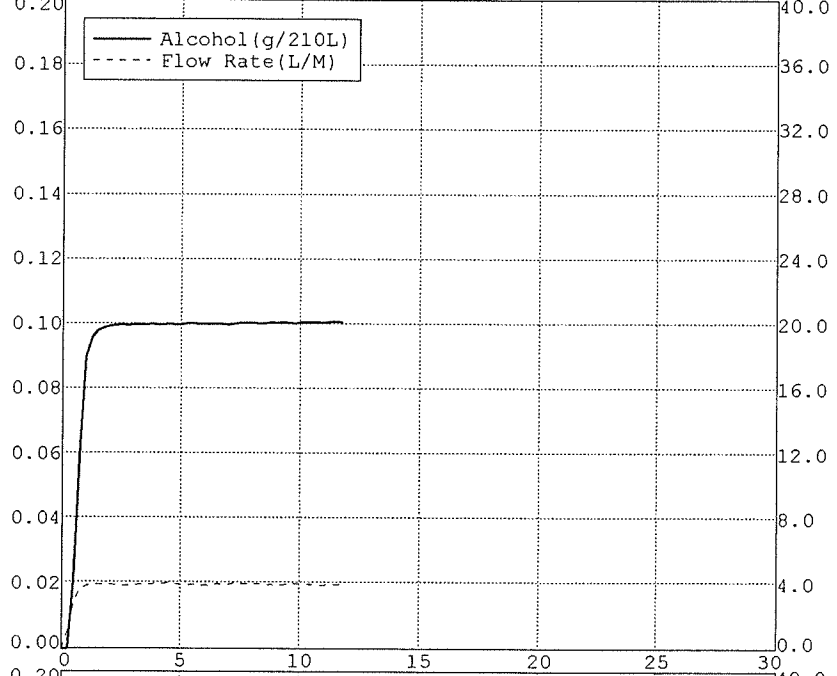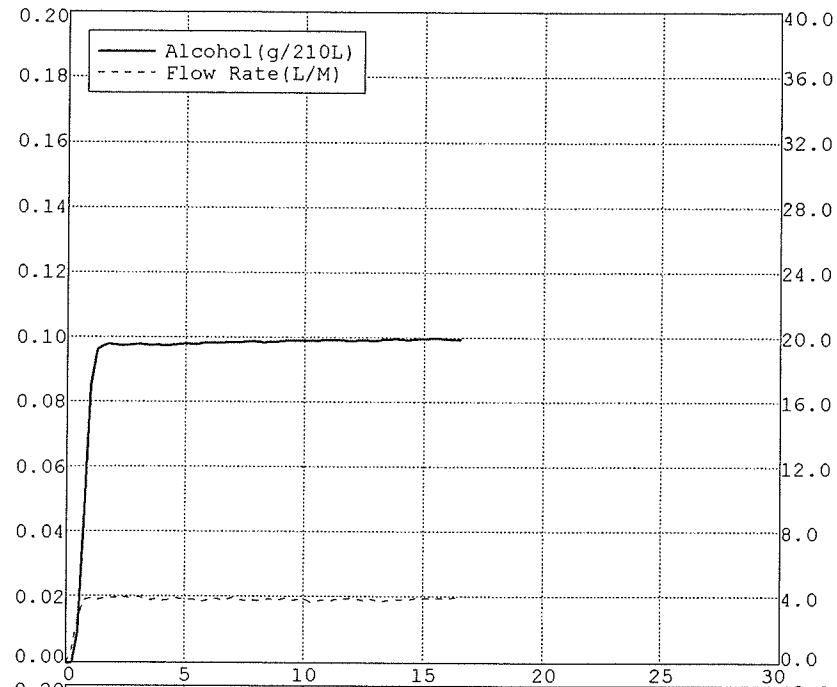

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 06/21/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:47
INTERNAL STANDARD	VERIFIED	17:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:47
BLANK TEST	0.00	17:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:48
BLANK TEST	0.00	17:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:49
BLANK TEST	0.00	17:50

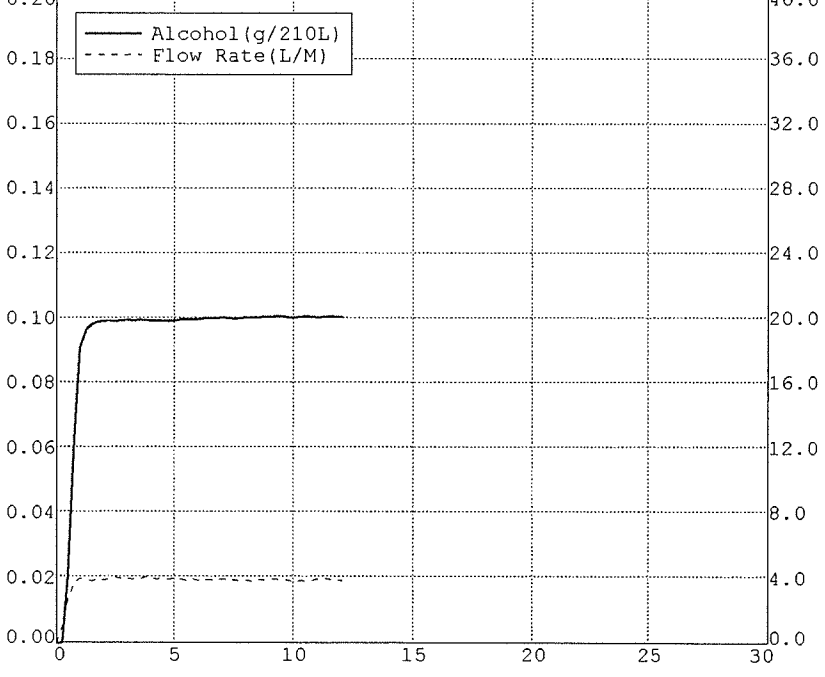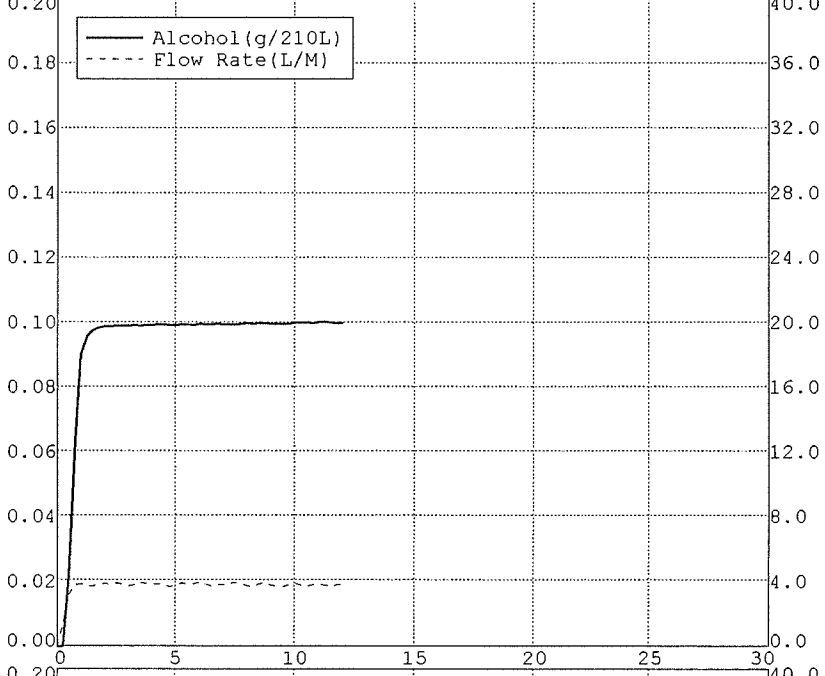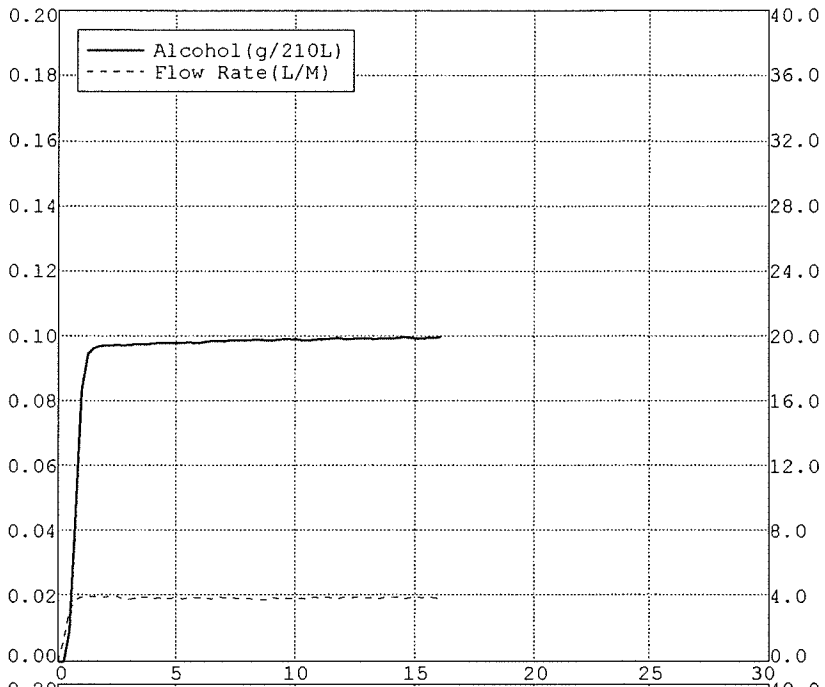

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 06/27/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:10
INTERNAL STANDARD	VERIFIED	16:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:10
BLANK TEST	0.00	16:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:12
BLANK TEST	0.00	16:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:13
BLANK TEST	0.00	16:14

