

# SOLUTION CHANGE




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 06/01/2025

OPERATOR NAME:  
MAKENZIE A HAYES  
Permit #: 49532  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 25110

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 18:38 |
| INTERNAL STANDARD       | VERIFIED | 18:39 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.09     | 18:39 |
| BLANK TEST              | 0.00     | 18:40 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.09     | 18:40 |
| BLANK TEST              | 0.00     | 18:41 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 18:41 |
| BLANK TEST              | 0.00     | 18:42 |

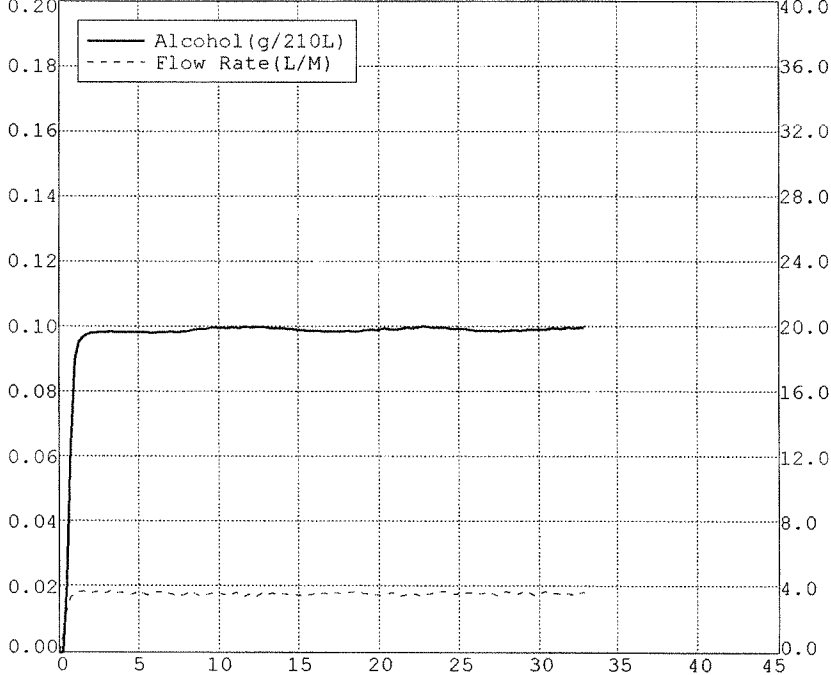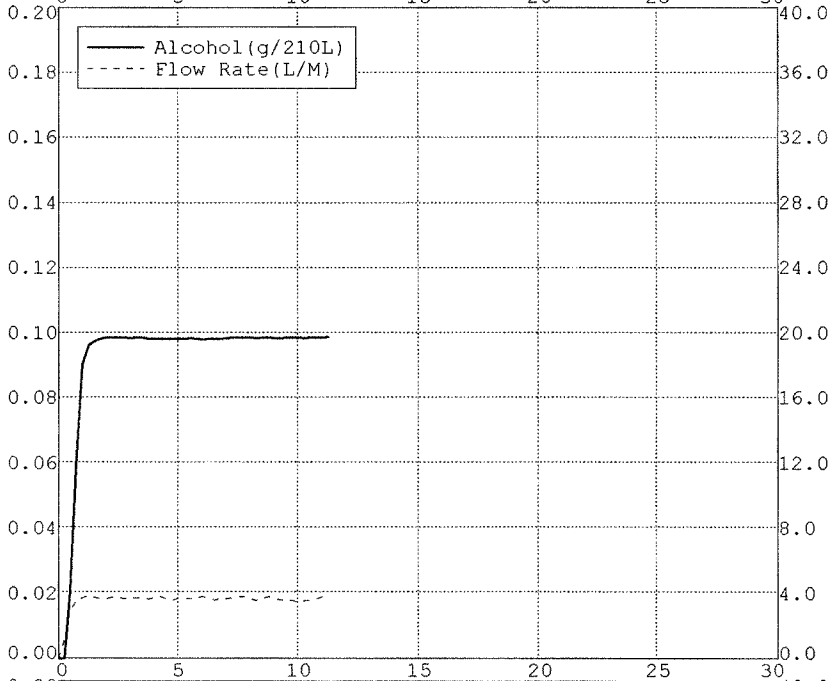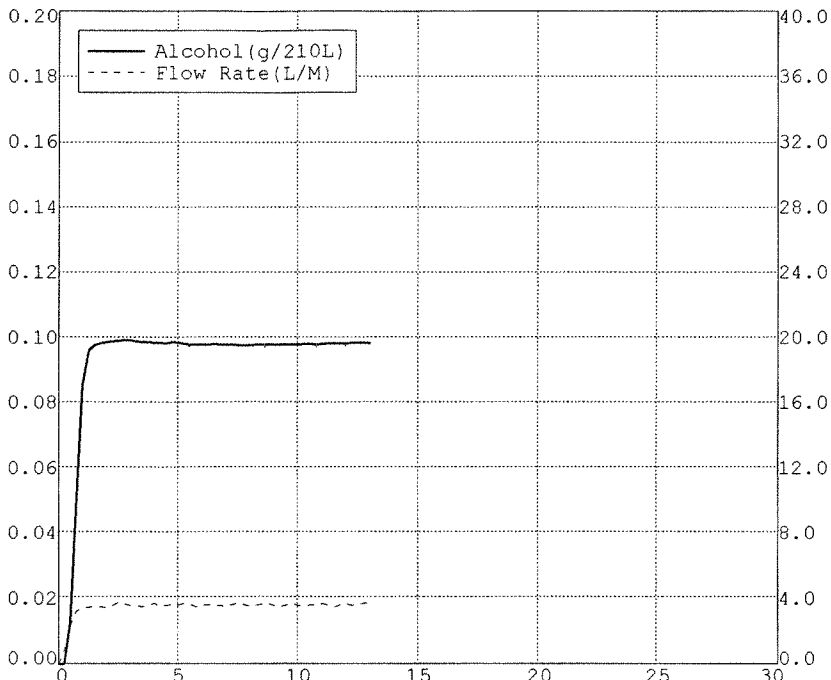

# SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 06/08/2025

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 25110

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 04:47 |
| INTERNAL STANDARD       | VERIFIED | 04:47 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 04:48 |
| BLANK TEST              | 0.00     | 04:49 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 04:49 |
| BLANK TEST              | 0.00     | 04:50 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 04:50 |
| BLANK TEST              | 0.00     | 04:51 |

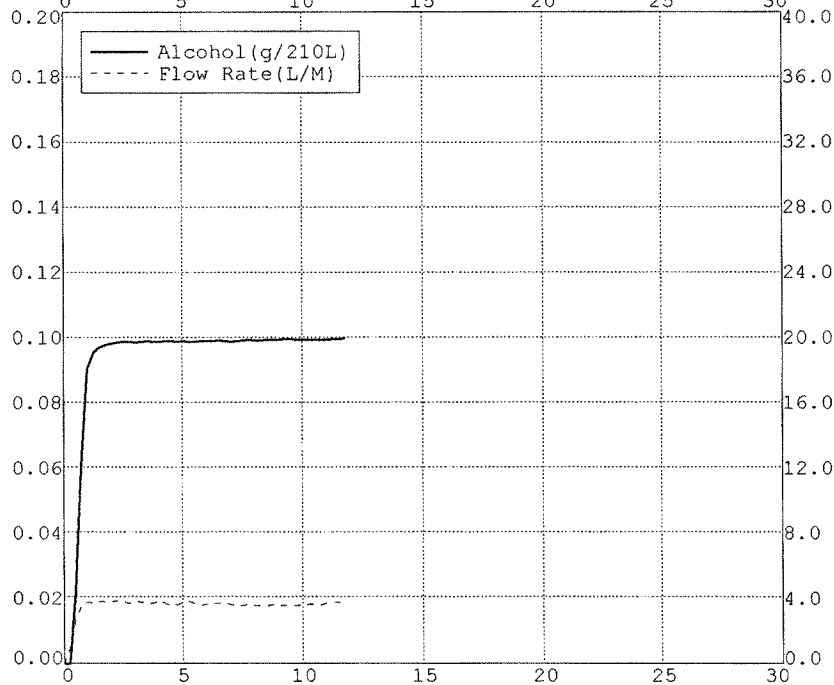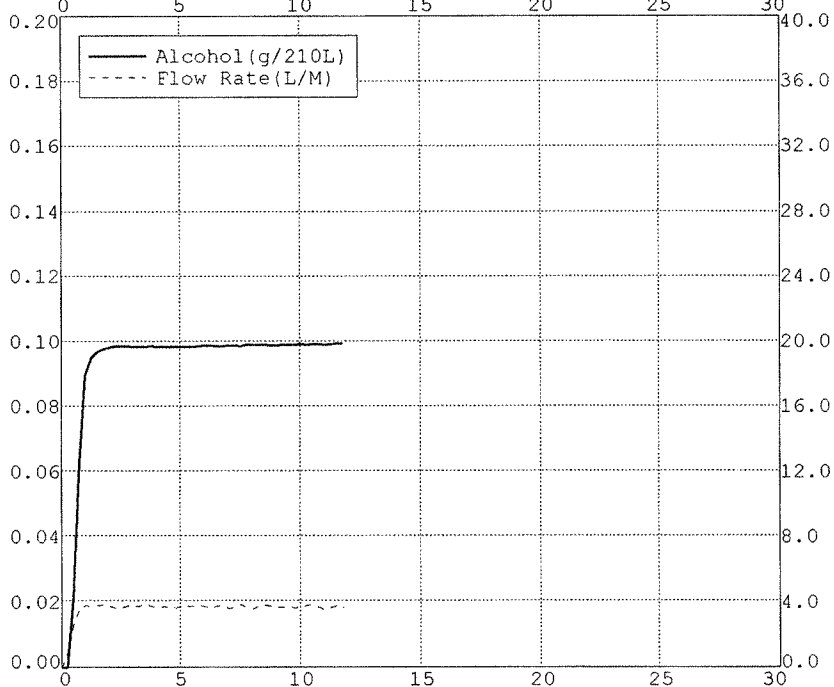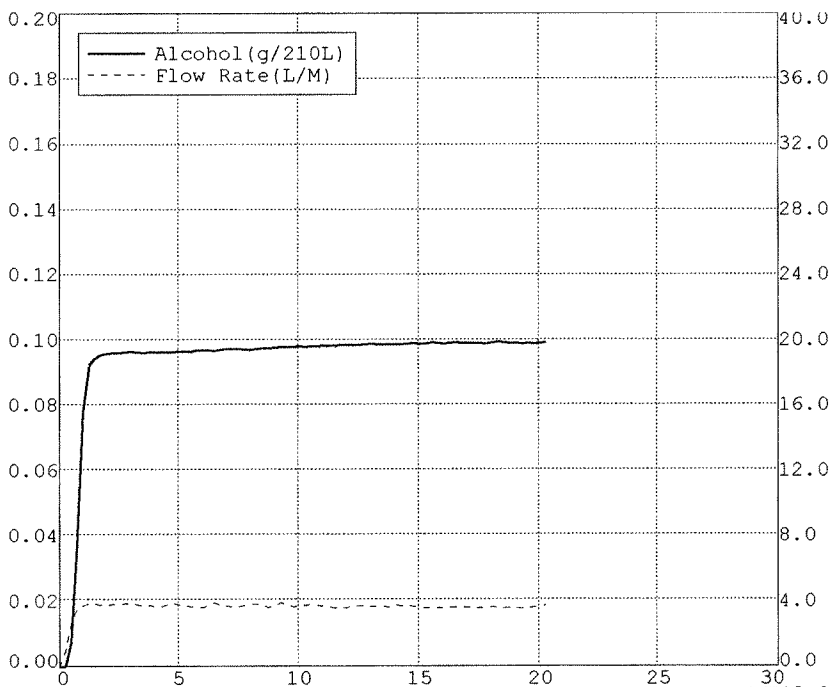

# SUPERVISOR TEST


LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 06/16/2025

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 25110

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 20:02 |
| INTERNAL STANDARD       | VERIFIED | 20:02 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.09     | 20:02 |
| BLANK TEST              | 0.00     | 20:03 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.09     | 20:03 |
| BLANK TEST              | 0.00     | 20:04 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.09     | 20:04 |
| BLANK TEST              | 0.00     | 20:05 |

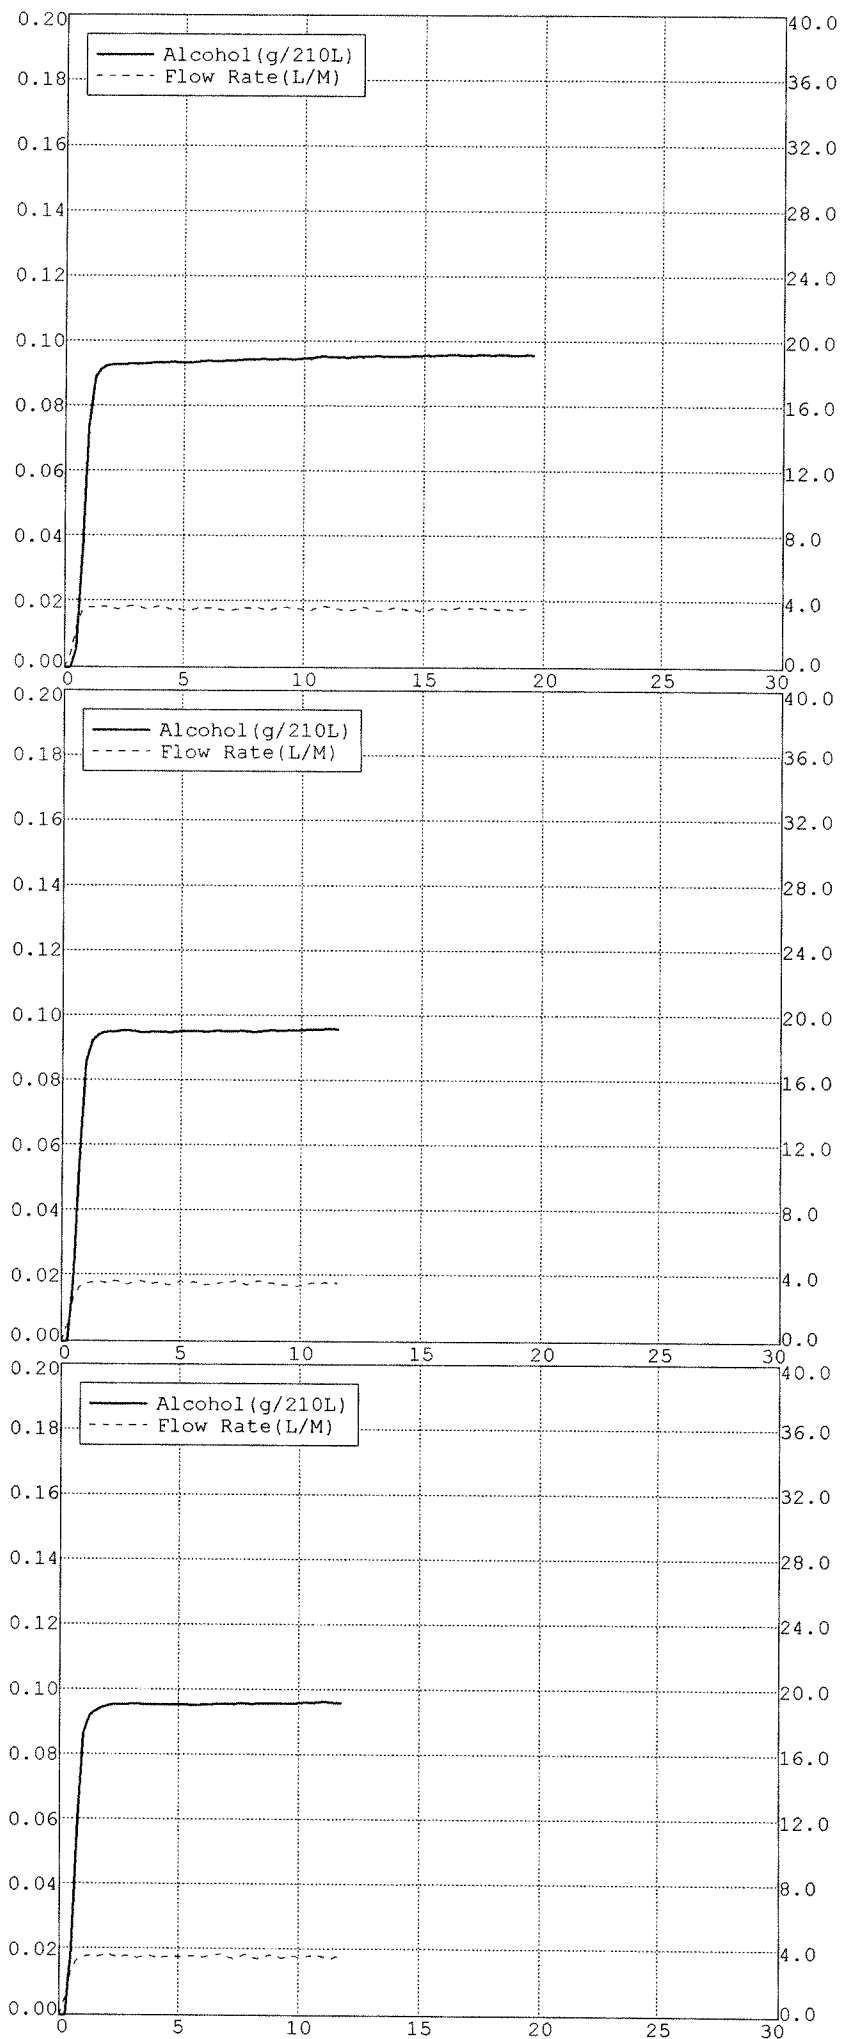

# SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 06/22/2025

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 25110

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 03:11 |
| INTERNAL STANDARD       | VERIFIED | 03:11 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.09     | 03:11 |
| BLANK TEST              | 0.00     | 03:12 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.09     | 03:12 |
| BLANK TEST              | 0.00     | 03:13 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.09     | 03:13 |
| BLANK TEST              | 0.00     | 03:14 |

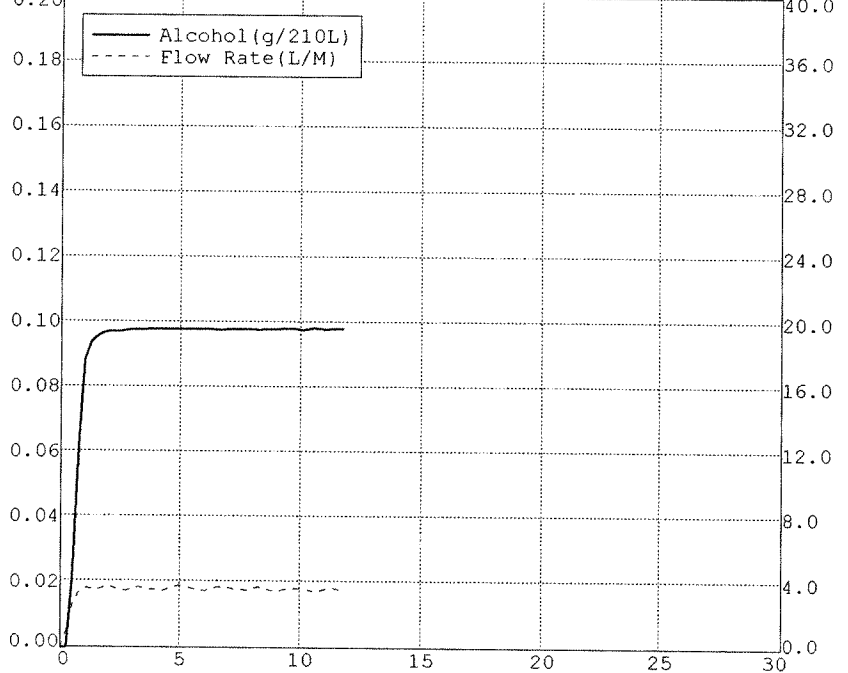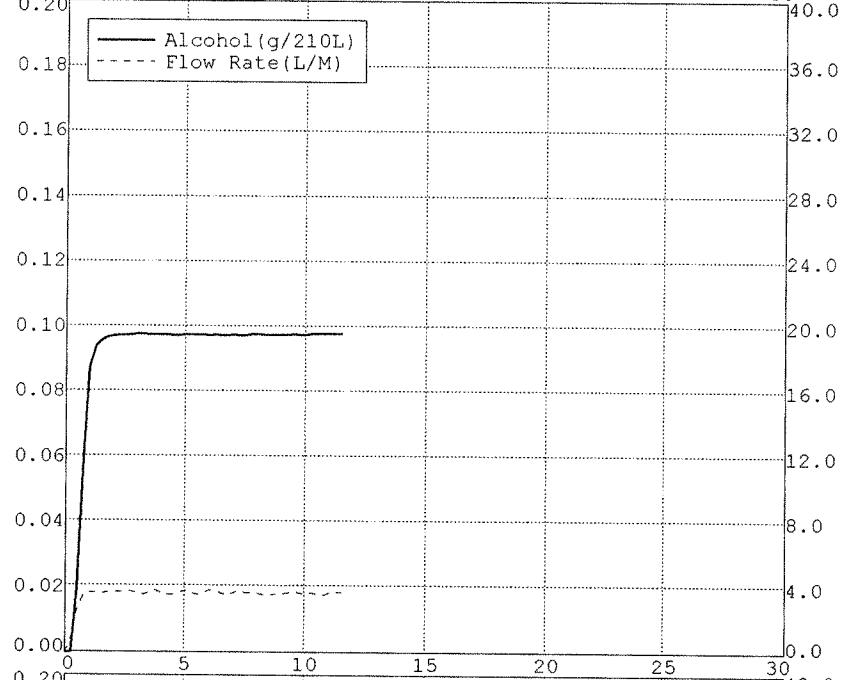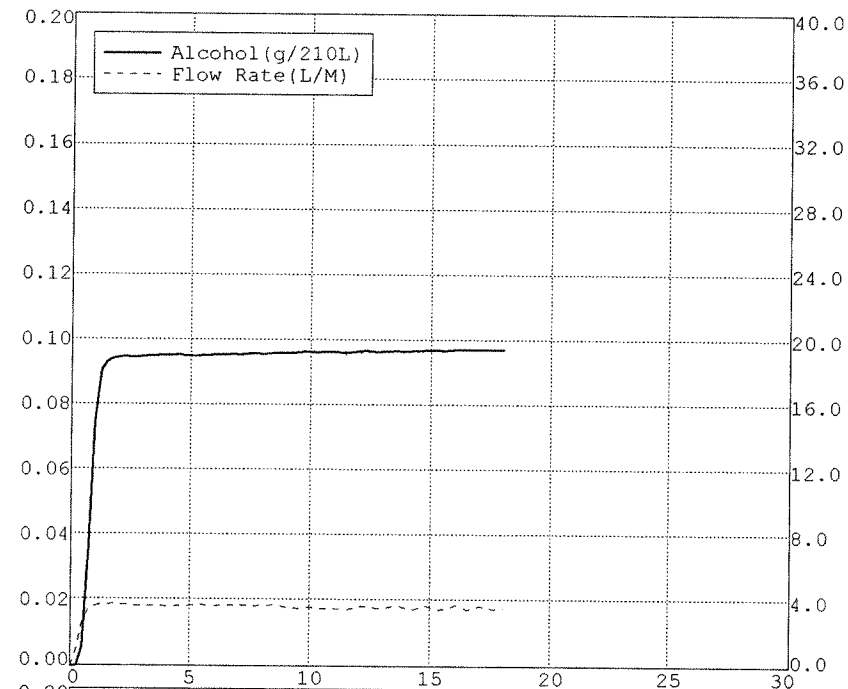

# SUPERVISOR TEST

LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 06/29/2025

OPERATOR NAME:  
MAKENZIE A HAYES  
Permit #: 49532  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 25110

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 08:10 |
| INTERNAL STANDARD       | VERIFIED | 08:10 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 08:10 |
| BLANK TEST              | 0.00     | 08:11 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 08:11 |
| BLANK TEST              | 0.00     | 08:12 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 08:12 |
| BLANK TEST              | 0.00     | 08:13 |

