

SUPERVISOR TEST



LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 10/03/2022

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:11
INTERNAL STANDARD	VERIFIED	18:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:11
BLANK TEST	0.00	18:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:12
BLANK TEST	0.00	18:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:13
BLANK TEST	0.00	18:14

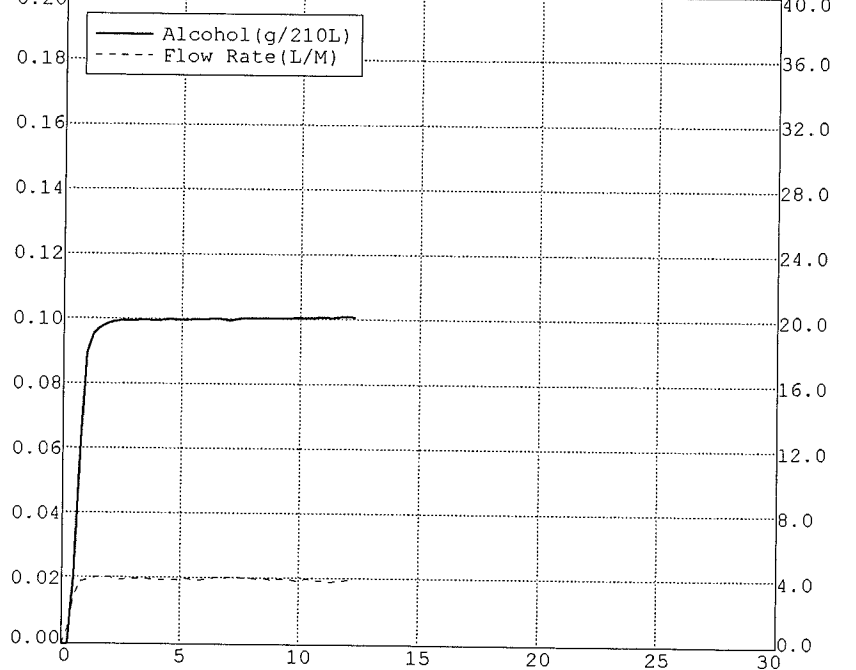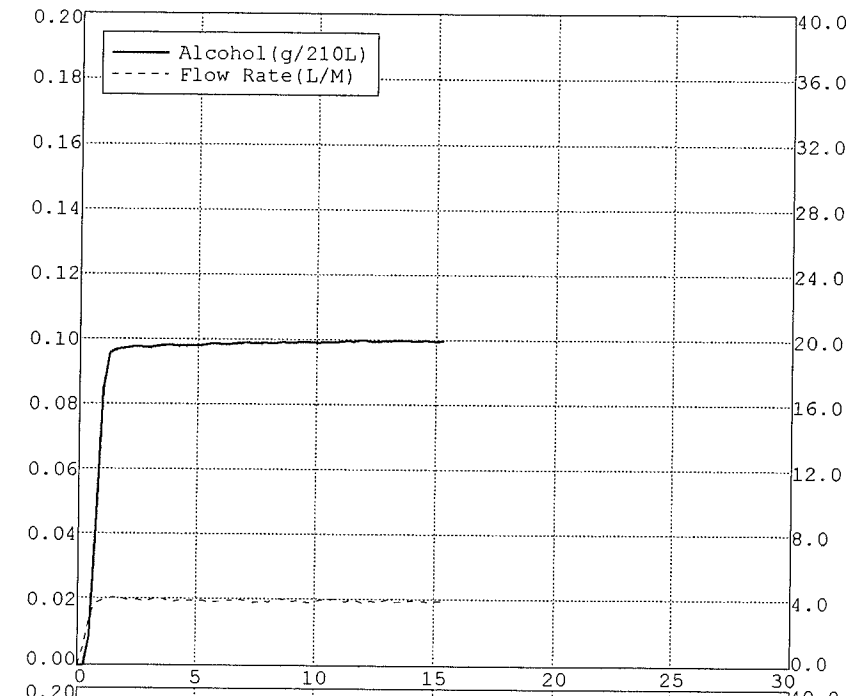

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 10/09/2022

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:23
INTERNAL STANDARD	VERIFIED	05:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:24
BLANK TEST	0.00	05:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:25
BLANK TEST	0.00	05:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:26
BLANK TEST	0.00	05:27

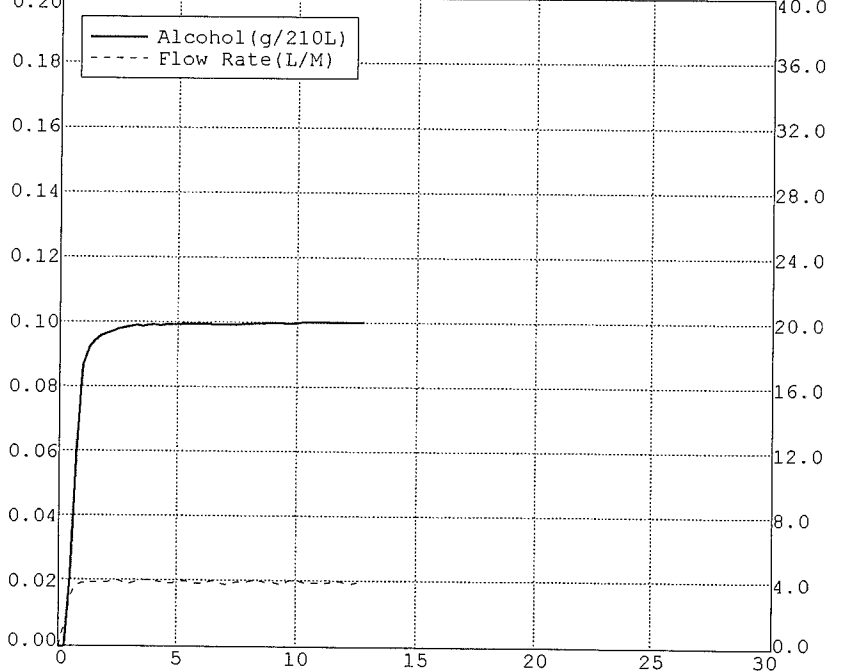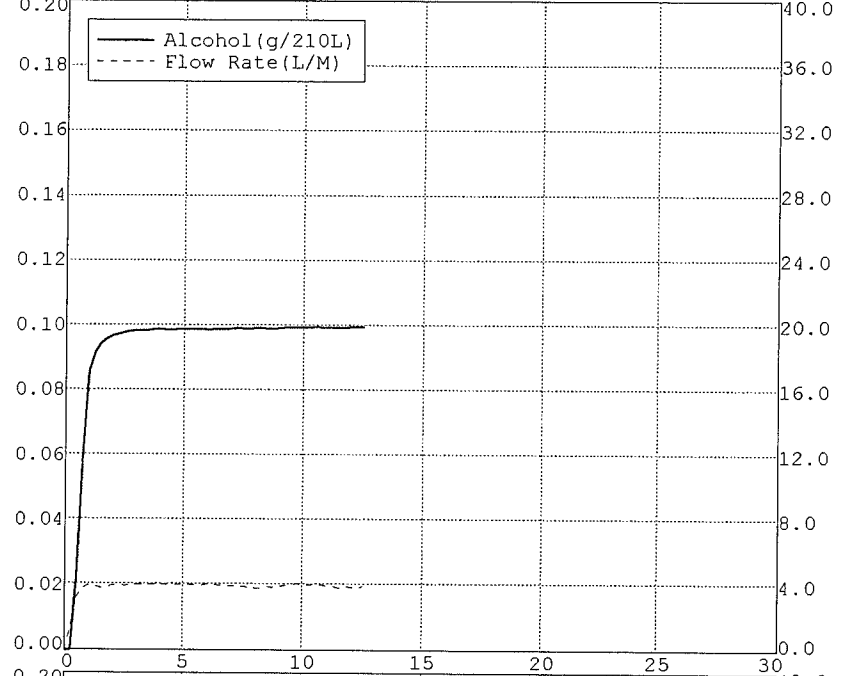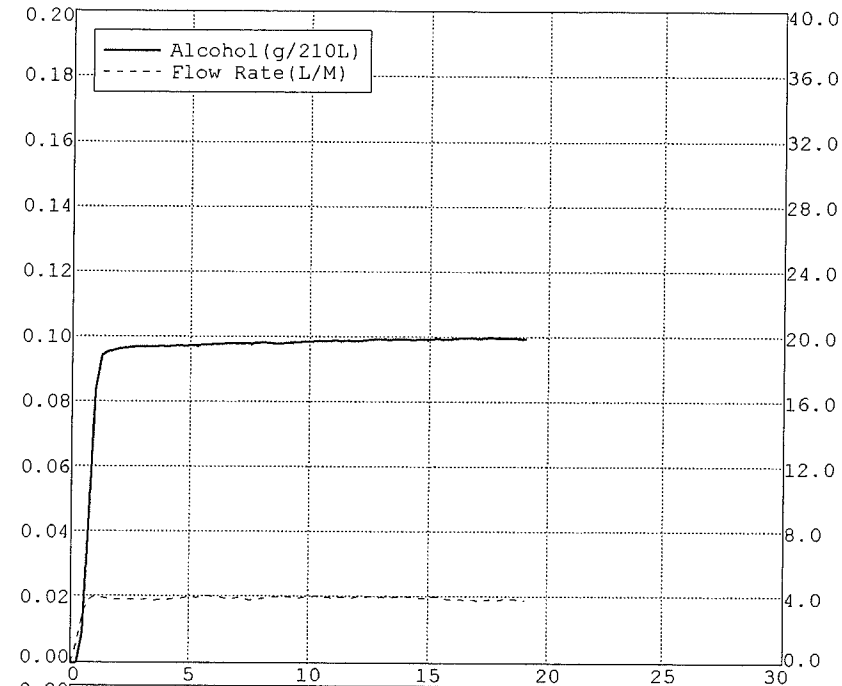

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 10/17/2022

OPERATOR NAME:
IAN GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:06
INTERNAL STANDARD	VERIFIED	18:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:07
BLANK TEST	0.00	18:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:08
BLANK TEST	0.00	18:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:09
BLANK TEST	0.00	18:10

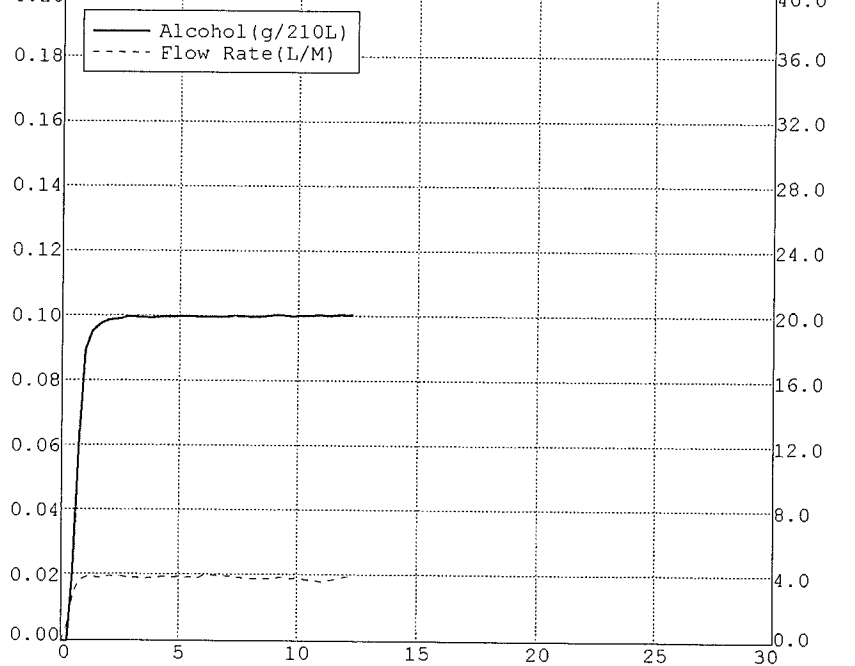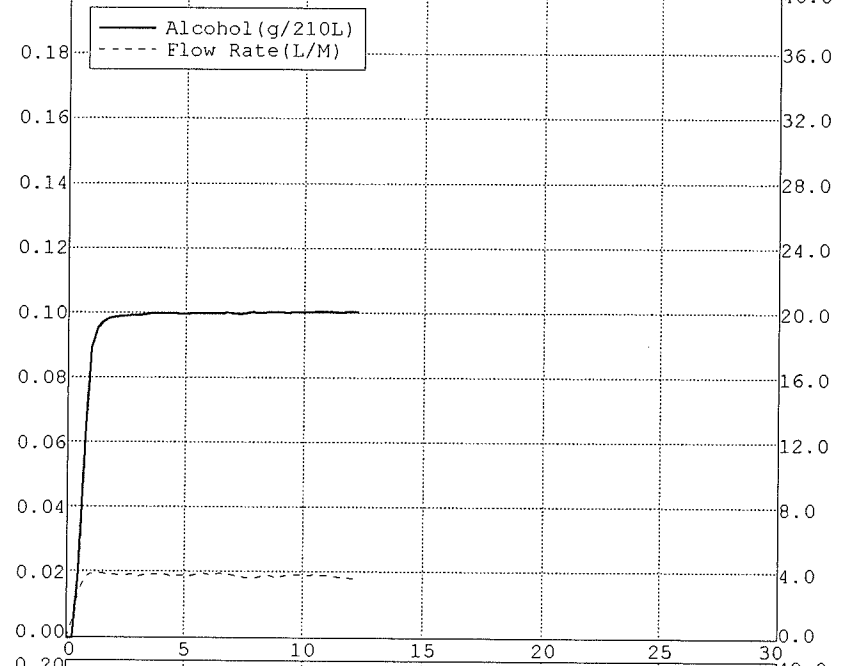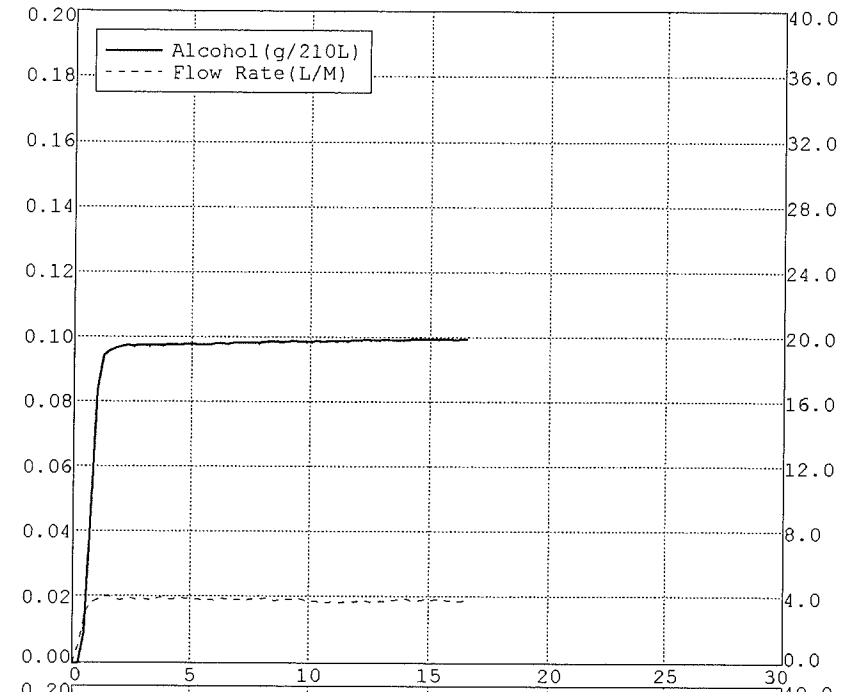

SUPERVISOR TEST

LAKE PLACID VILLAGE
 POLICE DEPT.
 DATAMASTER dmt: 100290

Date: 10/23/2022

OPERATOR NAME:
 IAN O GORDON
 Permit #: 50784
 Operator Agency/Dept: LAKE PLACID VILL. PD
 Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:51
INTERNAL STANDARD	VERIFIED	16:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:51
BLANK TEST	0.00	16:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:52
BLANK TEST	0.00	16:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:54
BLANK TEST	0.00	16:54

