

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 12/06/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:16
INTERNAL STANDARD	VERIFIED	08:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:16
BLANK TEST	0.00	08:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:17
BLANK TEST	0.00	08:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:19
BLANK TEST	0.00	08:19

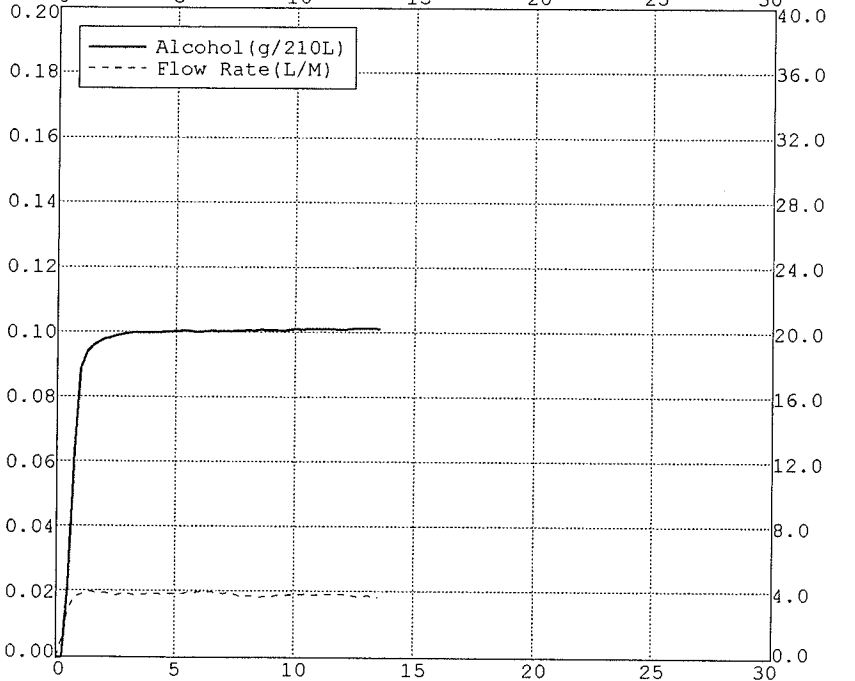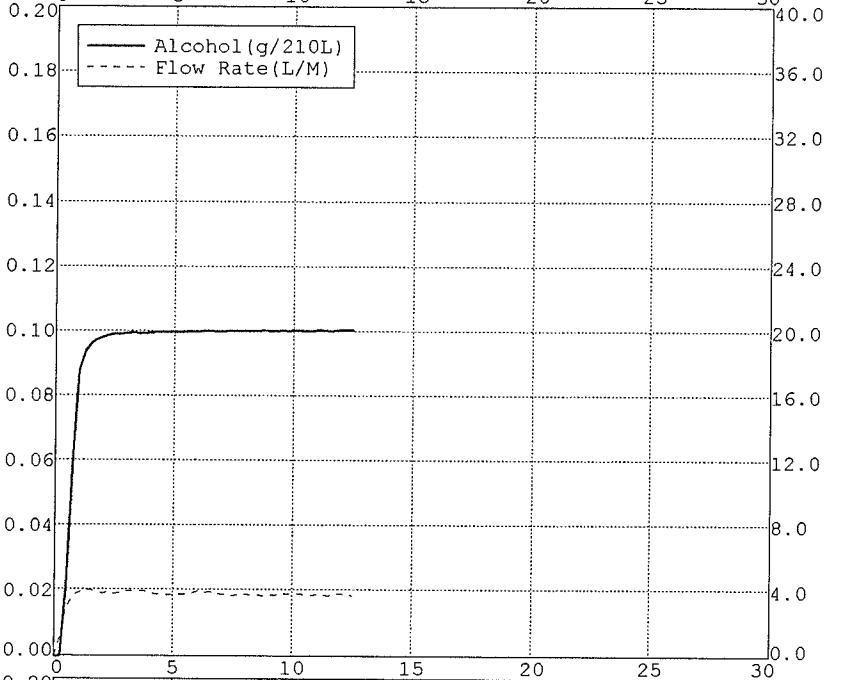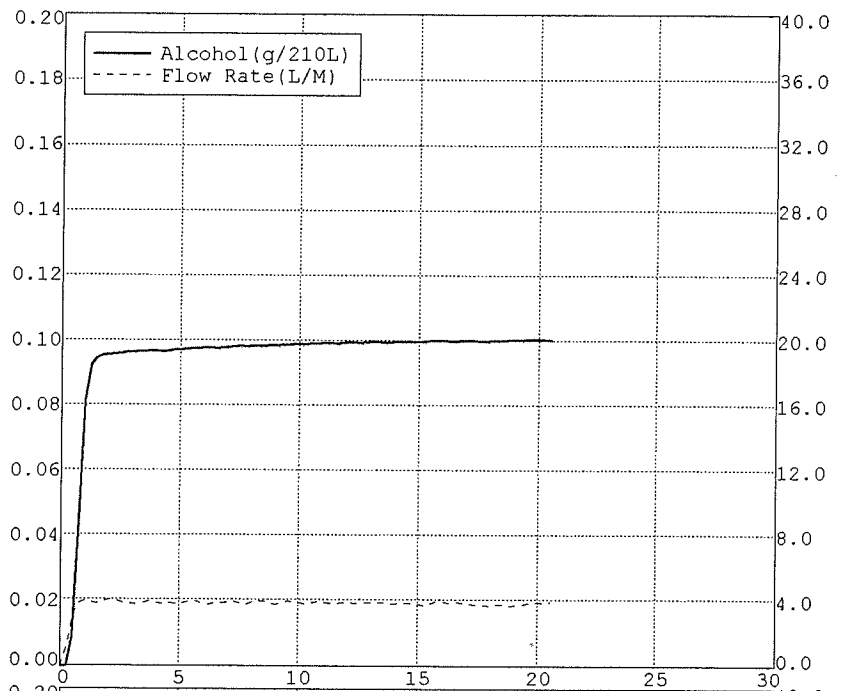

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 12/12/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:45
INTERNAL STANDARD	VERIFIED	09:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:45
BLANK TEST	0.00	09:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:46
BLANK TEST	0.00	09:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:47
BLANK TEST	0.00	09:48

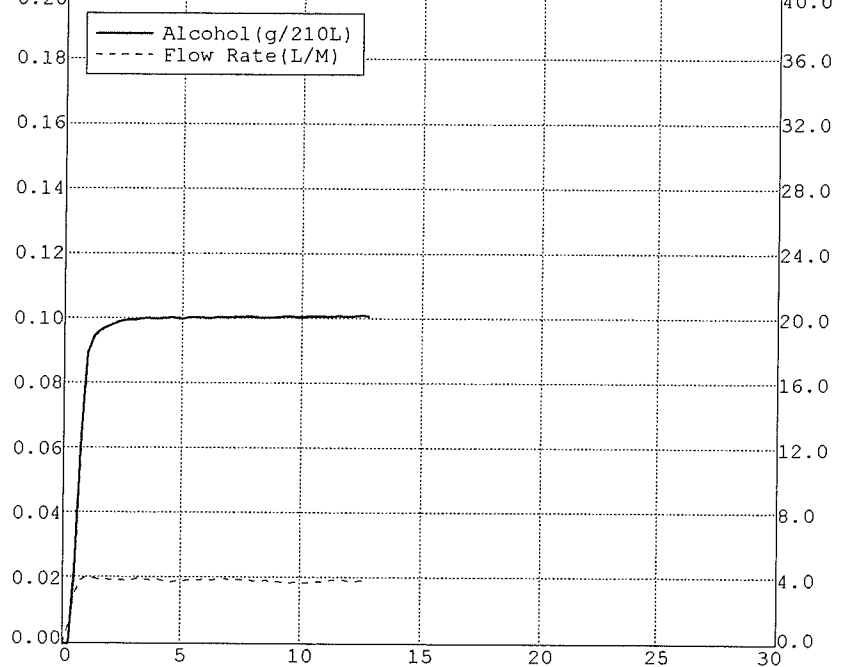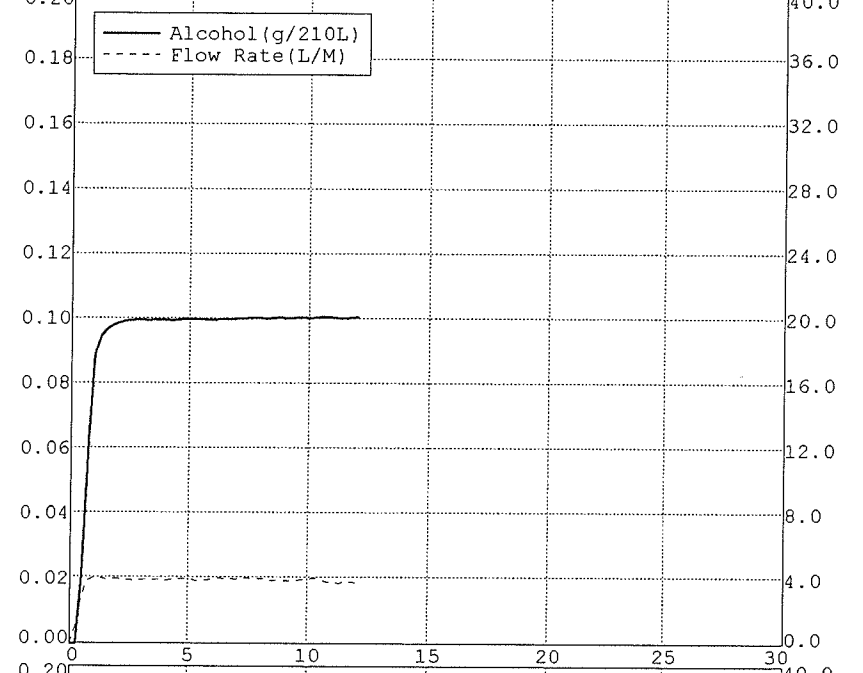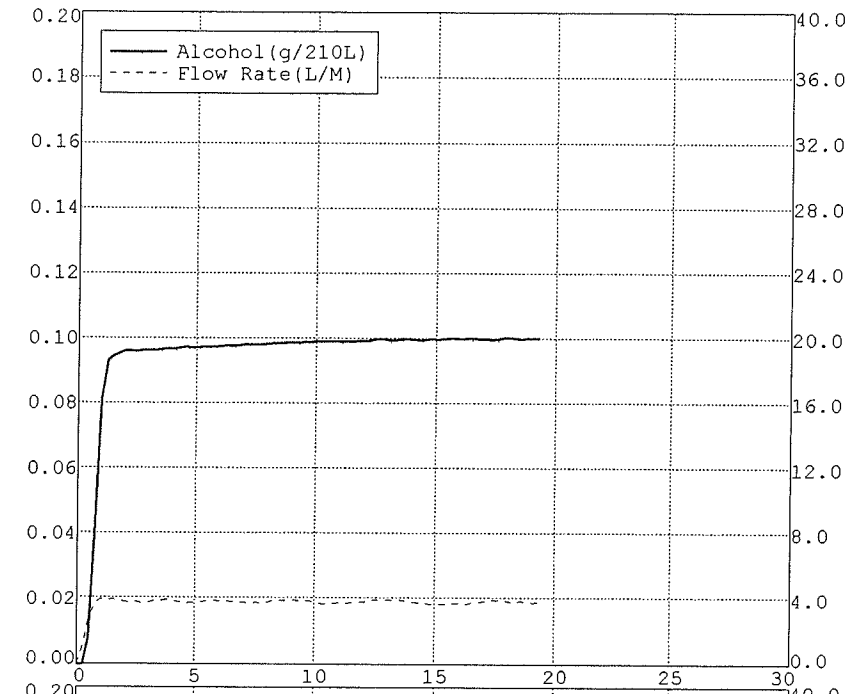

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 12/20/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:34
INTERNAL STANDARD	VERIFIED	17:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:34
BLANK TEST	0.00	17:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:36
BLANK TEST	0.00	17:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:37
BLANK TEST	0.00	17:38

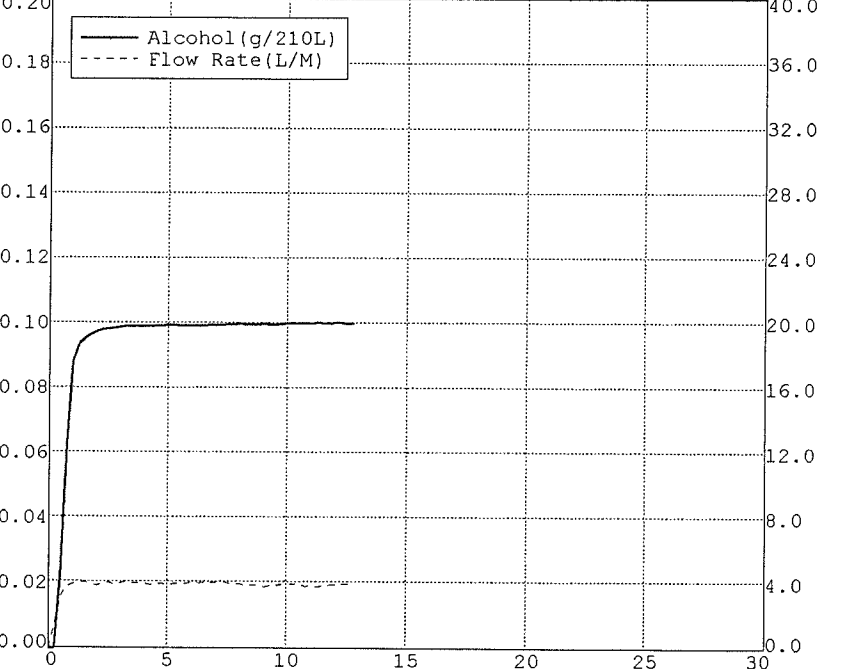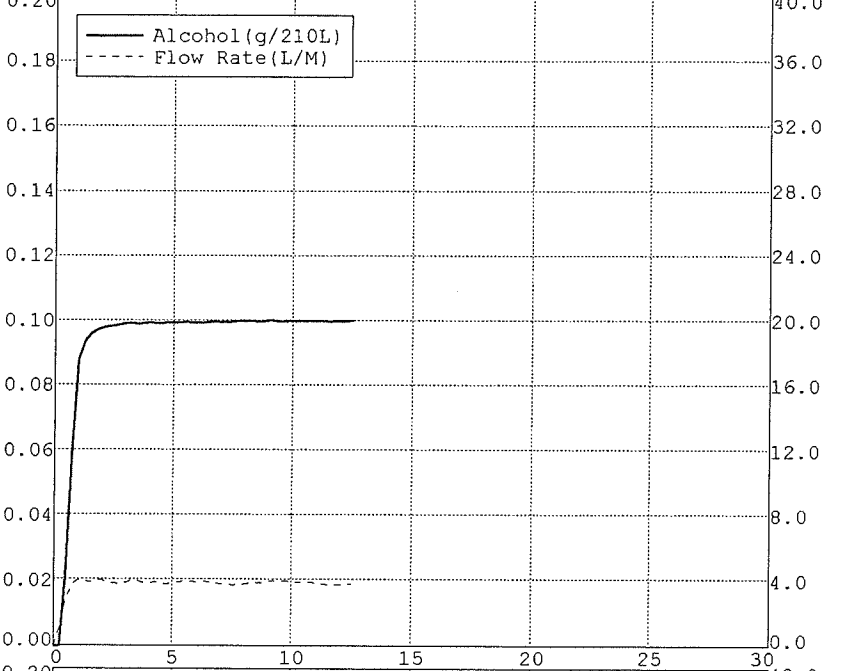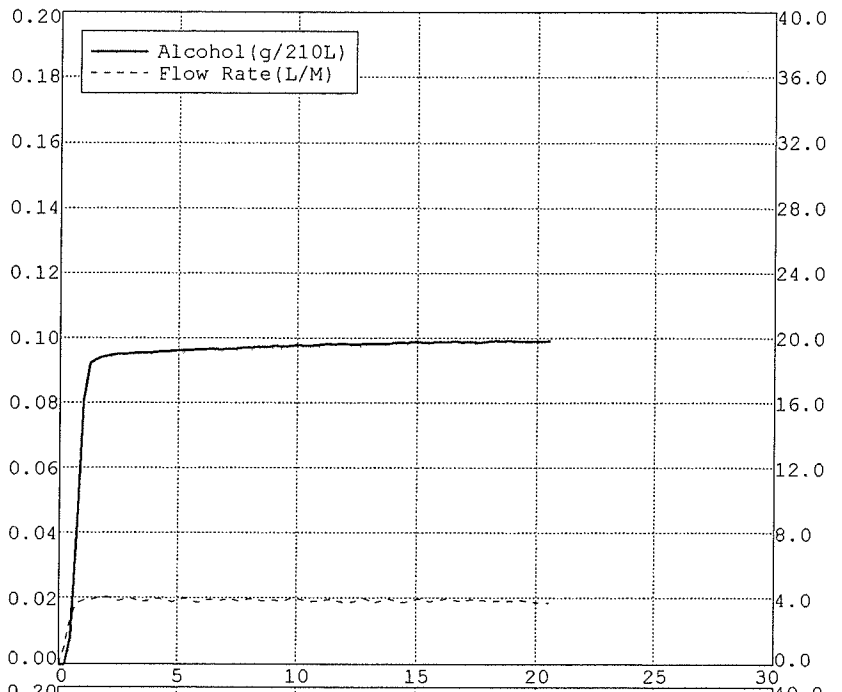

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 12/26/2021




OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:41
INTERNAL STANDARD	VERIFIED	10:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:42
BLANK TEST	0.00	10:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:43
BLANK TEST	0.00	10:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	INTERFERENCE	10:44

Interference Detected

*Datas left for an EMS
Call. Possibly caused by digital
radio*

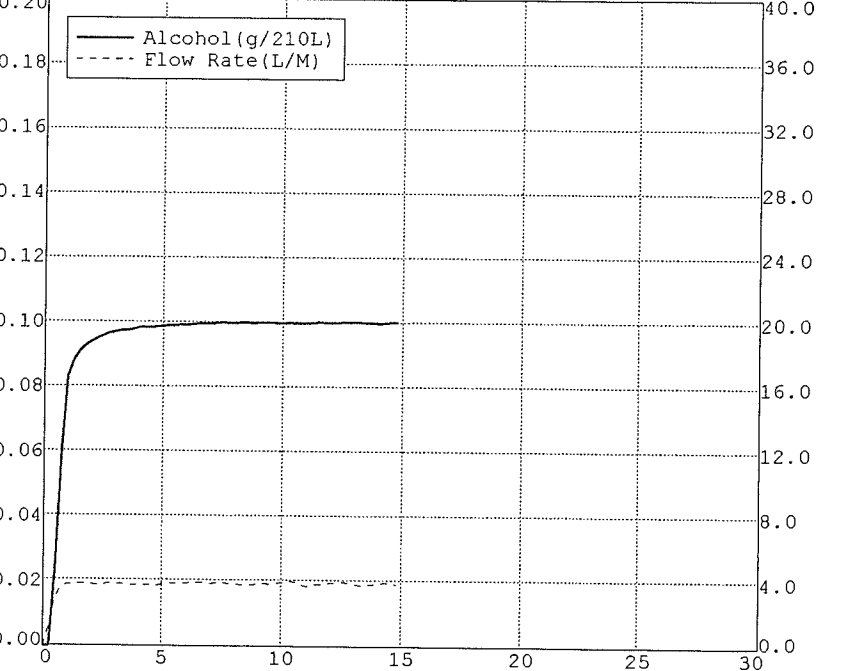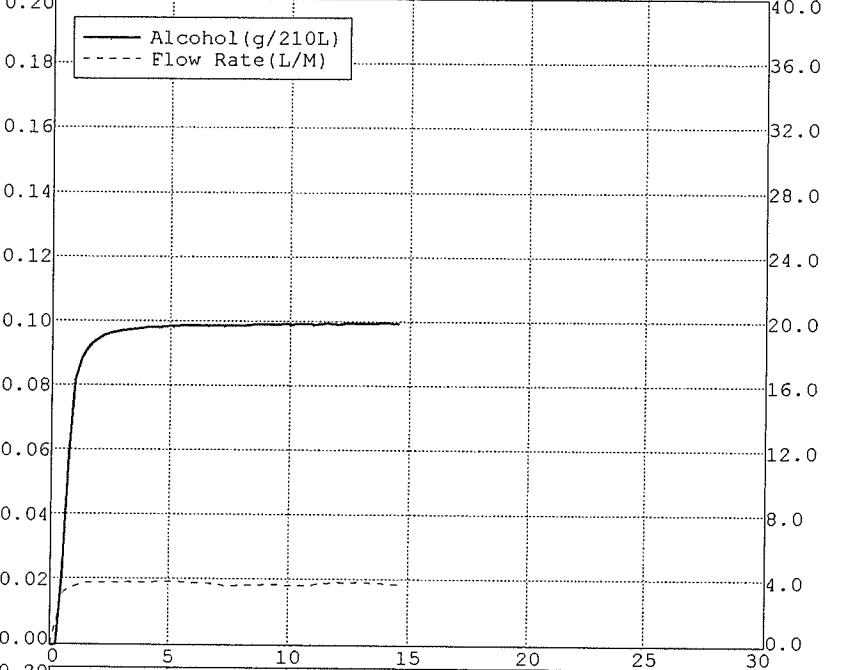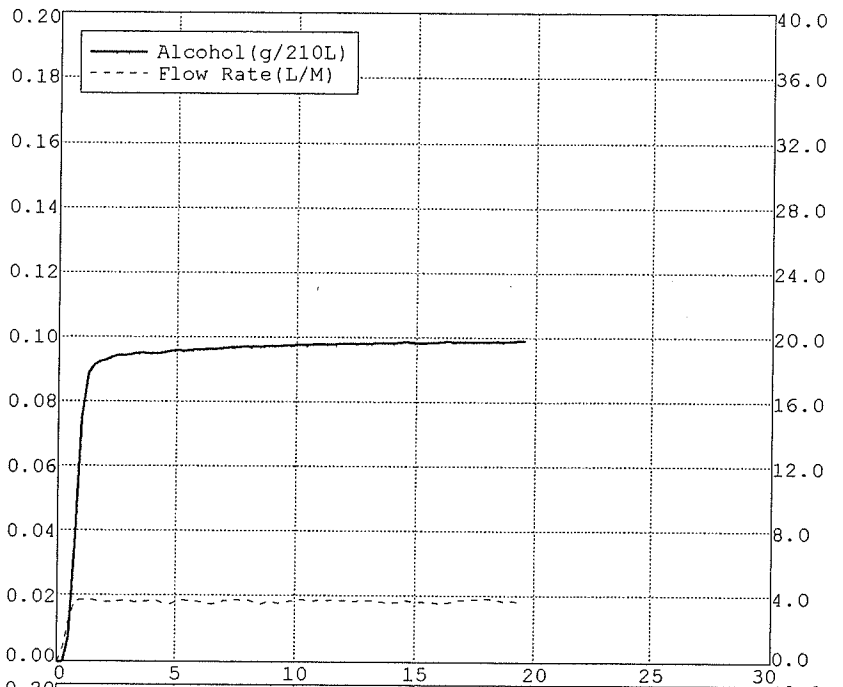

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 12/26/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:53
INTERNAL STANDARD	VERIFIED	17:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:54
BLANK TEST	0.00	17:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:55
BLANK TEST	0.00	17:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:56
BLANK TEST	0.00	17:57

