

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/05/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:17
INTERNAL STANDARD	VERIFIED	18:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:17
BLANK TEST	0.00	18:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:18
BLANK TEST	0.00	18:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:20
BLANK TEST	0.00	18:20

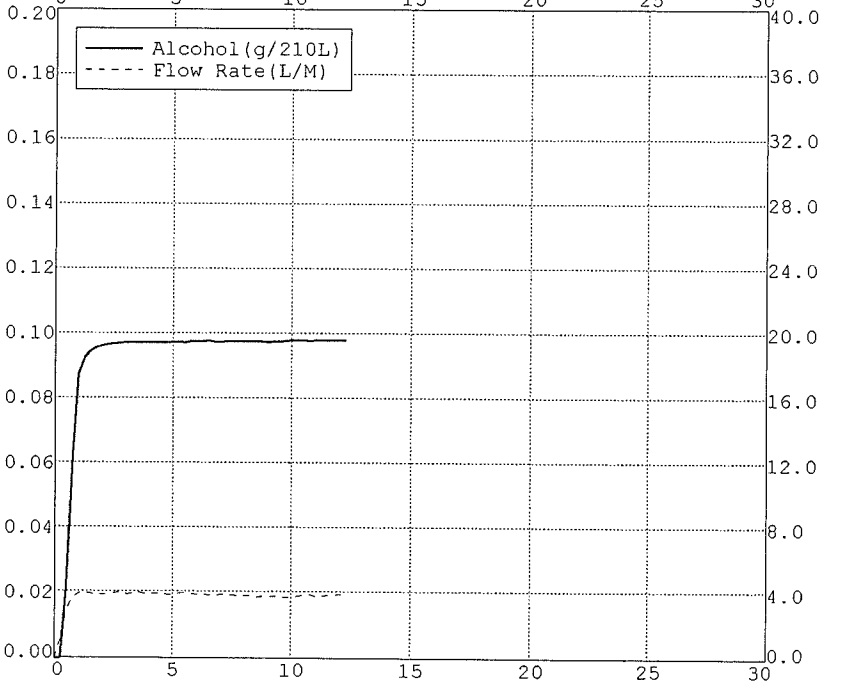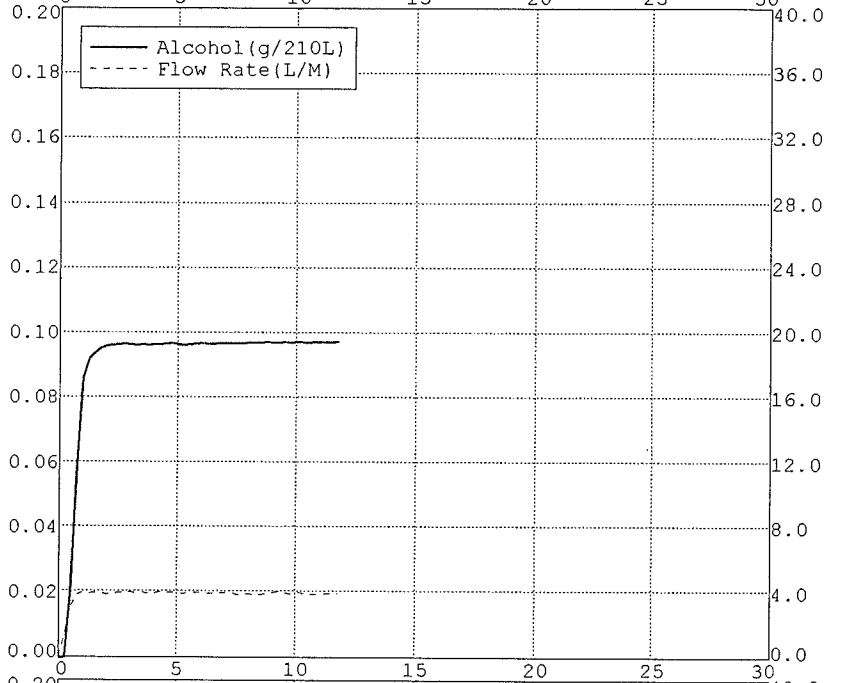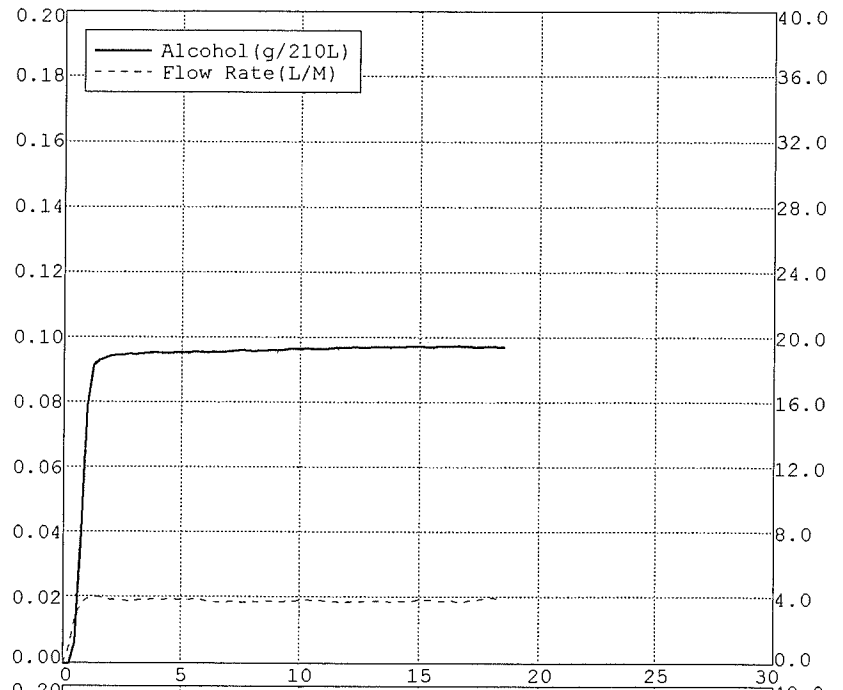

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/13/2023

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:37
INTERNAL STANDARD	VERIFIED	01:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:38
BLANK TEST	0.00	01:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:39
BLANK TEST	0.00	01:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:40
BLANK TEST	0.00	01:41

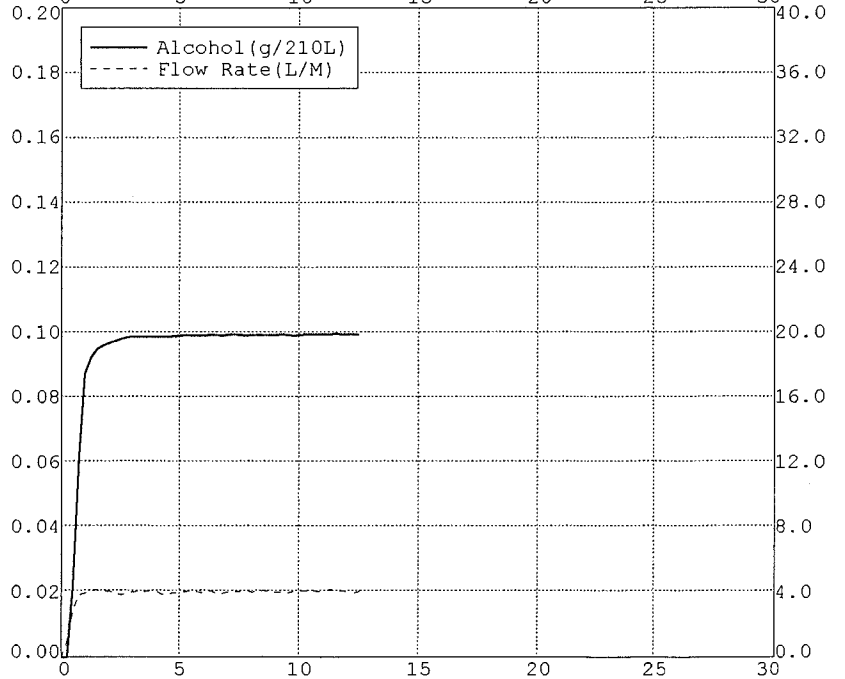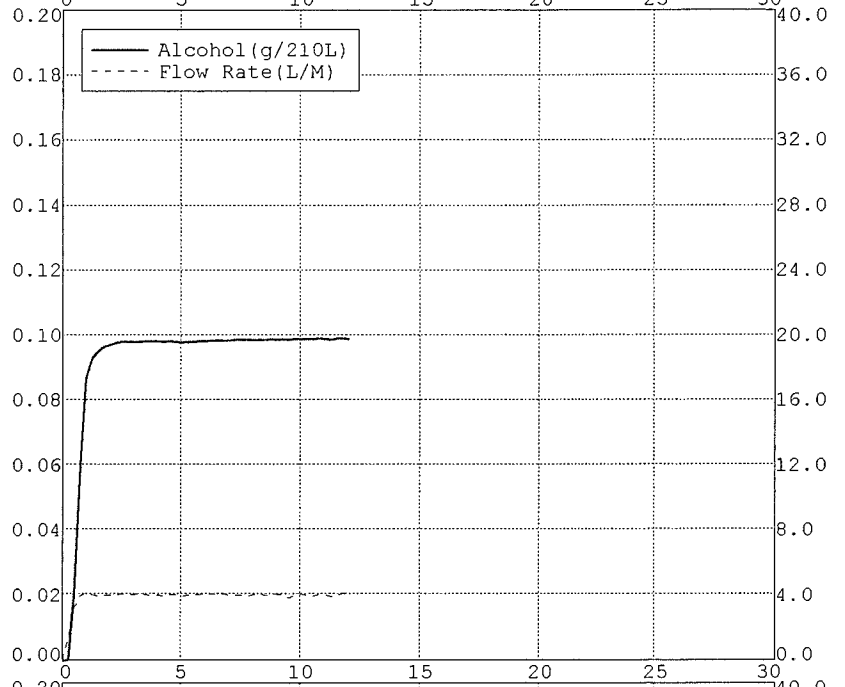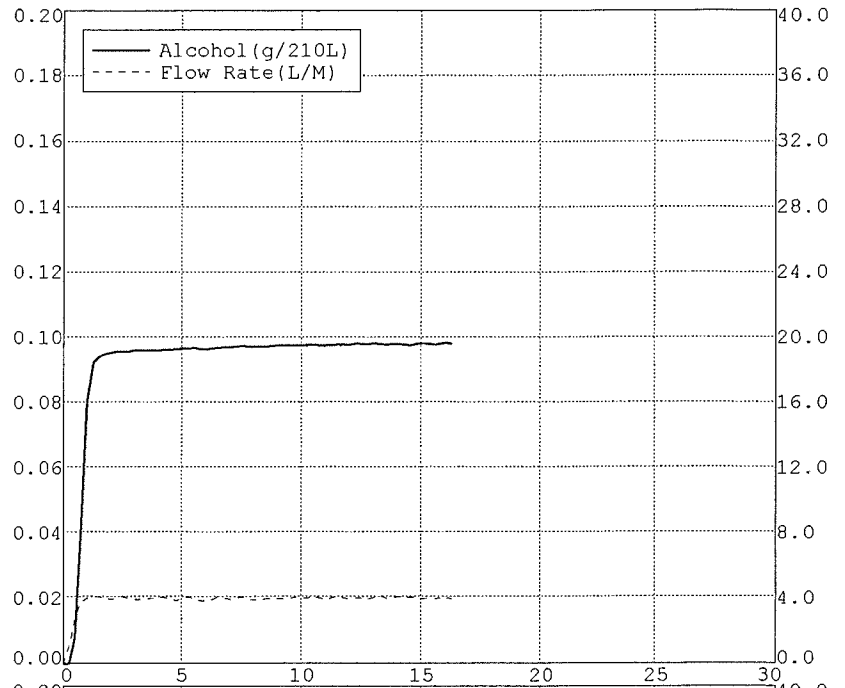

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/19/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:56
INTERNAL STANDARD	VERIFIED	15:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:56
BLANK TEST	0.00	15:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:57
BLANK TEST	0.00	15:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:58
BLANK TEST	0.00	15:59

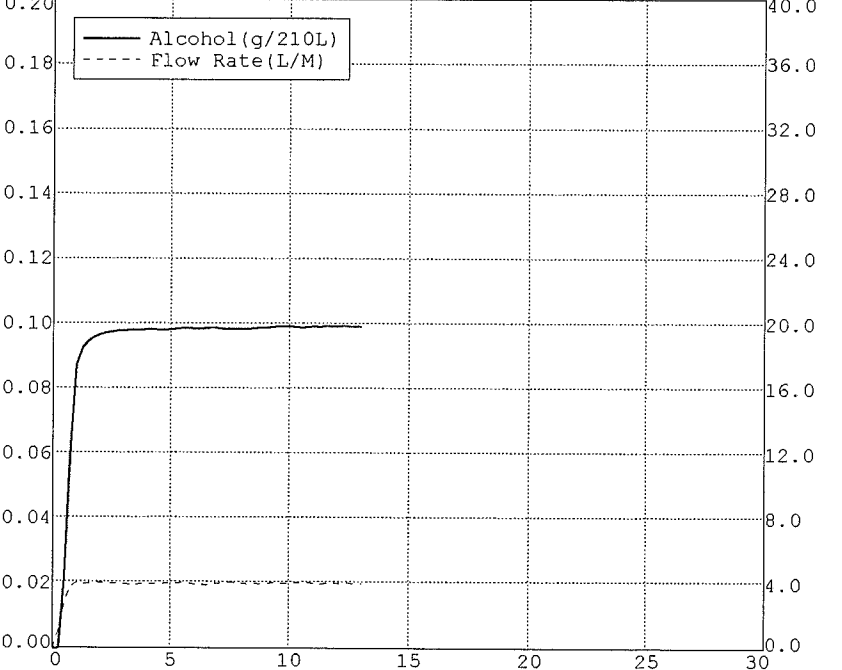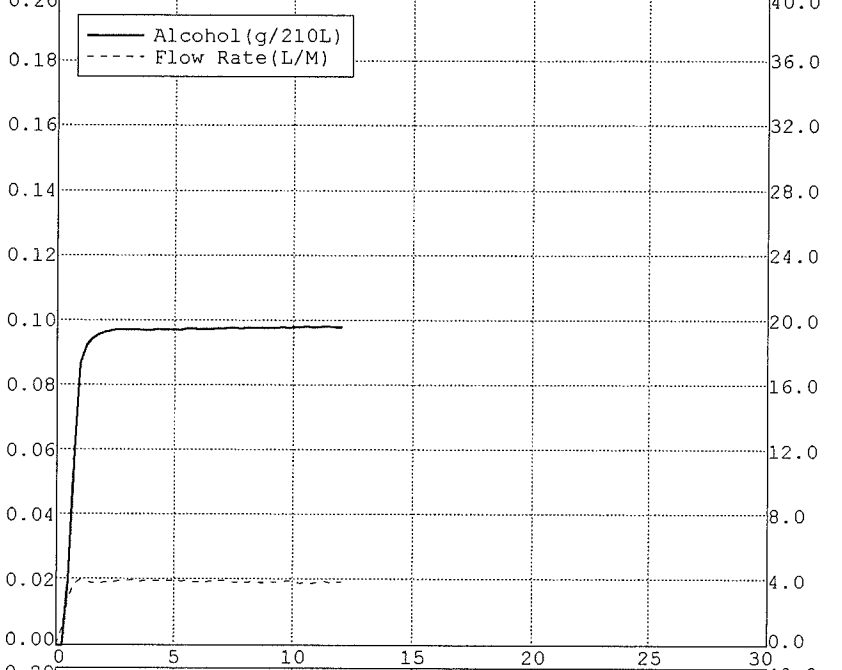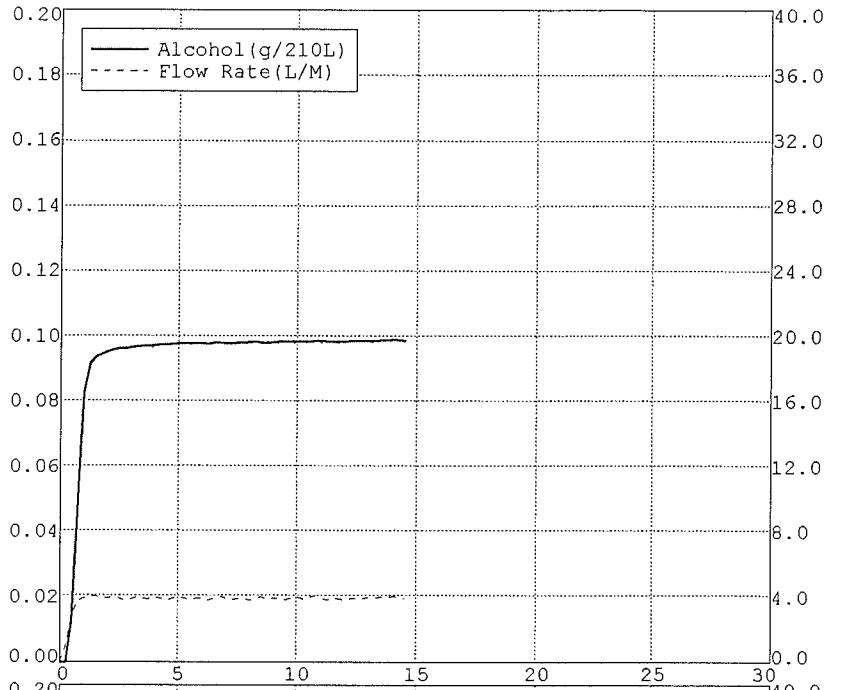

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/19/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:56
INTERNAL STANDARD	VERIFIED	15:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:56
BLANK TEST	0.00	15:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:57
BLANK TEST	0.00	15:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:58
BLANK TEST	0.00	15:59

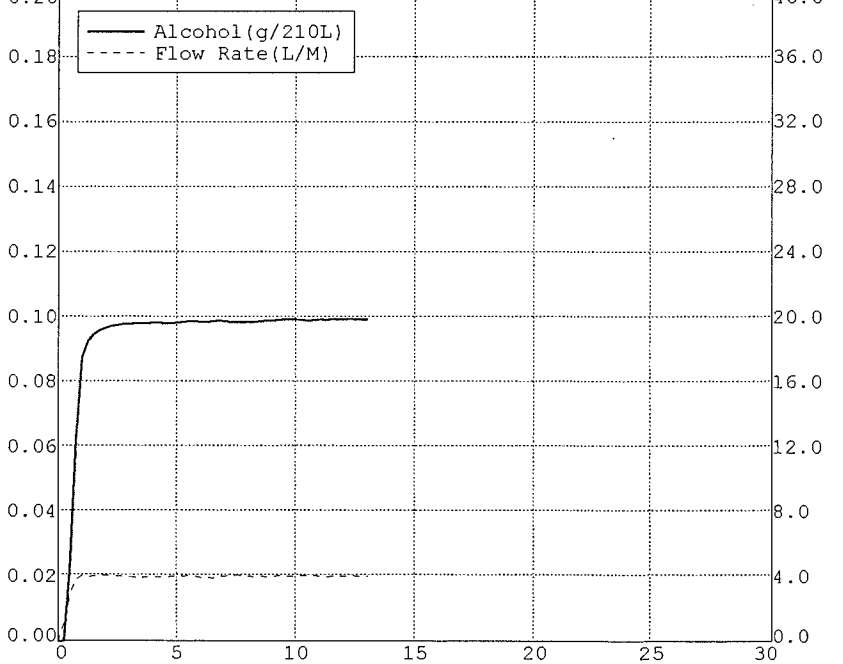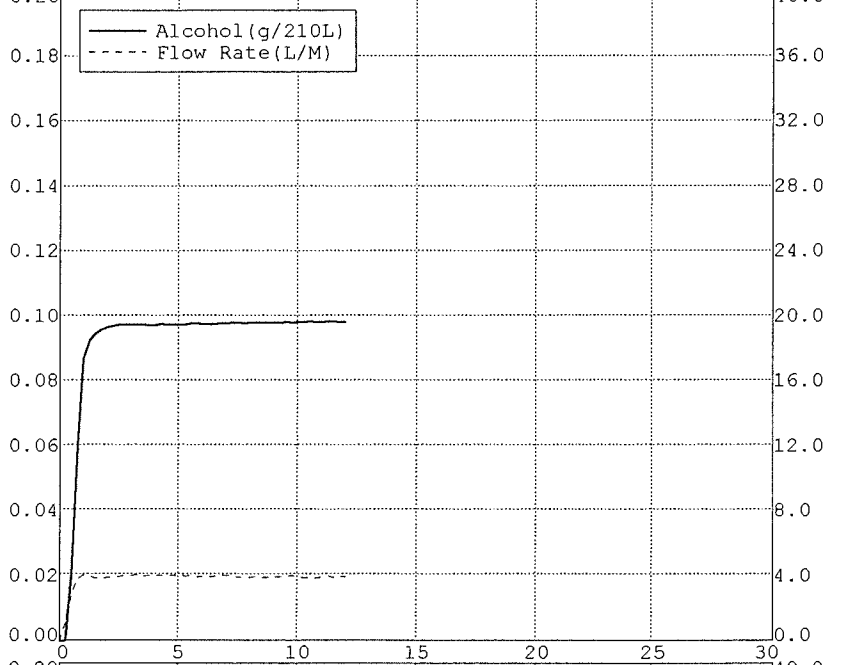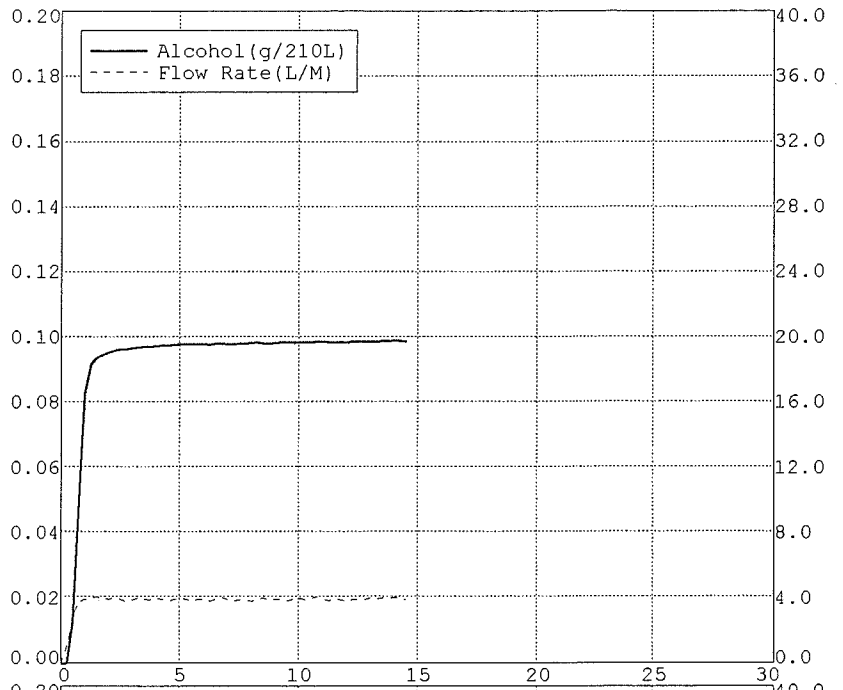

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/26/2023

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23350

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:42
INTERNAL STANDARD	VERIFIED	19:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:42
BLANK TEST	0.00	19:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:43
BLANK TEST	0.00	19:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:45
BLANK TEST	0.00	19:45

