

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 10/06/2024

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24270

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:03
INTERNAL STANDARD	VERIFIED	12:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:03
BLANK TEST	0.00	12:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:04
BLANK TEST	0.00	12:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:05
BLANK TEST	0.00	12:06

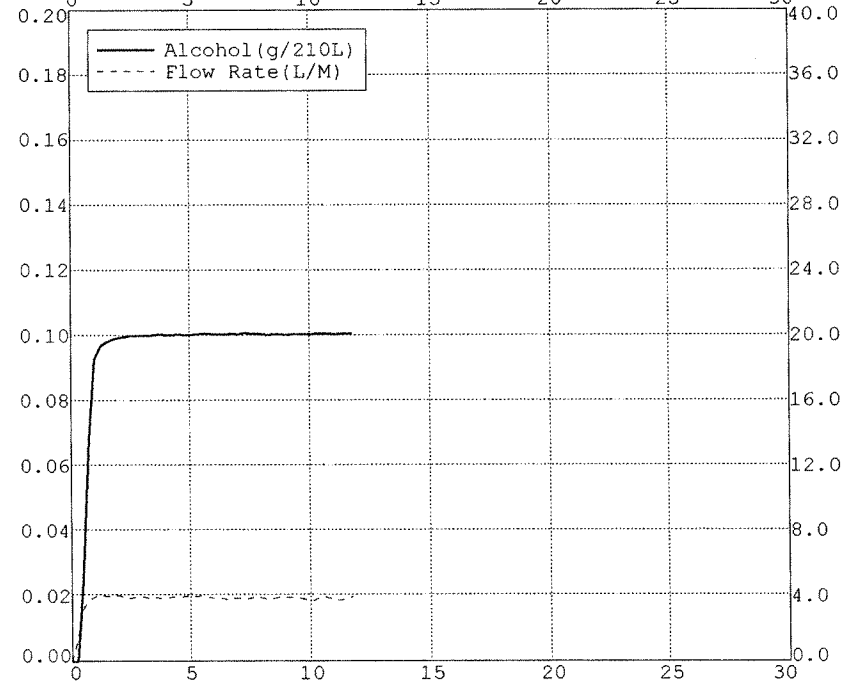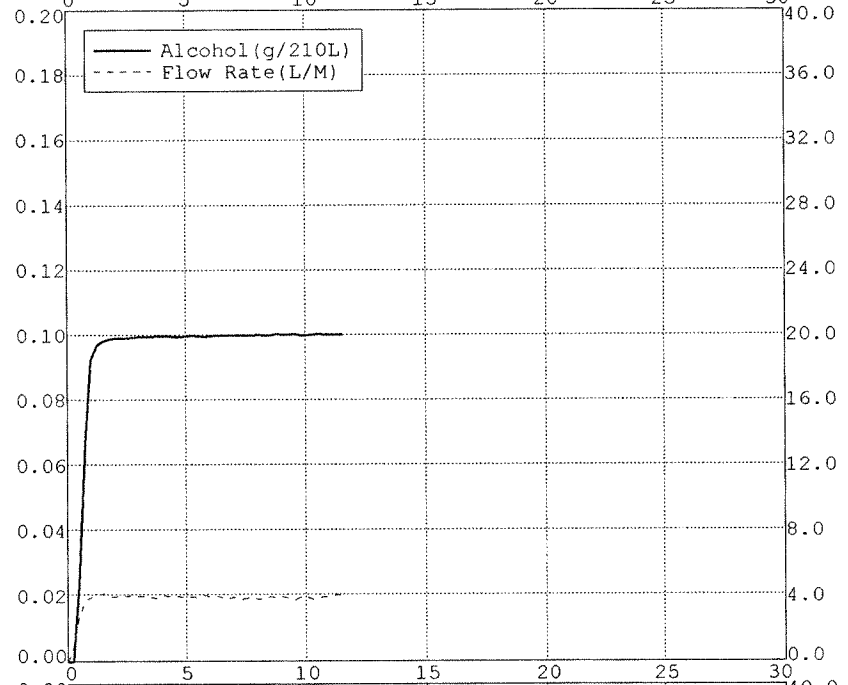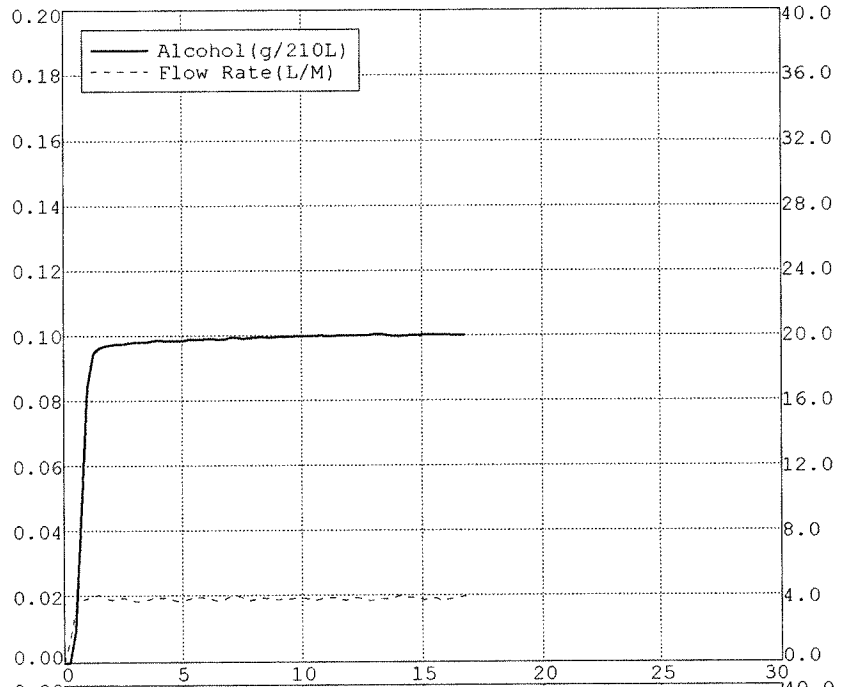

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 10/13/2024

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24270

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:29
INTERNAL STANDARD	VERIFIED	04:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:29
BLANK TEST	0.00	04:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:30
BLANK TEST	0.00	04:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:32
BLANK TEST	0.00	04:32

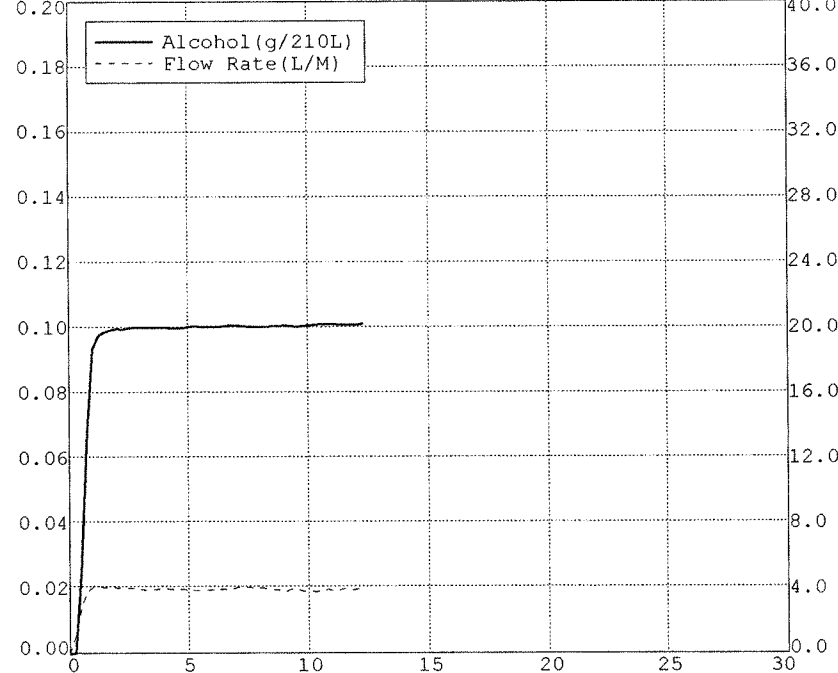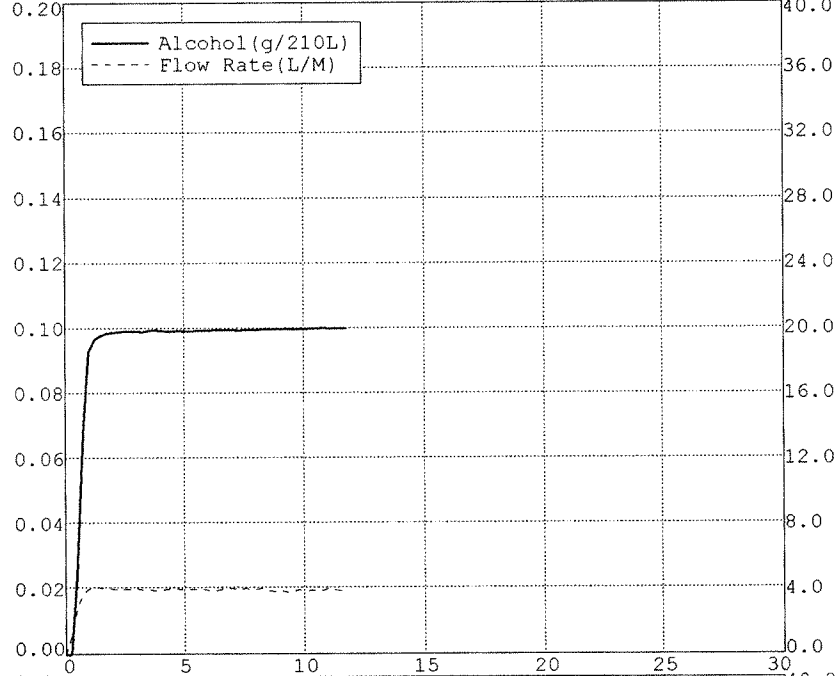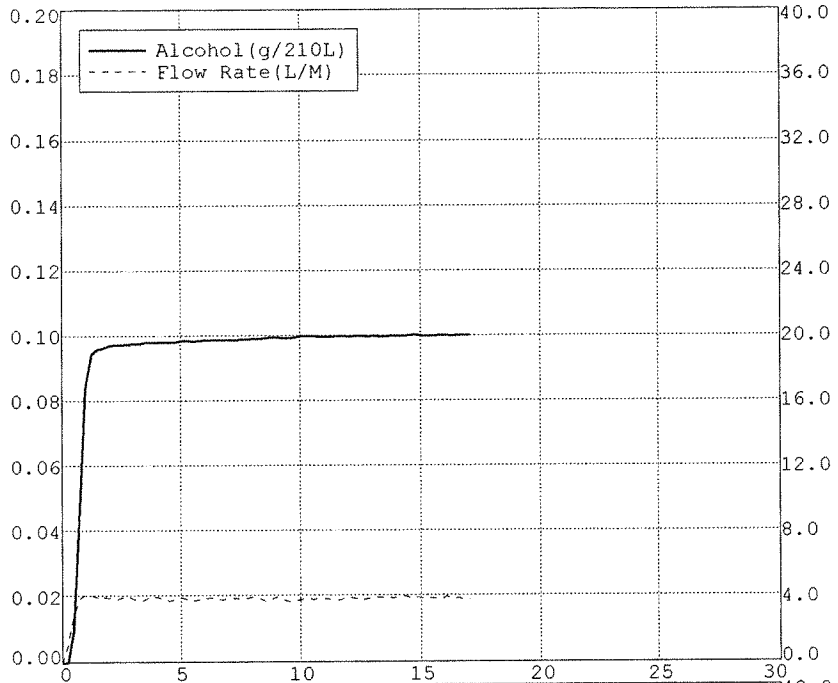

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 10/20/2024

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24270

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:46
INTERNAL STANDARD	VERIFIED	16:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:47
BLANK TEST	0.00	16:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:48
BLANK TEST	0.00	16:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:49
BLANK TEST	0.00	16:50

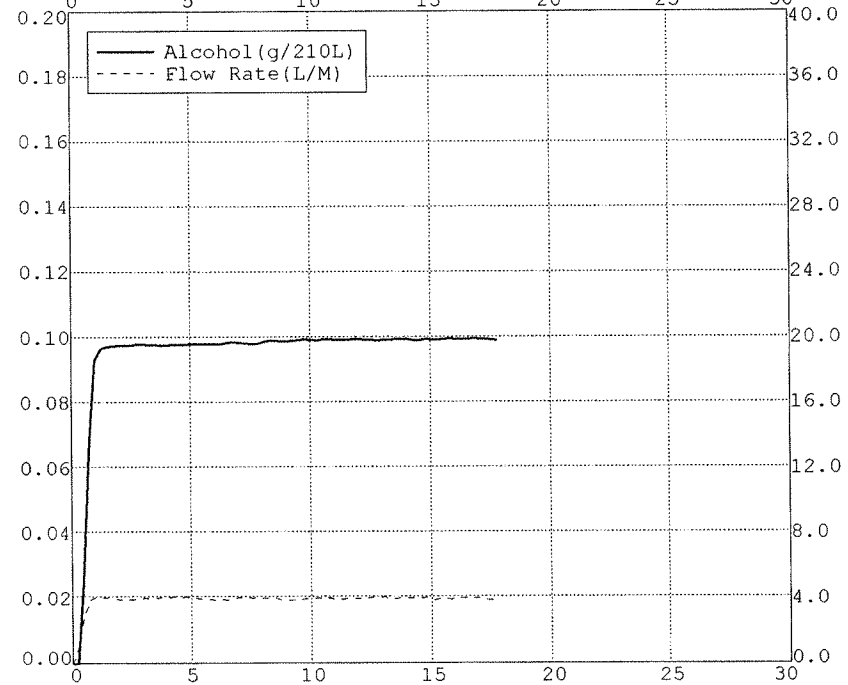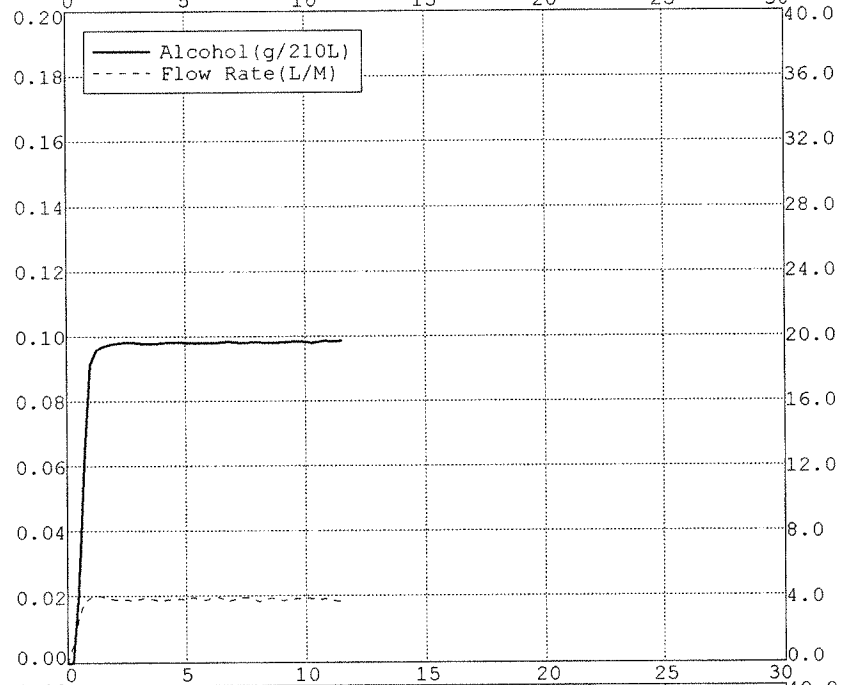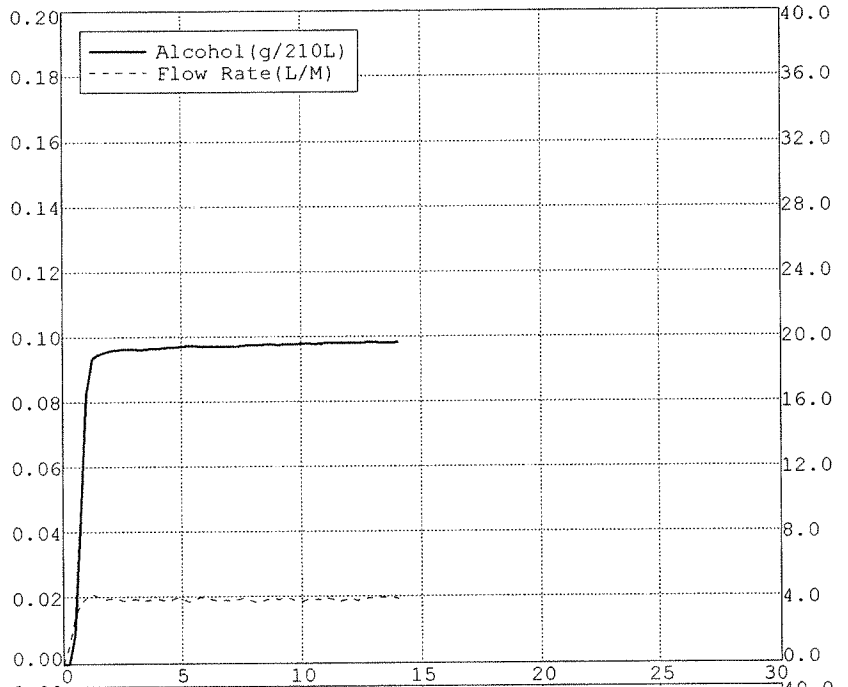

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 10/27/2024

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24270

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:35
INTERNAL STANDARD	VERIFIED	11:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:35
BLANK TEST	0.00	11:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:36
BLANK TEST	0.00	11:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:37
BLANK TEST	0.00	11:38

