

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/04/2024

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24190

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 18:08 |
| INTERNAL STANDARD | VERIFIED | 18:08 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:08 |
| BLANK TEST | 0.00 | 18:09 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:09 |
| BLANK TEST | 0.00 | 18:10 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:11 |
| BLANK TEST | 0.00 | 18:11 |

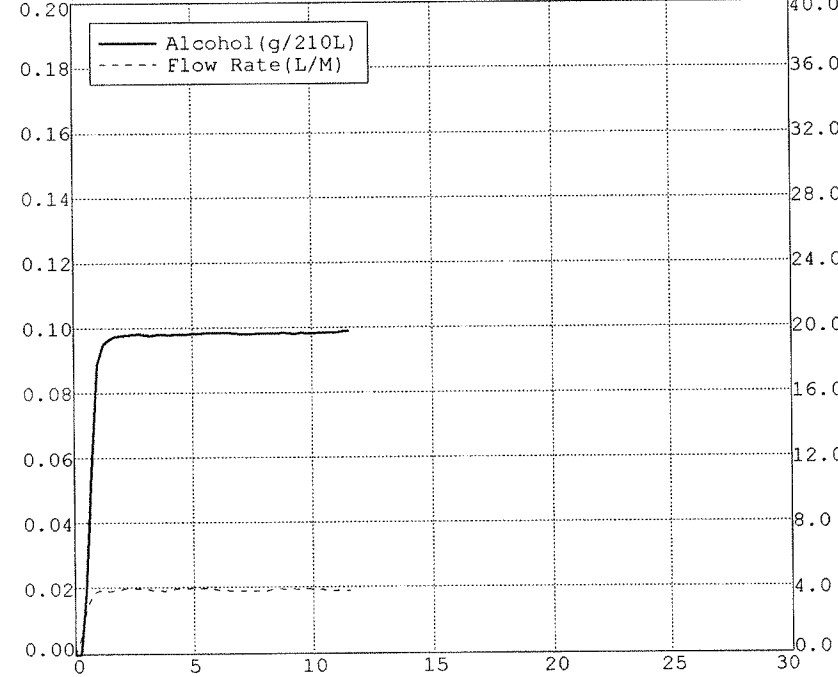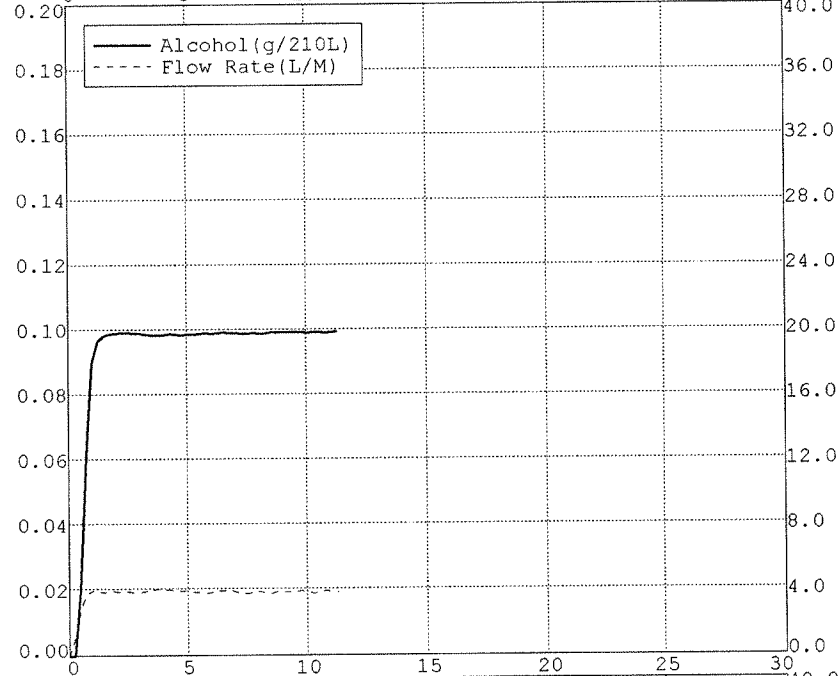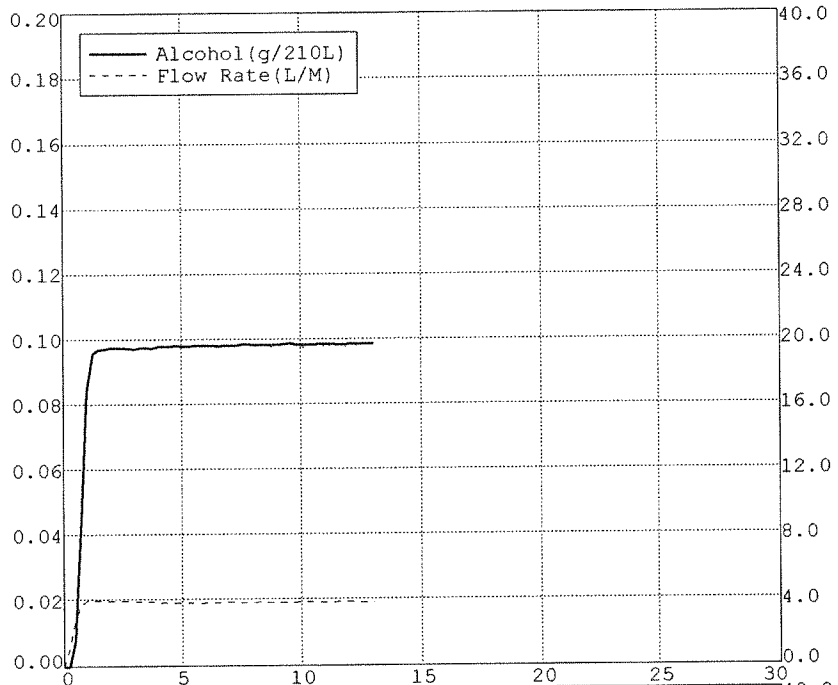

SUPERVISOR TEST



LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/11/2024

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24190

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 18:38 |
| INTERNAL STANDARD | VERIFIED | 18:38 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:39 |
| BLANK TEST | 0.00 | 18:40 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:40 |
| BLANK TEST | 0.00 | 18:41 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:41 |
| BLANK TEST | 0.00 | 18:42 |

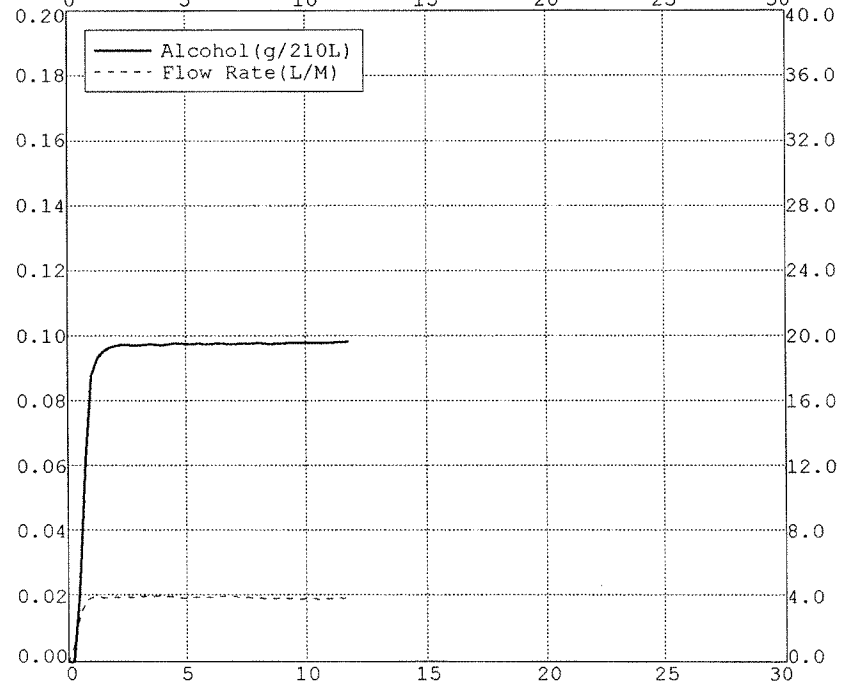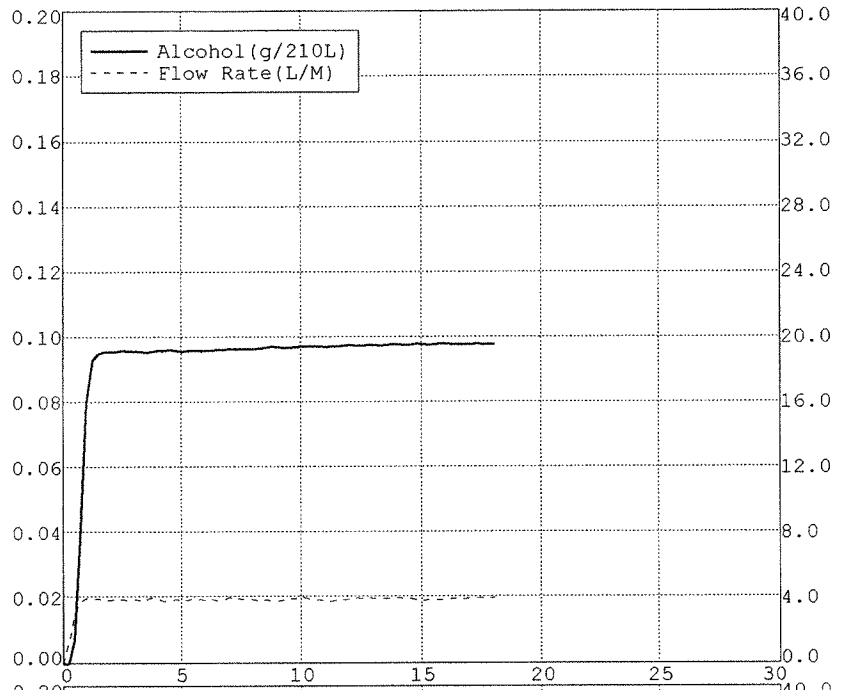

SUPERVISOR TEST



LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/18/2024

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24190

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 19:51 |
| INTERNAL STANDARD | VERIFIED | 19:51 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 19:51 |
| BLANK TEST | 0.00 | 19:52 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 19:53 |
| BLANK TEST | 0.00 | 19:53 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 19:54 |
| BLANK TEST | 0.00 | 19:54 |

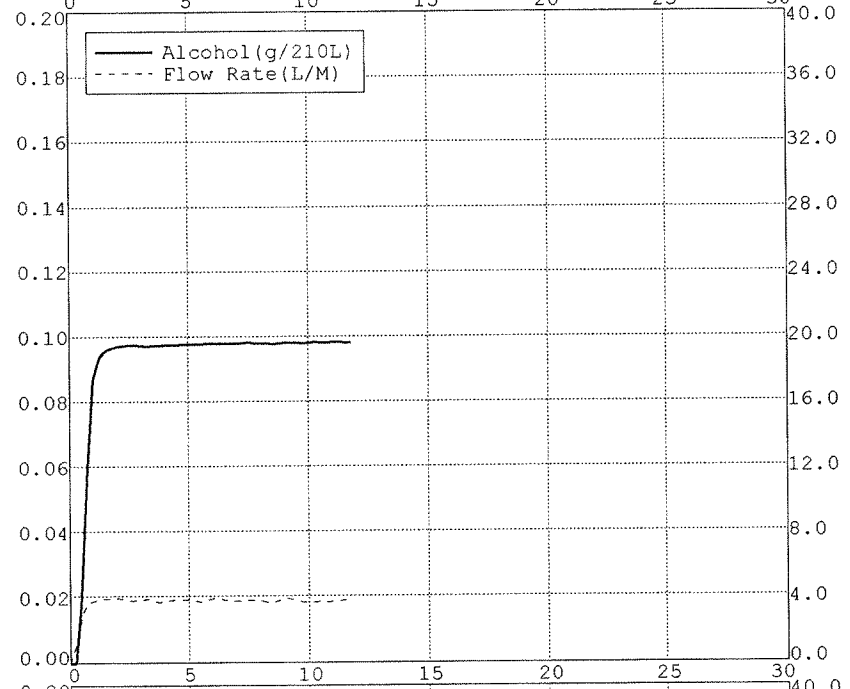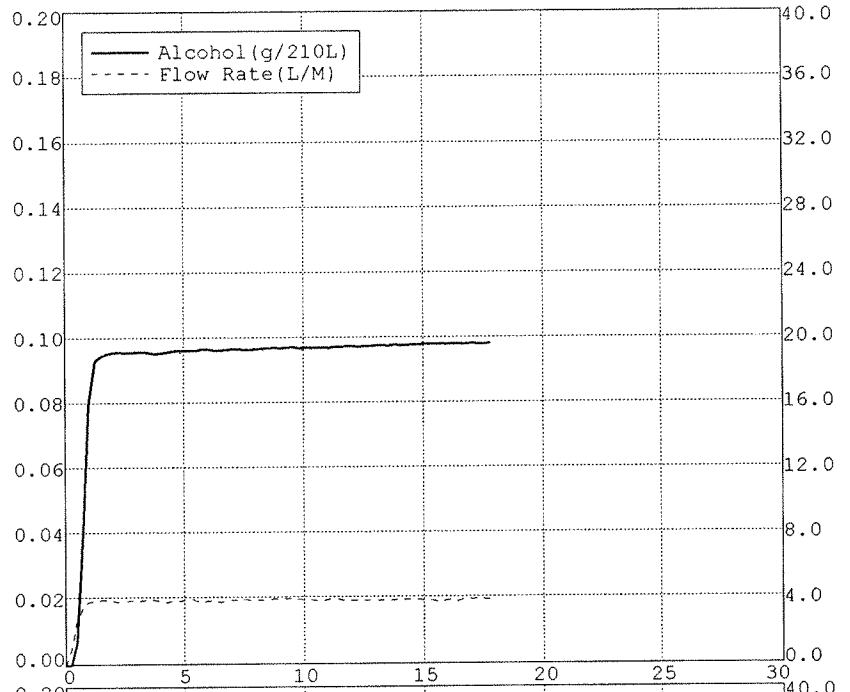

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/25/2024

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24190

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 16:03 |
| INTERNAL STANDARD | VERIFIED | 16:03 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 16:03 |
| BLANK TEST | 0.00 | 16:04 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 16:04 |
| BLANK TEST | 0.00 | 16:05 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 16:05 |
| BLANK TEST | 0.00 | 16:06 |

