

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 07/02/2023

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:18
INTERNAL STANDARD	VERIFIED	05:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:19
BLANK TEST	0.00	05:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:20
BLANK TEST	0.00	05:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:21
BLANK TEST	0.00	05:22

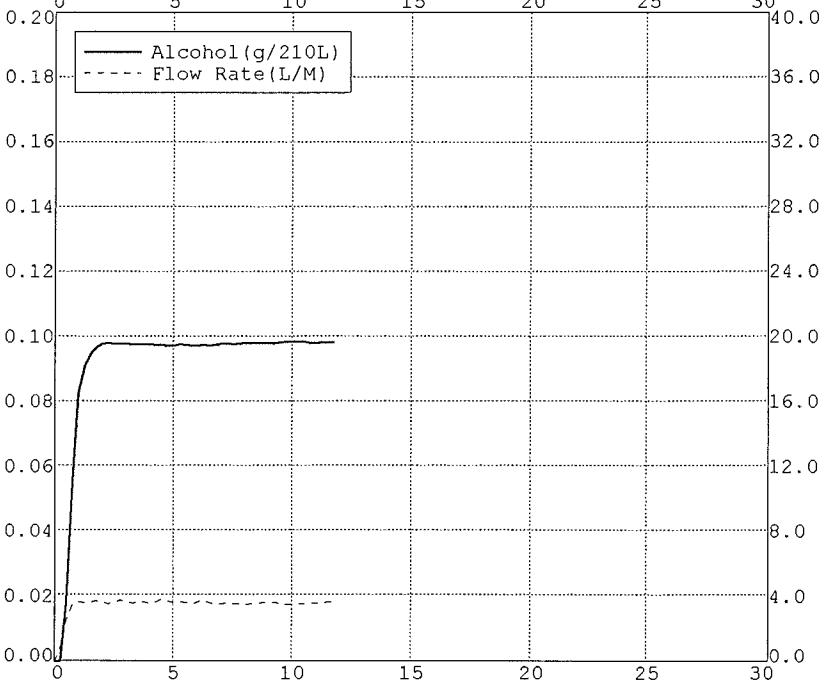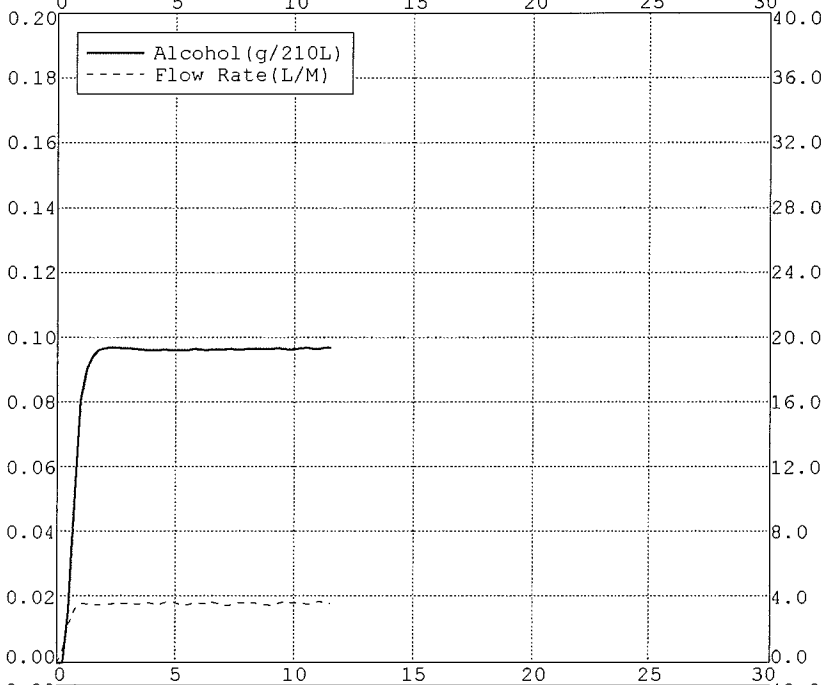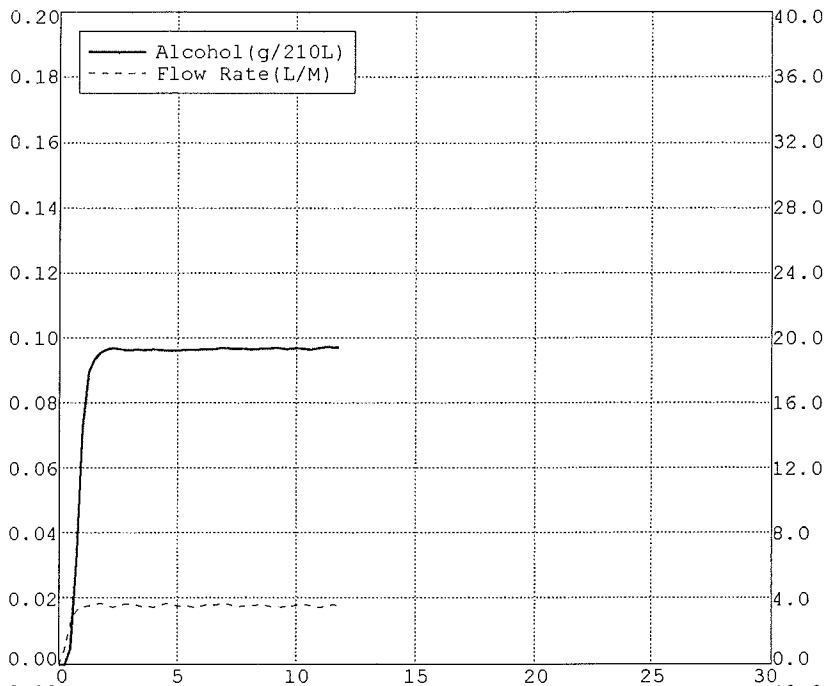

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 07/10/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:34
INTERNAL STANDARD	VERIFIED	21:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:34
BLANK TEST	0.00	21:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:35
BLANK TEST	0.00	21:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:36
BLANK TEST	0.00	21:37

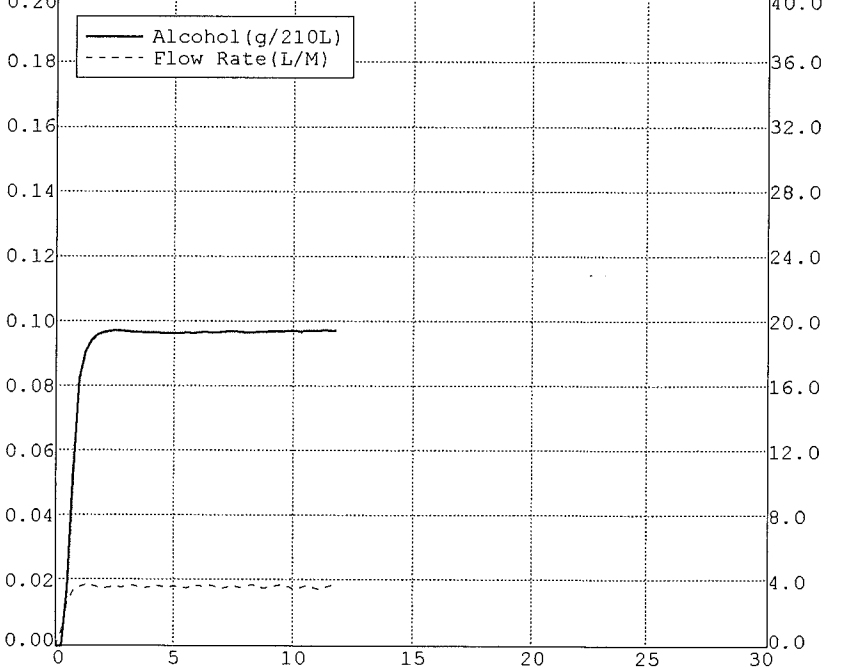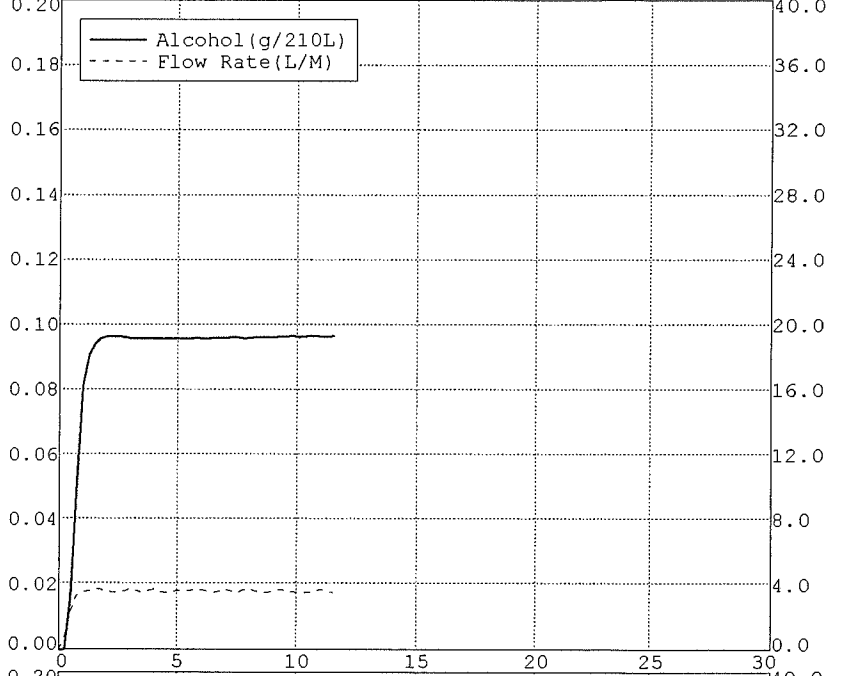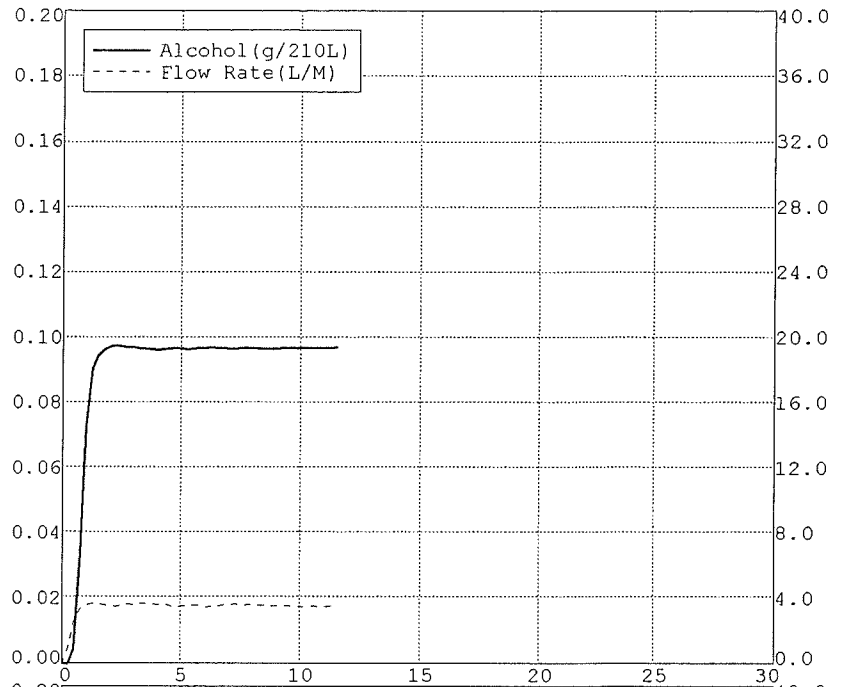

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 07/16/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:17
INTERNAL STANDARD	VERIFIED	02:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:18
BLANK TEST	0.00	02:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:19
BLANK TEST	0.00	02:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:20
BLANK TEST	0.00	02:21

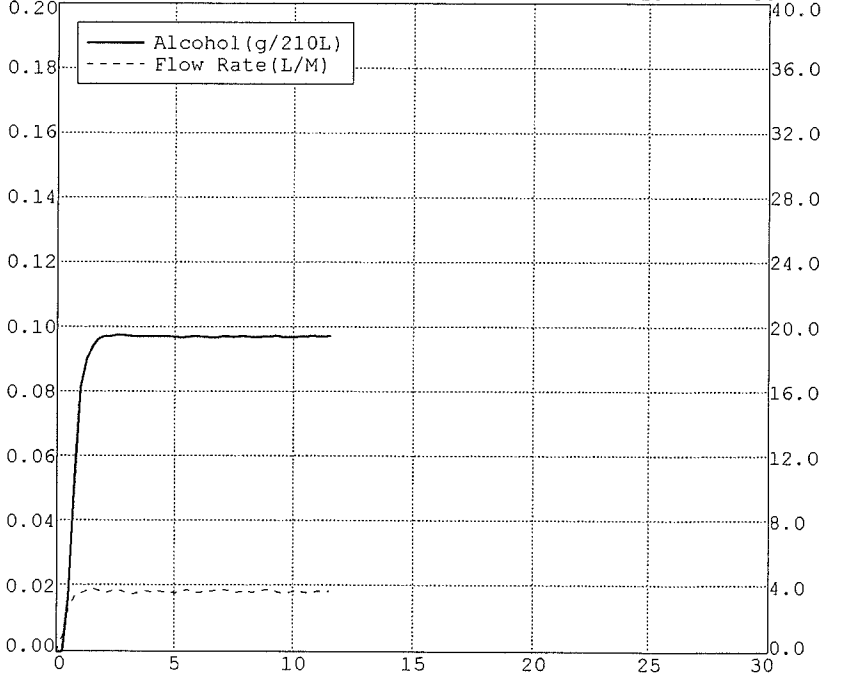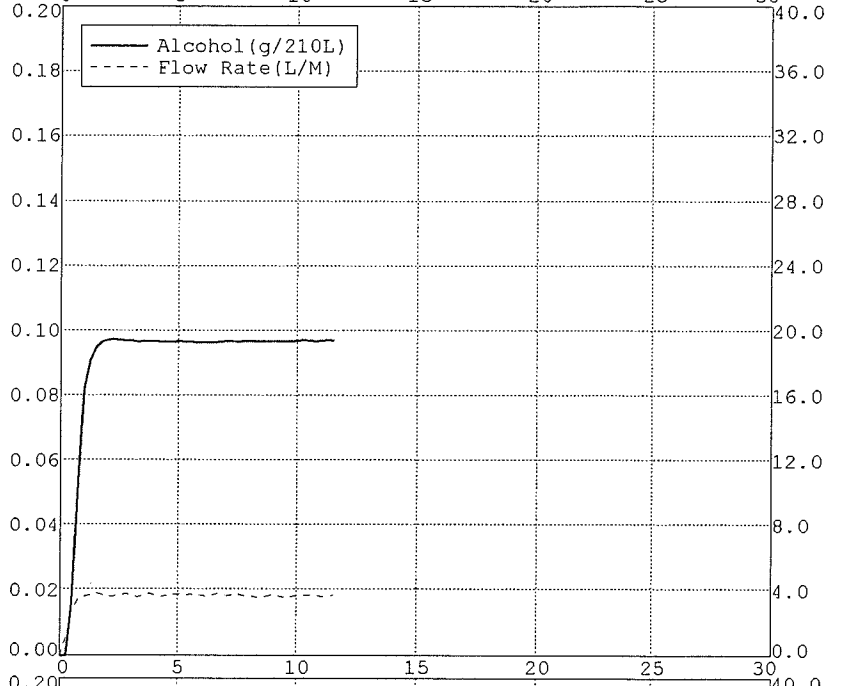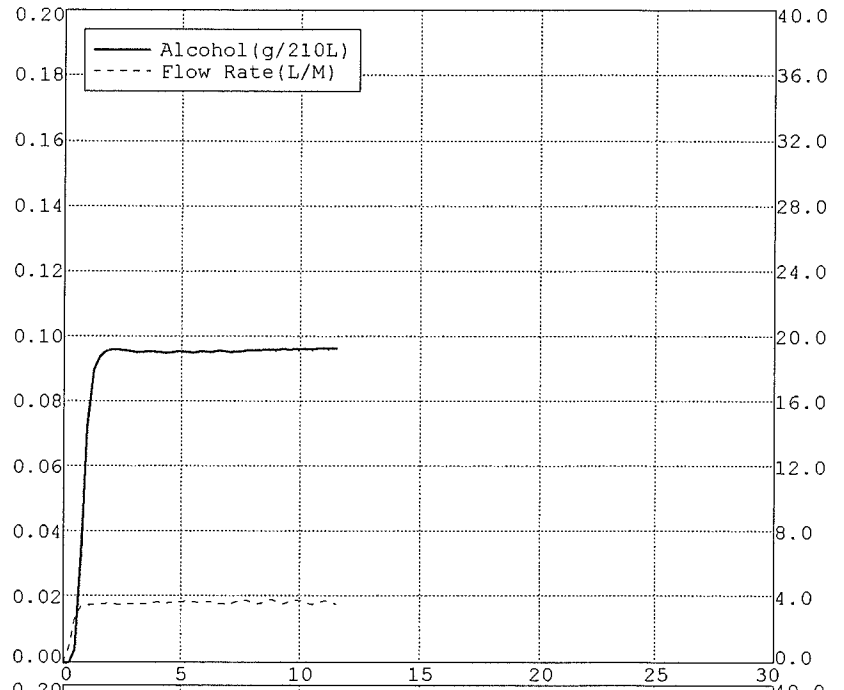

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 07/24/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:19
INTERNAL STANDARD	VERIFIED	19:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:19
BLANK TEST	0.00	19:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:20
BLANK TEST	0.00	19:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:21
BLANK TEST	0.00	19:22

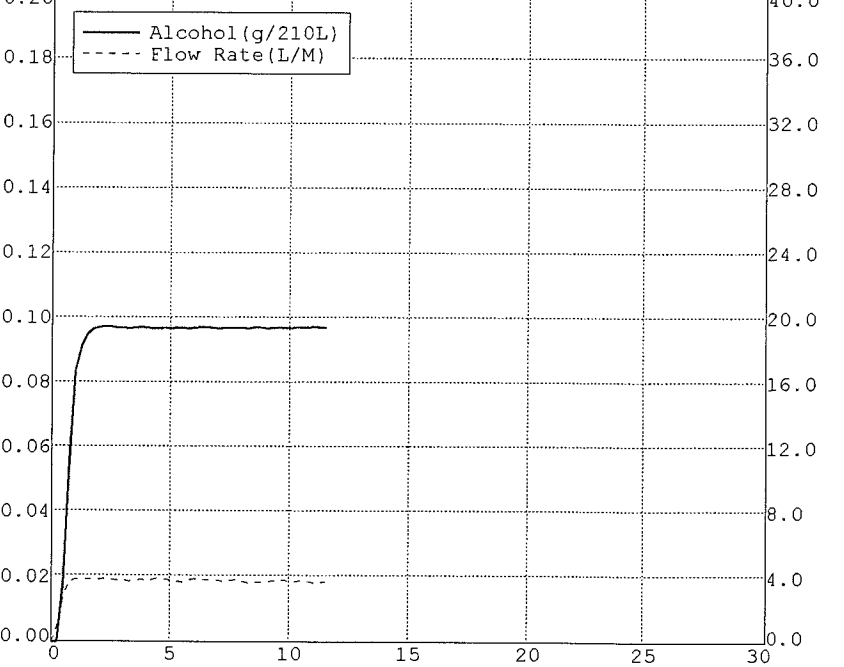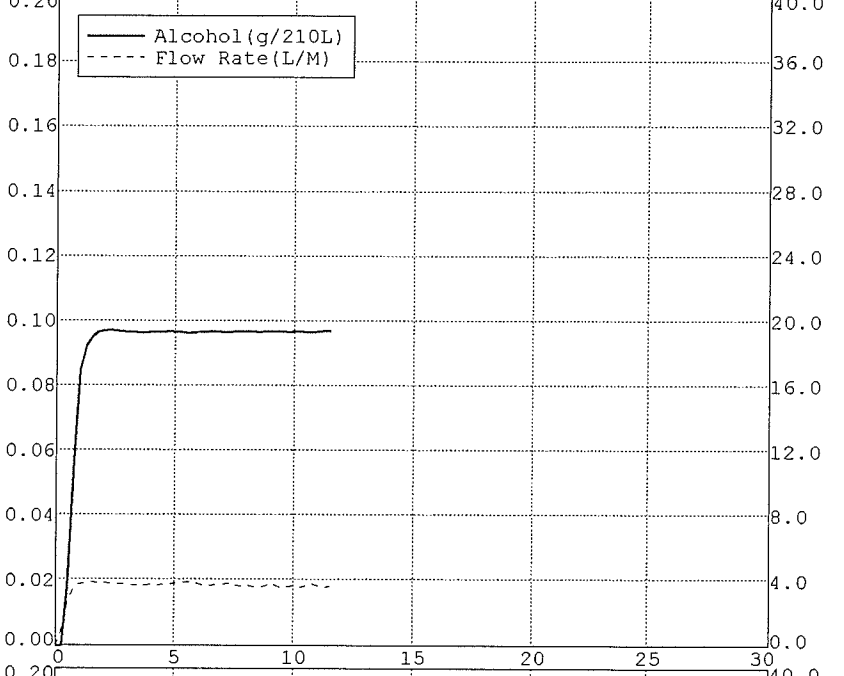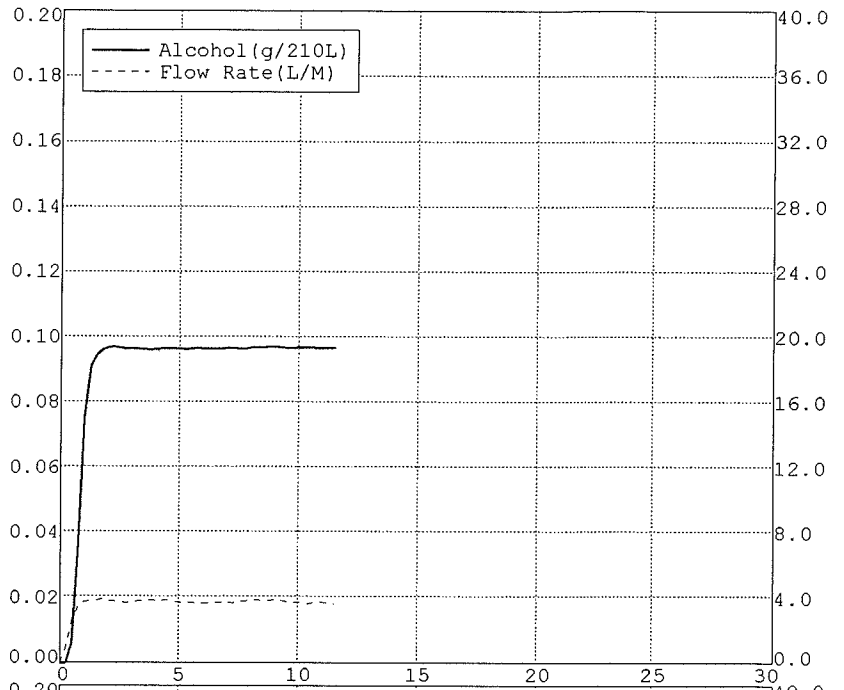

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 07/31/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:53
INTERNAL STANDARD	VERIFIED	04:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:53
BLANK TEST	0.00	04:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:54
BLANK TEST	0.00	04:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:55
BLANK TEST	0.00	04:56

