



Division of Criminal Justice Services

CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 100290, performed on February 19, 2021 by Office of Public Safety employee Jonathan Mascolo, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Joshua Vinehout".

Digitally signed under
ESRA by Joshua Vinehout
on 3/1/2021 9:11 AM

Joshua Vinehout
Supervisor of Public Safety Programs
Office of Public Safety

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Lake Placid Village Police Department
 Manufacturer: NAT'L PATENT ANALYTICAL SYS Model: DATAMASTER DMT
 Date: February 19, 2021 Serial Number: 100290

Reference Solution Lot Number: 20361
 Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.097 %	34.00 degrees centigrade
2	0.098 %	34.00 degrees centigrade
3	0.098 %	34.00 degrees centigrade
4	0.097 %	34.00 degrees centigrade

Reference Solution Lot Number: 20470
 Reference Solution Standard: 0.08 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.079 %	34.00 degrees centigrade
2	0.080 %	34.00 degrees centigrade
3	0.080 %	34.00 degrees centigrade
4	0.080 %	34.00 degrees centigrade


Reference Solution Lot Number: 20290
 Reference Solution Standard: 0.180 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.178 %	34.00 degrees centigrade
2	0.177 %	34.00 degrees centigrade
3	0.178 %	34.00 degrees centigrade
4	0.178 %	34.00 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 100290, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.


I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under
 ESRA by Jonathan Mascolo
 on 2/19/2021 1:56 PM

Reviewed by:



Digitally signed under
 ESRA by Frank Sgarlata
 on 2/23/2021 10:33 AM

Jonathan Mascolo
 Highway Safety Equipment Technician
 Breath Analysis Operator Permit # 45339

Frank Sgarlata
 Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Lake Placid Village Police Department
Manufacturer: NAT'L PATENT ANALYTICAL SYS
Model: DATAMASTER DMT
Serial Number: 100290
Date: February 19, 2021

1. General Appearance and condition of this device -----: INTERFERENCE ERROR

2. Check controls and indicators -----: OK


3. Check breath flow system -----: OK

4. Check printer operation -----: OK

5. System cycles through all modes -----: OK

6. Record any repairs made to this instrument and list services provided: INSPECTED INSTRUMENT, CLEANED FILTERS,CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.

Performed by:



Digitally signed under
ESRA by Jonathan Mascolo
on 2/19/2021 1:56 PM

Jonathan Mascolo
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 45339

Reviewed by:



Digitally signed under
ESRA by Frank Sgarlata
on 2/23/2021 10:33 AM

Frank Sgarlata
Breath Analysis Technical Supervisor

TECHNICIAN TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290


Date: 02/19/2021

OPERATOR NAME:
JONATHAN M MASCOLO
Permit #: 45339
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20361

Nominal = 0.100 g/210L

BLANK TEST	0.000	08:40
INTERNAL STANDARD	VERIFIED	08:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.097	08:41
BLANK TEST	0.000	08:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.098	08:42
BLANK TEST	0.000	08:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.098	08:43
BLANK TEST	0.000	08:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.097	08:44
BLANK TEST	0.000	08:45

Average = 0.0975
Std Dev = 0.0006



TECHNICIAN TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290





Date: 02/19/2021

OPERATOR NAME:
JONATHAN M MASCOLO
Permit #: 45339
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20470

Nominal = 0.080 g/210L

BLANK TEST	0.000	12:15
INTERNAL STANDARD	VERIFIED	12:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.079	12:15
BLANK TEST	0.000	12:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.080	12:16
BLANK TEST	0.000	12:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.080	12:18
BLANK TEST	0.000	12:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.080	12:19
BLANK TEST	0.000	12:20

Average = 0.0798
Std Dev = 0.0005

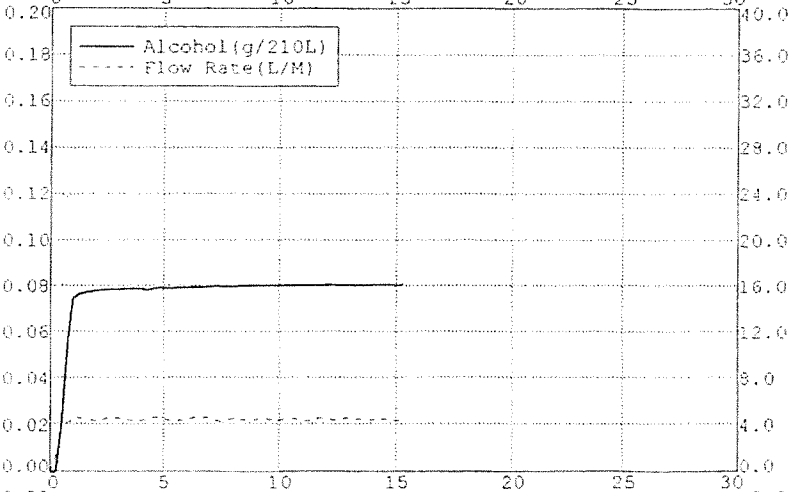

TECHNICIAN TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290





Date: 02/19/2021

OPERATOR NAME:
JONATHAN M MASCOLO
Permit #: 45339
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20290

Nominal = 0.180 g/210L

BLANK TEST	0.000	08:54
INTERNAL STANDARD	VERIFIED	08:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.178	08:55
BLANK TEST	0.000	08:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.177	08:56
BLANK TEST	0.000	08:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.178	08:57
BLANK TEST	0.000	08:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.178	08:58
BLANK TEST	0.000	08:59

Average = 0.1778
Std Dev = 0.0005



SERVICE AUTHORIZATION FORM
Highway Safety Technology Unit
 80 South Swan Street
 Albany, NY 12210
 Ph: 518-485-7636 / 518-402-0689
 Fax: 518-457-6869

2/19/21*

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

SECTION I - AGENCY INFORMATION

Name of Agency LAKE PLACID POLICE DEPARTMENT		Today's Date 2-10-2021
Address 2693 MAIN ST		City, State, ZIP LAKE PLACID, NY 12946
Contact Person CHARLES LANGLOIS DELIVERING-CHAD BLINN @ STATION		Contact Telephone 518-523-3306
Contact Email blinn@lakeplacidpd.com		Best Way to Reach You During Appointment Period 518-523-3306

SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle) NPAS DMT REPCO SIM Applied Concepts(Stalker) Decatur(Genesis) Kustom(Eagle/Falcon) MPH AVS FST Other:		
Model Number DMT*		Instrument Serial Number 100090*
Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 --		Type of maintenance (check appropriate) <input type="checkbox"/> Calibration Check <input type="checkbox"/> Repair
Brief Description of Malfunction Interference error*		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: <input checked="" type="checkbox"/> DMT 100270 <input checked="" type="checkbox"/> SIM M94114 <input checked="" type="checkbox"/> Tubes <input checked="" type="checkbox"/> Keyboard Other: Power CARDS		Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other:
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.		
Signature Pd Chad P R		Date 2-10-2021

DCJS USE ONLY

<p>Inspected instrument, cleaned filters, checked setup voltages Print and Remote operation. Performed Calibration/Adjustment Procedure, Ran subject, technician & Diagnostic tests, Verified Calibration * @ 2/19/21</p>



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 100290, performed on August 02, 2021 by Office of Public Safety employee Joseph Iavarone, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance/calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Joshua Vinehout".

Digitally signed under ESRA
by Joshua Vinehout
on 8/20/2021 9:17 AM

Joshua Vinehout
Supervisor of Public Safety Programs
Office of Public Safety

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Lake Placid Village Police Department
Manufacturer: NAT'L PATENT ANALYTICAL SYS Model: DATAMASTER DMT
Serial Number: 100290
Date: August 02, 2021

Reference Solution Lot Number: 21170
Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.096 %	34.01 degrees centigrade
2	0.096 %	34.01 degrees centigrade
3	0.098 %	34.01 degrees centigrade
4	0.098 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 100290, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.


Performed by:



Digitally signed under
ESRA by Joseph Iavarone
on 8/2/2021 9:49 AM

Joseph Iavarone
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 44106

Reviewed by:



Digitally signed under
ESRA by Frank Sgarlata
on 8/17/2021 8:44 AM

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Lake Placid Village Police Department
Manufacturer: NAT'L PATENT ANALYTICAL SYS
Model: DATAMASTER DMT
Serial Number: 100290
Date: August 02, 2021

- 1. General Appearance and condition of this device -----: N/A

- 2. Check controls and indicators -----: OK


- 3. Check breath flow system -----: OK

- 4. Check printer operation -----: N/A

- 5. System cycles through all modes -----: OK

- 6. Record any repairs made to this instrument and list services provided: **CHECKED REMOTE OPERATION, RAN DIAGNOSTIC AND TECHNICIAN TESTS, VERIFIED CALIBRATION.**


Performed by:



Digitally signed under
ESRA by Joseph Iavarone
on 8/2/2021 9:49 AM

Joseph Iavarone
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 44106

Reviewed by:



Digitally signed under
ESRA by Frank Sgarlata
on 8/17/2021 8:44 AM

Frank Sgarlata
Breath Analysis Technical Supervisor

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dnt: 100290

Date: 08/02/2021

Nominal = 0.100 g/210L

BLANK TEST	0.000	09:25
INTERNAL STANDARD	VERIFIED	09:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.096	09:26
BLANK TEST	0.000	09:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.096	09:27
BLANK TEST	0.000	09:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.098	09:28
BLANK TEST	0.000	09:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.098	09:29
BLANK TEST	0.000	09:30

Average = 0.0970
Std Dev = 0.0012

Control Test Record

Serial Number: 100290
Test Date: 03-01-2021 16:06:58
Location: 334

LAKE PLACID POLICE DEPT.

Supervisor Information

First Name: Chad P
Last Name: Blinn
Permit: 23024
Agency: LAKE PLACID WILL. PD

Simulator Information


Lot: 21170 Nominal: 0.100

Test Results

Alcohol 1: 0.10 34.01
Alcohol 2: 0.10 34.01
Alcohol 3: 0.10 34.01

Solution Change:

Plot 1 of 3



Status

Status Code:
Date Time:
Message: