

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 10/03/2021

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:09
INTERNAL STANDARD	VERIFIED	08:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:10
BLANK TEST	0.00	08:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:11
BLANK TEST	0.00	08:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:12
BLANK TEST	0.00	08:13

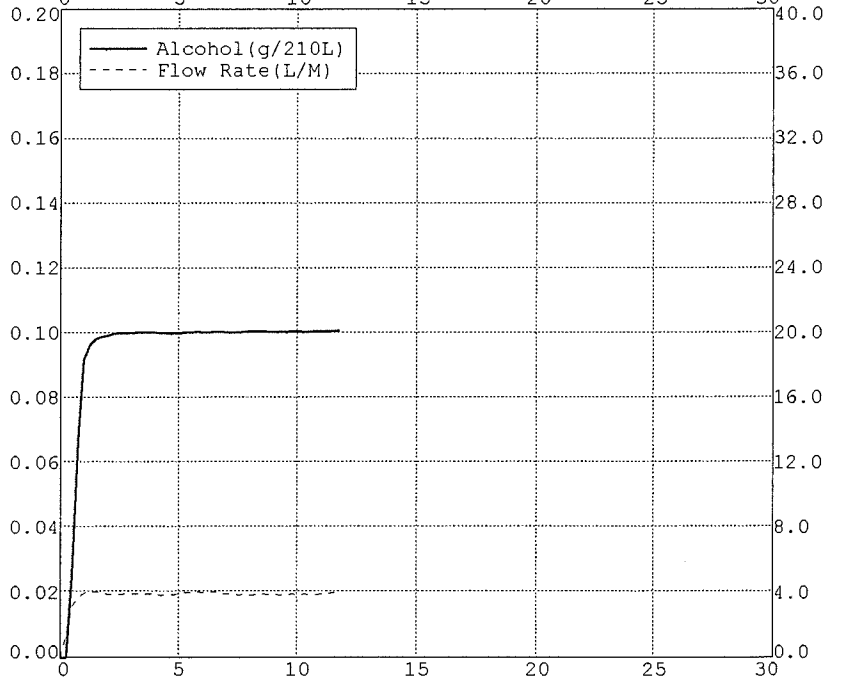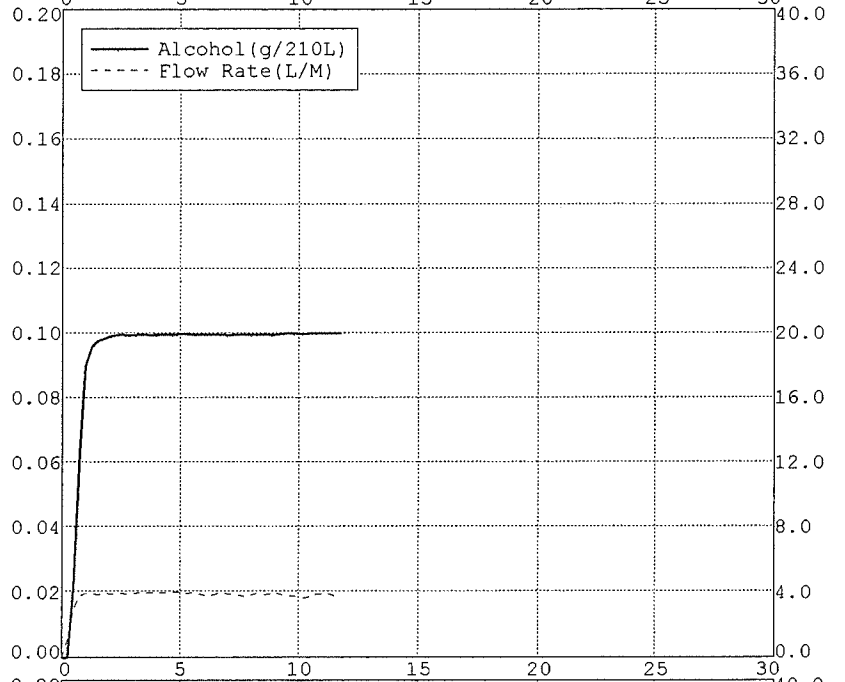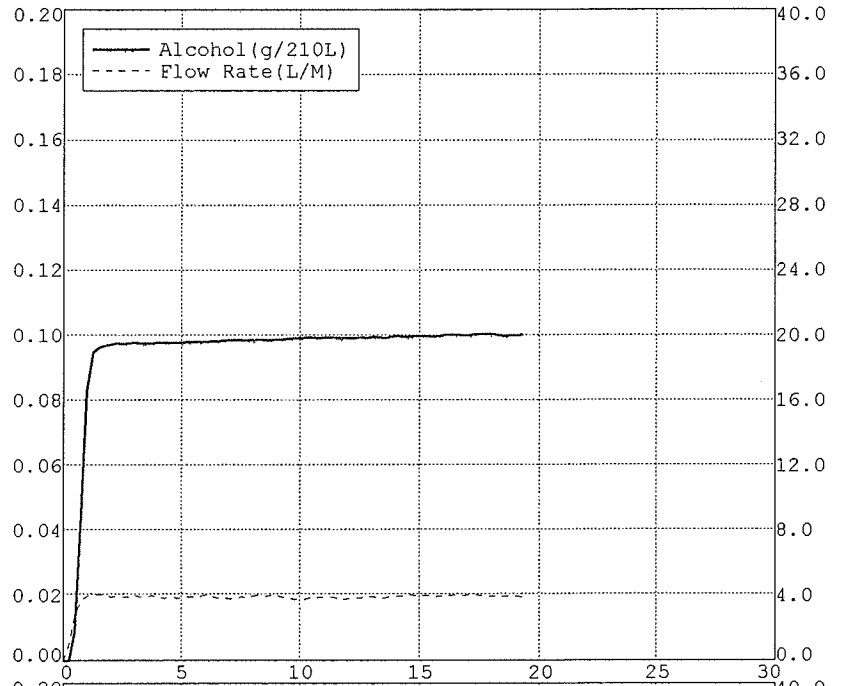

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 10/11/2021

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:23
INTERNAL STANDARD	VERIFIED	11:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:24
BLANK TEST	0.00	11:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:25
BLANK TEST	0.00	11:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:26
BLANK TEST	0.00	11:27

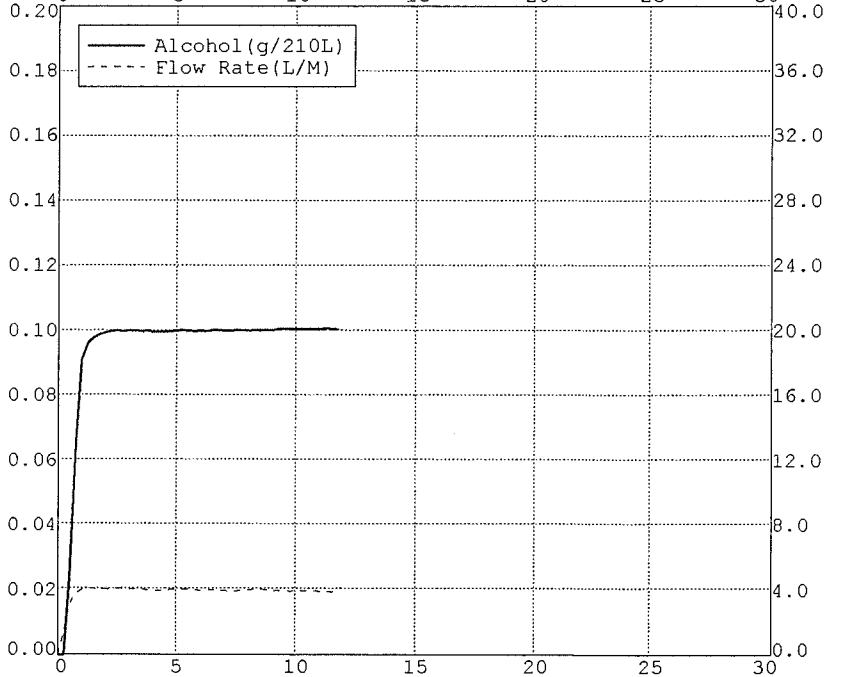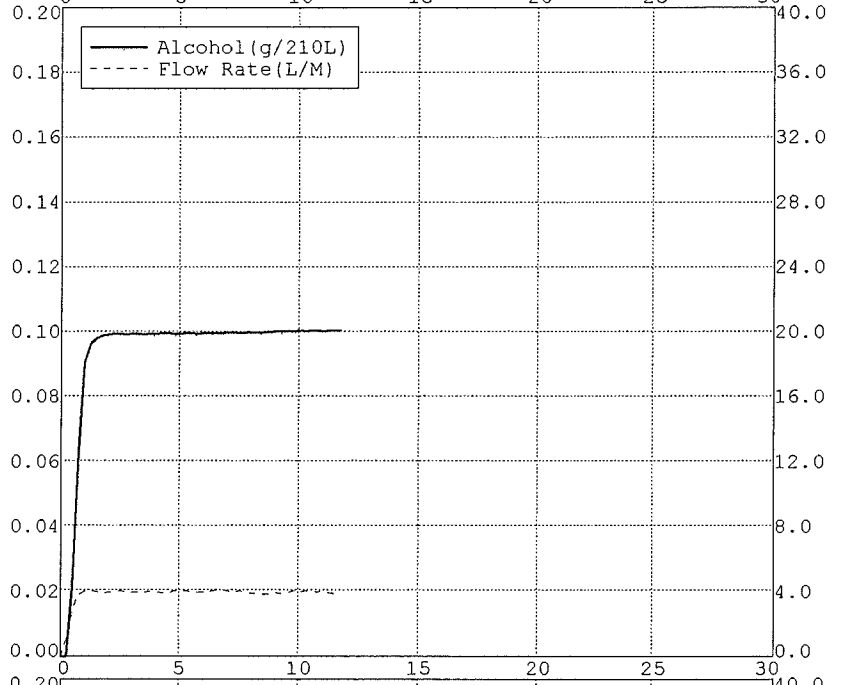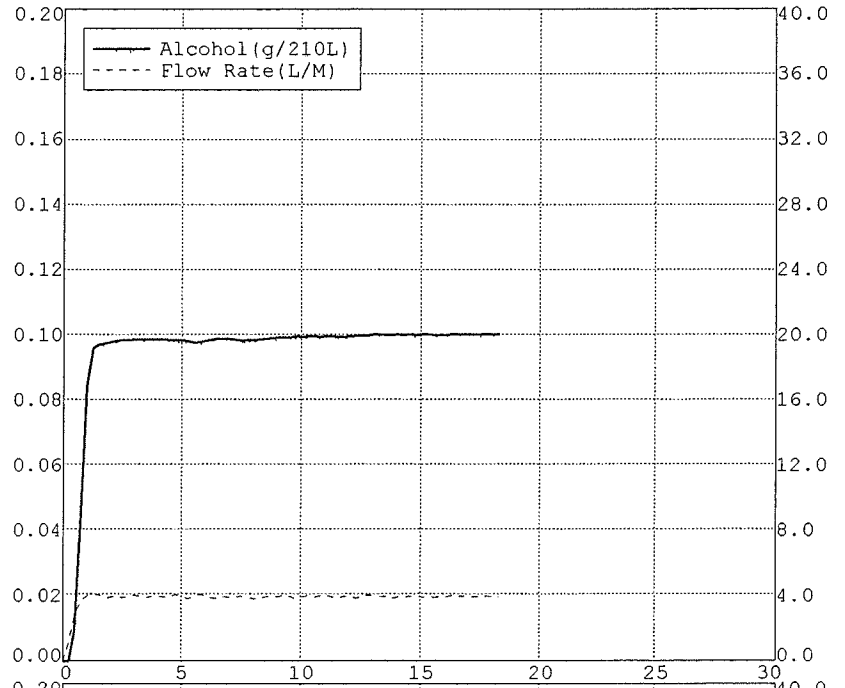

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 10/18/2021

OPERATOR NAME:  
DORAN H SORRELL  
Permit #: 47507  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:45
INTERNAL STANDARD	VERIFIED	03:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:45
BLANK TEST	0.00	03:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:47
BLANK TEST	0.00	03:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:48
BLANK TEST	0.00	03:49

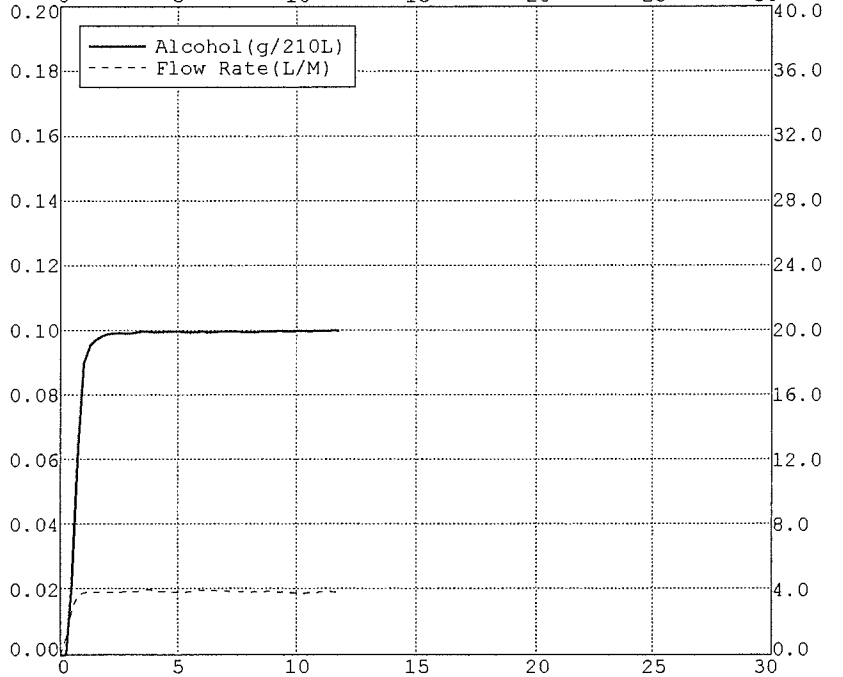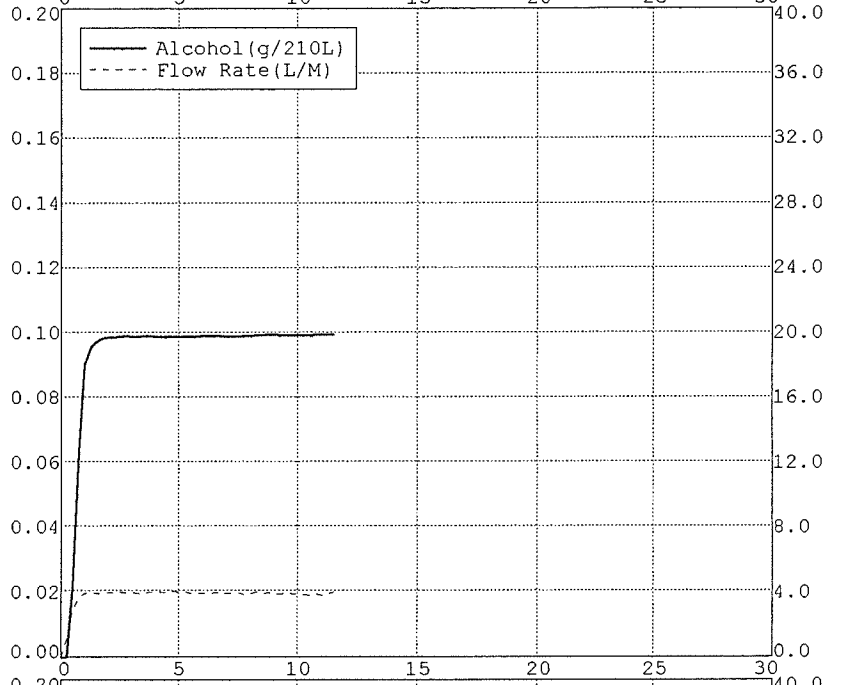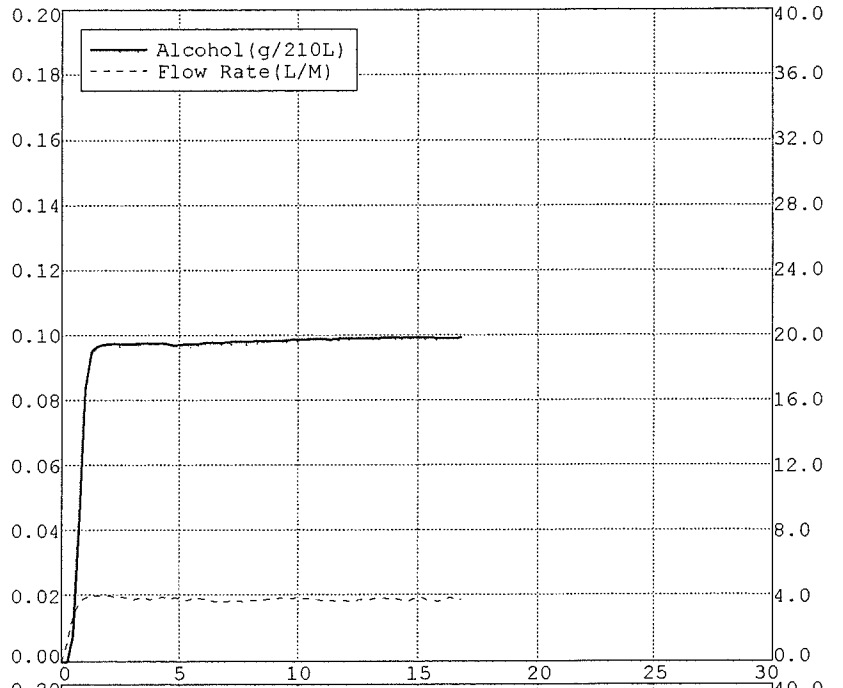

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 10/25/2021

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:04
INTERNAL STANDARD	VERIFIED	08:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:04
BLANK TEST	0.00	08:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:06
BLANK TEST	0.00	08:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:07
BLANK TEST	0.00	08:08

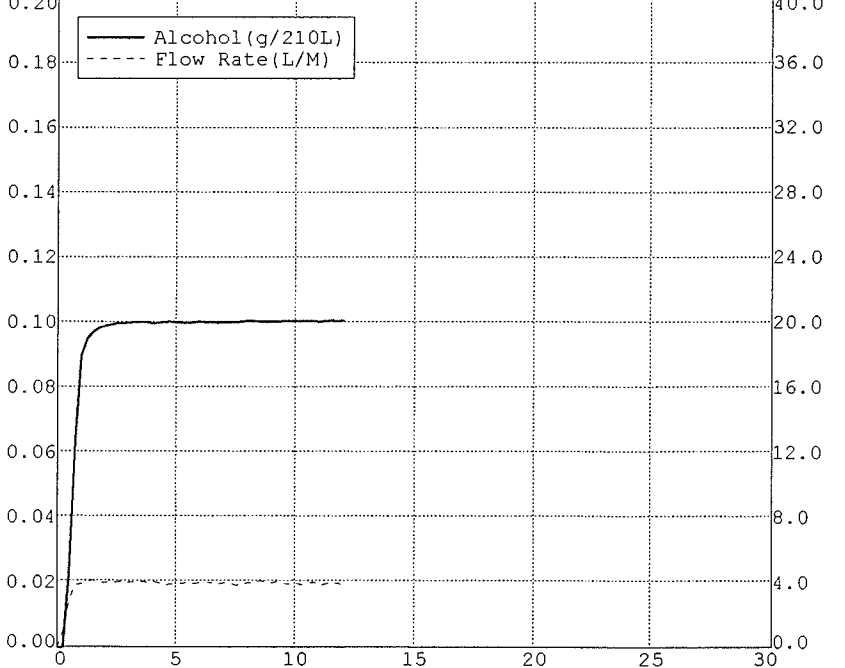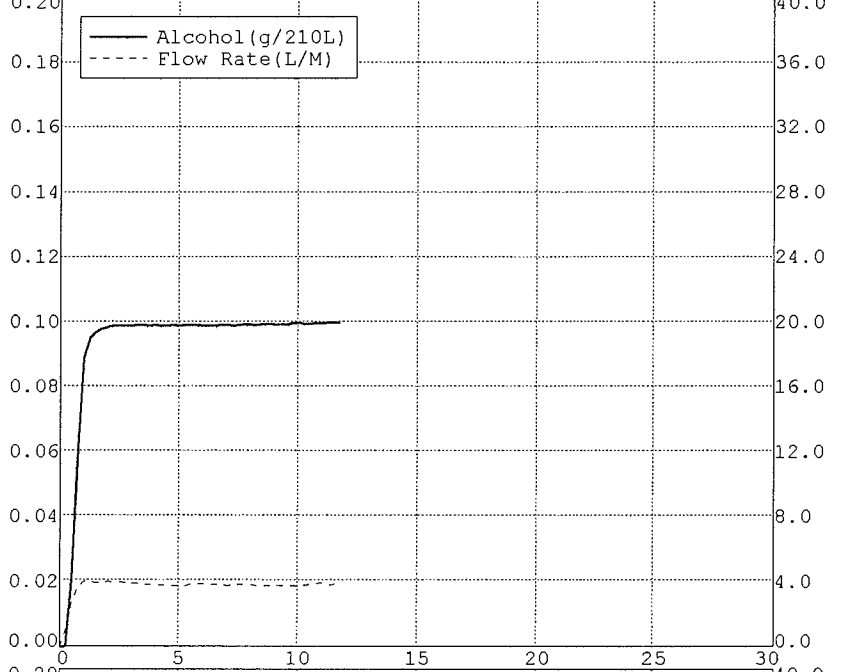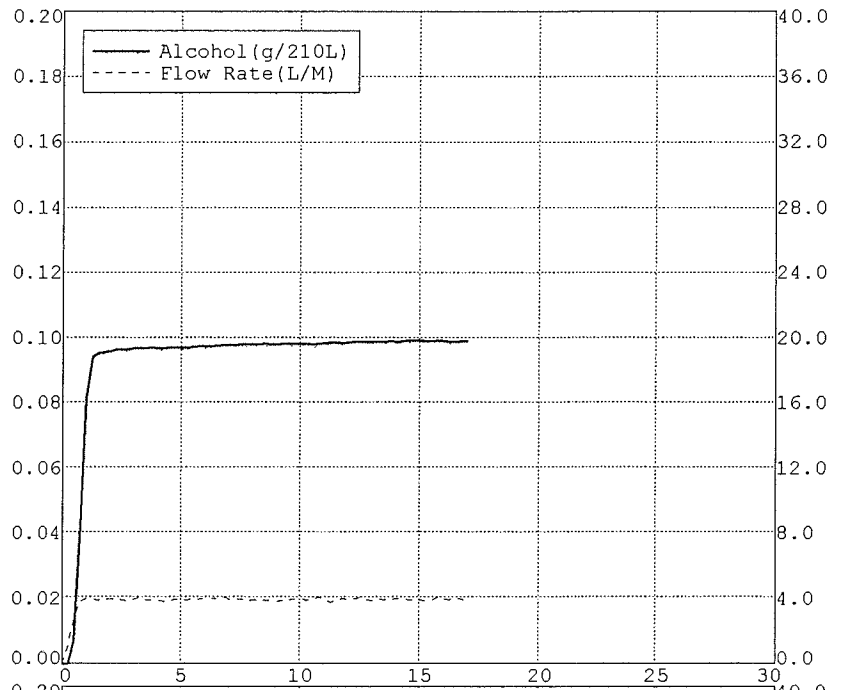

SUPERVISOR TEST

LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 10/31/2021

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:06
INTERNAL STANDARD	VERIFIED	09:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:06
BLANK TEST	0.00	09:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:07
BLANK TEST	0.00	09:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:08
BLANK TEST	0.00	09:09

