

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/01/2019

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:16
INTERNAL STANDARD	VERIFIED	08:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:17
BLANK TEST	0.00	08:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:18
BLANK TEST	0.00	08:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:19
BLANK TEST	0.00	08:20

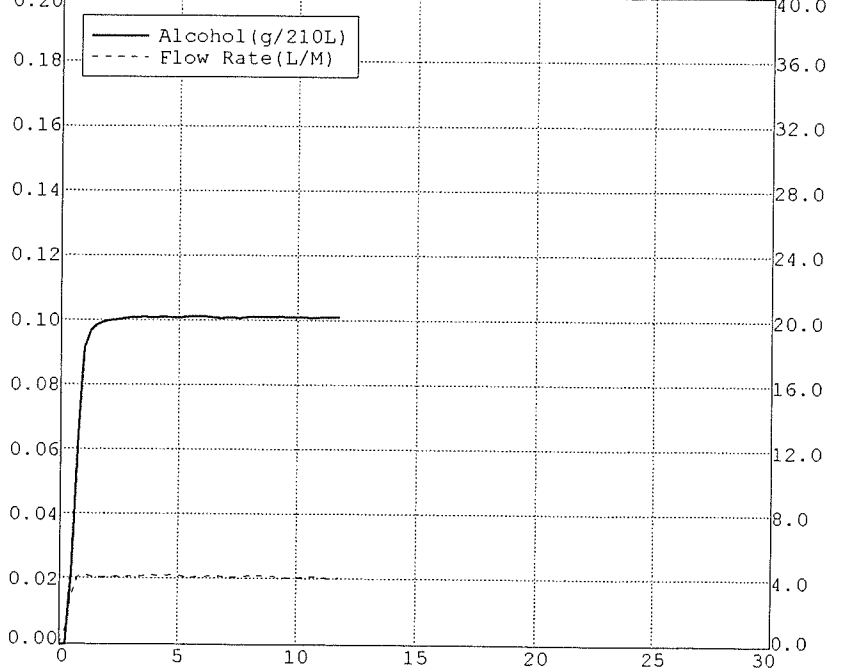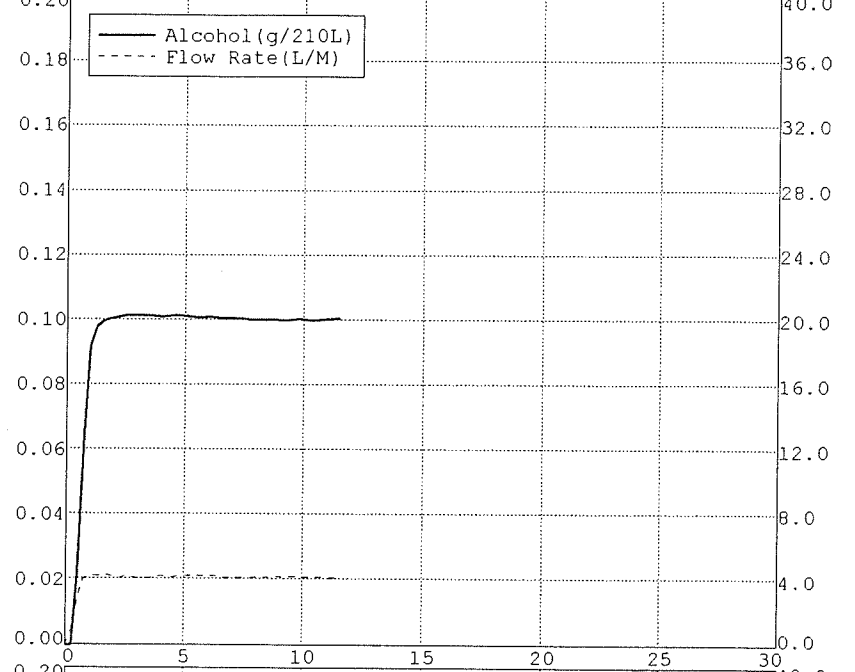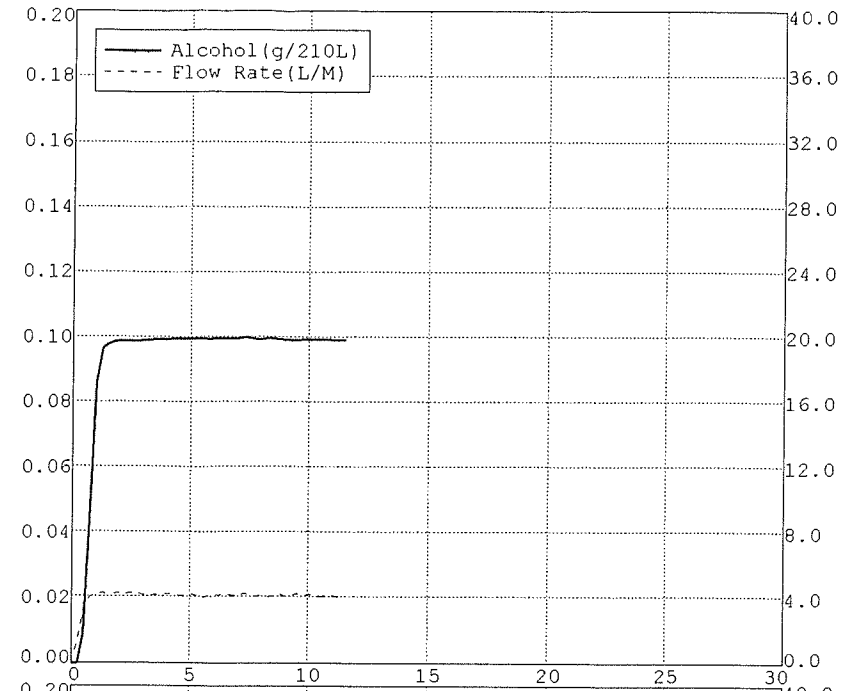

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/09/2019

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:48
INTERNAL STANDARD	VERIFIED	02:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:48
BLANK TEST	0.00	02:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:49
BLANK TEST	0.00	02:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:51
BLANK TEST	0.00	02:51

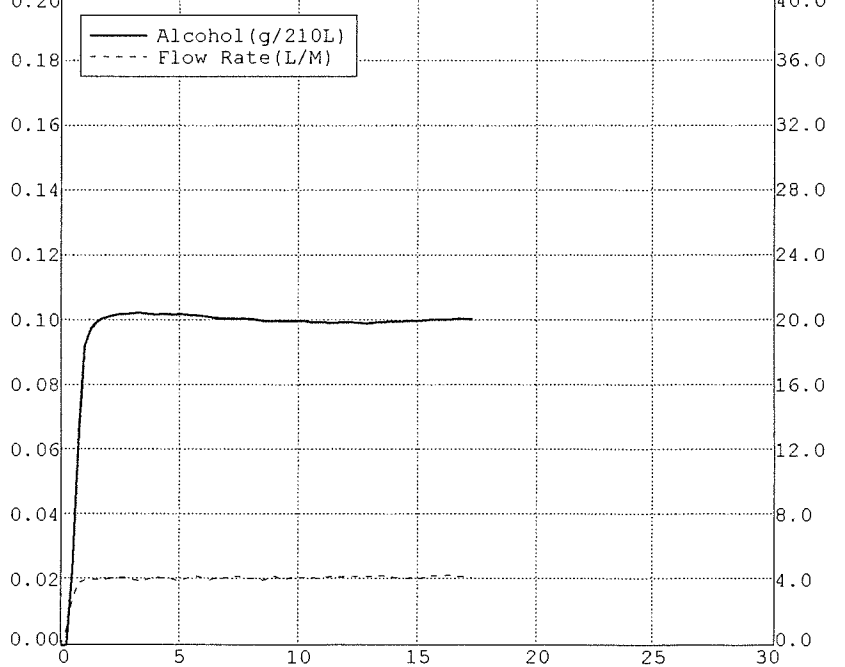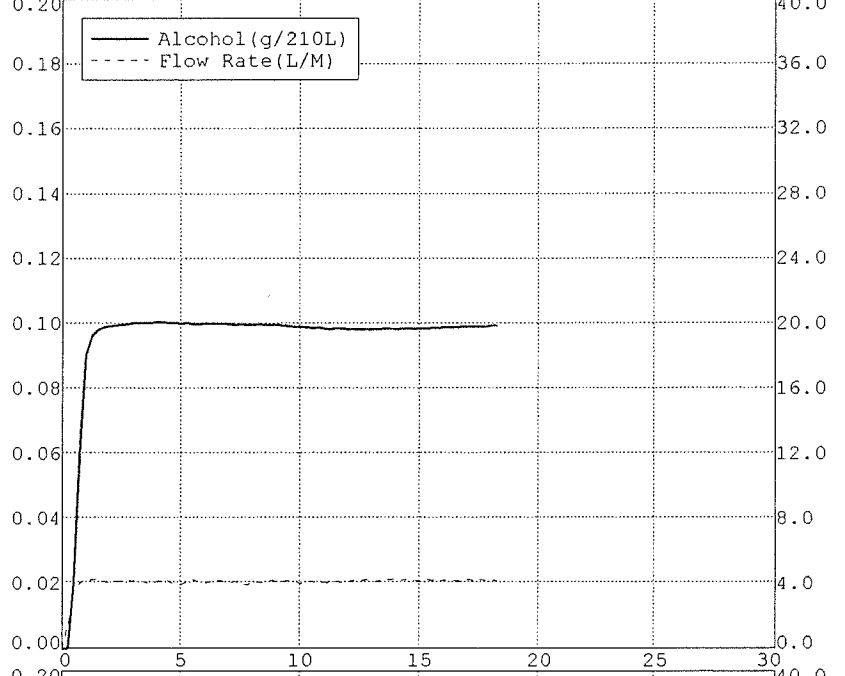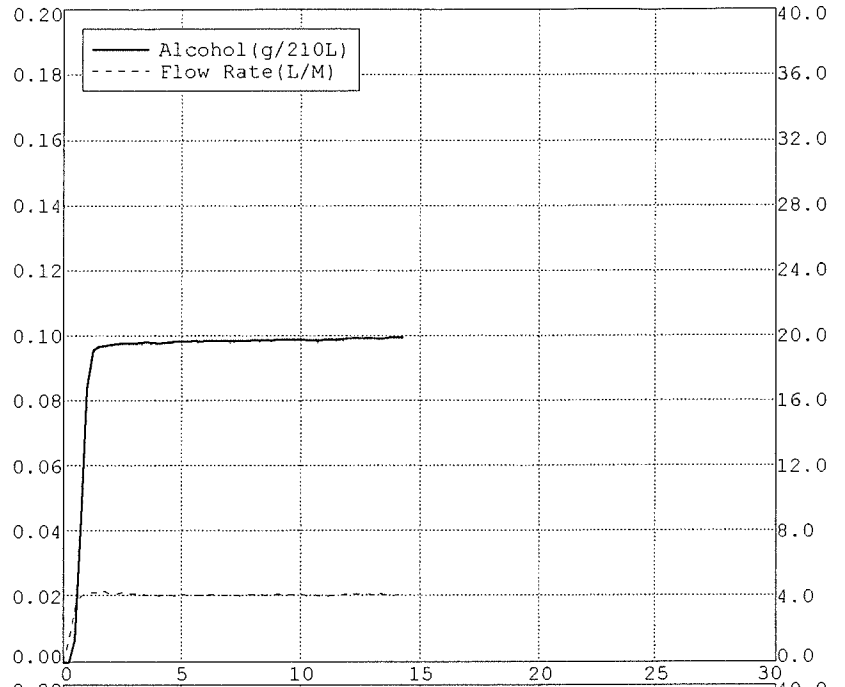

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/16/2019

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:28
INTERNAL STANDARD	VERIFIED	06:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:28
BLANK TEST	0.00	06:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:30
BLANK TEST	0.00	06:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:31
BLANK TEST	0.00	06:32

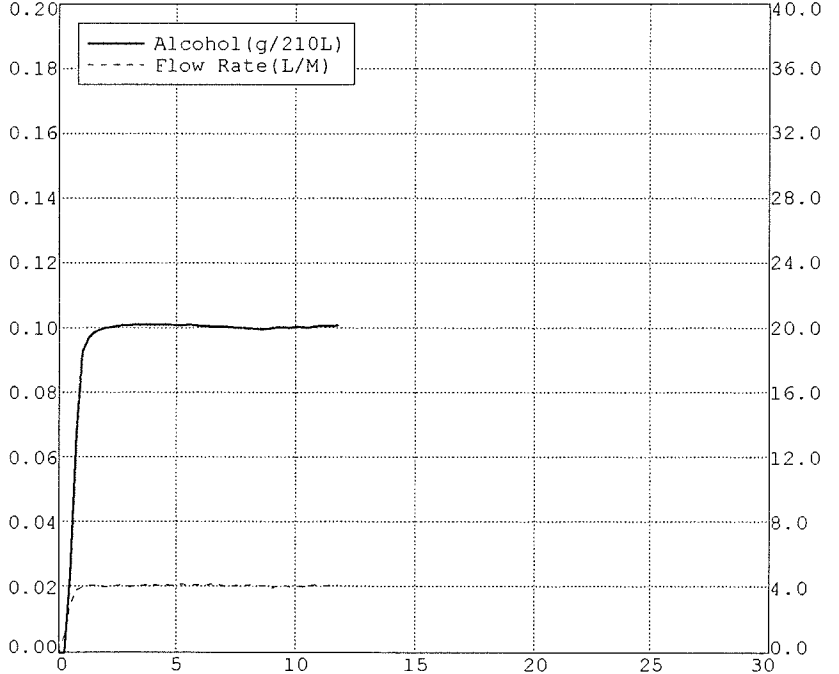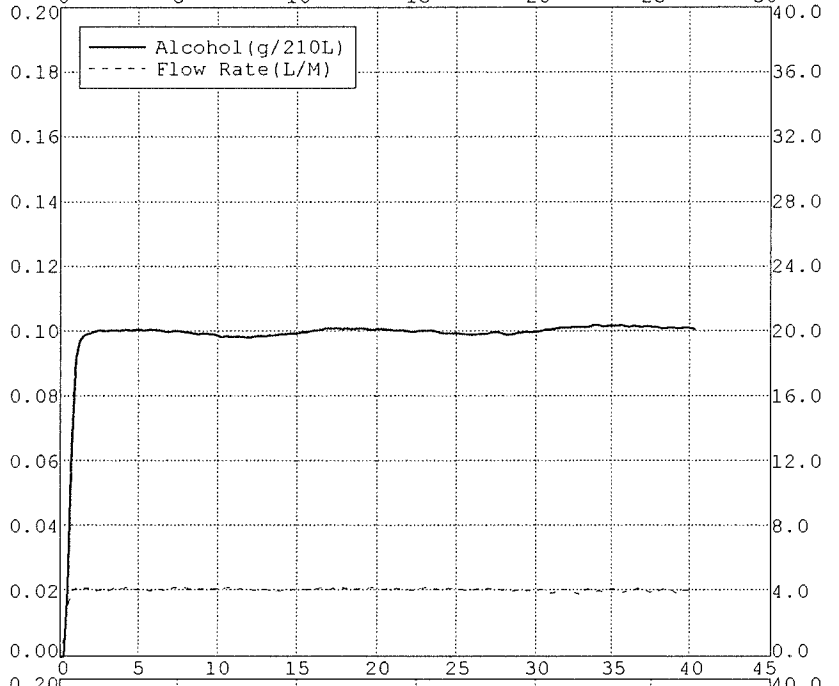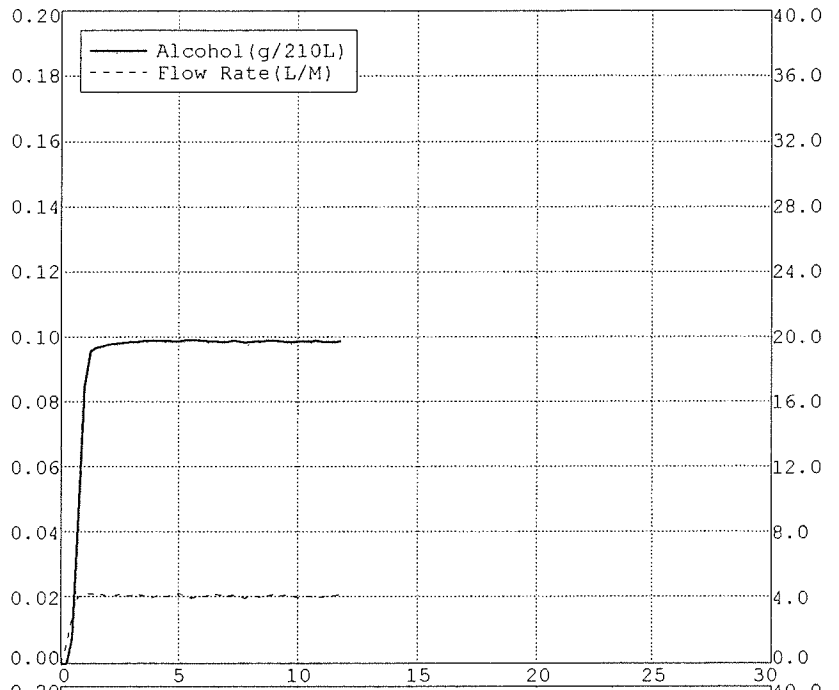

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/22/2019

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:06
INTERNAL STANDARD	VERIFIED	13:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:07
BLANK TEST	0.00	13:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:08
BLANK TEST	0.00	13:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:09
BLANK TEST	0.00	13:10

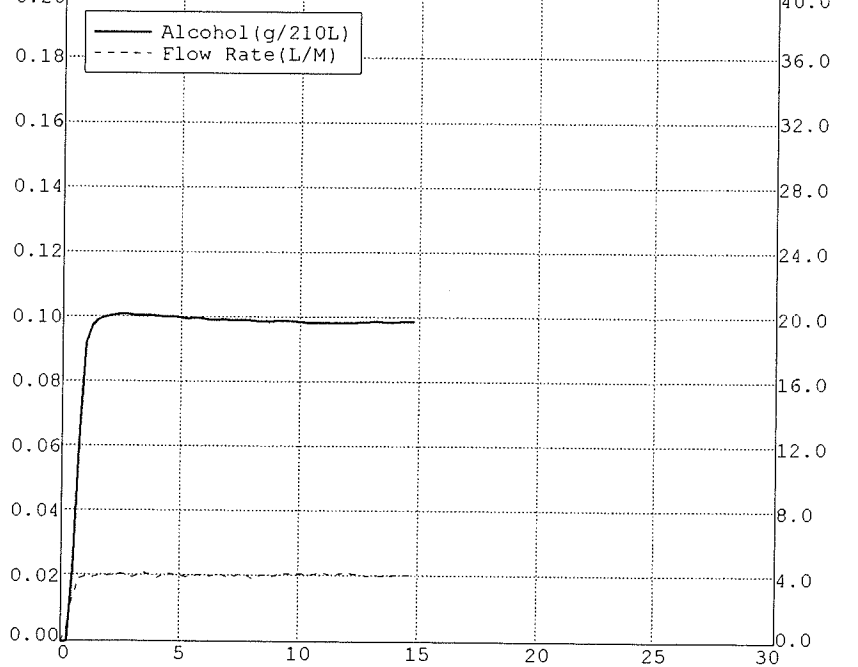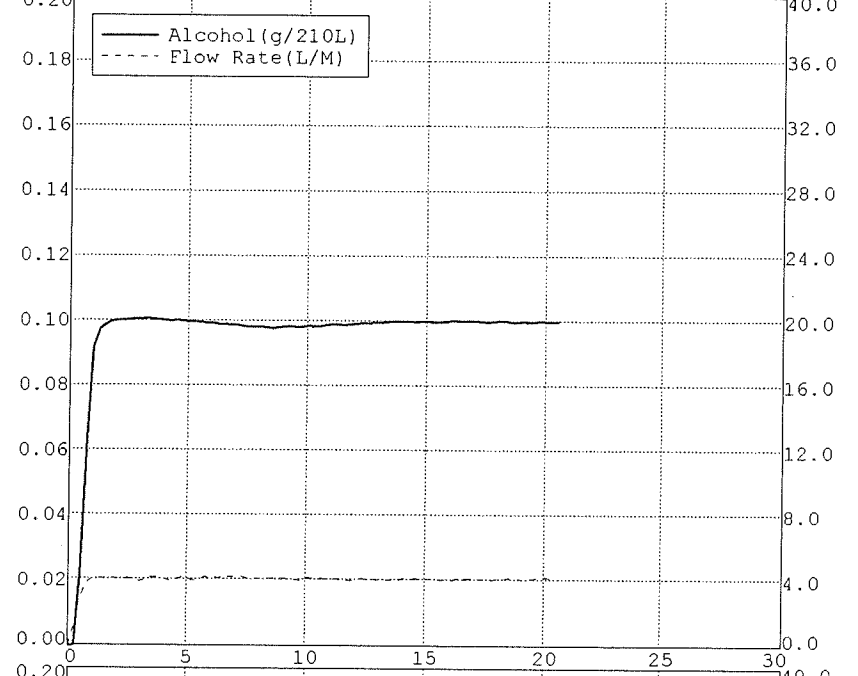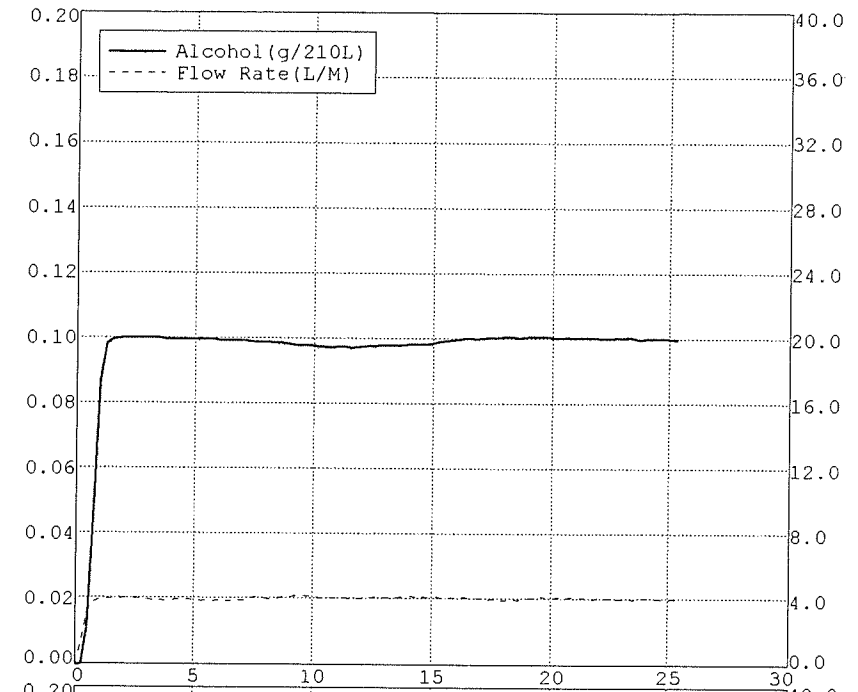

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/30/2019

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:21
INTERNAL STANDARD	VERIFIED	19:21

Simulator Timed Out

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/30/2019

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:28
INTERNAL STANDARD	VERIFIED	19:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:28
BLANK TEST	0.00	19:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:29
BLANK TEST	0.00	19:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:30
BLANK TEST	0.00	19:31

