

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/03/2020

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:17
INTERNAL STANDARD	VERIFIED	09:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:17
BLANK TEST	0.00	09:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:18
BLANK TEST	0.00	09:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:19
BLANK TEST	0.00	09:20

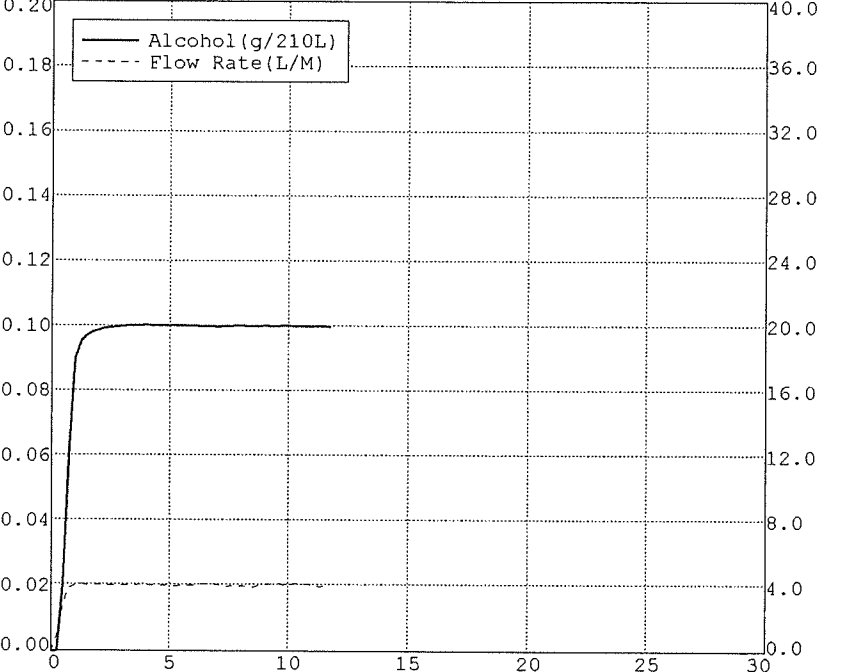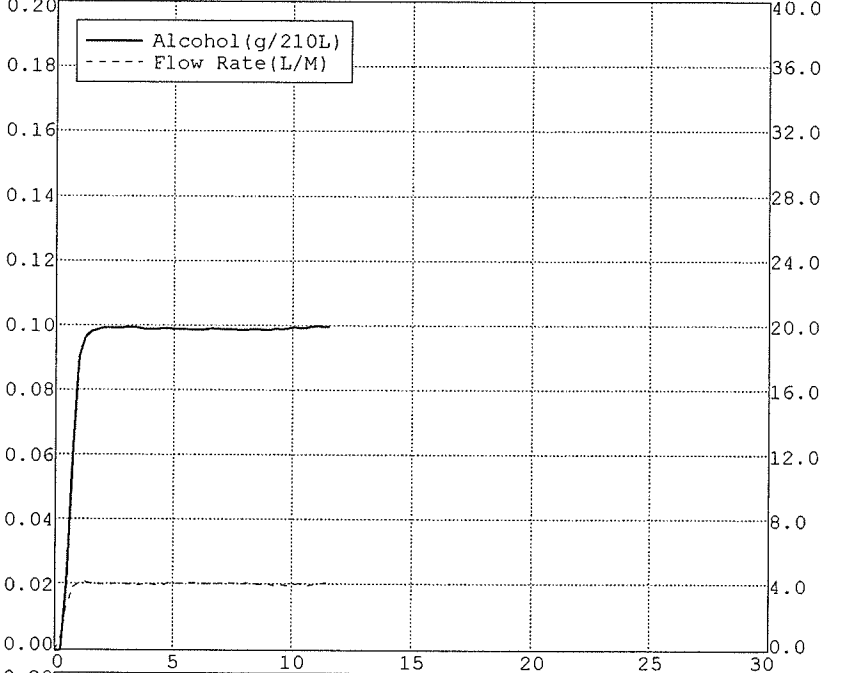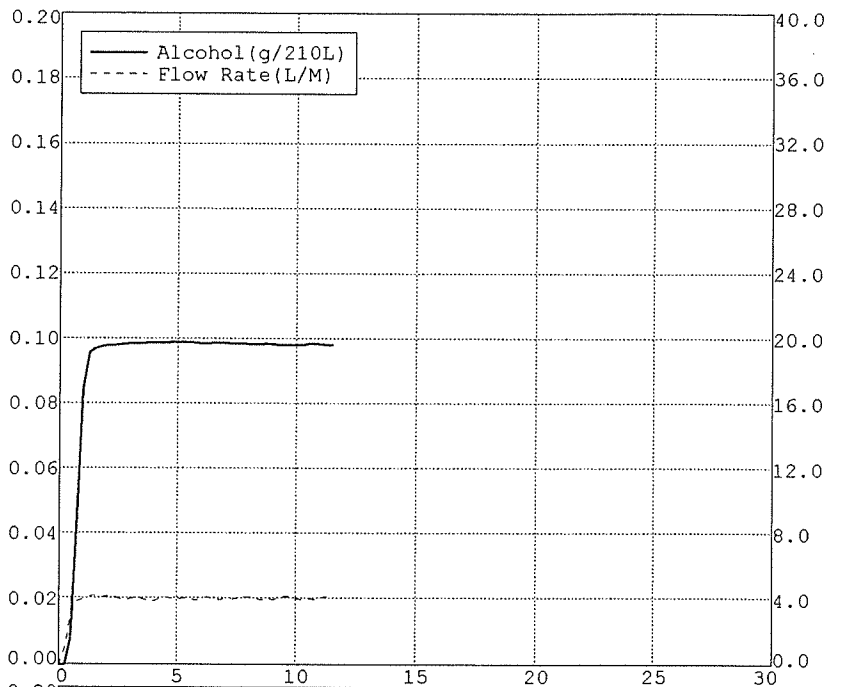

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/11/2020

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:40
INTERNAL STANDARD	VERIFIED	11:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:41
BLANK TEST	0.00	11:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:42
BLANK TEST	0.00	11:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:43
BLANK TEST	0.00	11:44

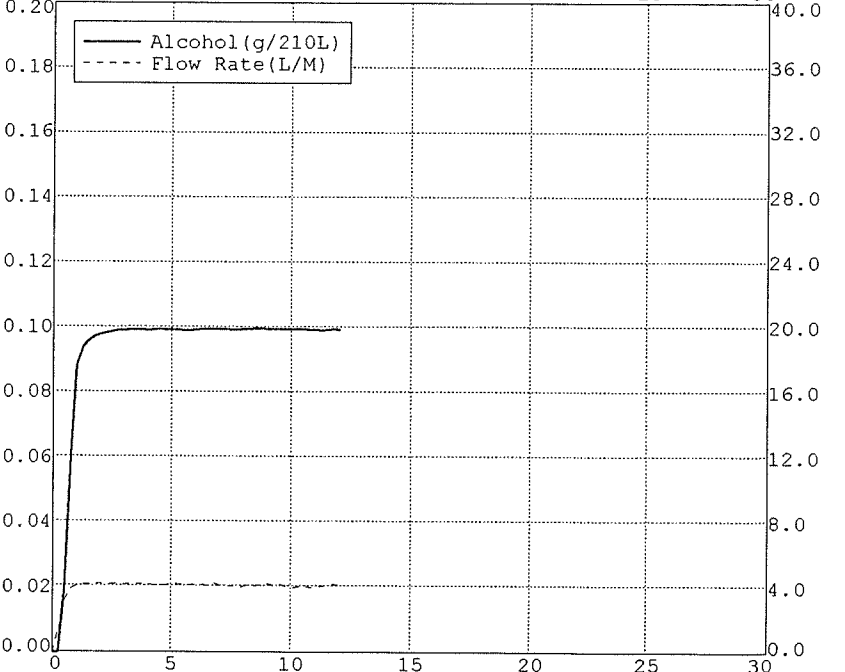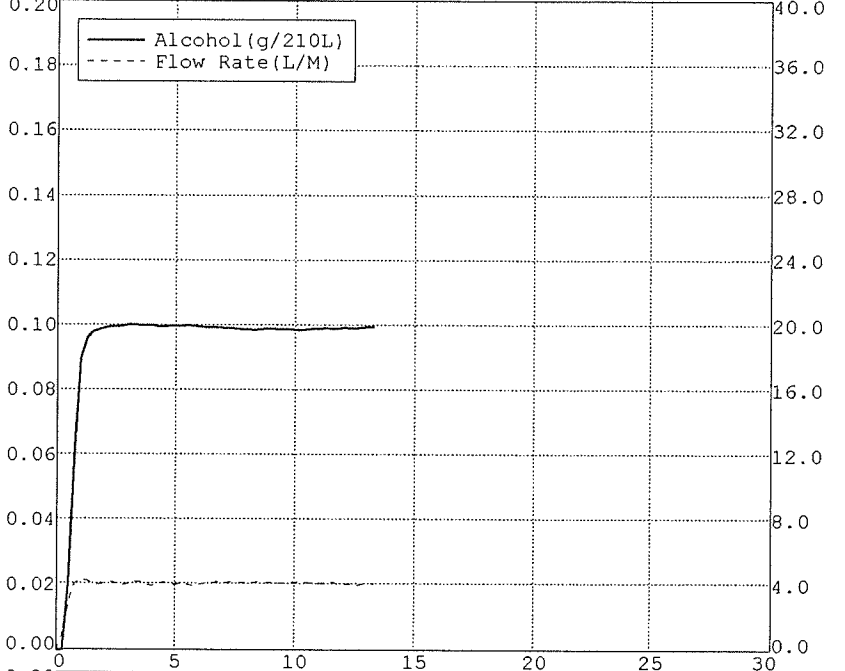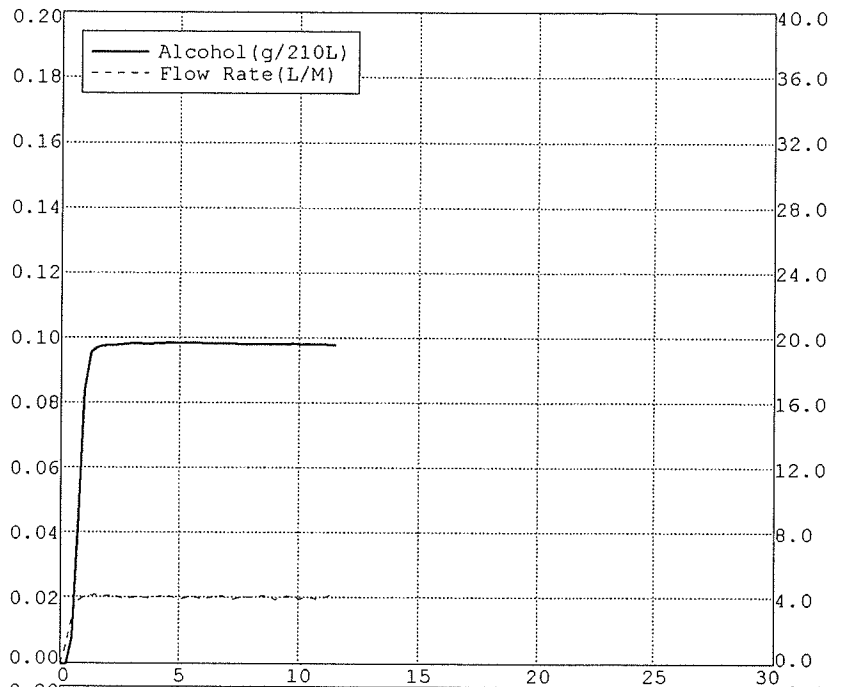

SUPERVISOR TEST




LAKE PLACID VILLAGE
 POLICE DEPT.
 DATAMASTER dmt: 100290

Date: 05/17/2020

OPERATOR NAME:
 CHAD P BLINN
 Permit #: 33034
 Operator Agency/Dept: LAKE PLACID VILL. PD
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:07
INTERNAL STANDARD	VERIFIED	08:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:08
BLANK TEST	0.00	08:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:09
BLANK TEST	0.00	08:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:10
BLANK TEST	0.00	08:11

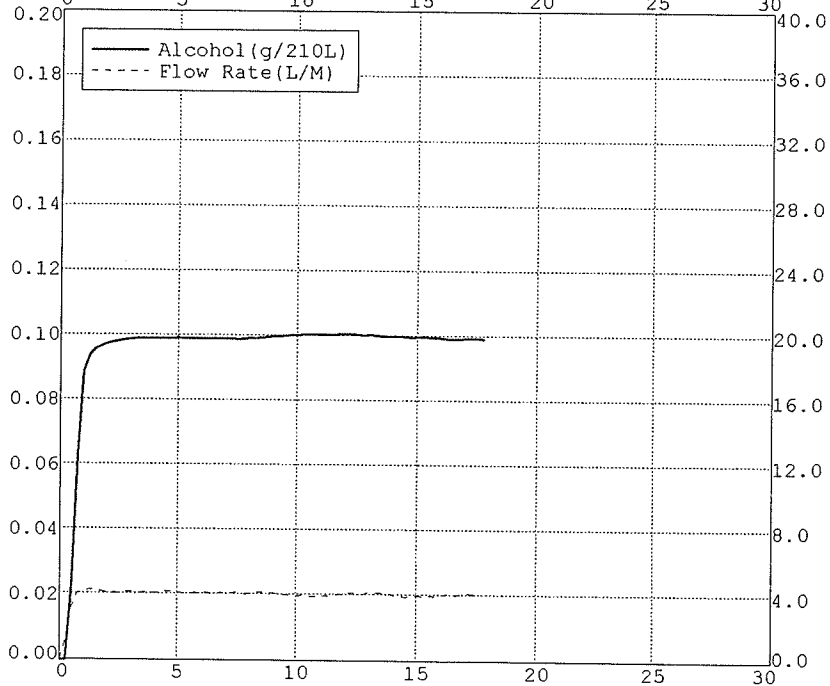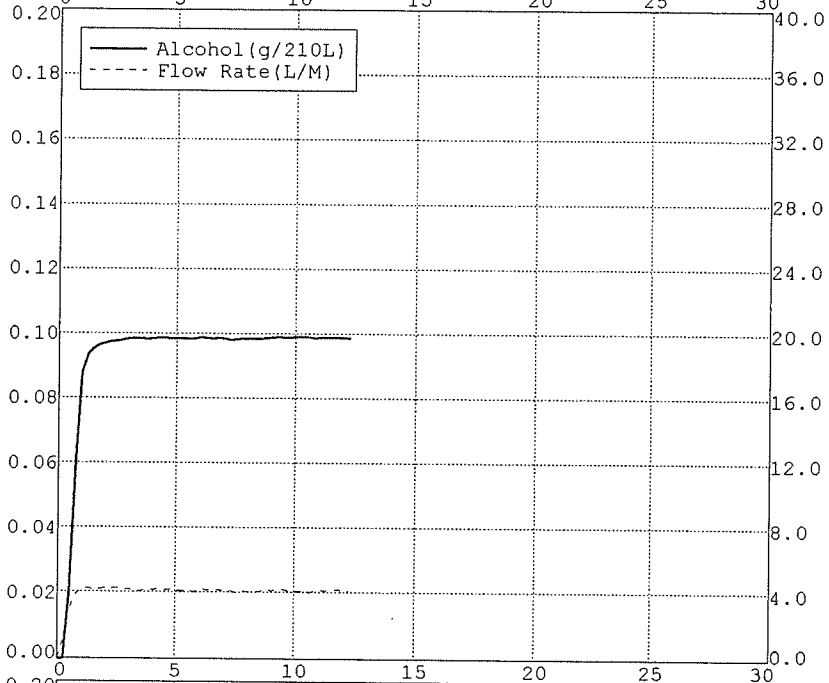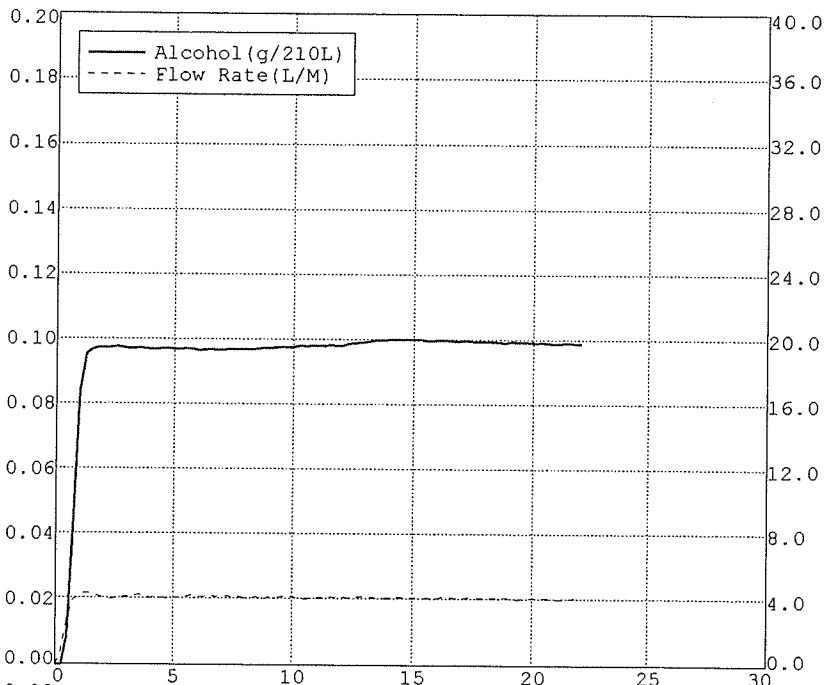

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/25/2020

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:39
INTERNAL STANDARD	ERROR	06:39

Internal Standard Error

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/25/2020

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:42
INTERNAL STANDARD	VERIFIED	06:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:42
BLANK TEST	0.00	06:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:43
BLANK TEST	0.00	06:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:45
BLANK TEST	0.00	06:45

