

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 02/06/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:07
INTERNAL STANDARD	VERIFIED	18:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:07
BLANK TEST	0.00	18:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:08
BLANK TEST	0.00	18:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:09
BLANK TEST	0.00	18:10

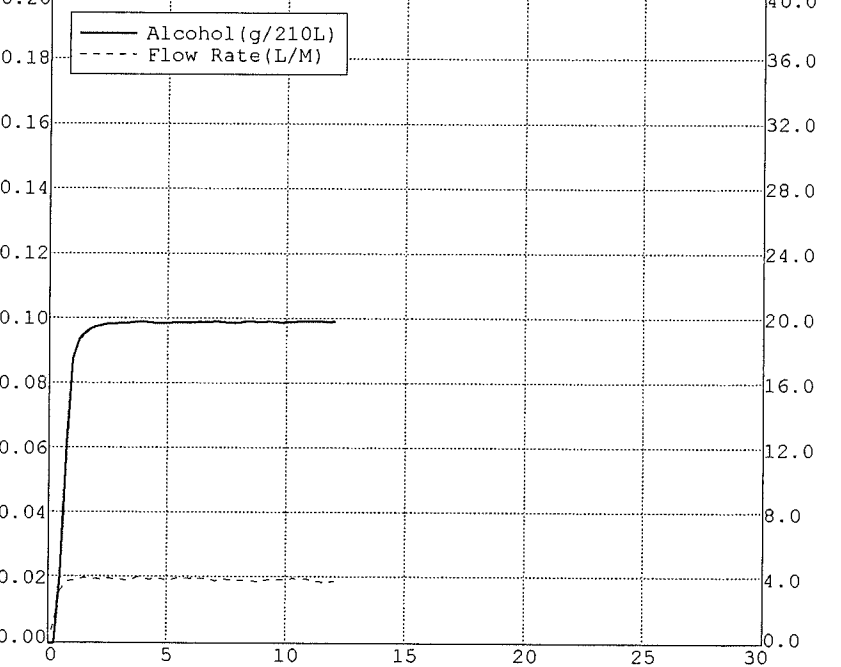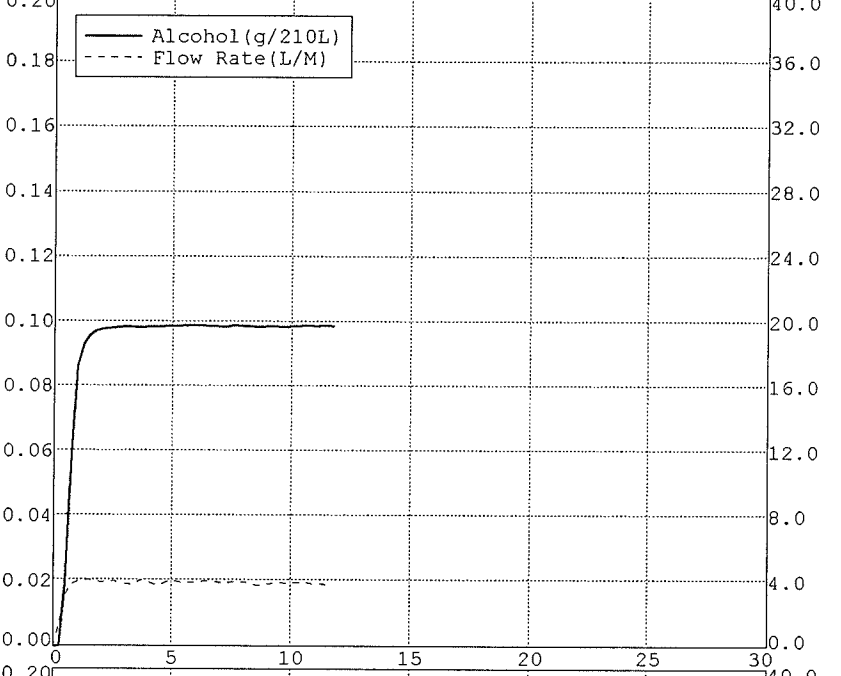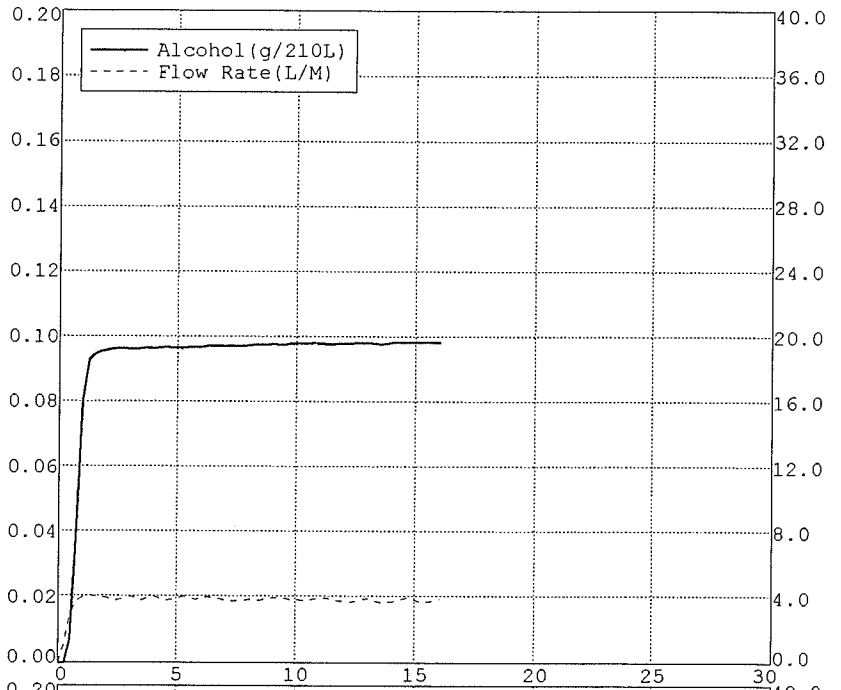

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 02/12/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:33
INTERNAL STANDARD	VERIFIED	20:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.08	20:33
BLANK TEST	0.00	20:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.08	20:34
BLANK TEST	0.00	20:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:35
BLANK TEST	0.00	20:36

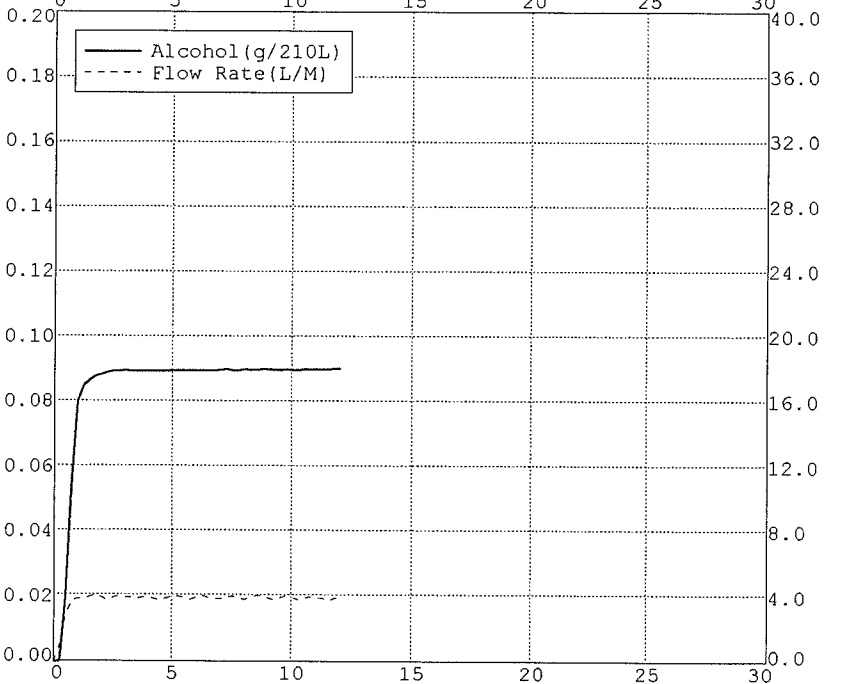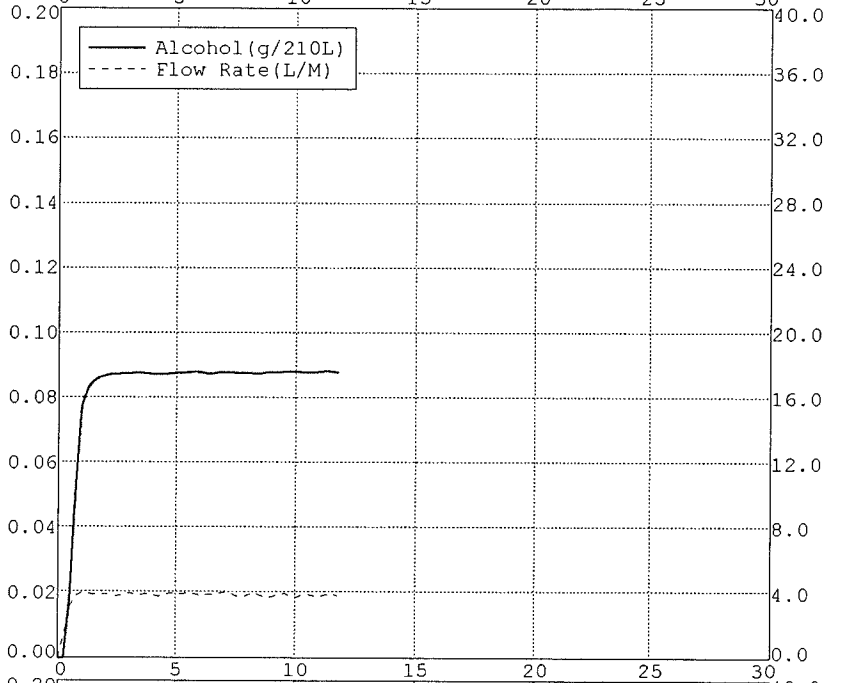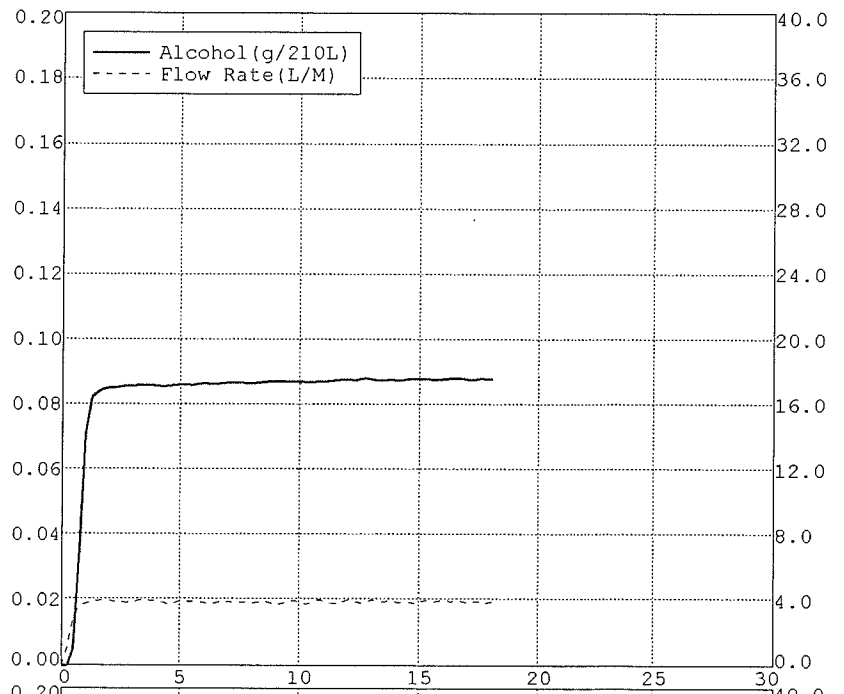

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 02/12/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:02
INTERNAL STANDARD	VERIFIED	21:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:03
BLANK TEST	0.00	21:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:04
BLANK TEST	0.00	21:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:05
BLANK TEST	0.00	21:06

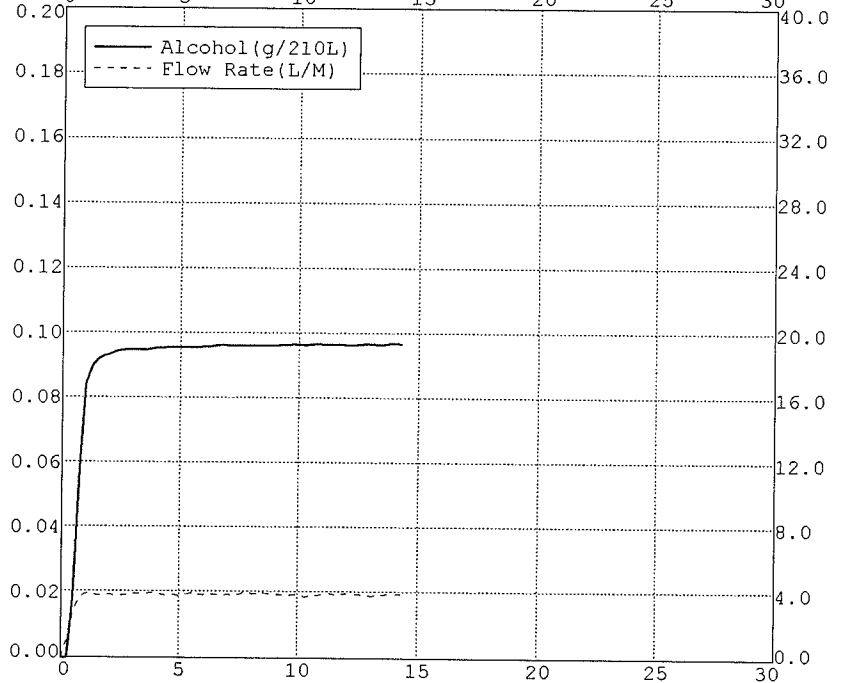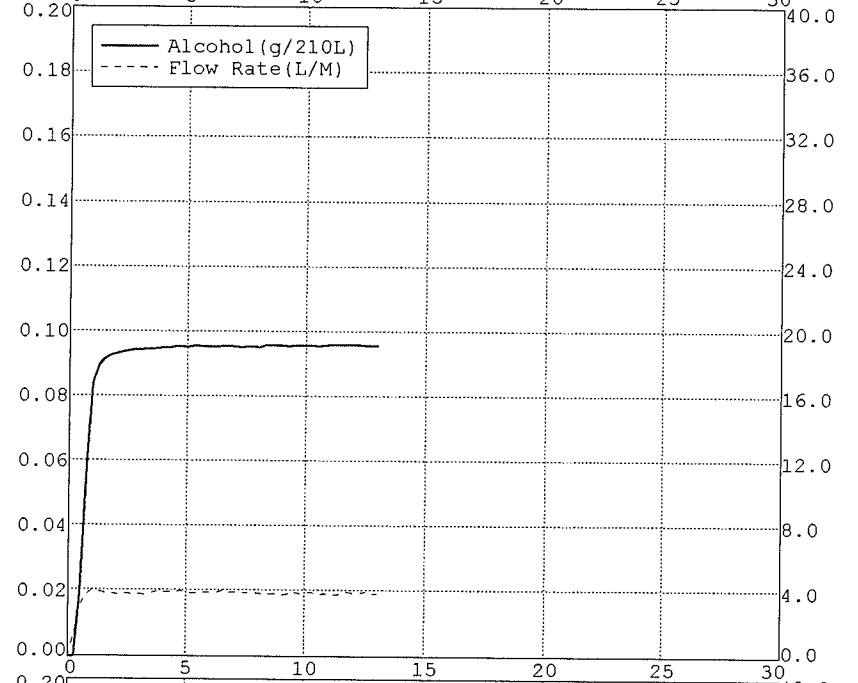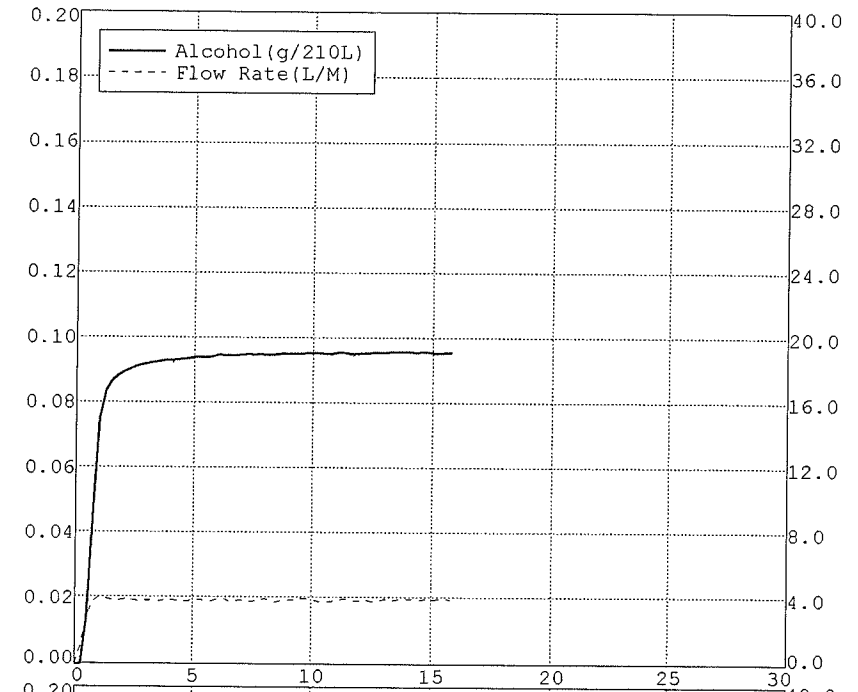

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 02/20/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:03
INTERNAL STANDARD	VERIFIED	18:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:03
BLANK TEST	0.00	18:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:05
BLANK TEST	0.00	18:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:06
BLANK TEST	0.00	18:07

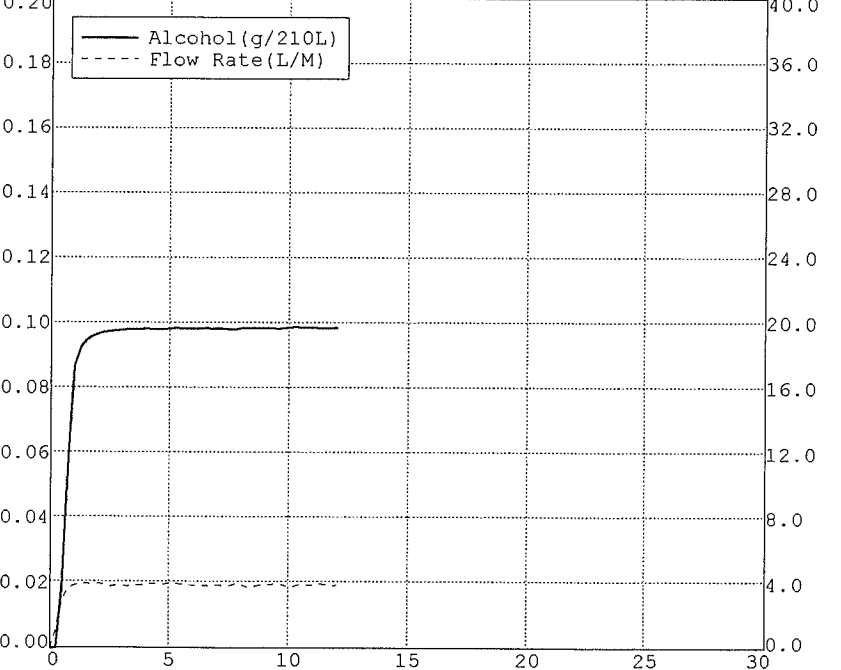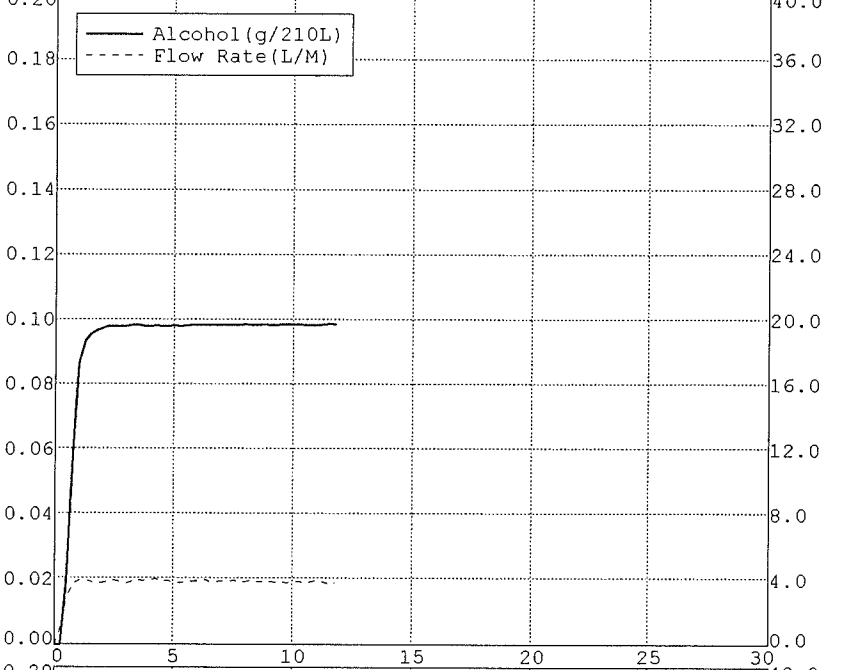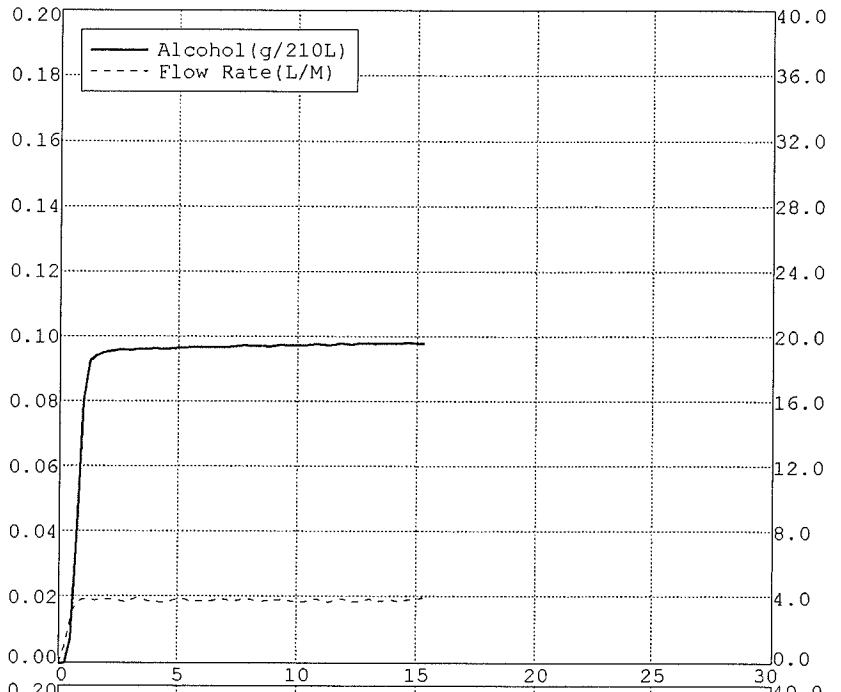

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 02/26/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:31
INTERNAL STANDARD	VERIFIED	18:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:31
BLANK TEST	0.00	18:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:32
BLANK TEST	0.00	18:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:33
BLANK TEST	0.00	18:34

