

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/06/2025

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25040

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:13
INTERNAL STANDARD	VERIFIED	18:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:13
BLANK TEST	0.00	18:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:14
BLANK TEST	0.00	18:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:16
BLANK TEST	0.00	18:16

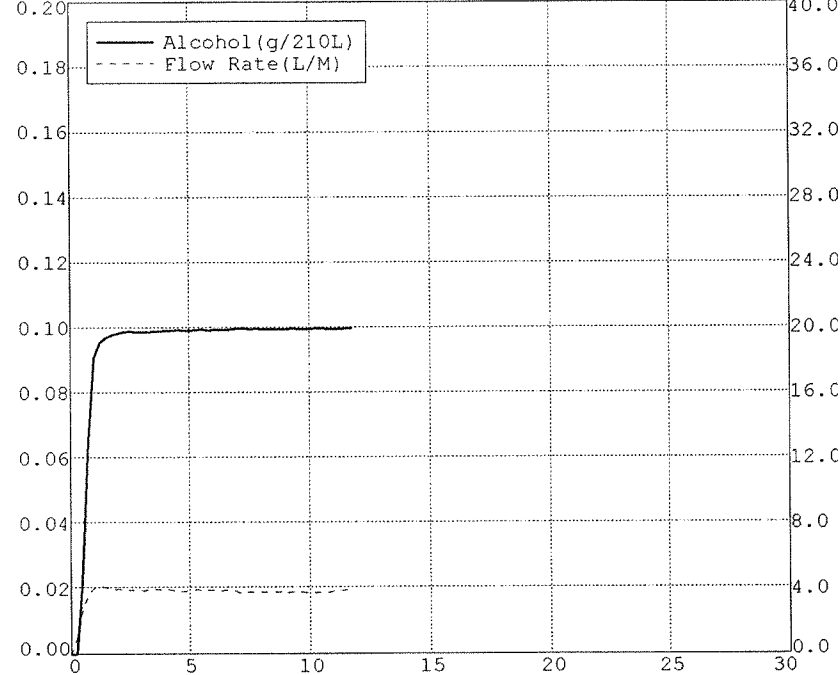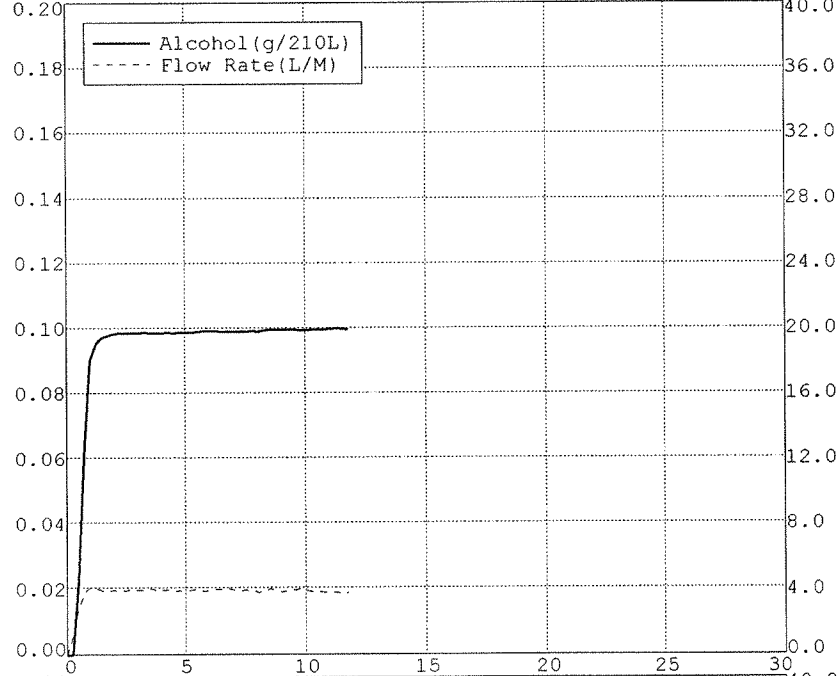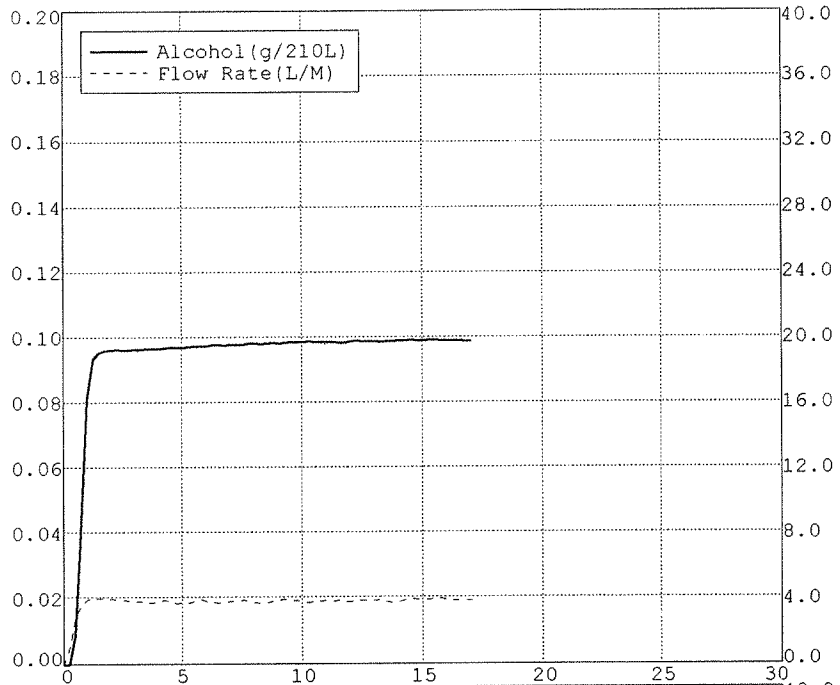

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/14/2025

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25040

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:47
INTERNAL STANDARD	VERIFIED	22:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:47
BLANK TEST	0.00	22:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:48
BLANK TEST	0.00	22:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:49
BLANK TEST	0.00	22:50

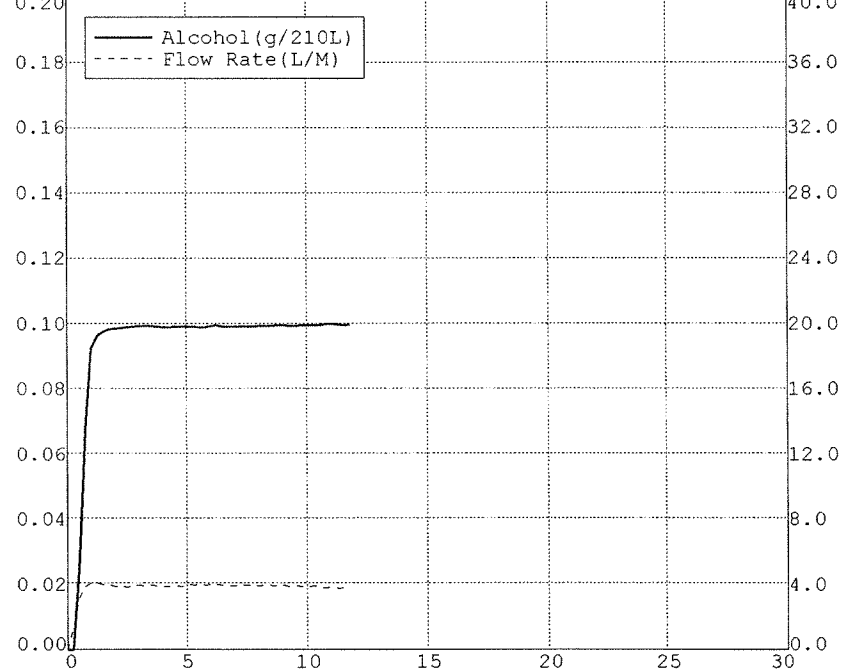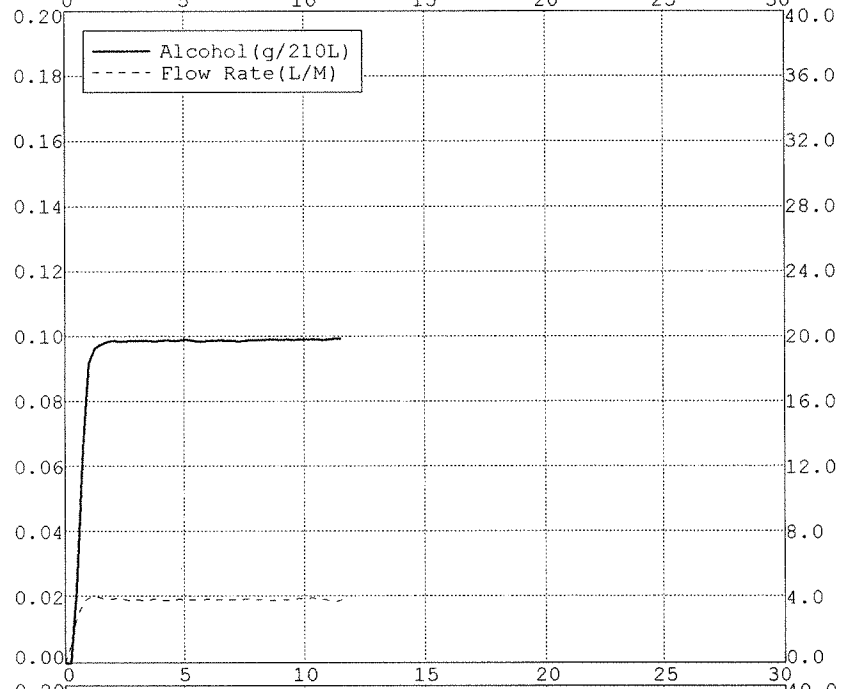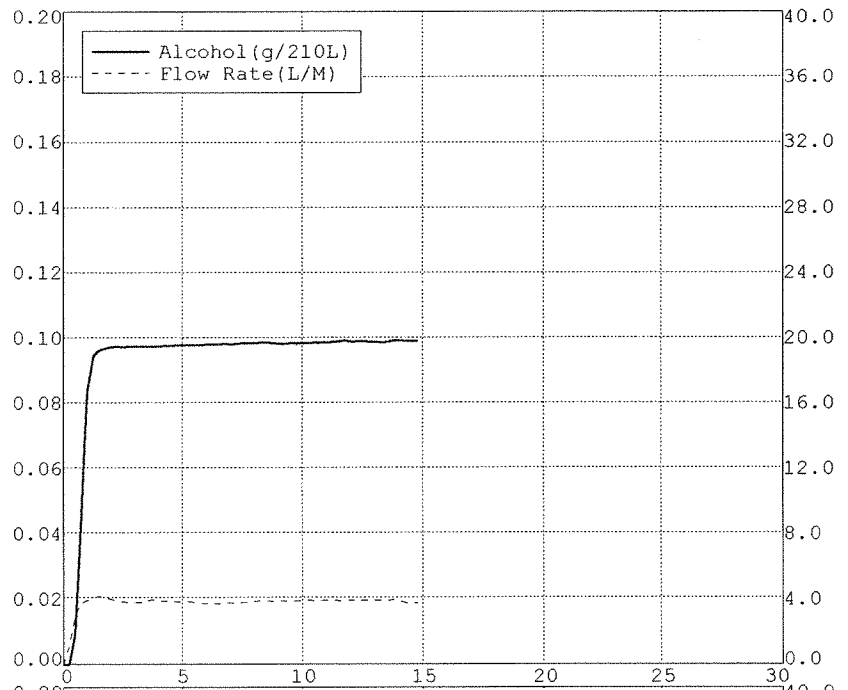

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/20/2025

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25040

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:50
INTERNAL STANDARD	VERIFIED	06:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:50
BLANK TEST	0.00	06:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:51
BLANK TEST	0.00	06:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:52
BLANK TEST	0.00	06:53

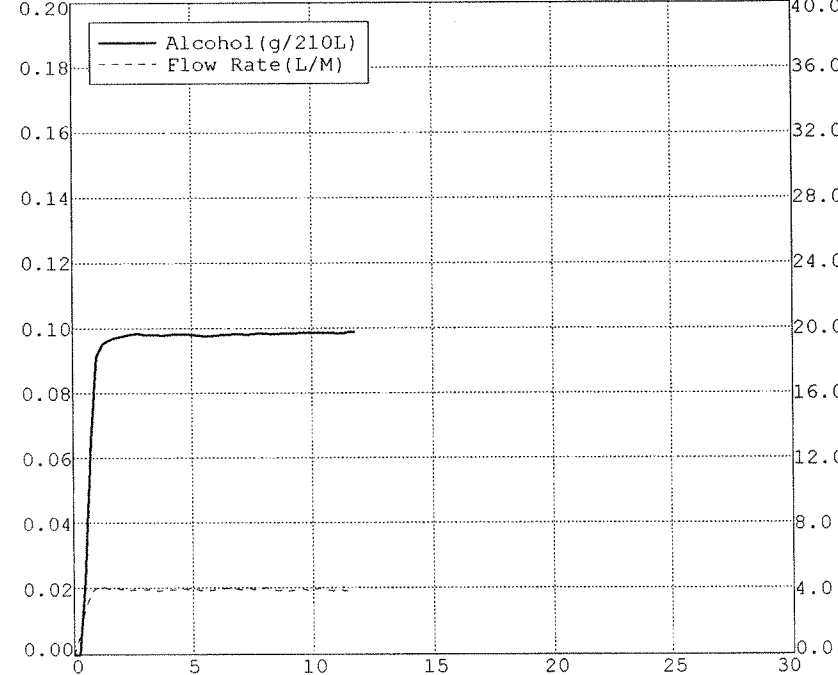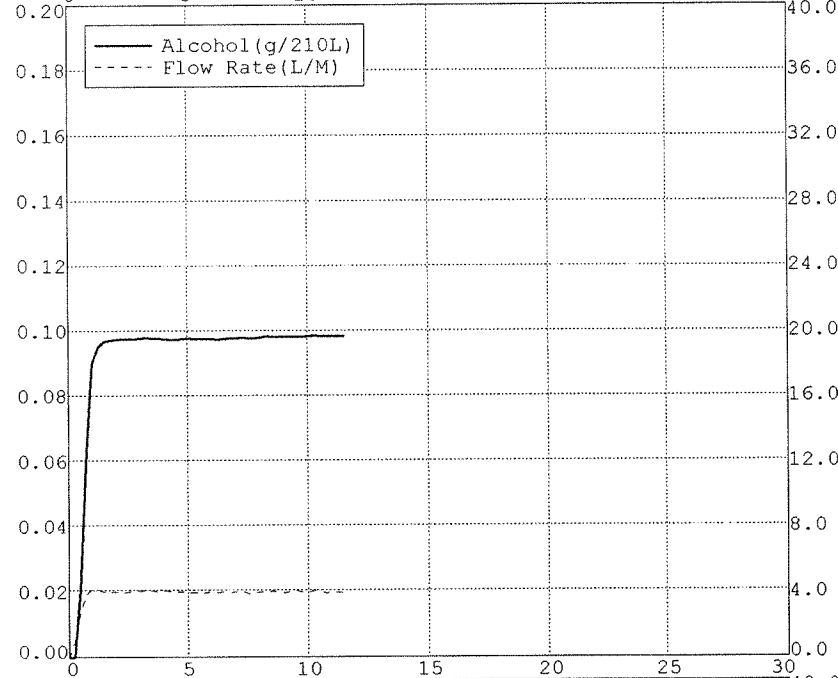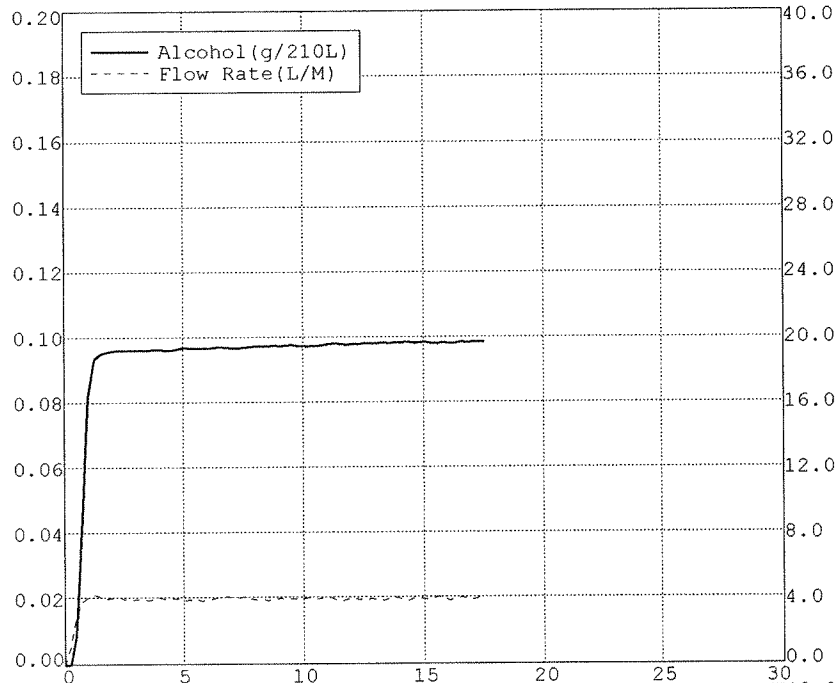

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/27/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25040

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:40
INTERNAL STANDARD	VERIFIED	08:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:40
BLANK TEST	0.00	08:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:41
BLANK TEST	0.00	08:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:42
BLANK TEST	0.00	08:43

