

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/01/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:10
INTERNAL STANDARD	VERIFIED	18:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:11
BLANK TEST	0.00	18:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:12
BLANK TEST	0.00	18:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:13
BLANK TEST	0.00	18:14

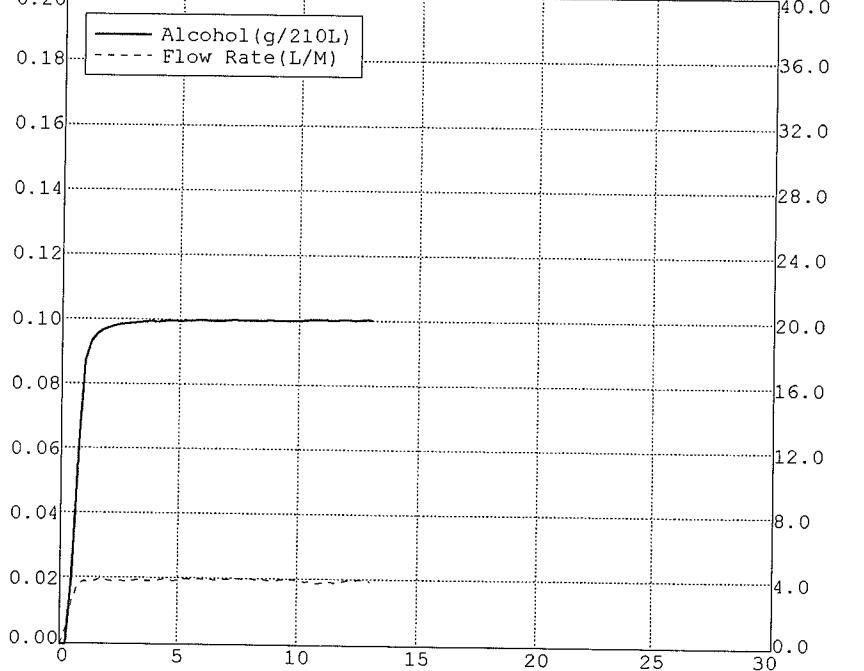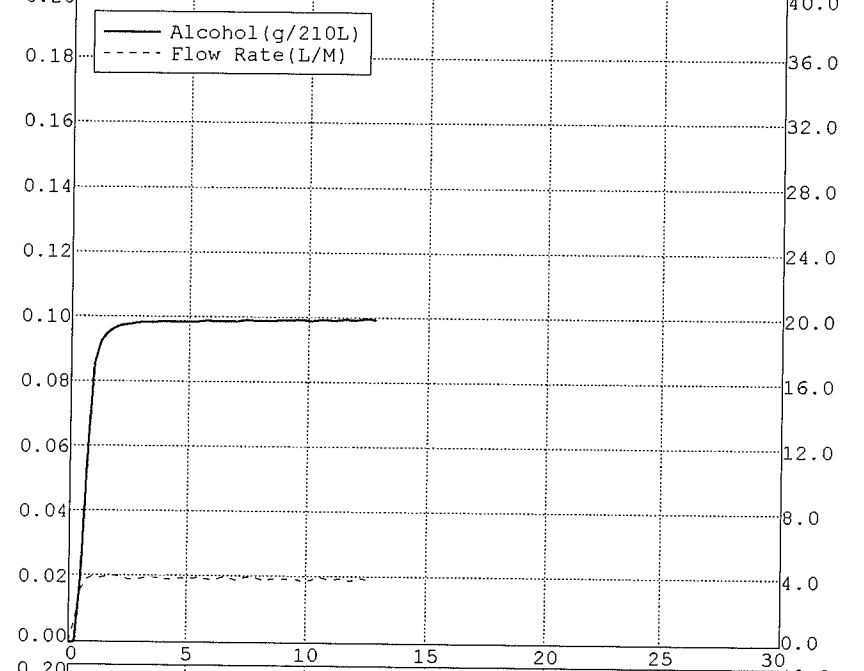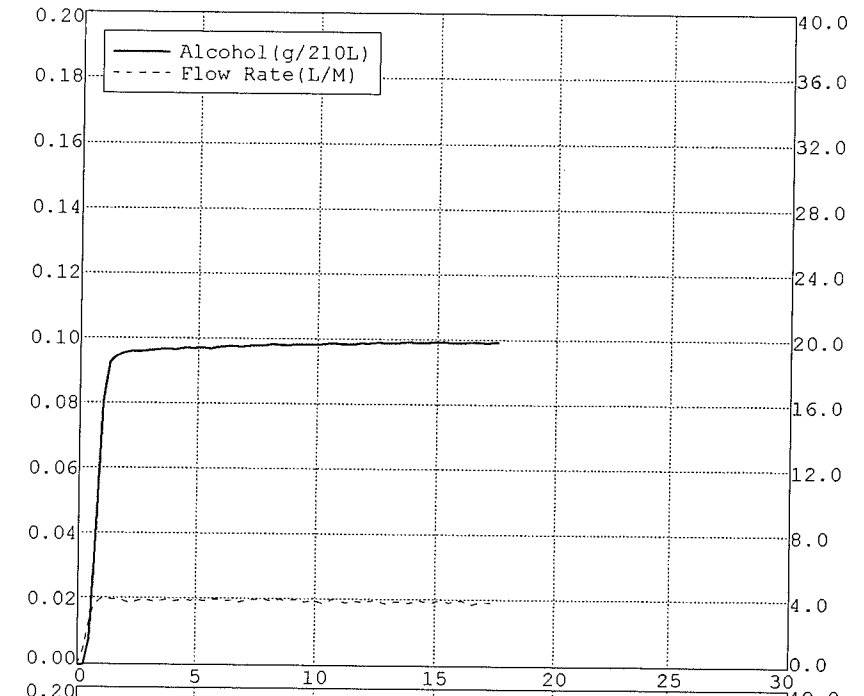

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/01/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22390

Nominal = 0.10 g/210L

RFI Detected

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/09/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:25
INTERNAL STANDARD	VERIFIED	18:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:25
BLANK TEST	0.00	18:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:26
BLANK TEST	0.00	18:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:27
BLANK TEST	0.00	18:28

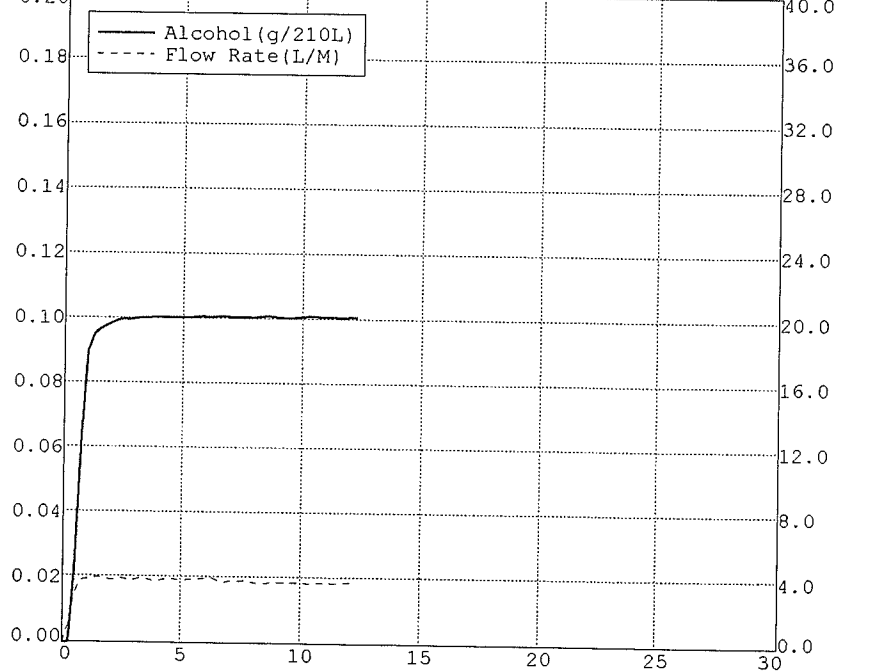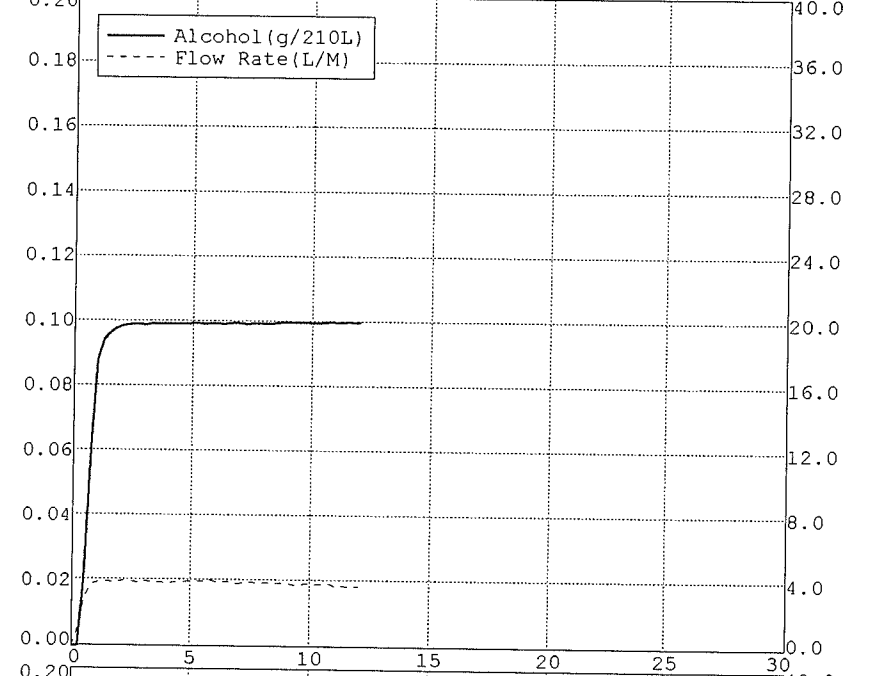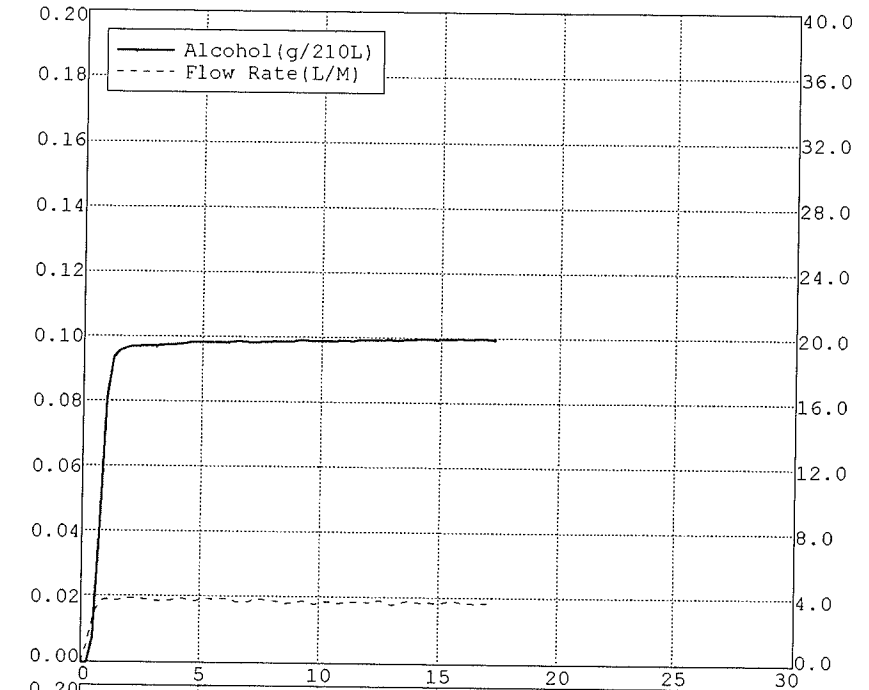

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/15/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:12
INTERNAL STANDARD	VERIFIED	18:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:13
BLANK TEST	0.00	18:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:14
BLANK TEST	0.00	18:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:15
BLANK TEST	0.00	18:16

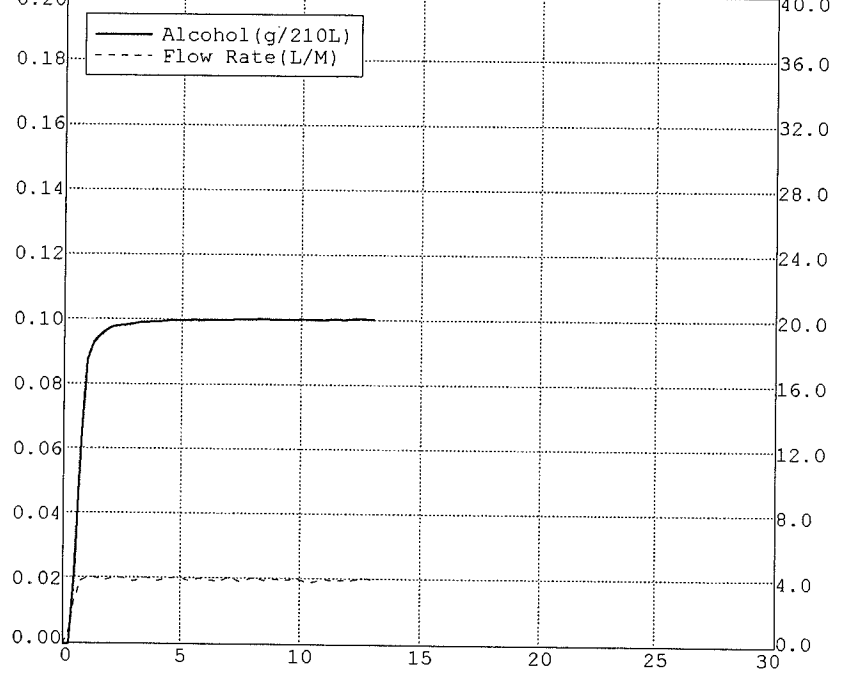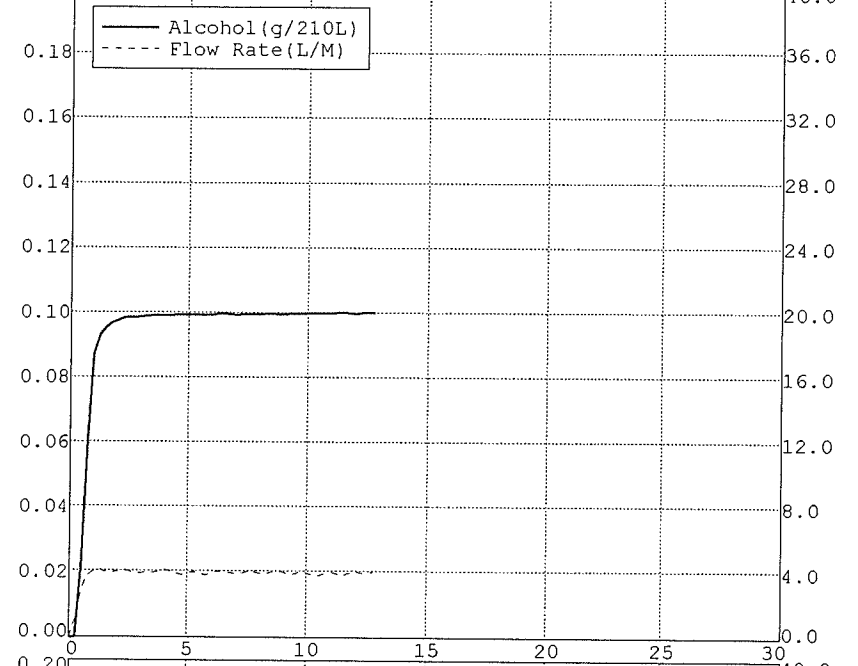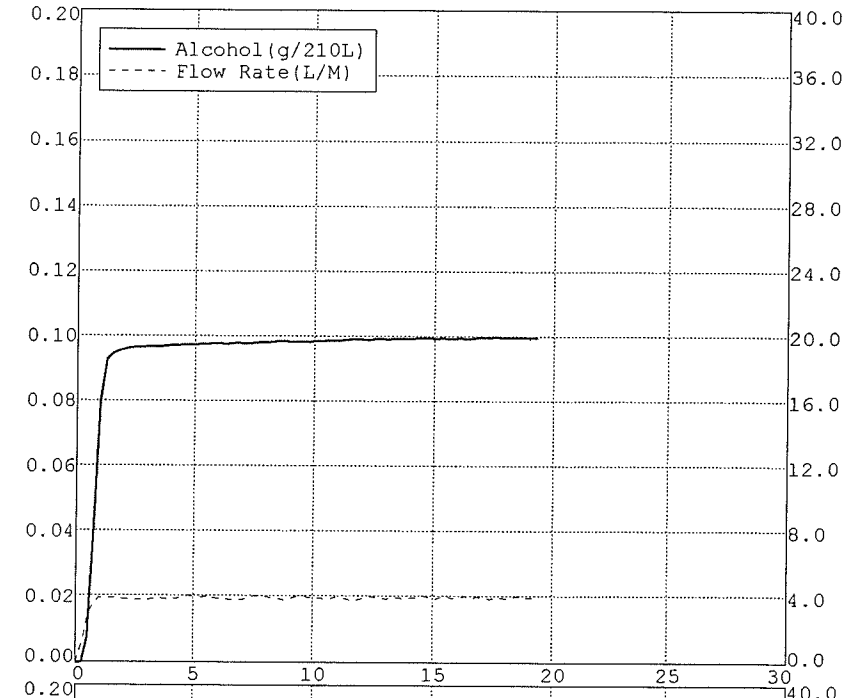

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/23/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:06
INTERNAL STANDARD	VERIFIED	18:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:07
BLANK TEST	0.00	18:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:08
BLANK TEST	0.00	18:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:09
BLANK TEST	0.00	18:10

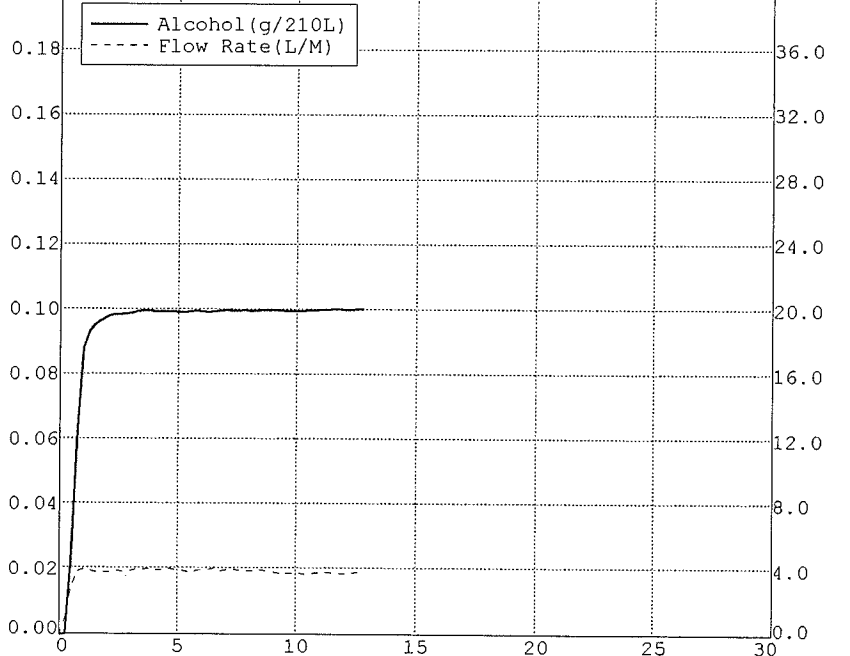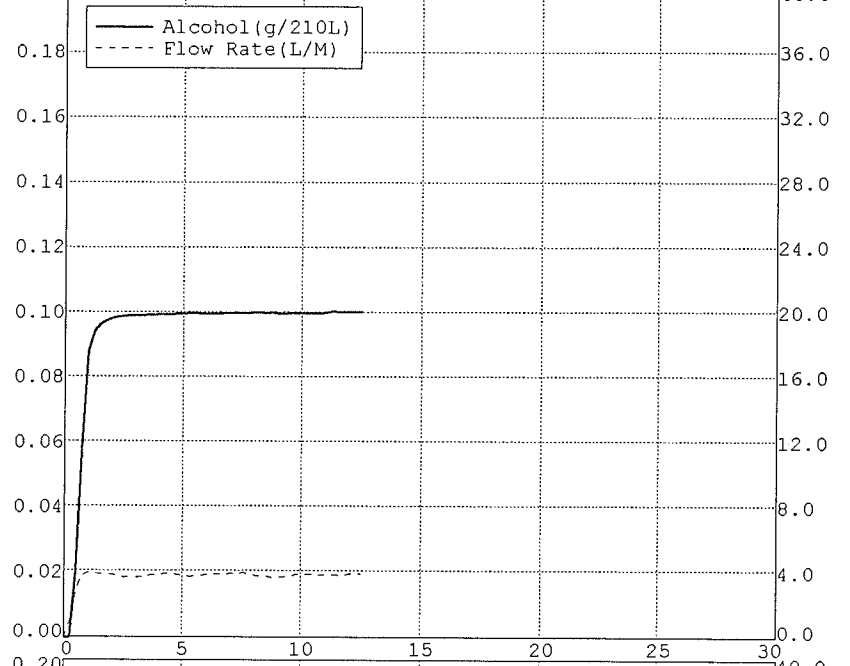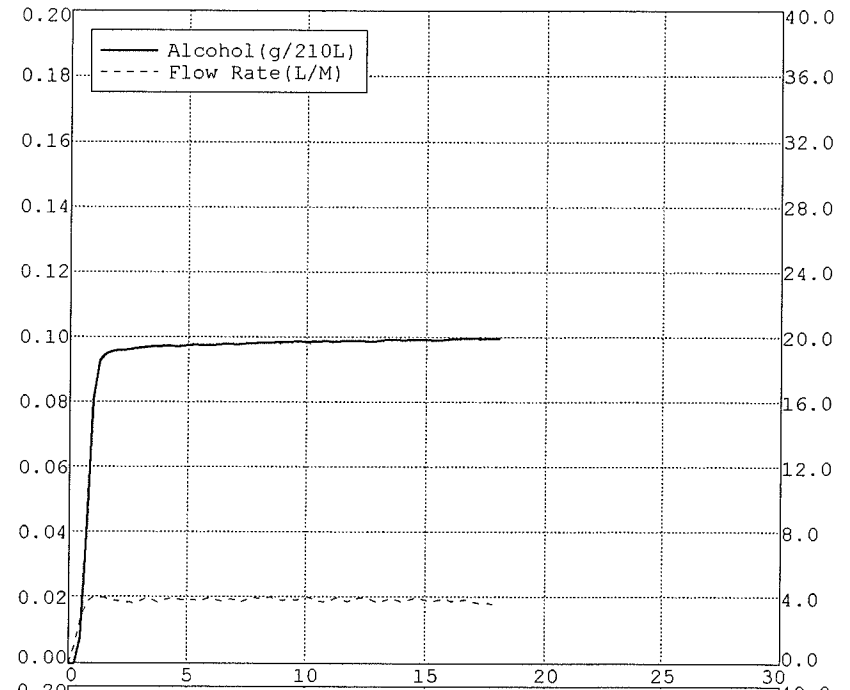

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/29/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:42
INTERNAL STANDARD	VERIFIED	19:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:42
BLANK TEST	0.00	19:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:43
BLANK TEST	0.00	19:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:45
BLANK TEST	0.00	19:45

