

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/03/2024

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24270

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:43
INTERNAL STANDARD	VERIFIED	06:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:43
BLANK TEST	0.00	06:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:44
BLANK TEST	0.00	06:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:45
BLANK TEST	0.00	06:46

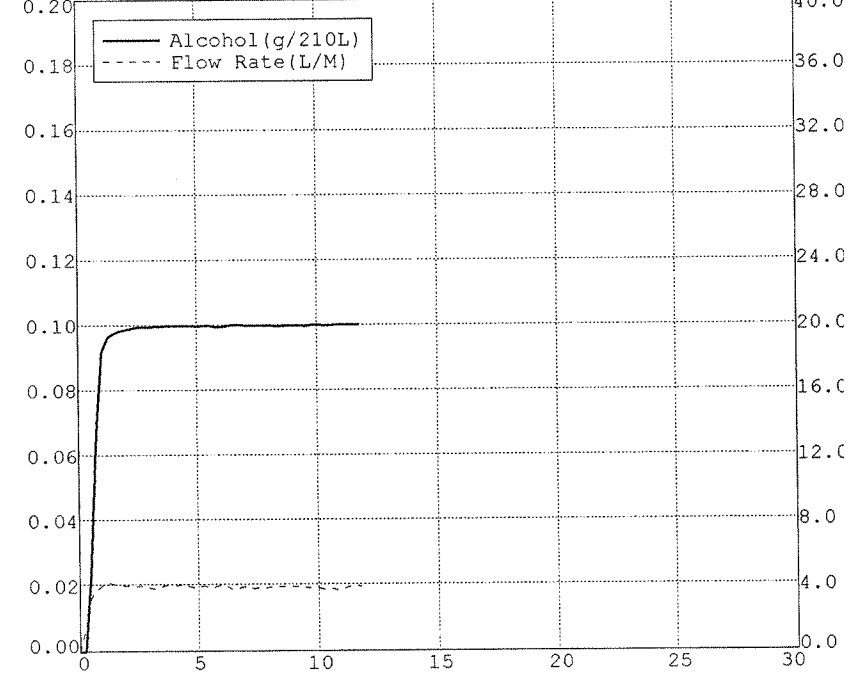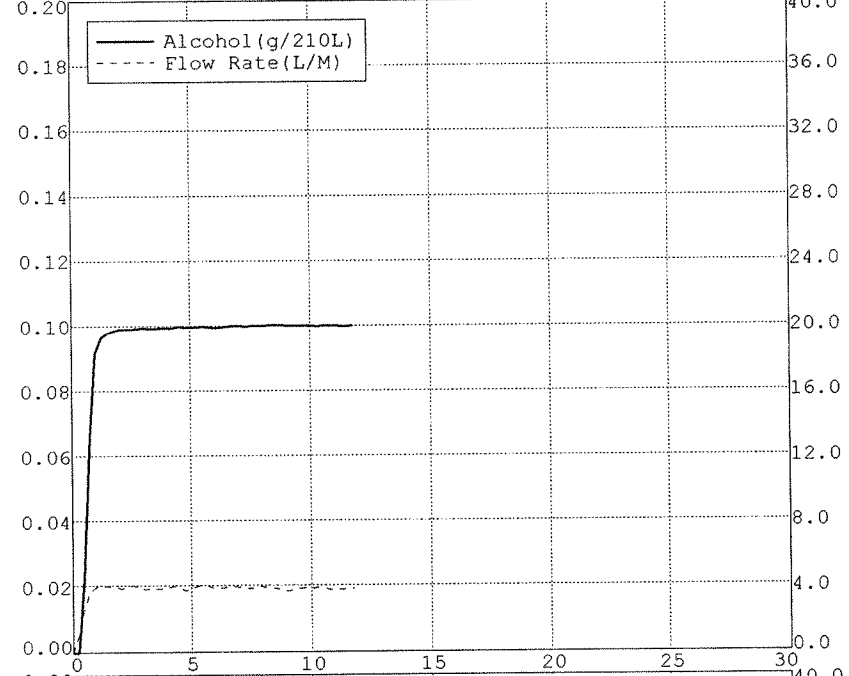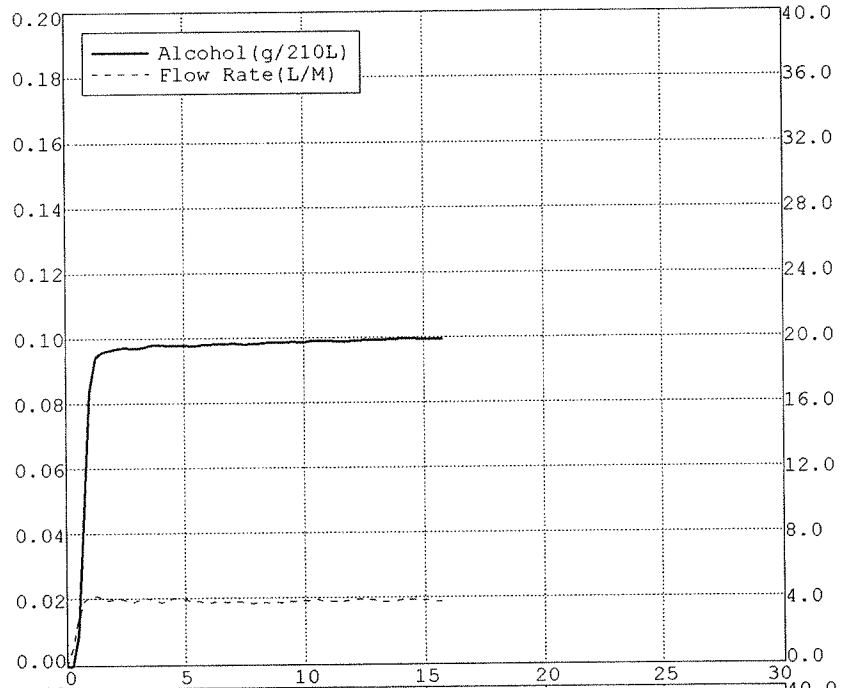

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/10/2024

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24270

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:12
INTERNAL STANDARD	VERIFIED	05:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:13
BLANK TEST	0.00	05:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:14
BLANK TEST	0.00	05:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:15
BLANK TEST	0.00	05:16

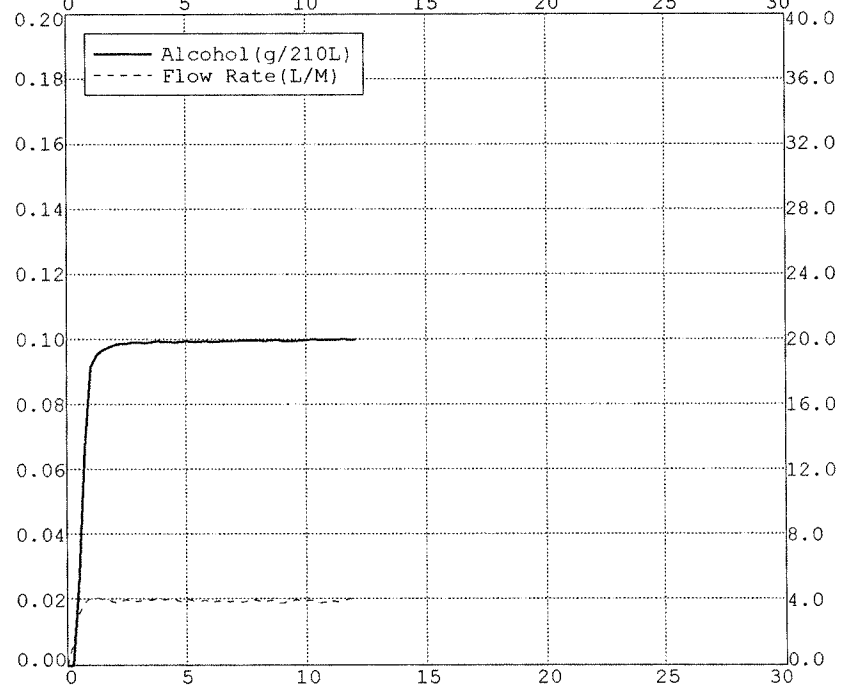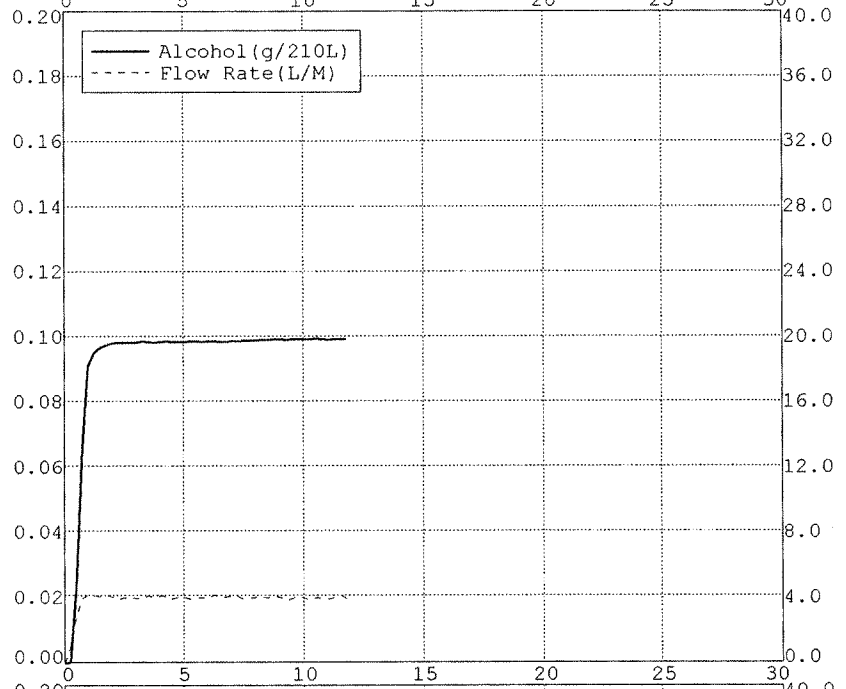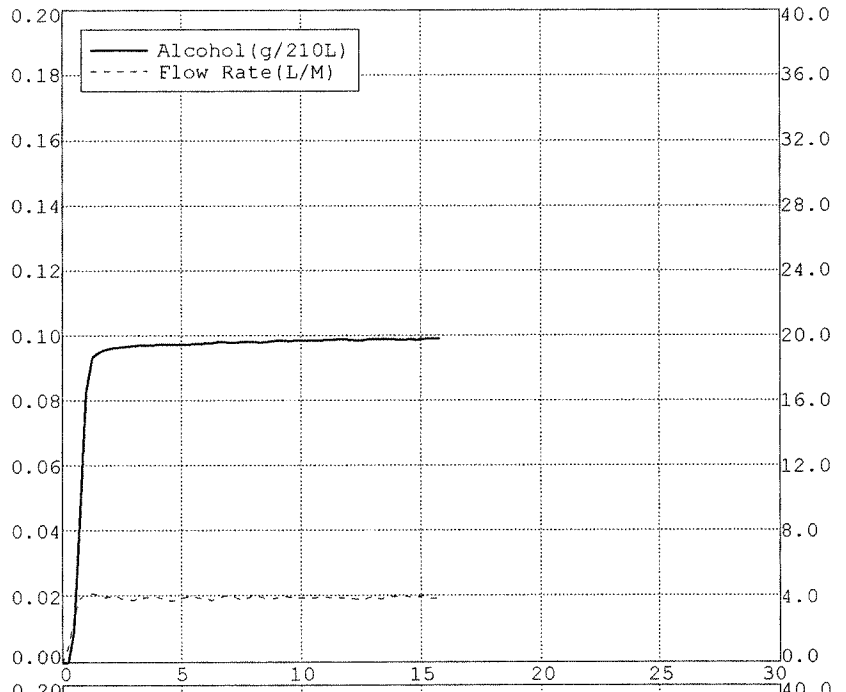

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/17/2024

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24270

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:34
INTERNAL STANDARD	VERIFIED	09:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:35
BLANK TEST	0.00	09:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:36
BLANK TEST	0.00	09:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:37
BLANK TEST	0.00	09:38

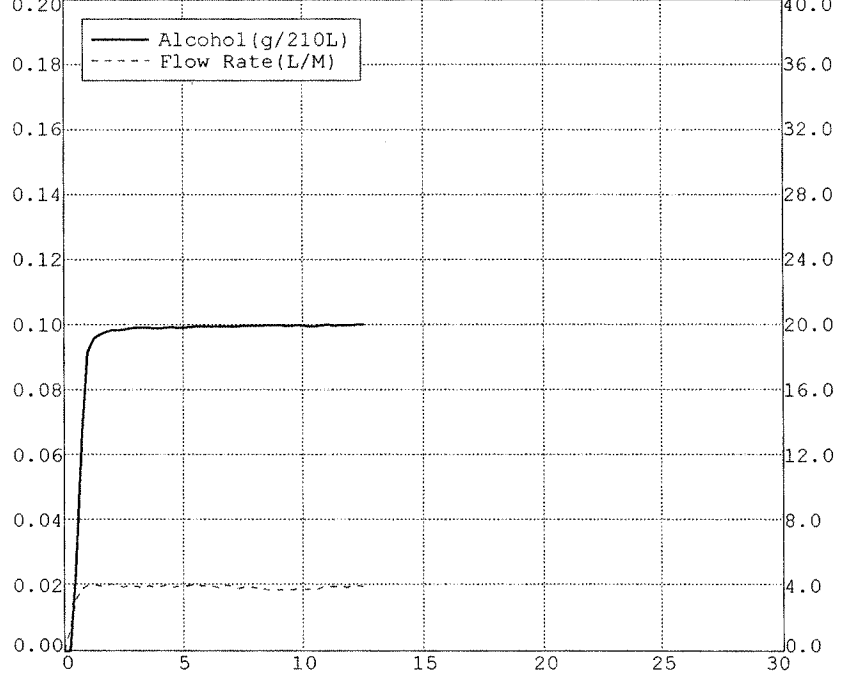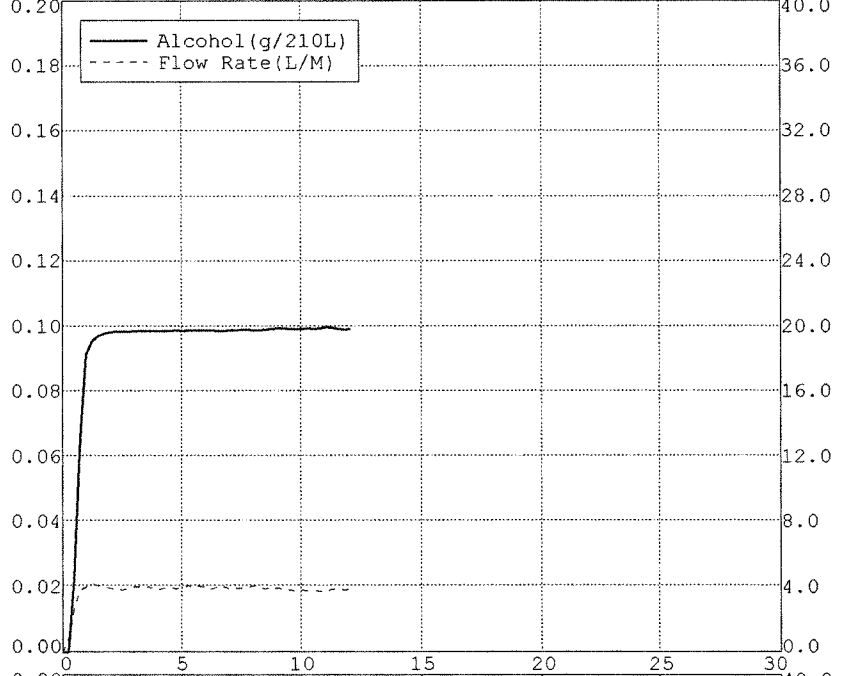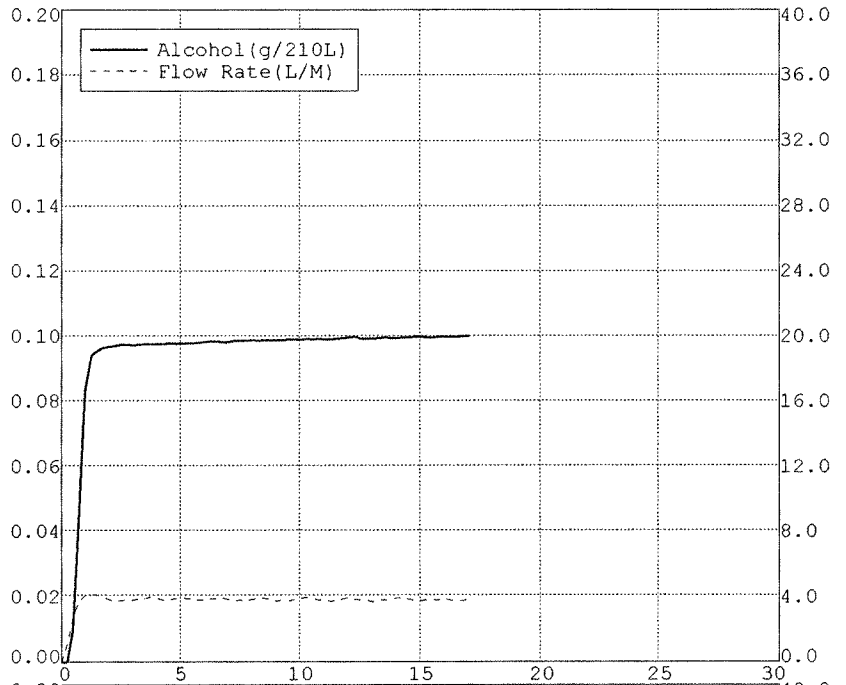

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/24/2024

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24270

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:11
INTERNAL STANDARD	VERIFIED	19:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:12
BLANK TEST	0.00	19:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:13
BLANK TEST	0.00	19:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:14
BLANK TEST	0.00	19:15

