

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/03/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25170

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:56
INTERNAL STANDARD	VERIFIED	18:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:57
BLANK TEST	0.00	18:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:58
BLANK TEST	0.00	18:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:59
BLANK TEST	0.00	19:00

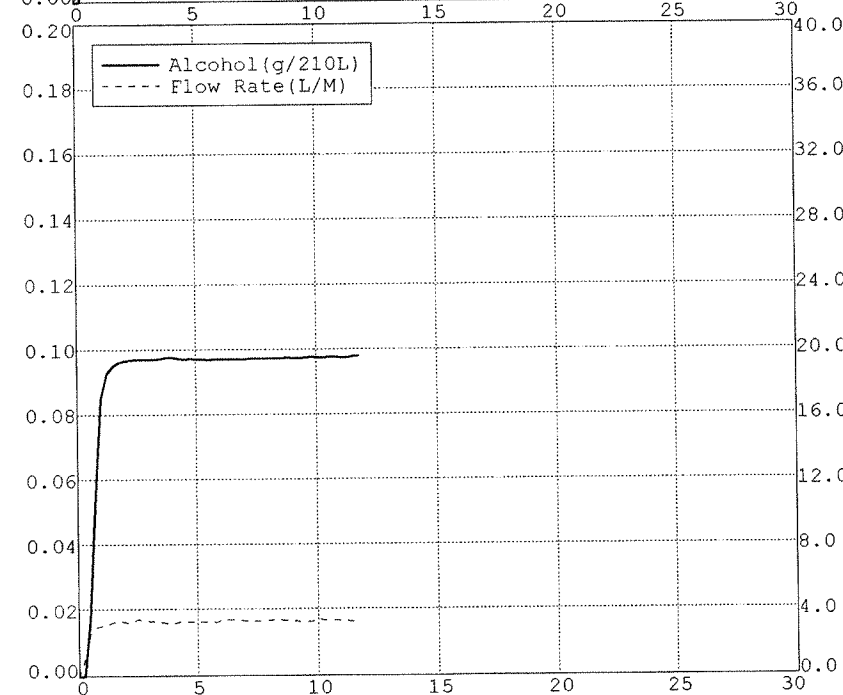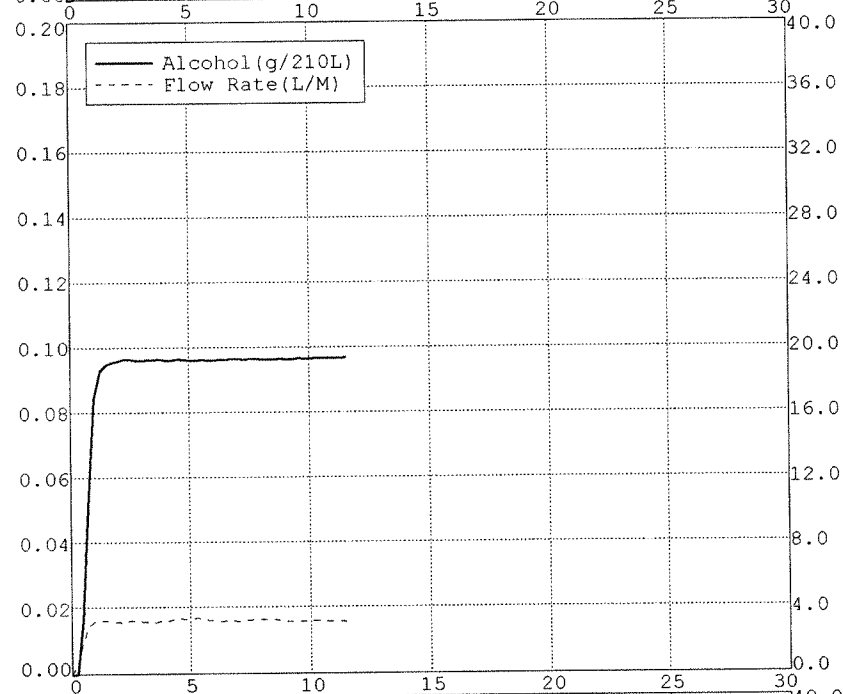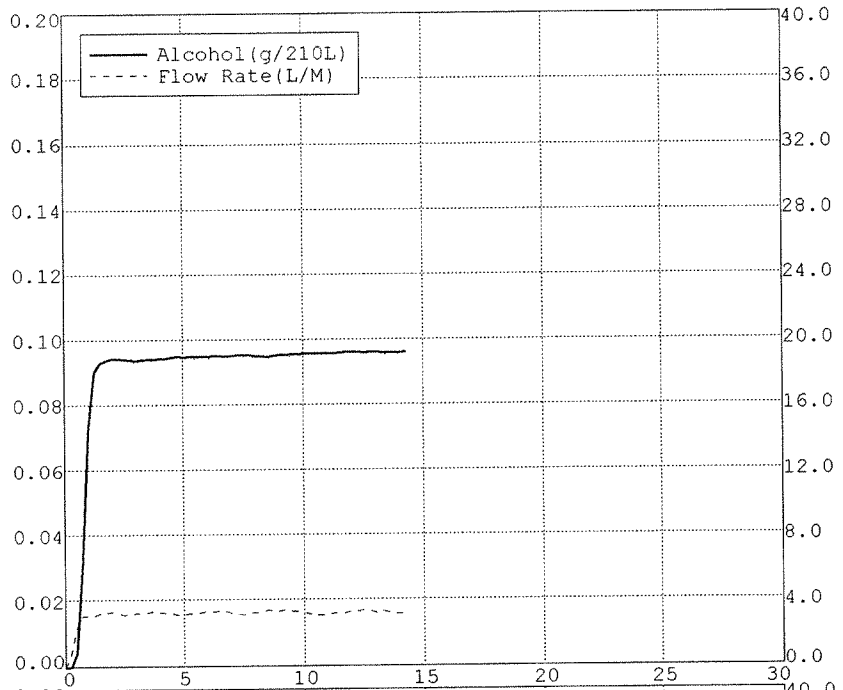

SUPERVISOR TEST


LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/10/2025

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25170

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:53
INTERNAL STANDARD	VERIFIED	11:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:53
BLANK TEST	0.00	11:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:54
BLANK TEST	0.00	11:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:56
BLANK TEST	0.00	11:56

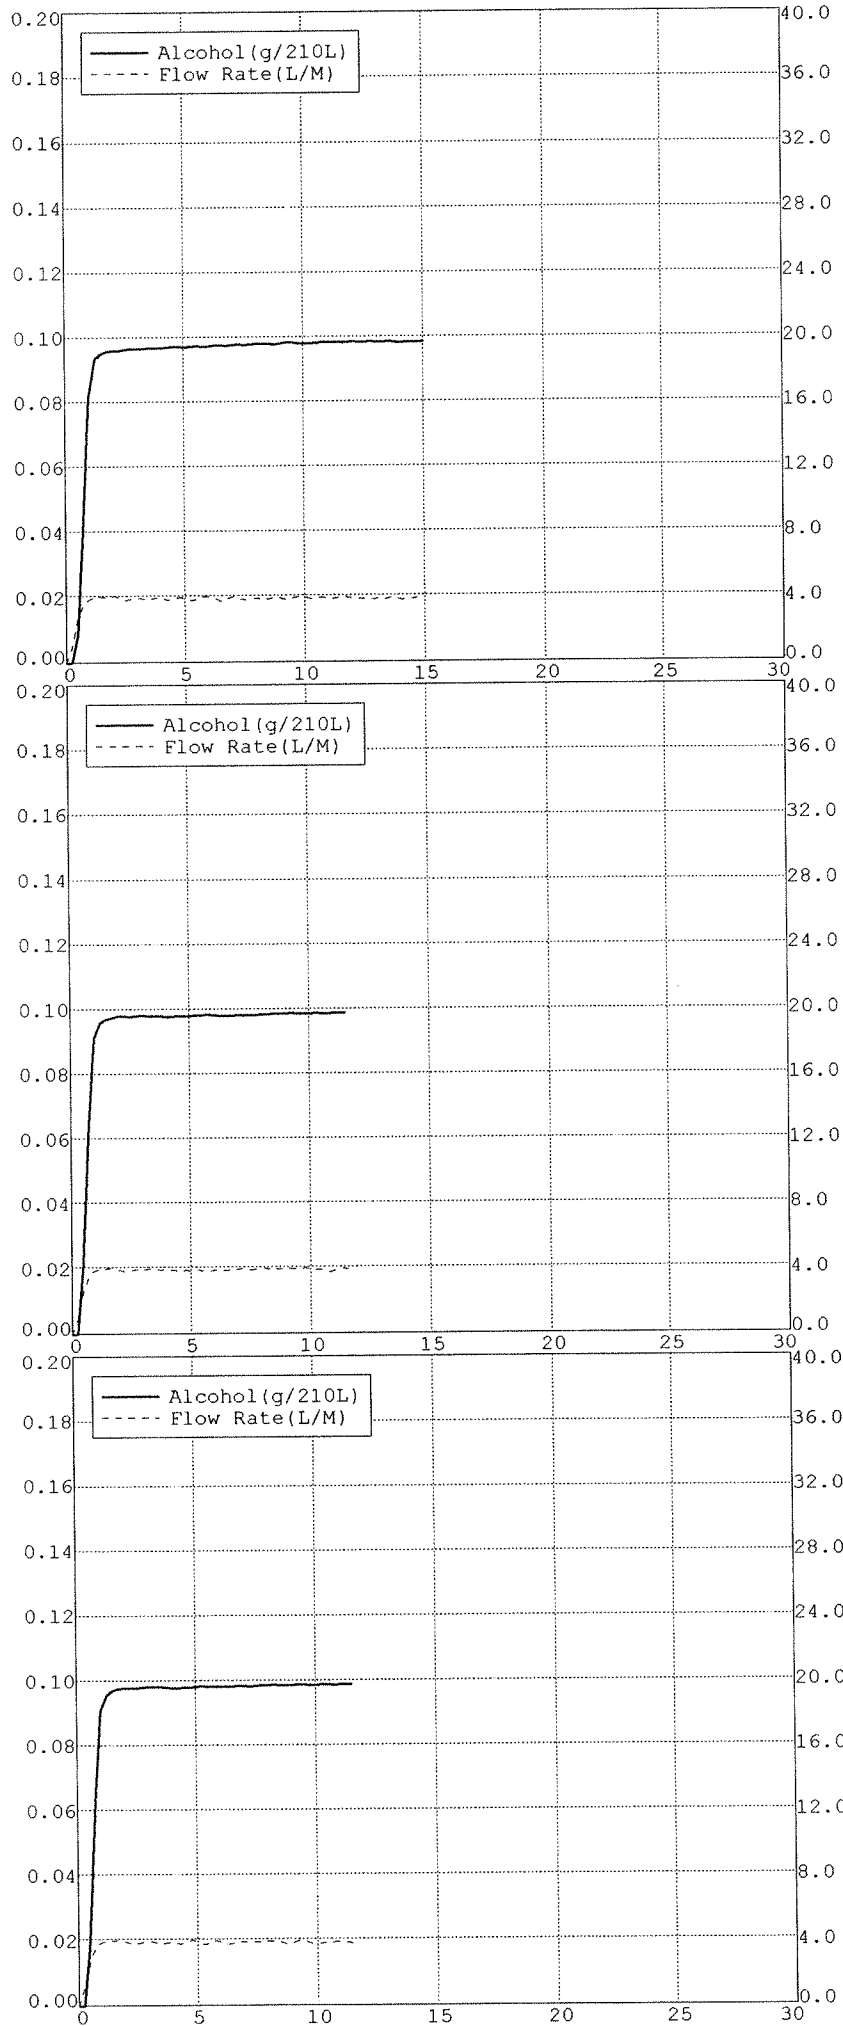

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/17/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25170

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:51
INTERNAL STANDARD	VERIFIED	10:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:51
BLANK TEST	0.00	10:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:52
BLANK TEST	0.00	10:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:53
BLANK TEST	0.00	10:54

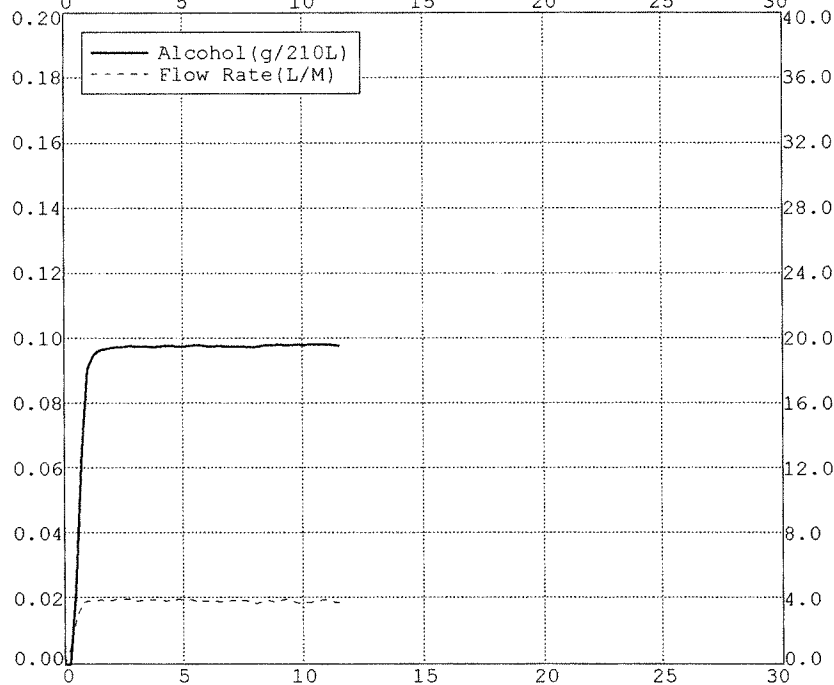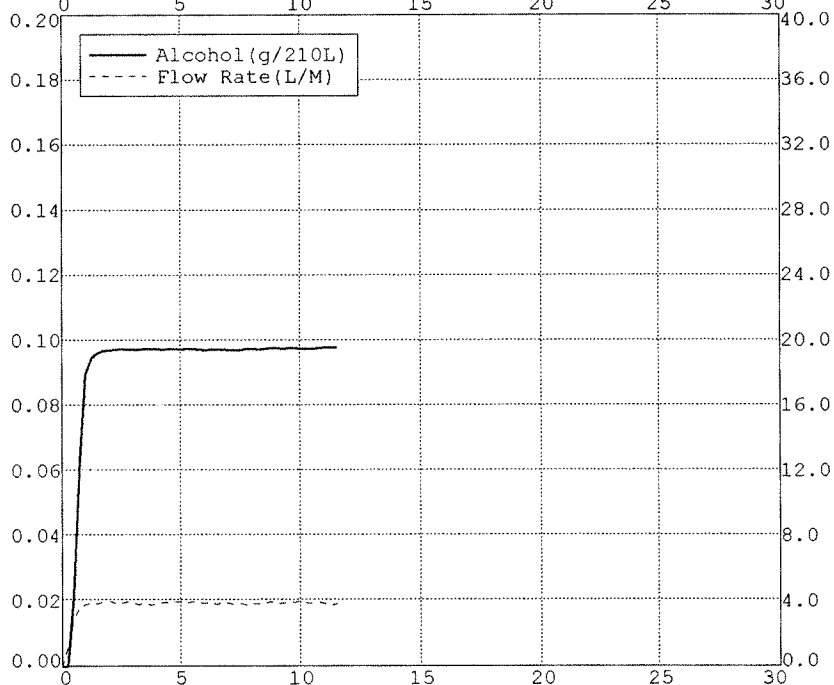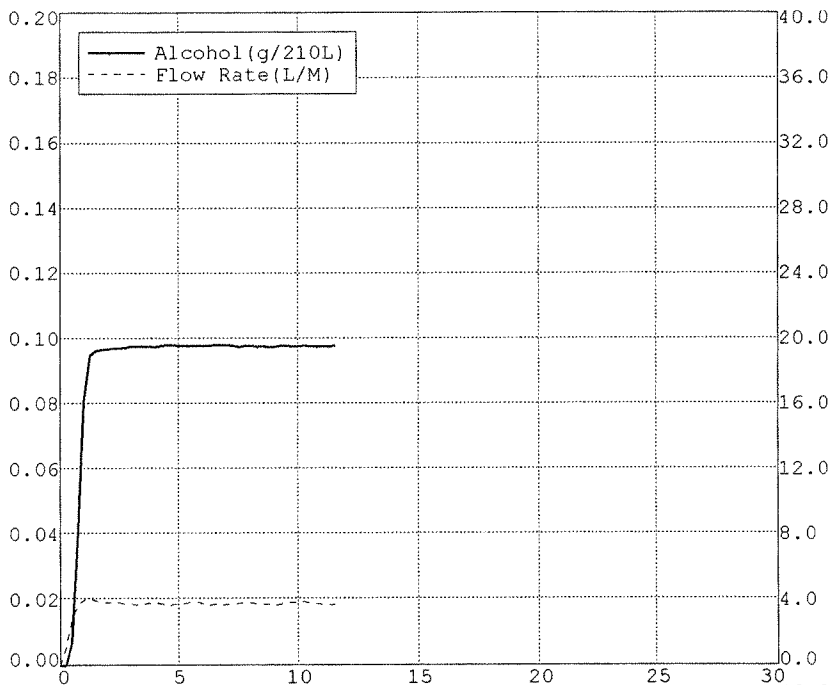

SUPERVISOR TEST


LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/24/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25170

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:14
INTERNAL STANDARD	VERIFIED	14:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:15
BLANK TEST	0.00	14:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:16
BLANK TEST	0.00	14:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:17
BLANK TEST	0.00	14:18

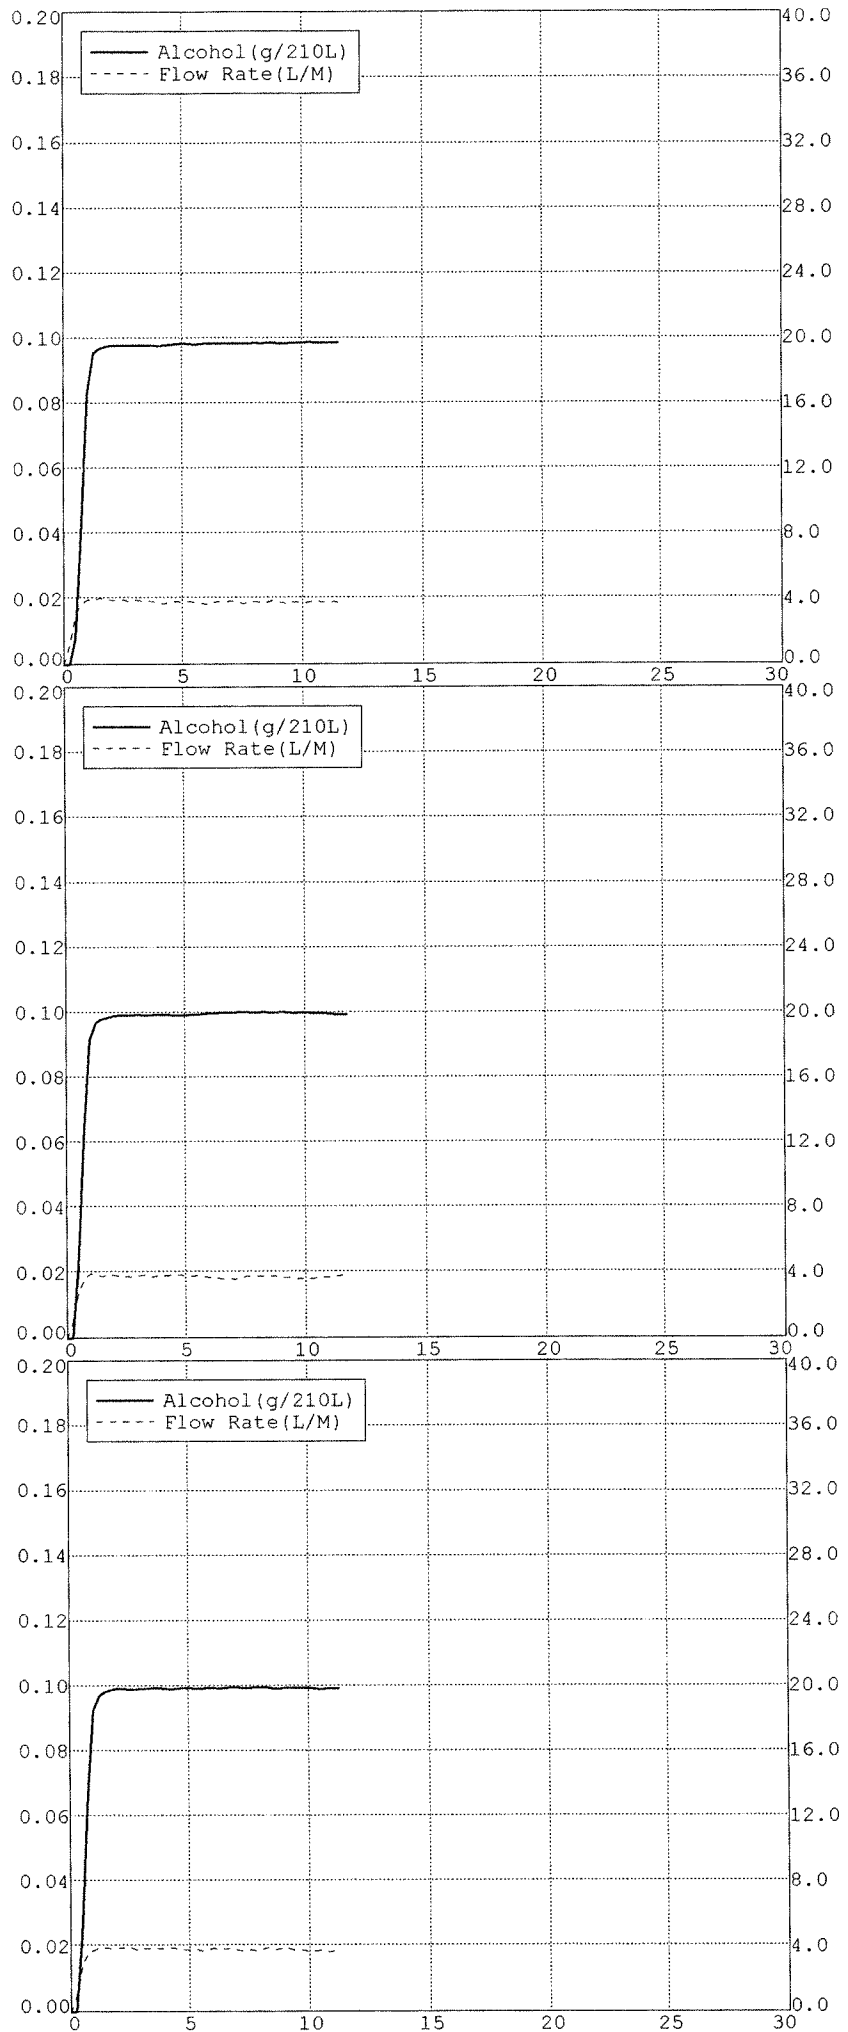

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/31/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25170

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:18
INTERNAL STANDARD	VERIFIED	19:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:19
BLANK TEST	0.00	19:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:20
BLANK TEST	0.00	19:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:21
BLANK TEST	0.00	19:22

