

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/08/2022

OPERATOR NAME:  
IAN O GORDON  
Permit #: 50784  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:03
INTERNAL STANDARD	VERIFIED	18:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:03
BLANK TEST	0.00	18:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:04
BLANK TEST	0.00	18:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:06
BLANK TEST	0.00	18:06

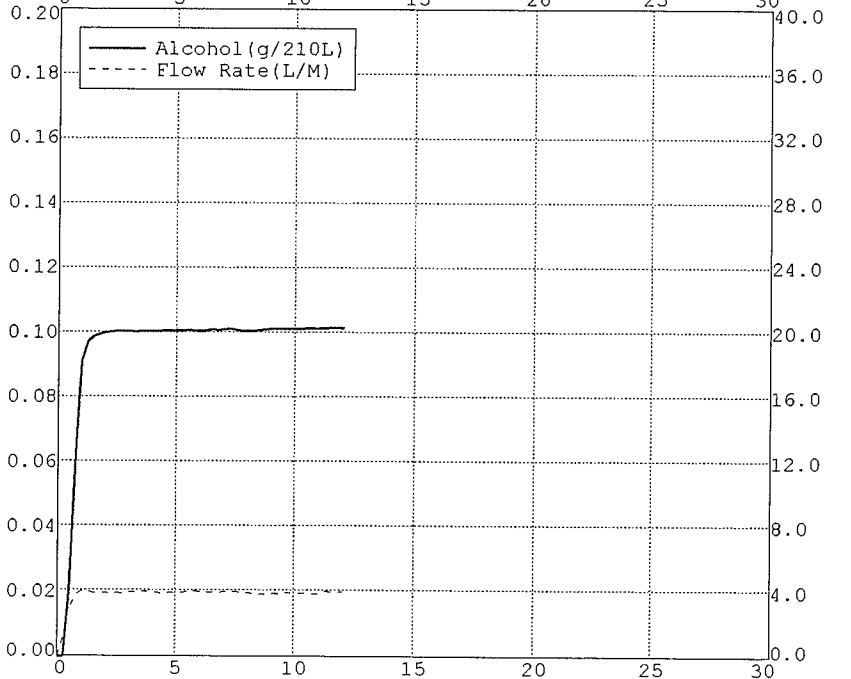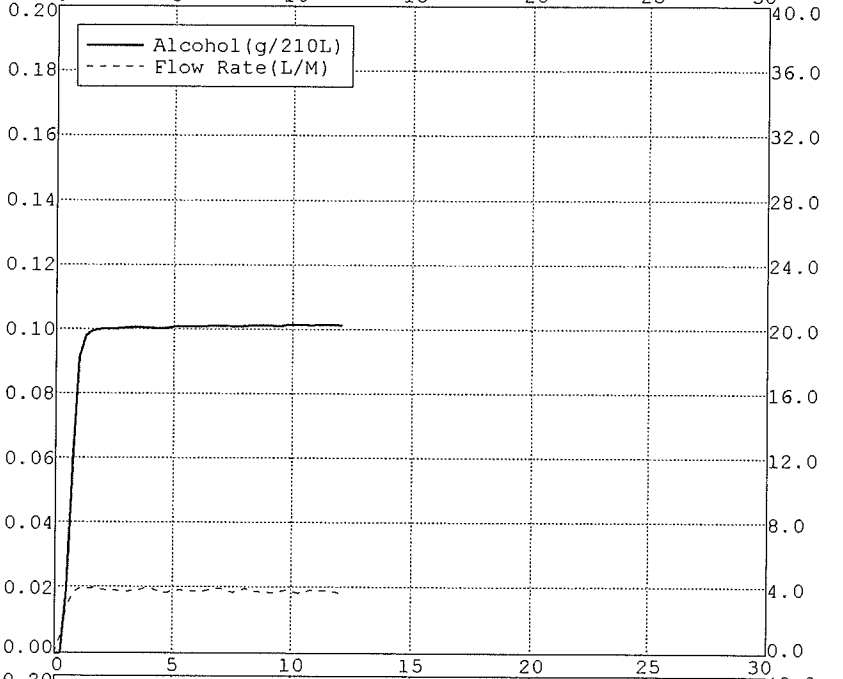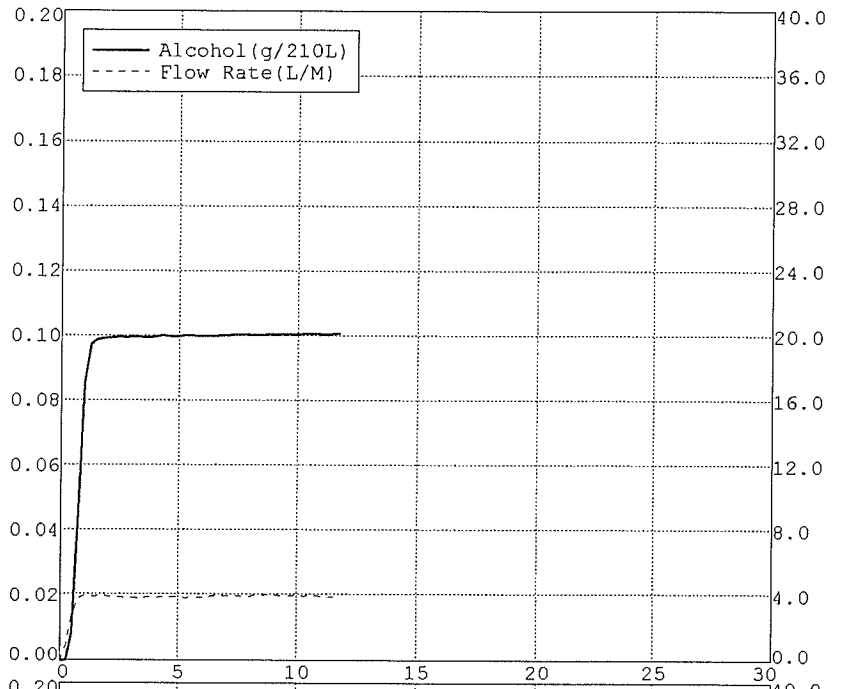

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/14/2022

OPERATOR NAME:  
IAN O GORDON  
Permit #: 50784  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:25
INTERNAL STANDARD	VERIFIED	05:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:26
BLANK TEST	0.00	05:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:27
BLANK TEST	0.00	05:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:28
BLANK TEST	0.00	05:29

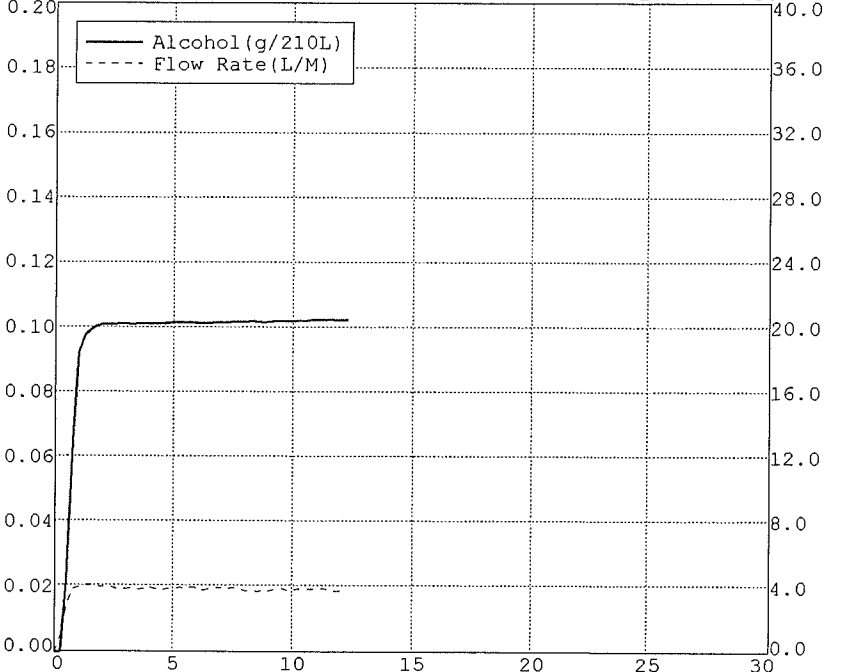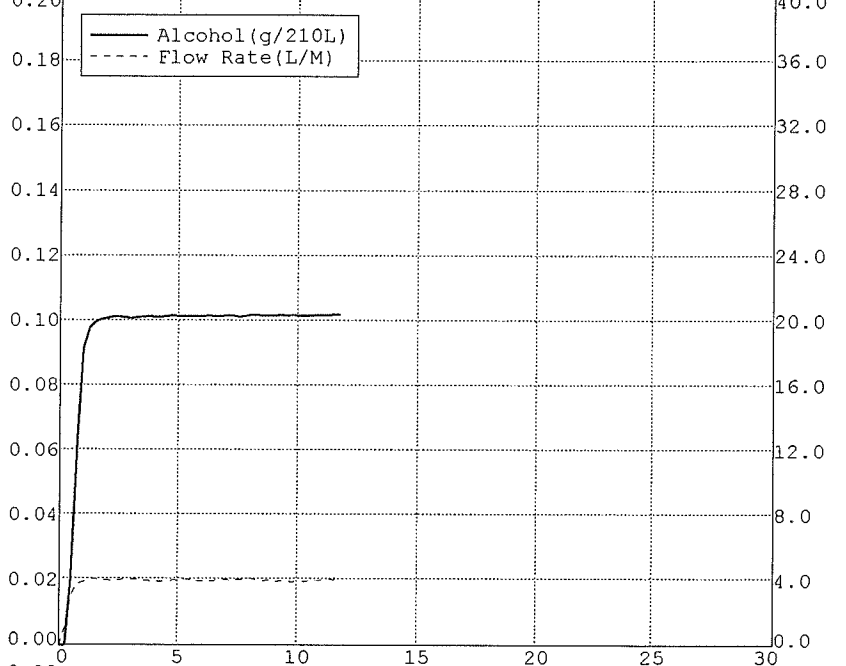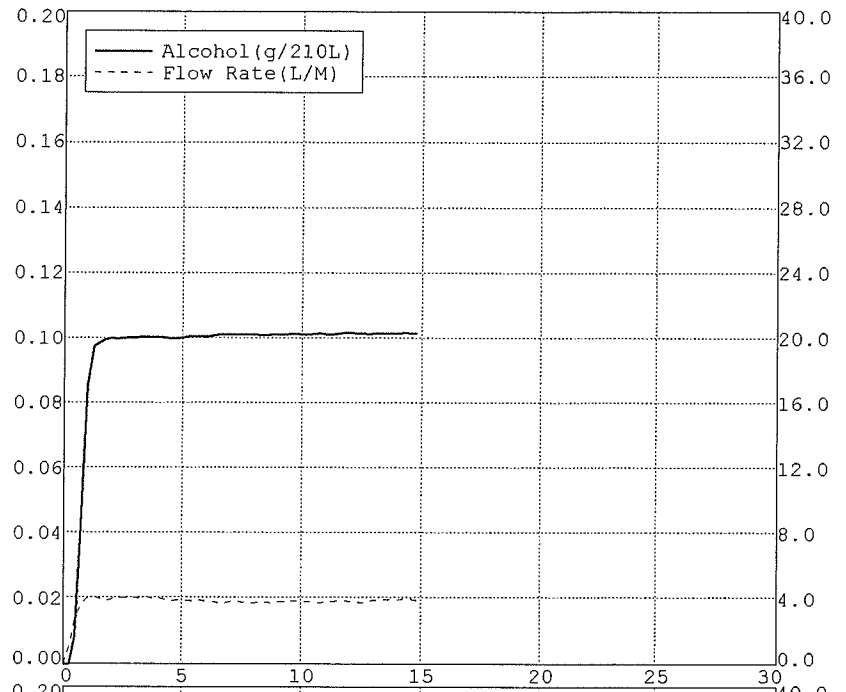

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/23/2022

OPERATOR NAME:  
IAN O GGORDON  
Permit #: 50784  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:22
INTERNAL STANDARD	VERIFIED	00:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:23
BLANK TEST	0.00	00:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:24
BLANK TEST	0.00	00:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:25
BLANK TEST	0.00	00:26

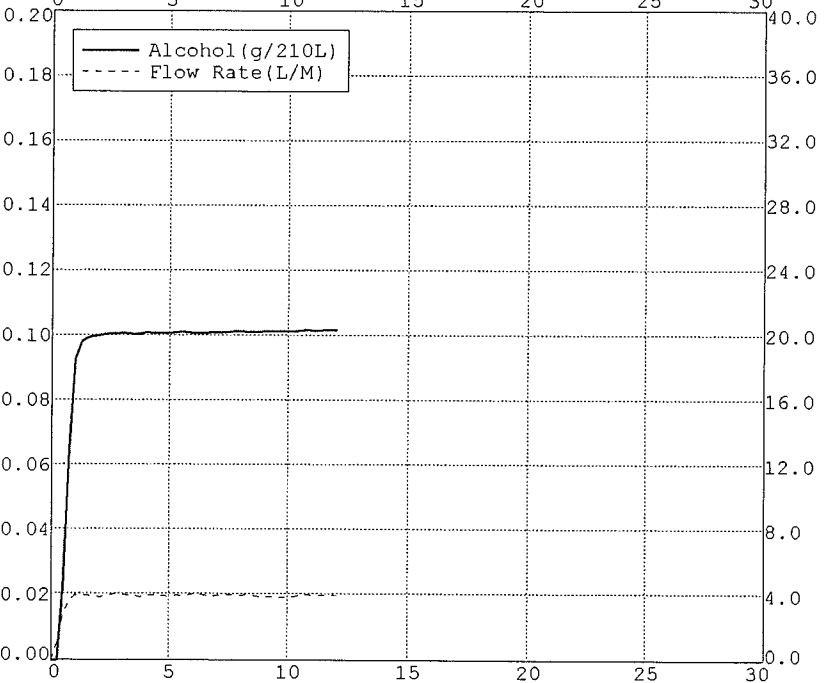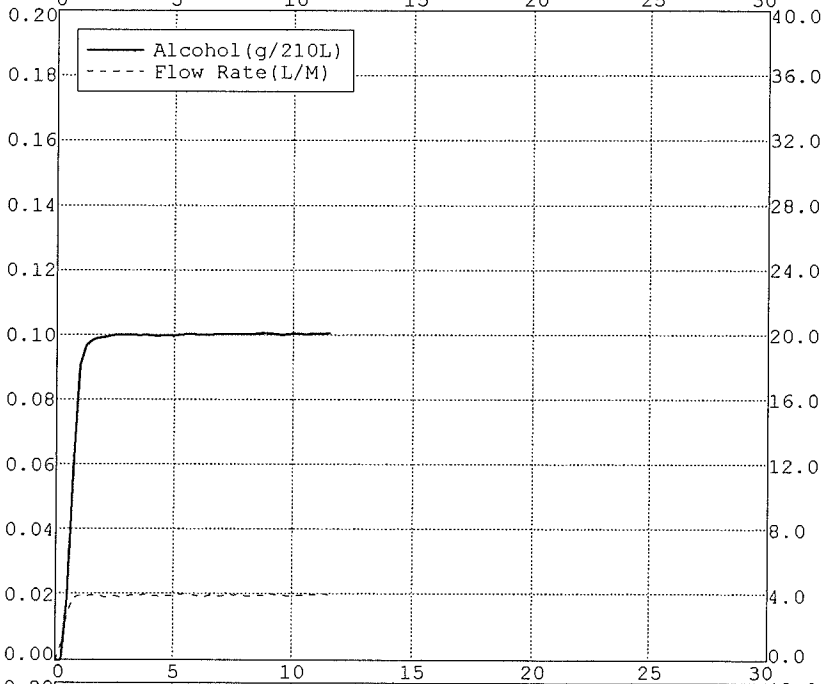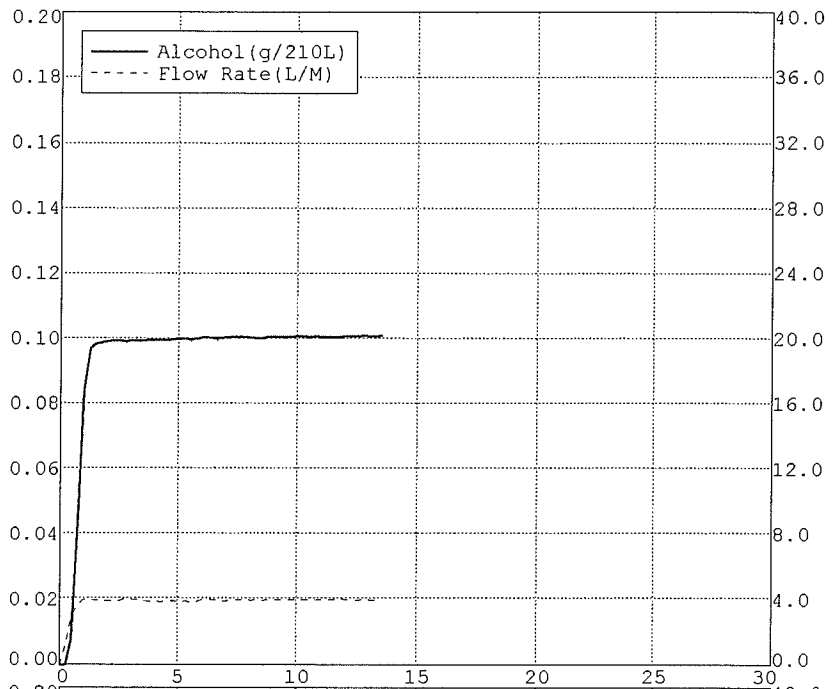




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/28/2022

OPERATOR NAME:  
IAN O GORDON  
Permit #: 50784  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:21
INTERNAL STANDARD	VERIFIED	18:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:22
BLANK TEST	0.00	18:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:23
BLANK TEST	0.00	18:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:24
BLANK TEST	0.00	18:25

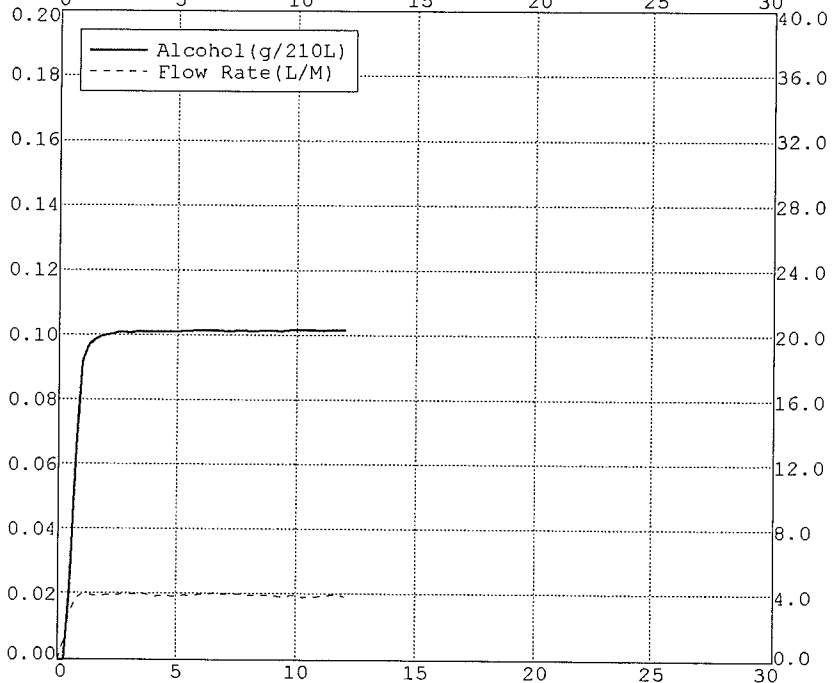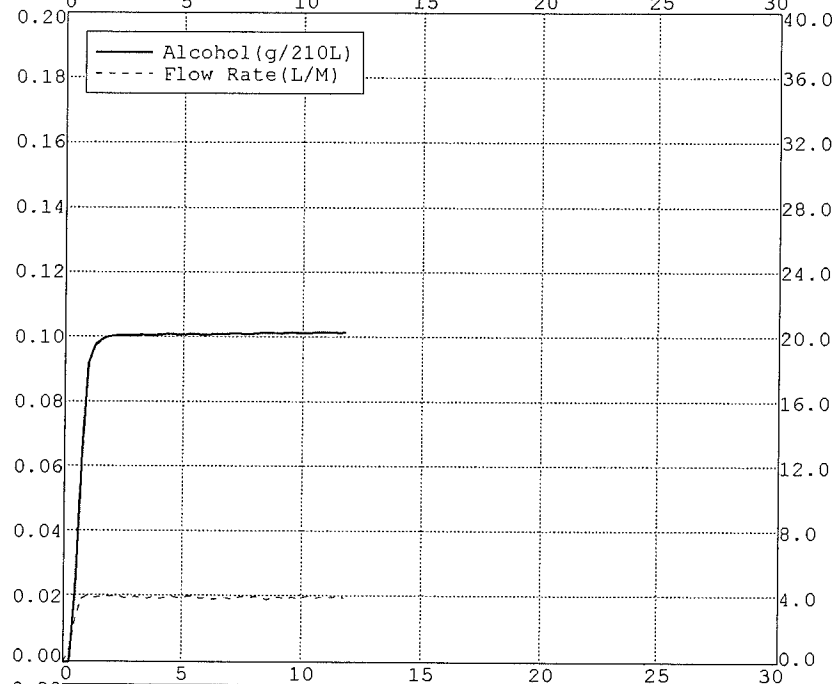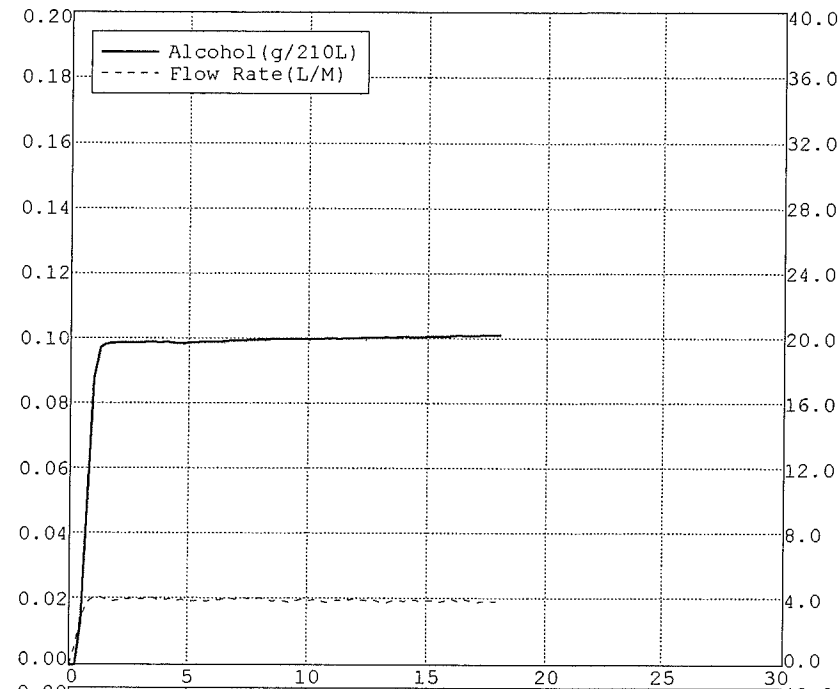

SUPERVISOR TEST

LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/28/2022

OPERATOR NAME:  
IAN O GORDON  
Permit #: 50784  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:40
INTERNAL STANDARD	VERIFIED	18:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:41
BLANK TEST	0.00	18:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:42
BLANK TEST	0.00	18:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:43
BLANK TEST	0.00	18:44

