

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/03/2020

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:41
INTERNAL STANDARD	VERIFIED	06:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:41
BLANK TEST	0.00	06:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:42
BLANK TEST	0.00	06:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:44
BLANK TEST	0.00	06:44

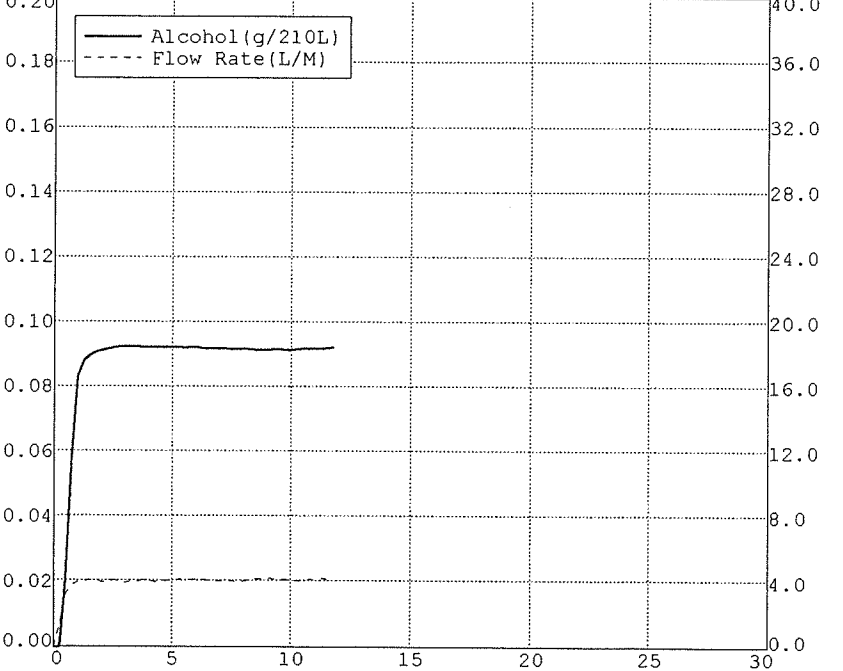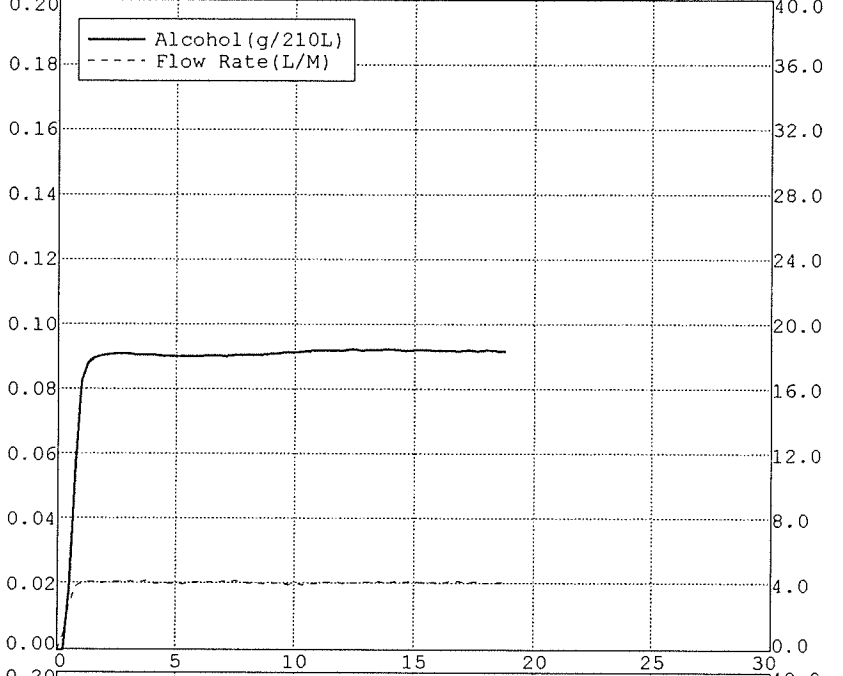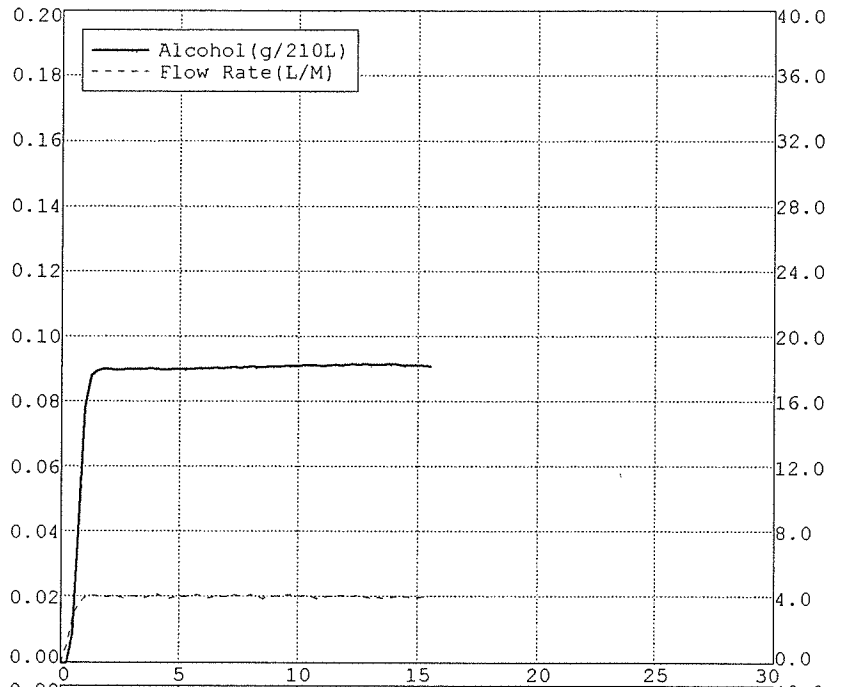

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/09/2020

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:53
INTERNAL STANDARD	VERIFIED	05:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:53
BLANK TEST	0.00	05:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:54
BLANK TEST	0.00	05:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:55
BLANK TEST	0.00	05:56

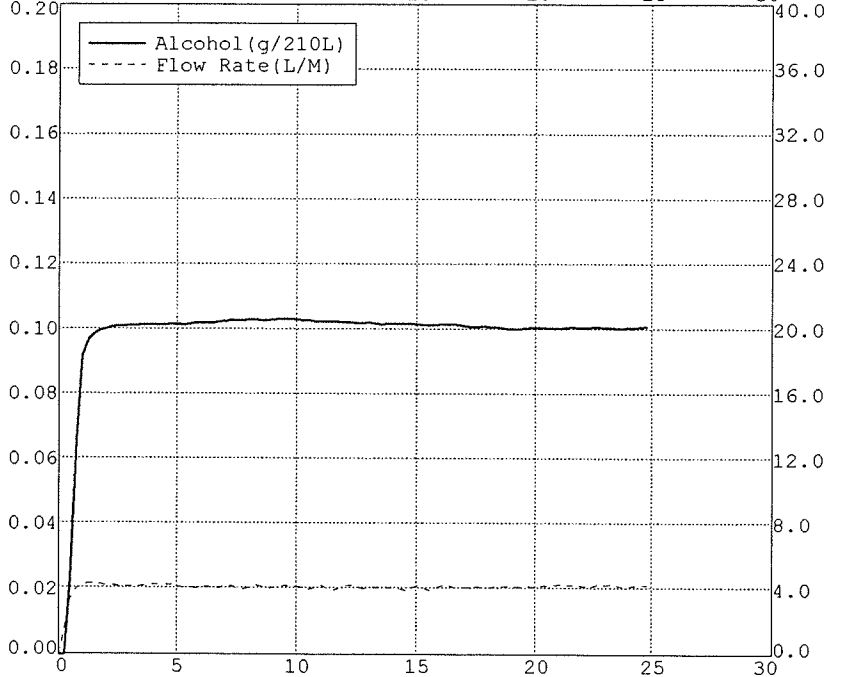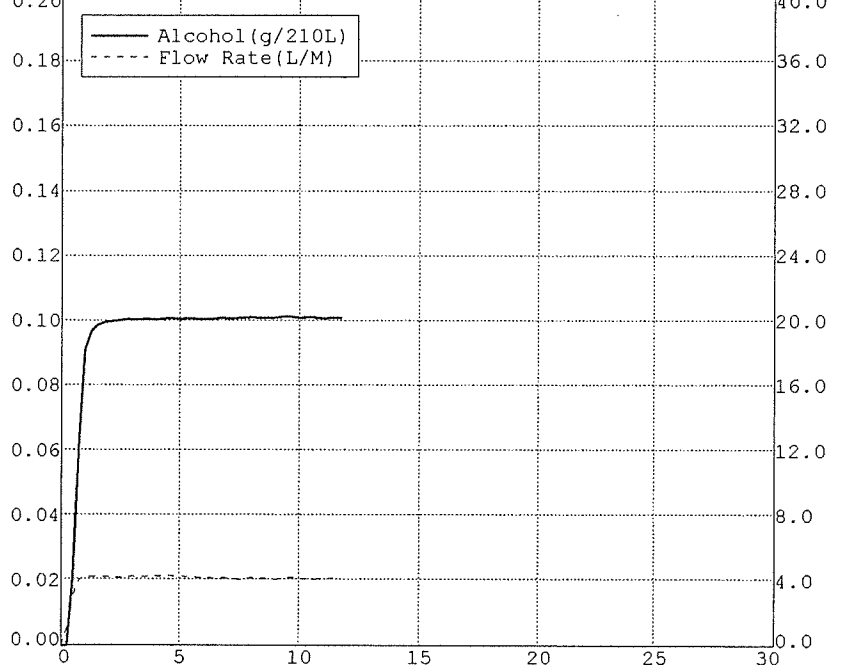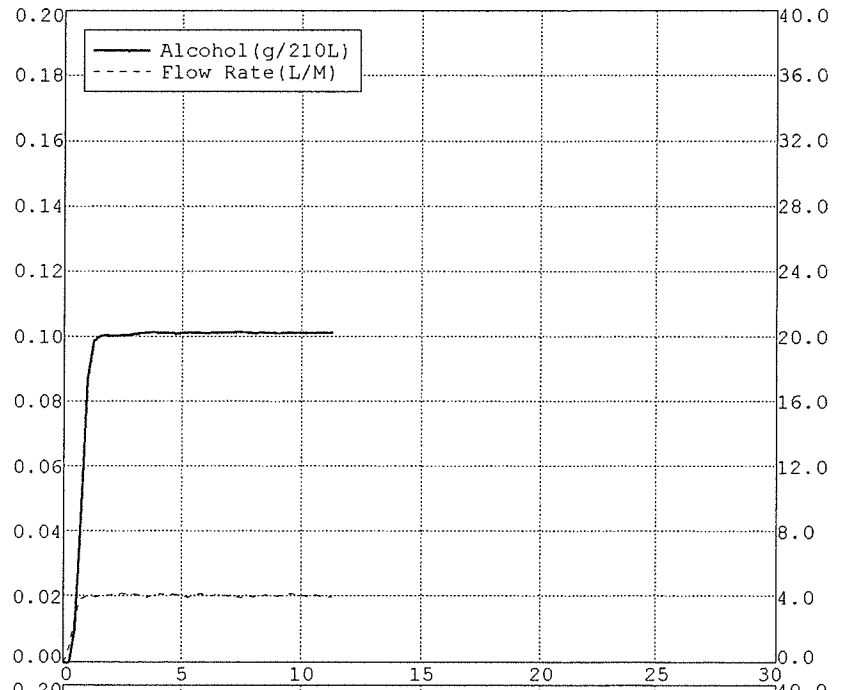

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/15/2020

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:03
INTERNAL STANDARD	VERIFIED	10:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:04
BLANK TEST	0.00	10:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:05
BLANK TEST	0.00	10:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:06
BLANK TEST	0.00	10:07

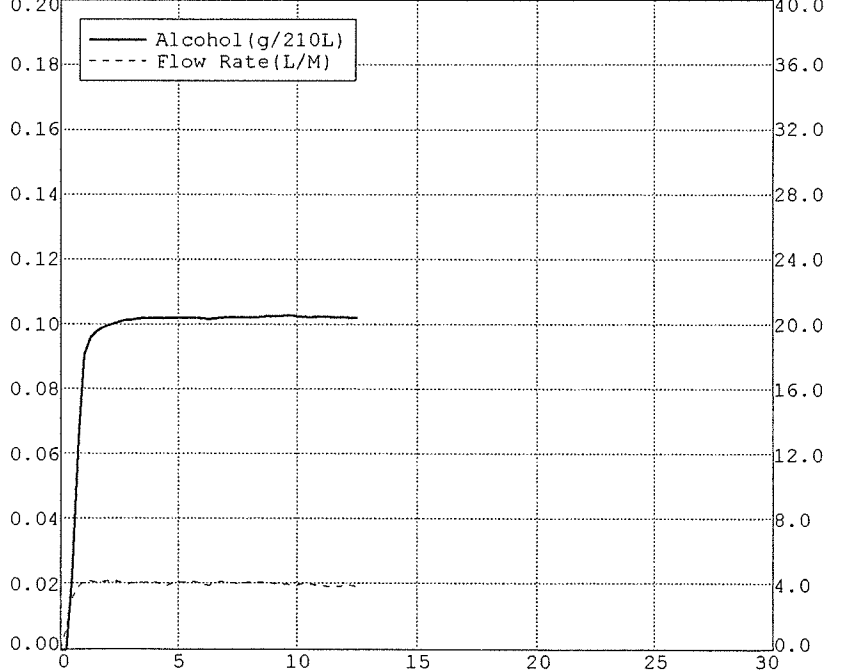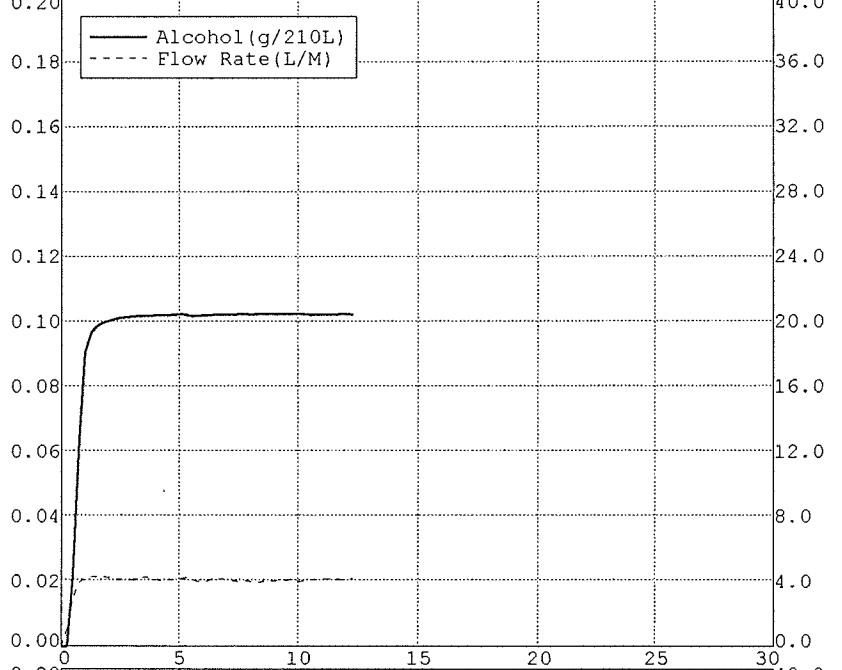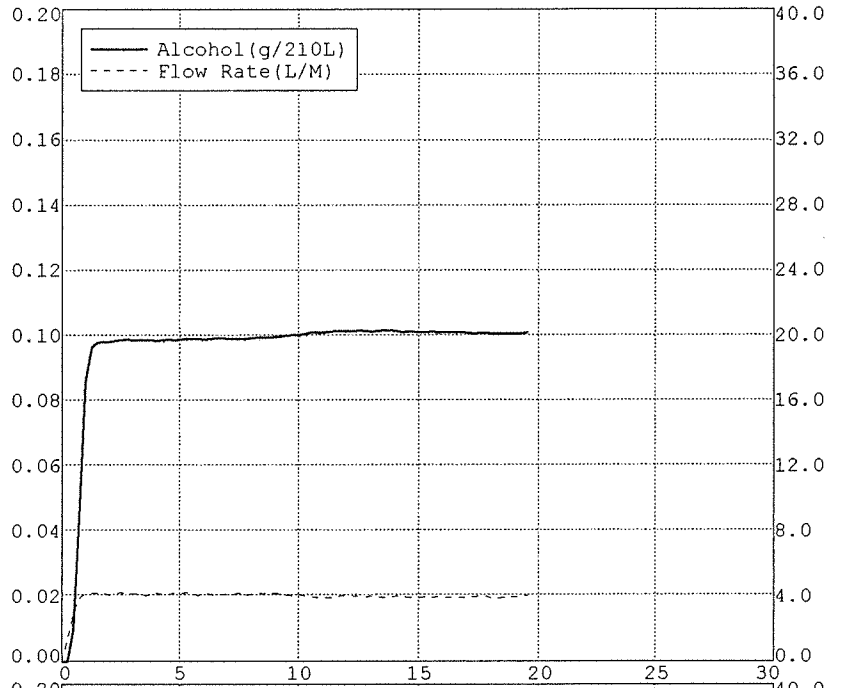

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/23/2020

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:59
INTERNAL STANDARD	VERIFIED	17:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:59
BLANK TEST	0.00	18:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:01
BLANK TEST	0.00	18:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:02
BLANK TEST	0.00	18:02

