

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/05/2022

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:00
INTERNAL STANDARD	VERIFIED	18:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:01
BLANK TEST	0.00	18:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:02
BLANK TEST	0.00	18:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:03
BLANK TEST	0.00	18:04

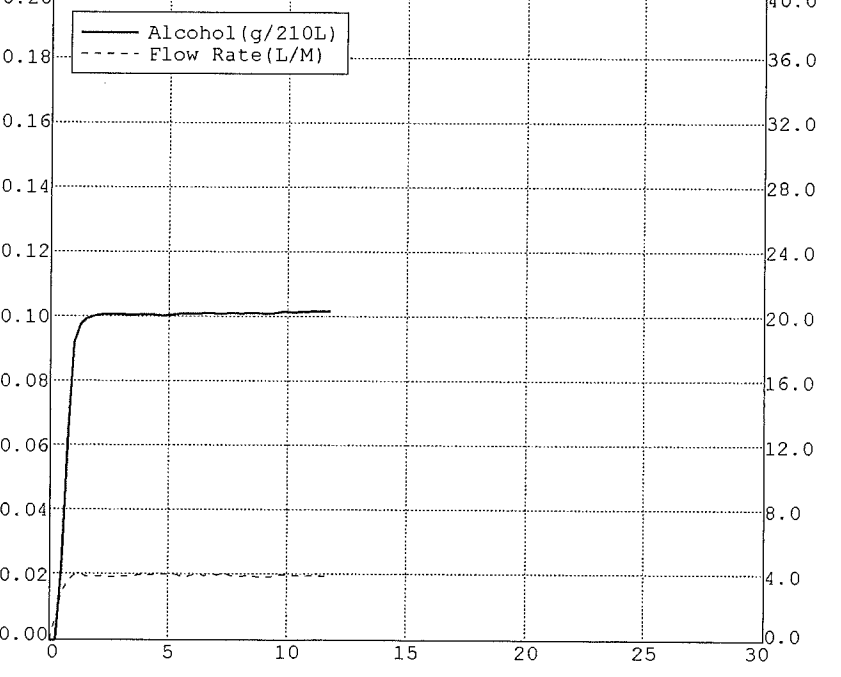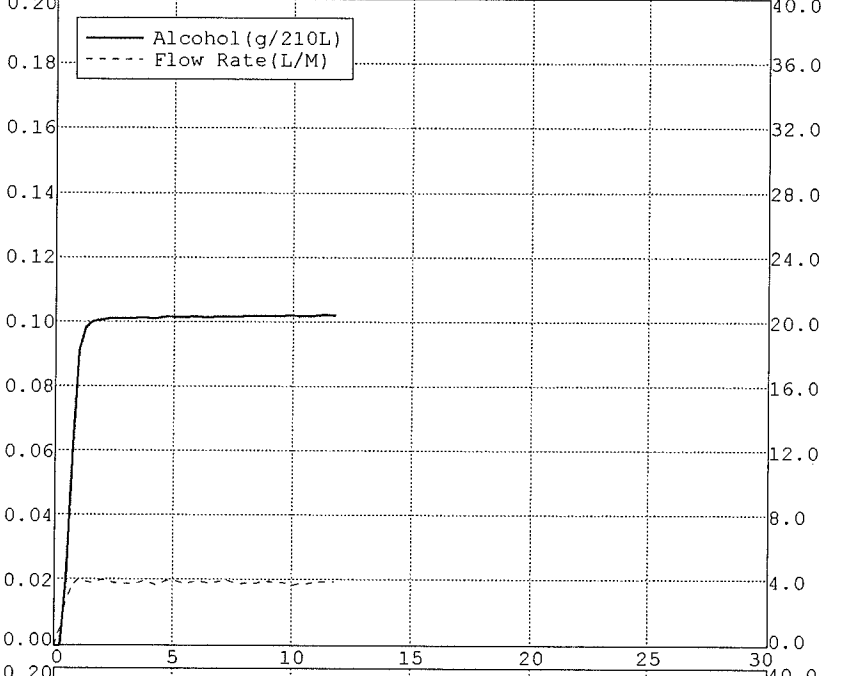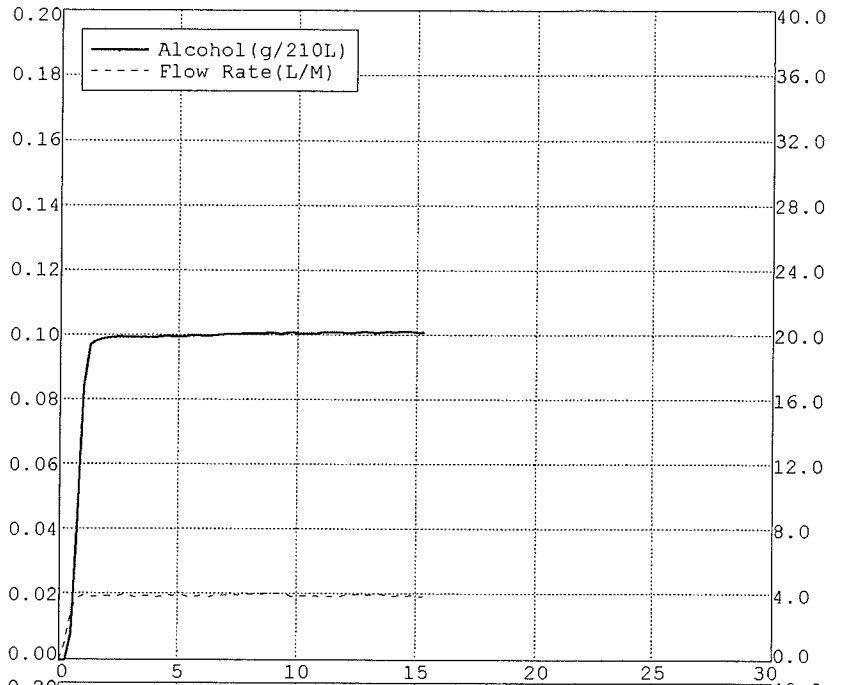

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/11/2022

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:07
INTERNAL STANDARD	VERIFIED	21:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:07
BLANK TEST	0.00	21:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:08
BLANK TEST	0.00	21:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:10
BLANK TEST	0.00	21:10

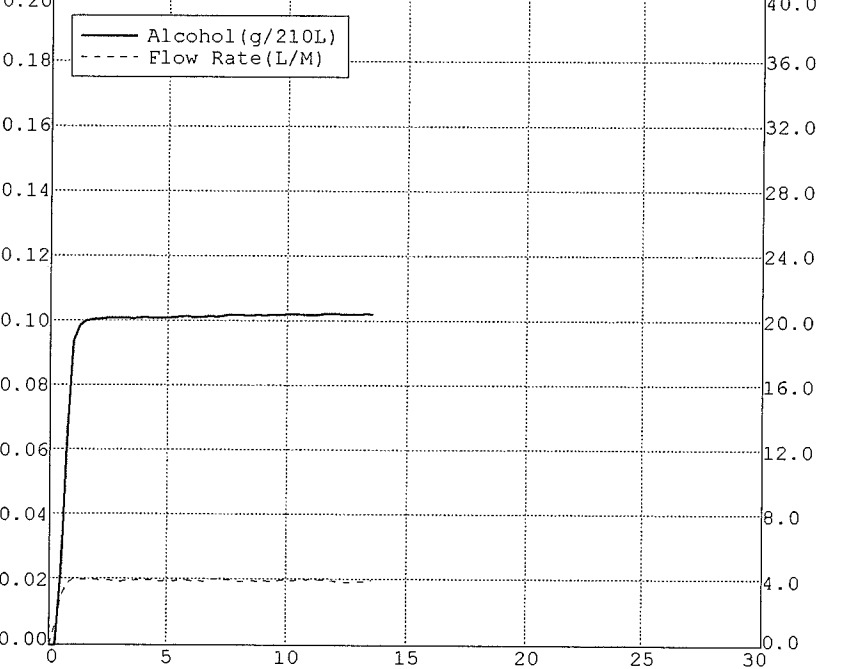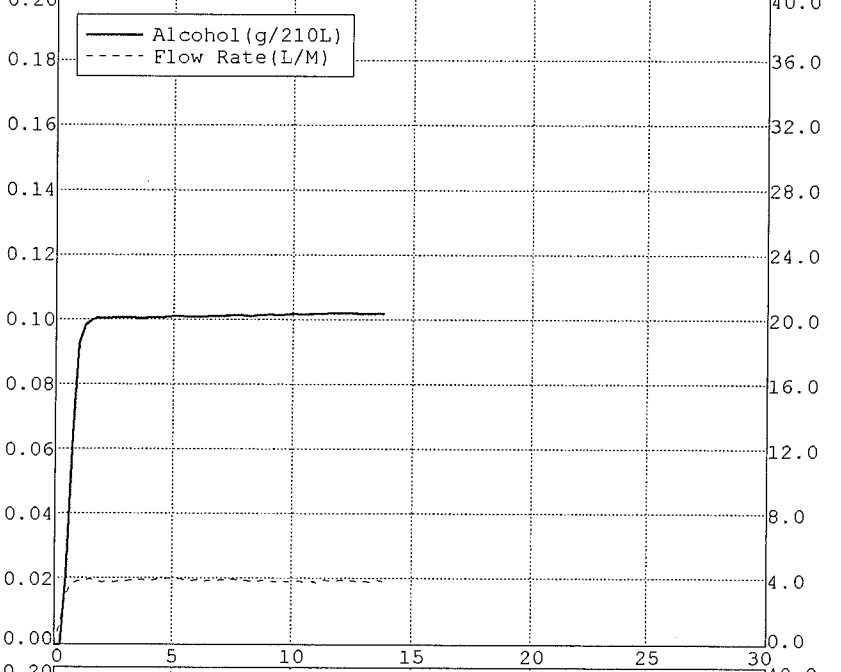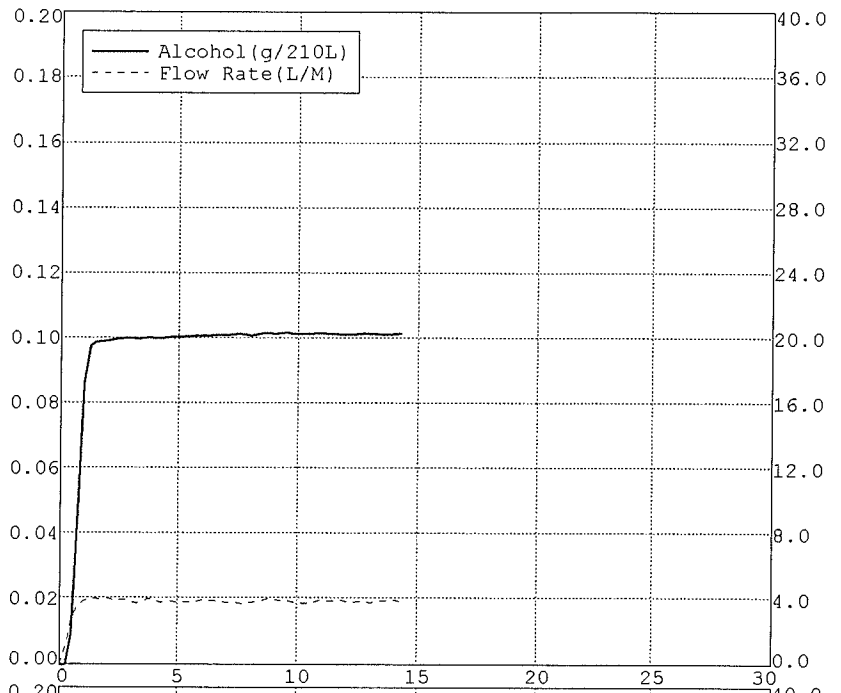

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/19/2022

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:09
INTERNAL STANDARD	VERIFIED	18:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:10
BLANK TEST	0.00	18:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:11
BLANK TEST	0.00	18:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:12
BLANK TEST	0.00	18:13

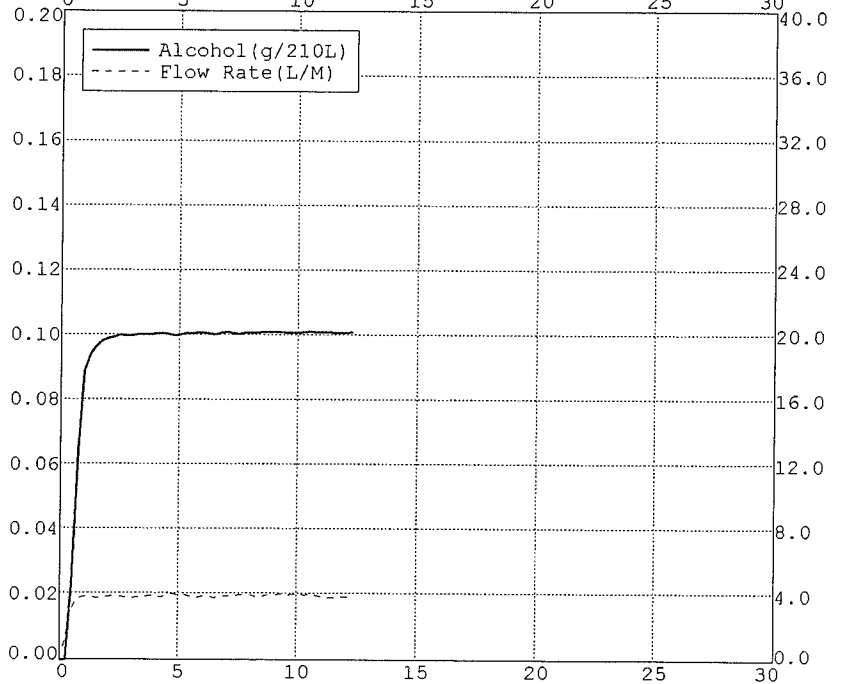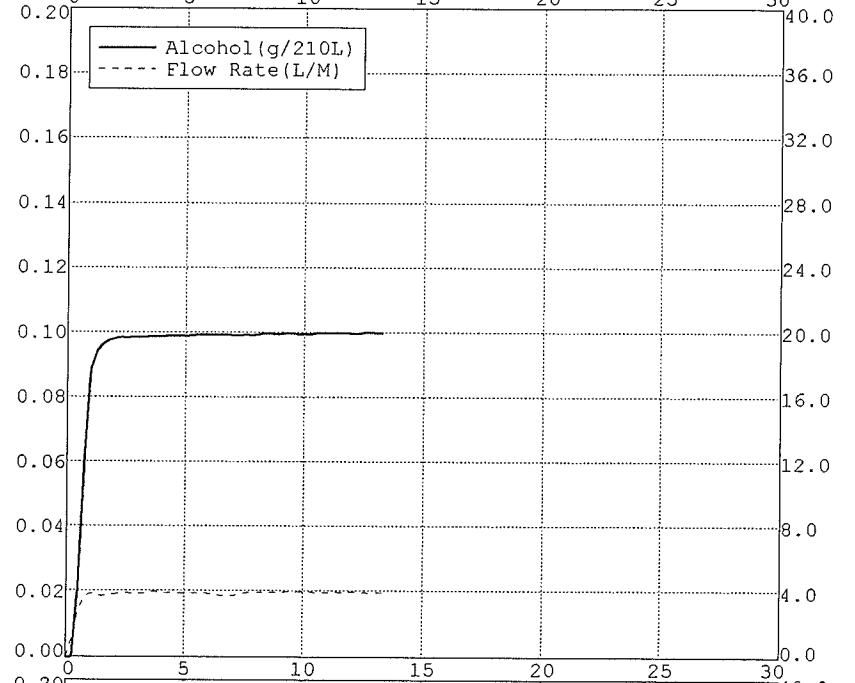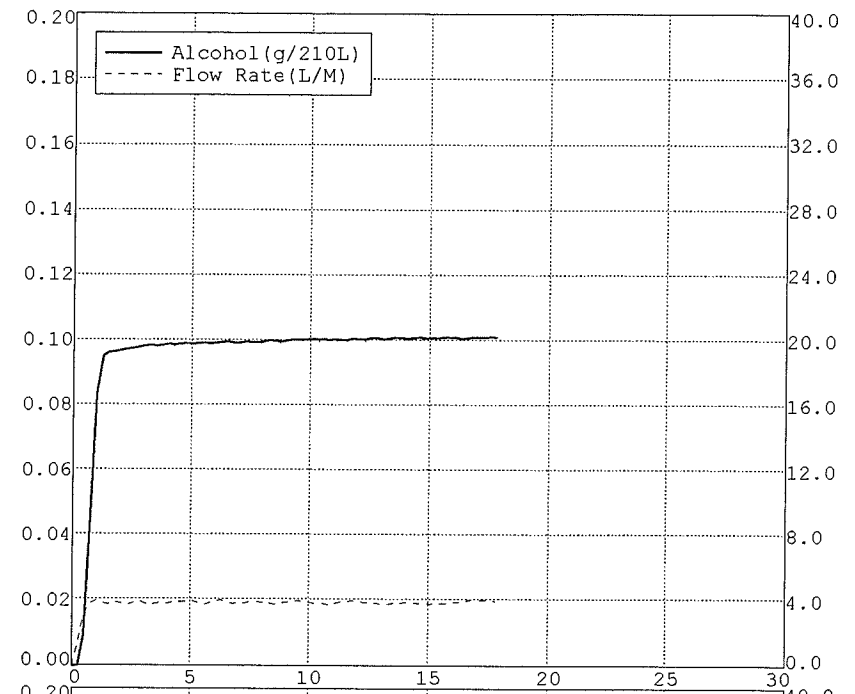

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/22/2022

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:27
INTERNAL STANDARD	VERIFIED	16:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:27
BLANK TEST	0.00	16:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:28
BLANK TEST	0.00	16:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:29
BLANK TEST	0.00	16:30

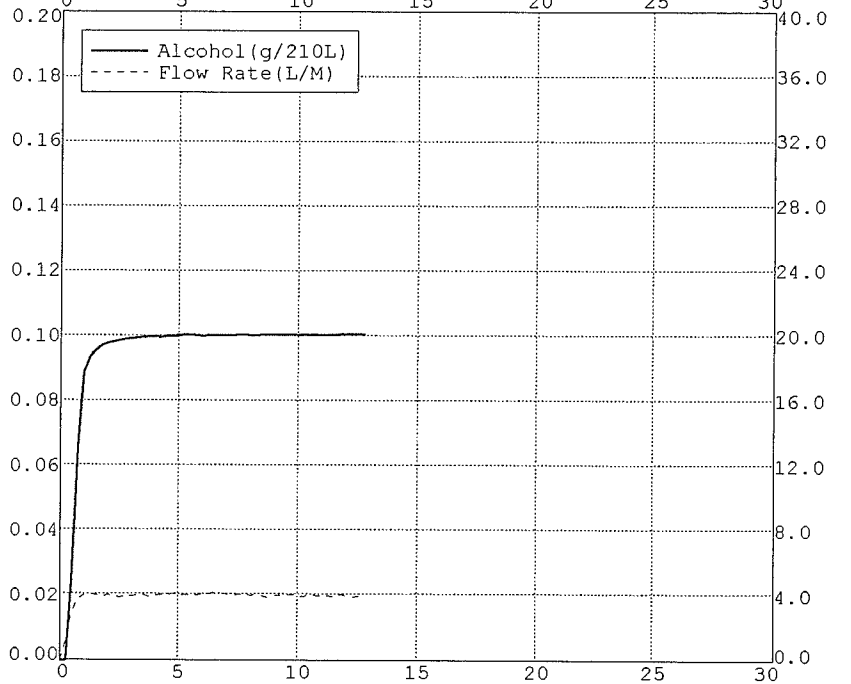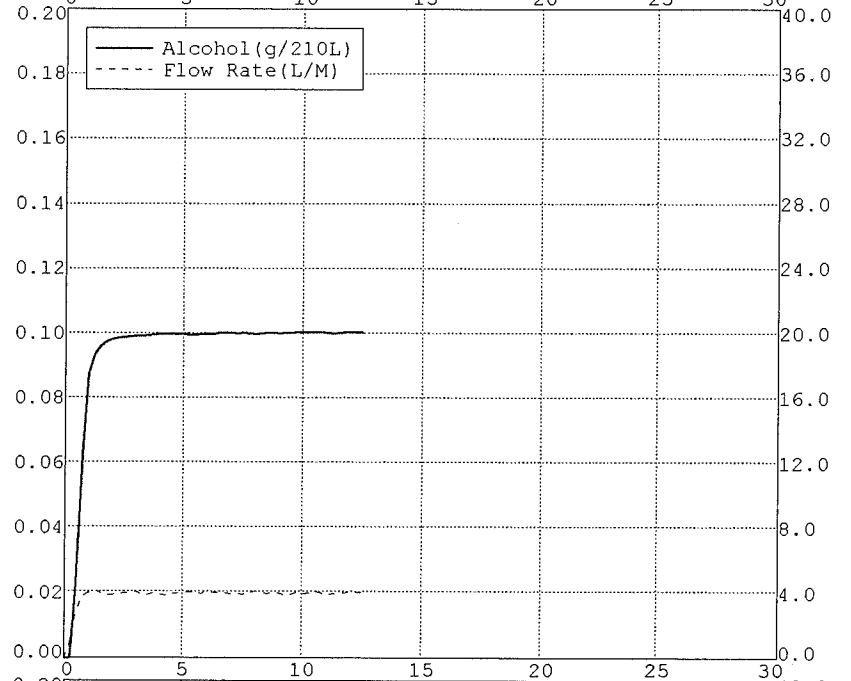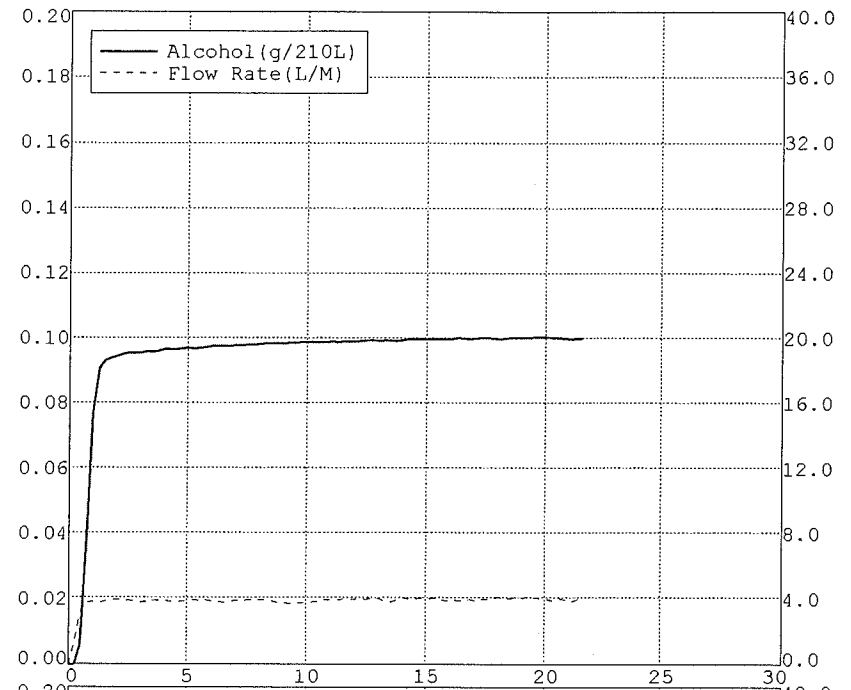

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/25/2022

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:42
INTERNAL STANDARD	VERIFIED	18:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:43
BLANK TEST	0.00	18:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:44
BLANK TEST	0.00	18:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:45
BLANK TEST	0.00	18:46

