

SOLUTION CHANGE




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 02/01/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:38
INTERNAL STANDARD	VERIFIED	15:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:39
BLANK TEST	0.00	15:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:40
BLANK TEST	0.00	15:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:41
BLANK TEST	0.00	15:42

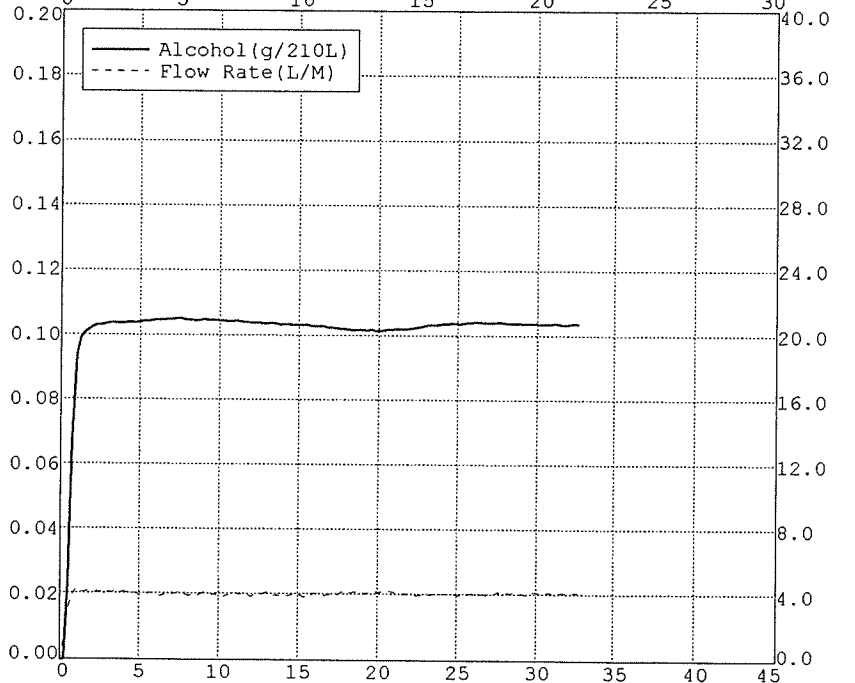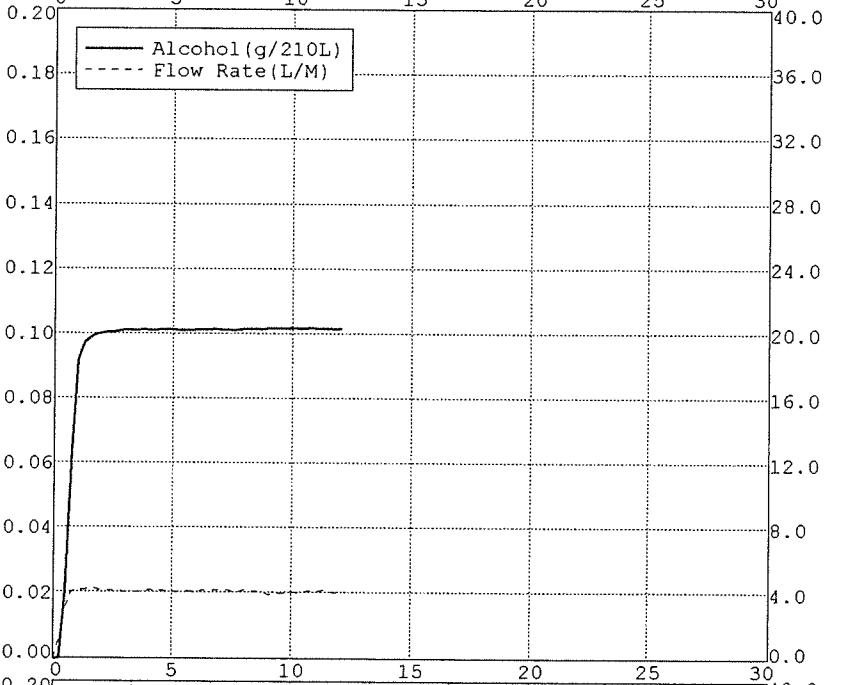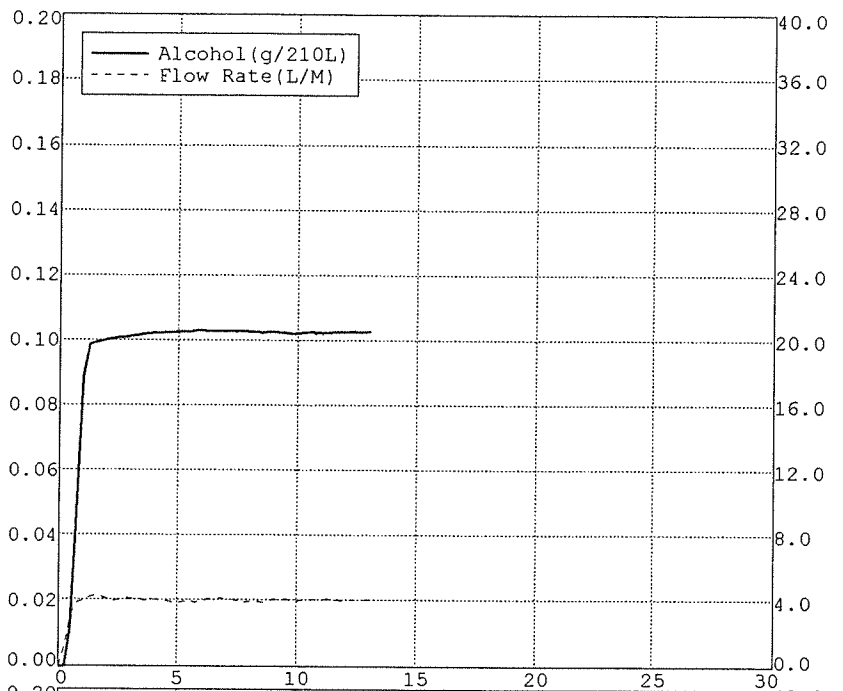

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 02/07/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:26
INTERNAL STANDARD	VERIFIED	12:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:26
BLANK TEST	0.00	12:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:27
BLANK TEST	0.00	12:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:28
BLANK TEST	0.00	12:29

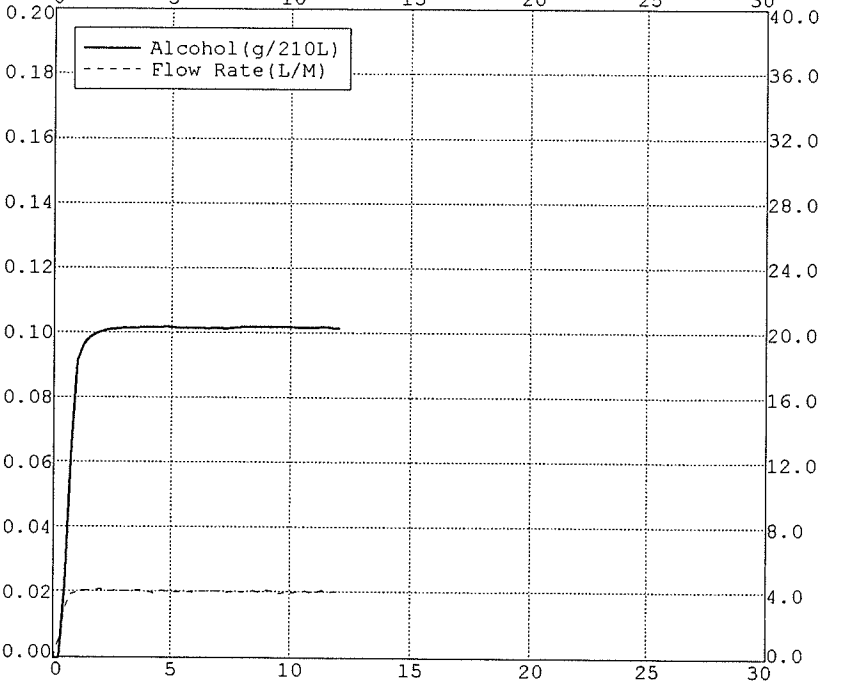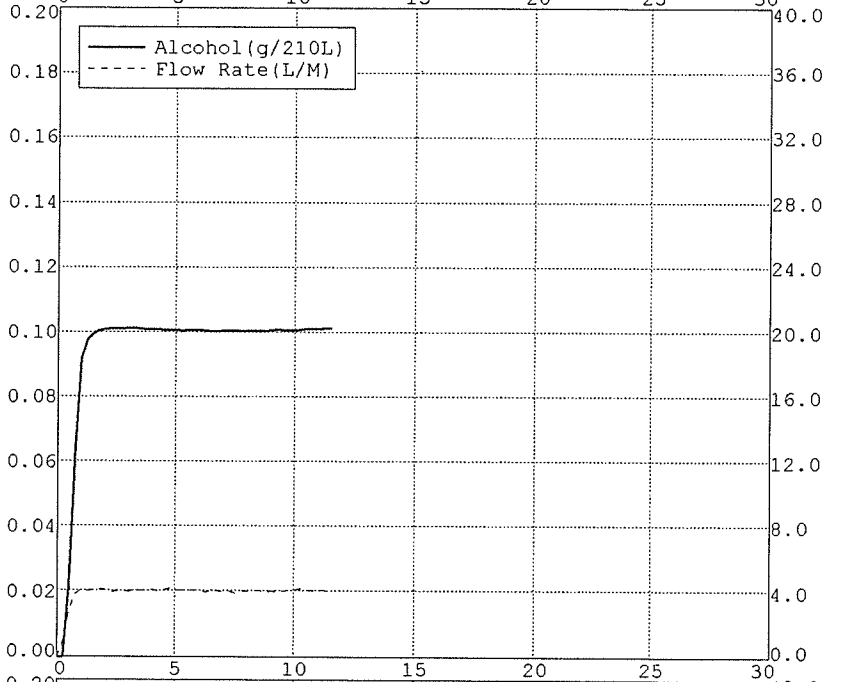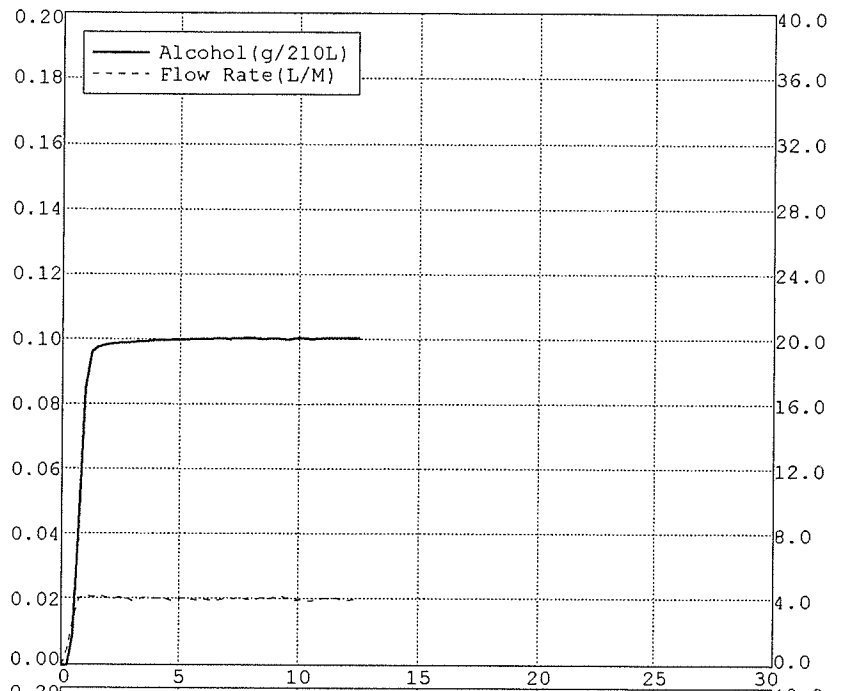

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 02/20/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:51
INTERNAL STANDARD	VERIFIED	09:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:52
BLANK TEST	0.00	09:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:53
BLANK TEST	0.00	09:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:54
BLANK TEST	0.00	09:55

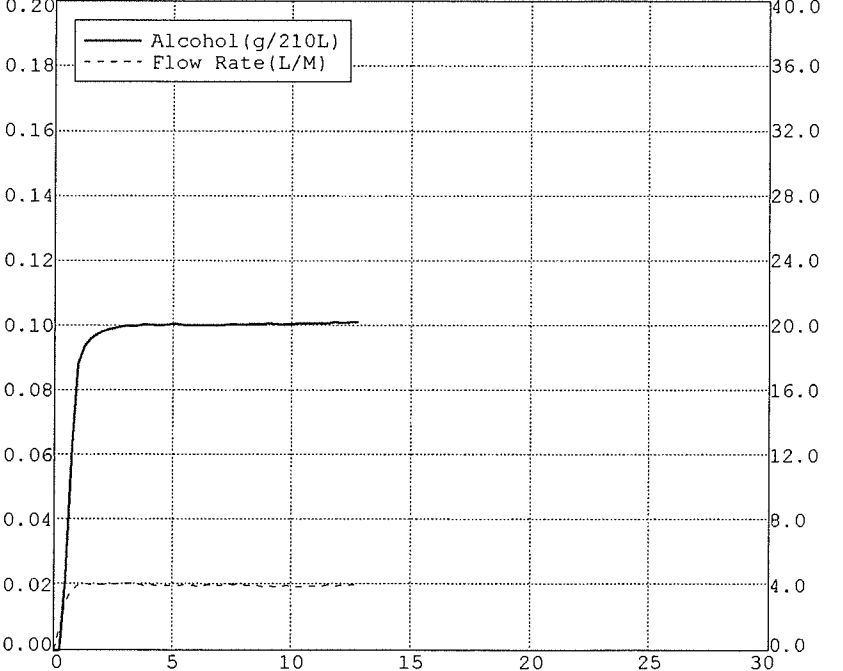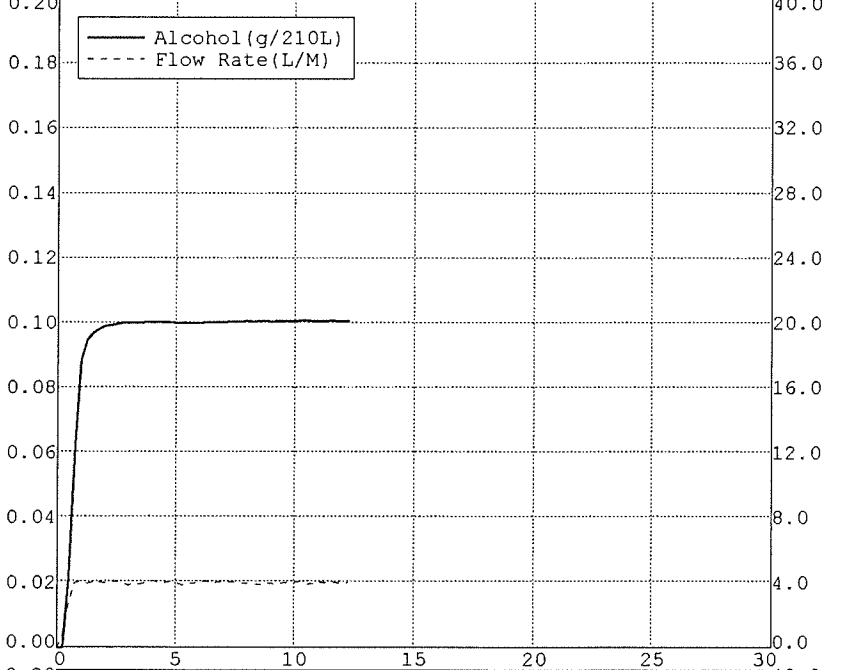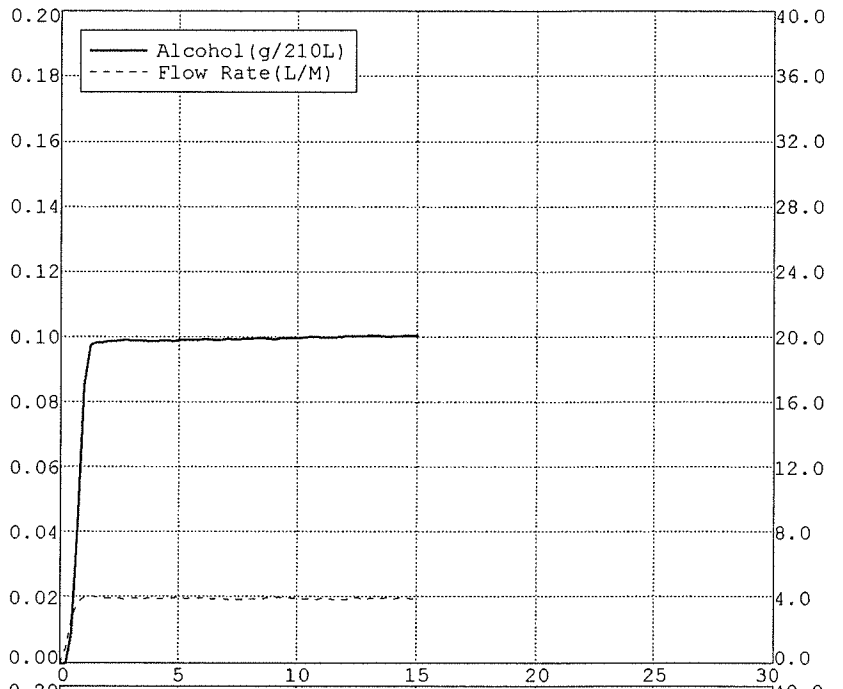

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 02/21/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:26
INTERNAL STANDARD	VERIFIED	12:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:26
BLANK TEST	0.00	12:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:28
BLANK TEST	0.00	12:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:29
BLANK TEST	0.00	12:29

