

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/01/2024

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:30
INTERNAL STANDARD	VERIFIED	05:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:31
BLANK TEST	0.00	05:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:32
BLANK TEST	0.00	05:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:33
BLANK TEST	0.00	05:34



SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/08/2024

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:56
INTERNAL STANDARD	VERIFIED	11:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:57
BLANK TEST	0.00	11:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:58
BLANK TEST	0.00	11:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:59
BLANK TEST	0.00	12:00

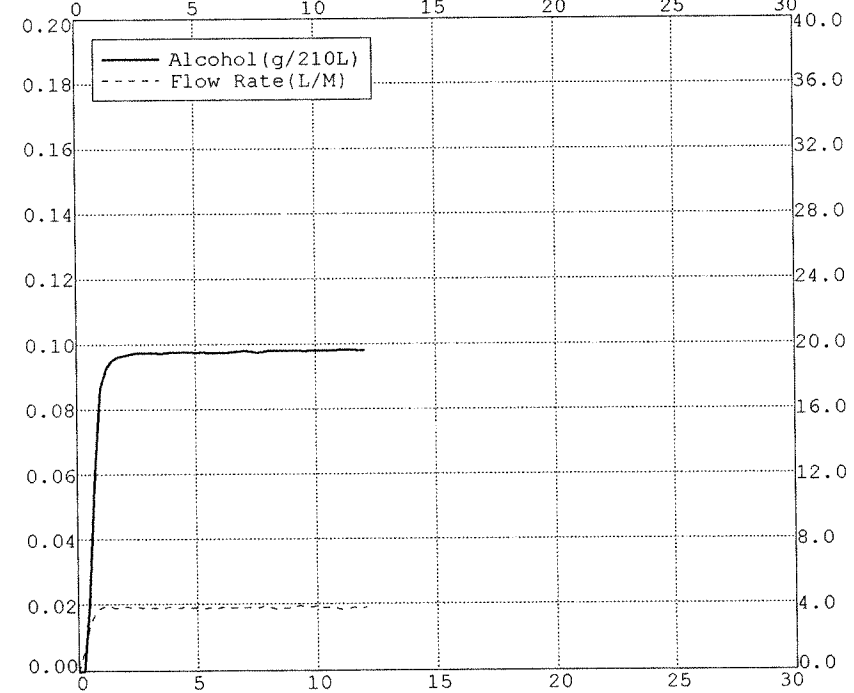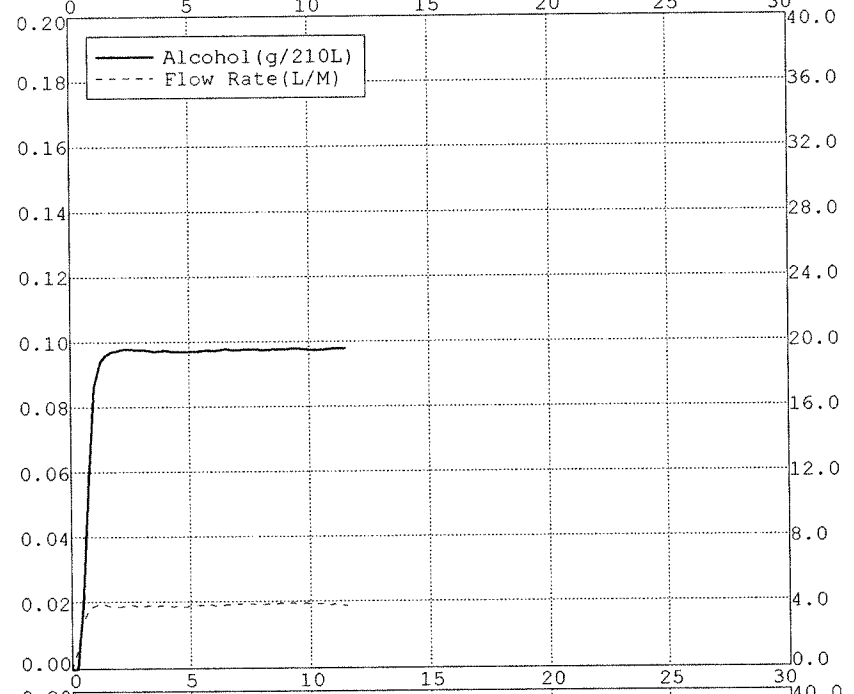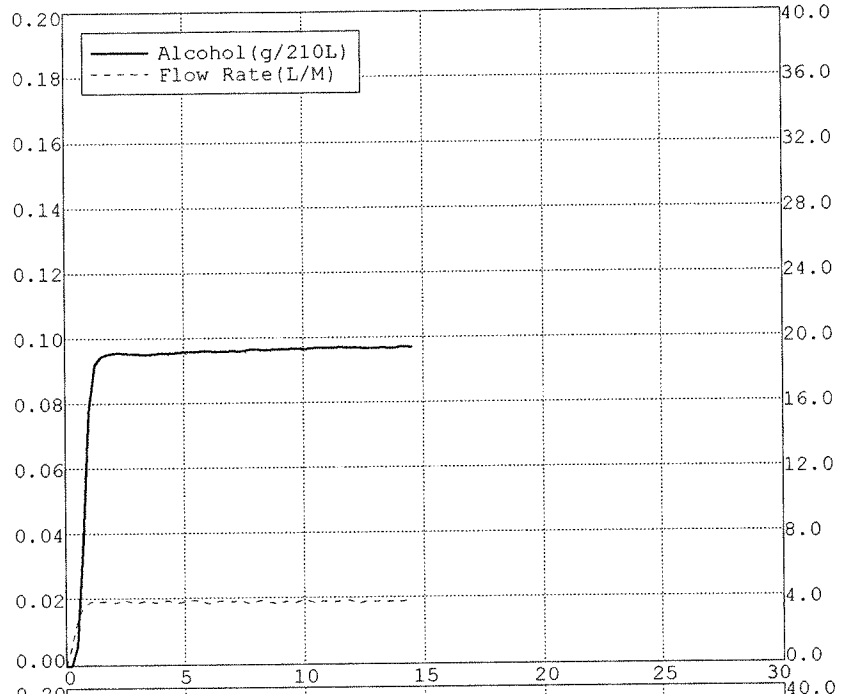

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/15/2024

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:41
INTERNAL STANDARD	VERIFIED	06:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:41
BLANK TEST	0.00	06:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:42
BLANK TEST	0.00	06:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:43
BLANK TEST	0.00	06:44

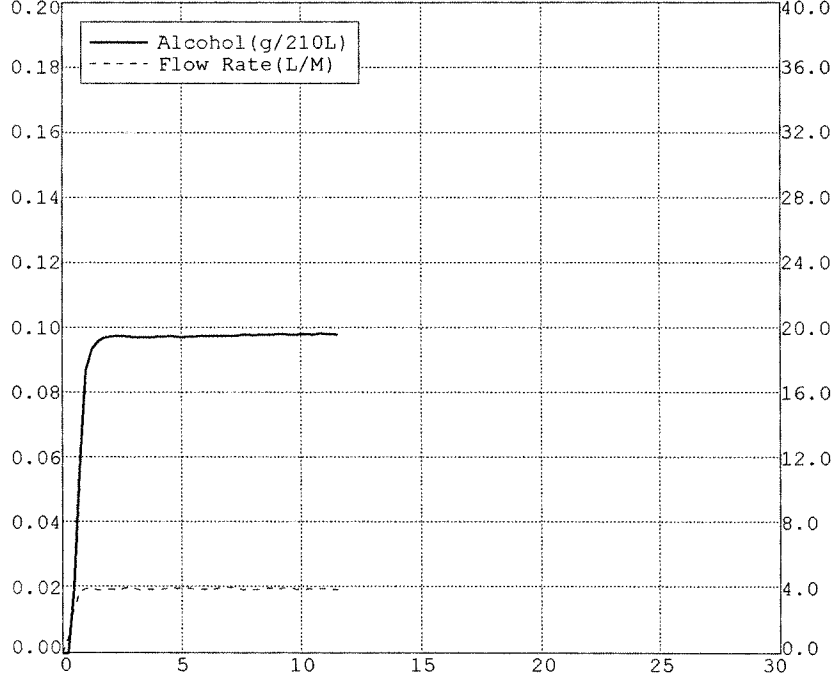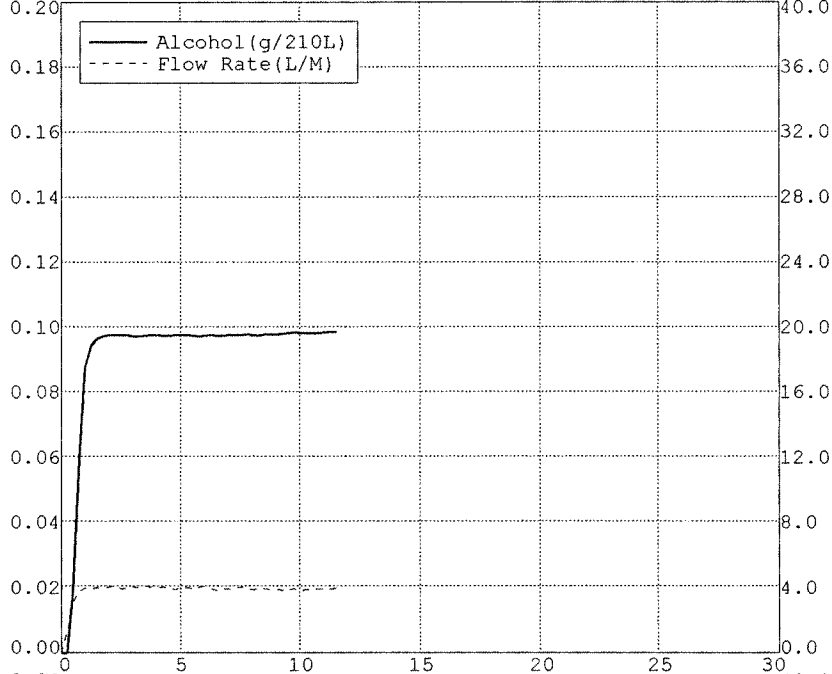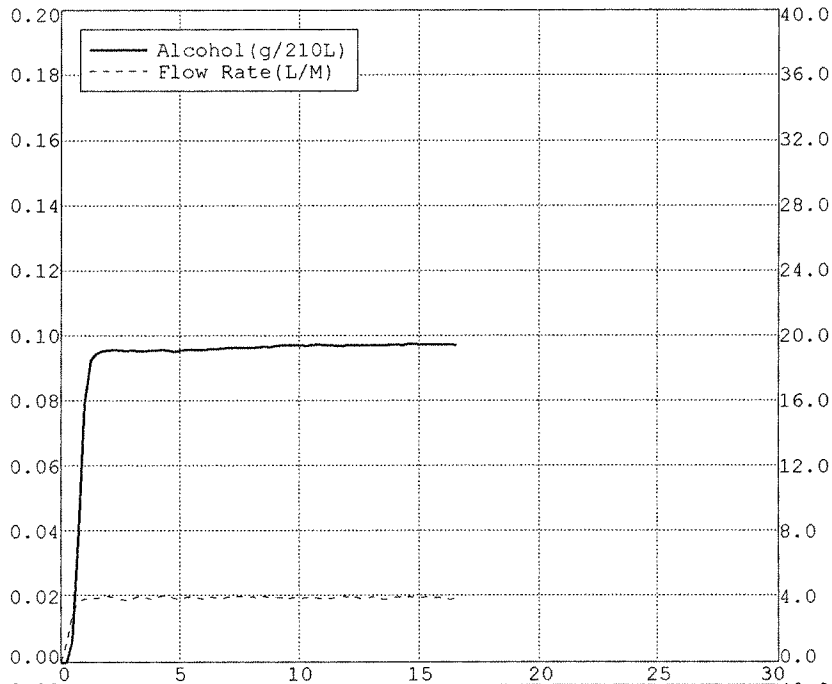

SUPERVISOR TEST


LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/16/2024

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:50
INTERNAL STANDARD	VERIFIED	16:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:50
BLANK TEST	0.00	16:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:51
BLANK TEST	0.00	16:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:53
BLANK TEST	0.00	16:53

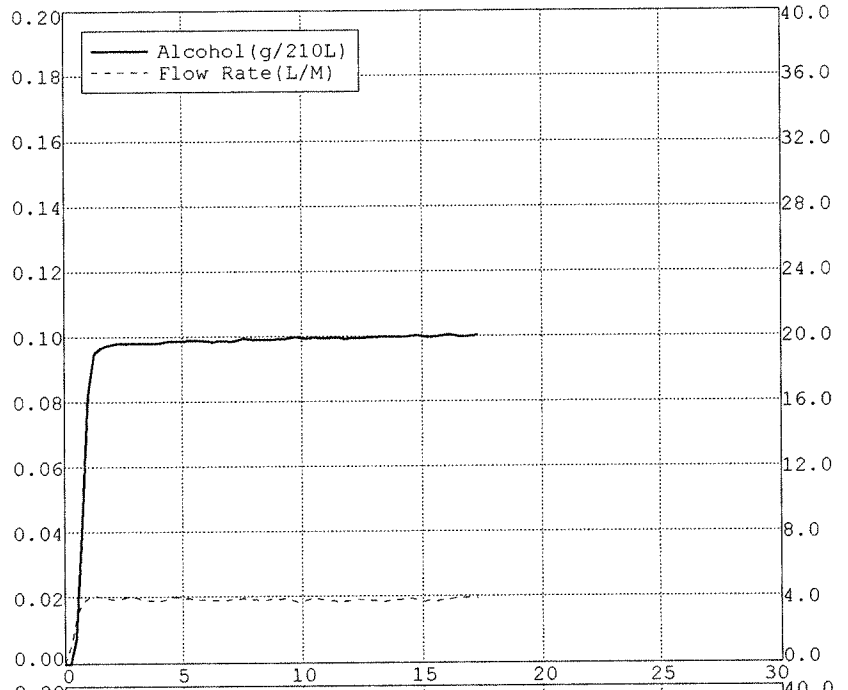

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/22/2024

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24190

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:44
INTERNAL STANDARD	VERIFIED	13:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:44
BLANK TEST	0.00	13:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:46
BLANK TEST	0.00	13:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:47
BLANK TEST	0.00	13:48

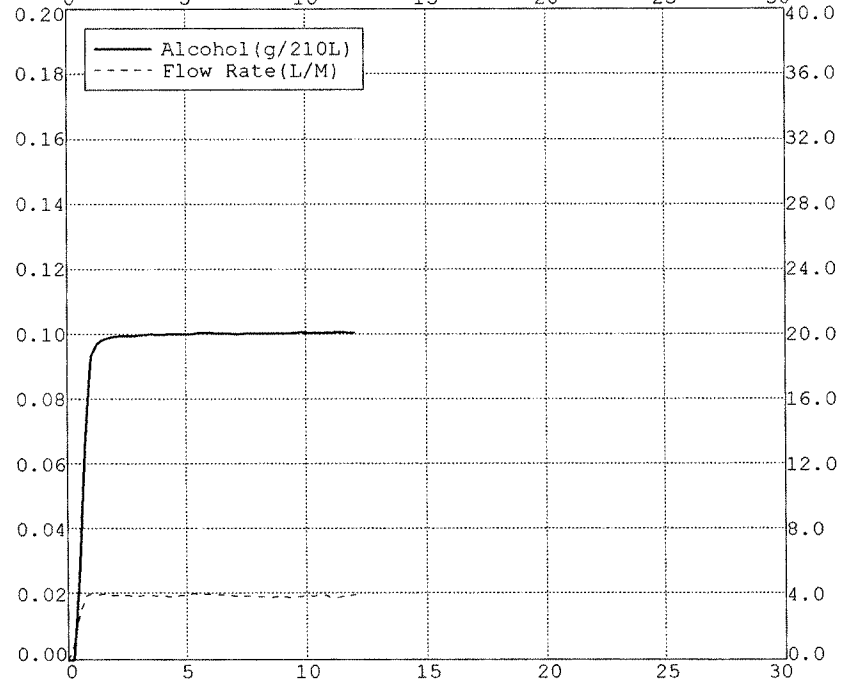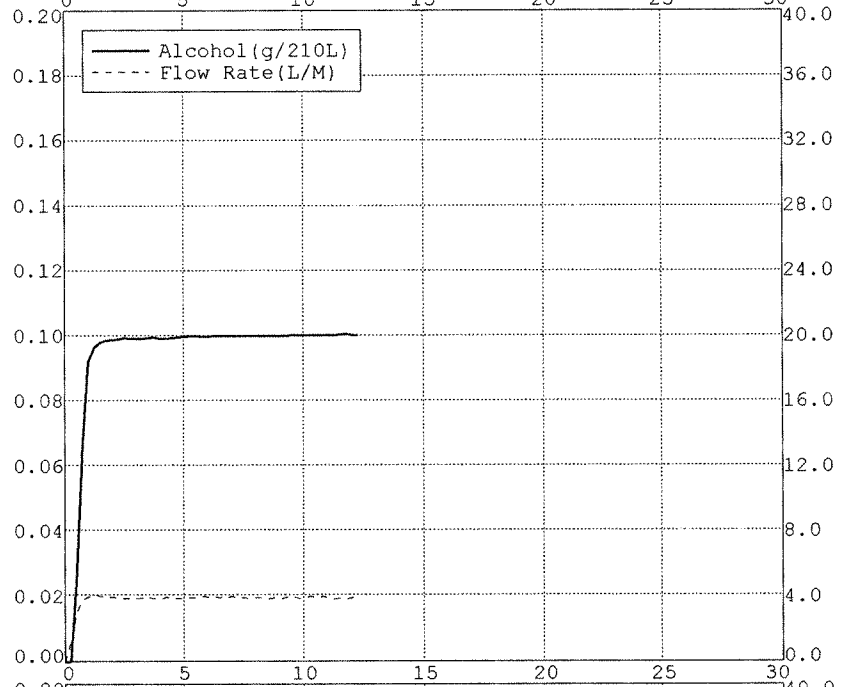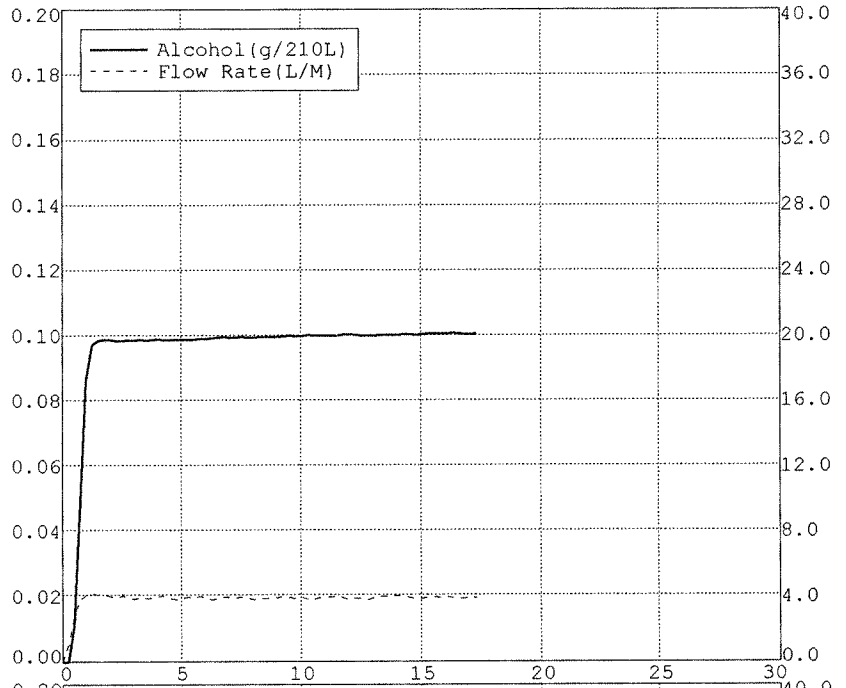

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/29/2024

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24270

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:52
INTERNAL STANDARD	VERIFIED	13:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:53
BLANK TEST	0.00	13:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:54
BLANK TEST	0.00	13:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:55
BLANK TEST	0.00	13:56

