

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290



Date: 01/04/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:06
INTERNAL STANDARD	VERIFIED	09:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:07
BLANK TEST	0.00	09:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	INTERFERENCE	09:08

Interference Detected

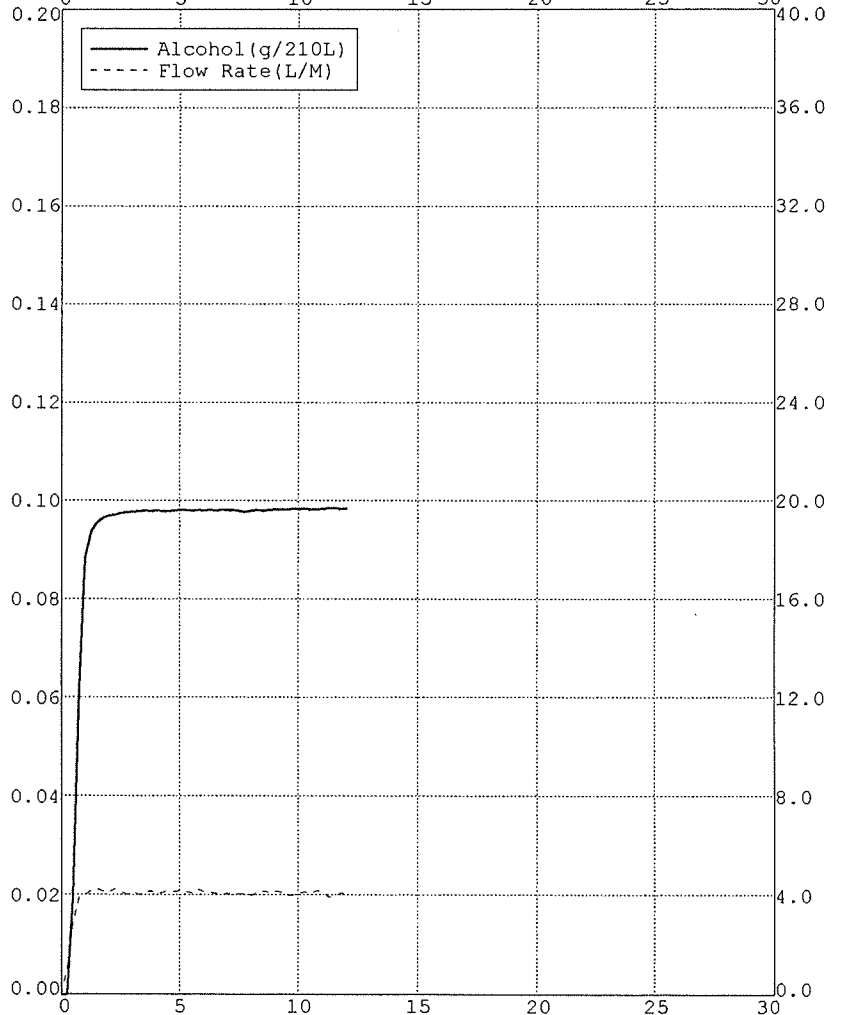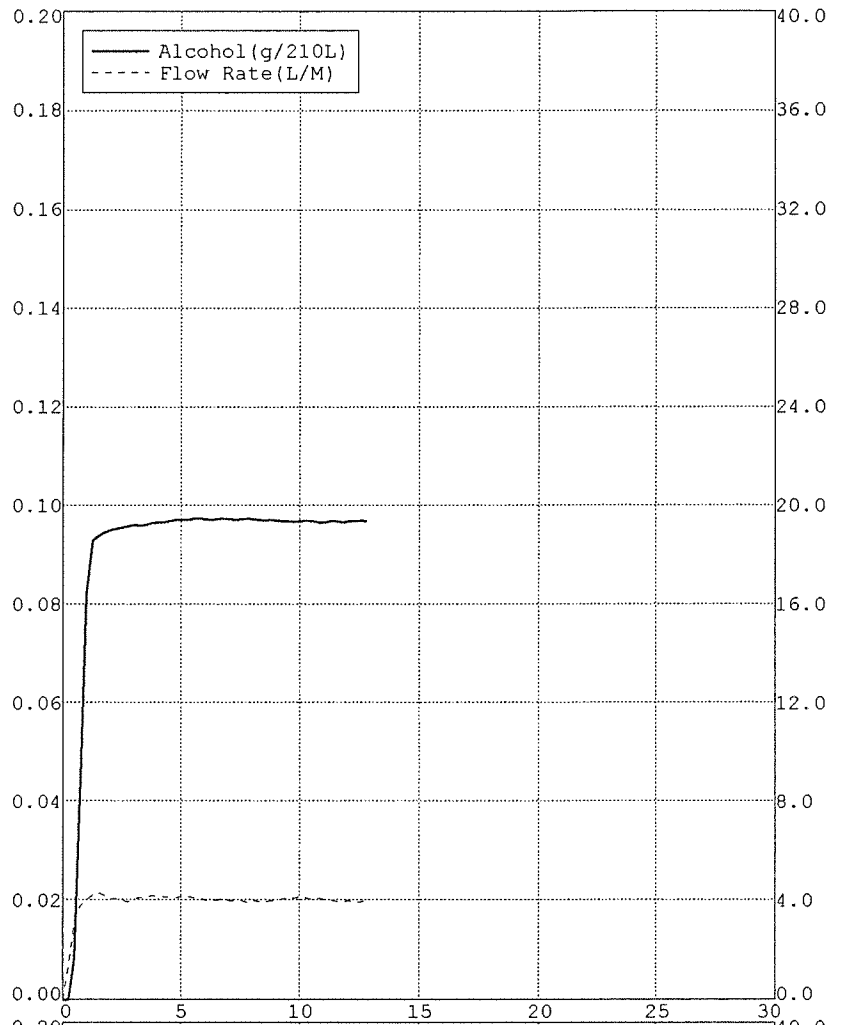

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/04/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:12
INTERNAL STANDARD	VERIFIED	09:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:13
BLANK TEST	0.00	09:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:14
BLANK TEST	0.00	09:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:15
BLANK TEST	0.00	09:16

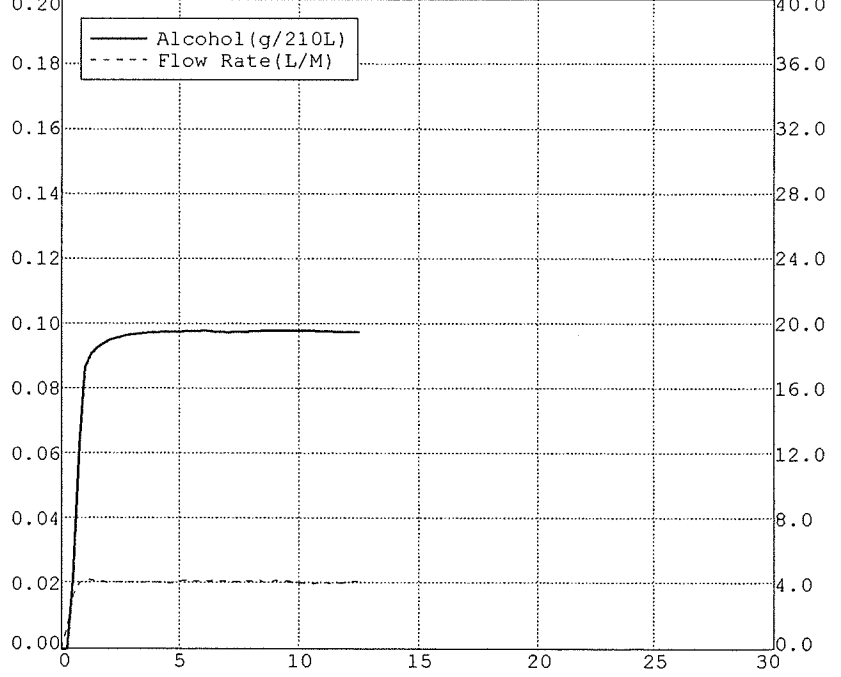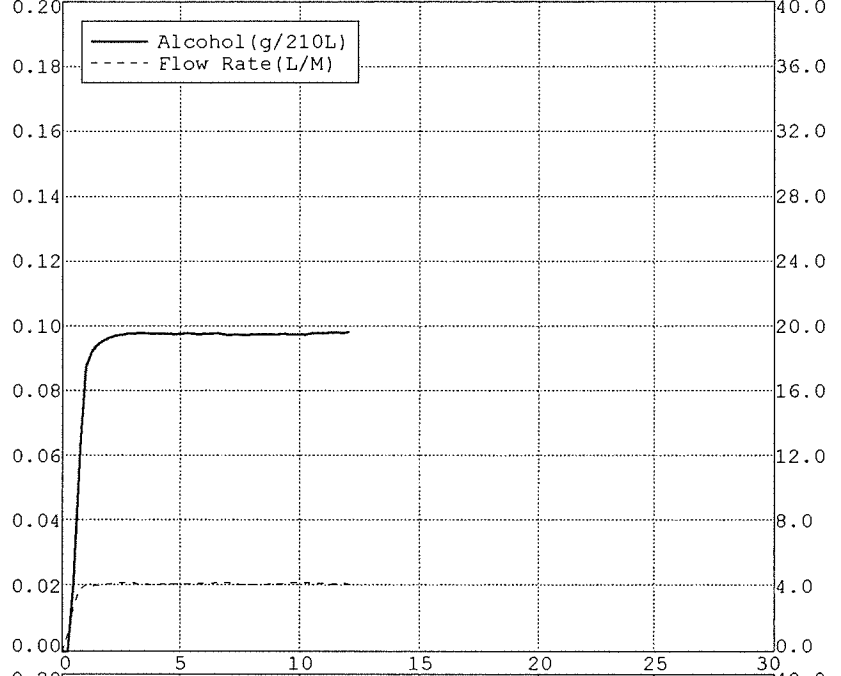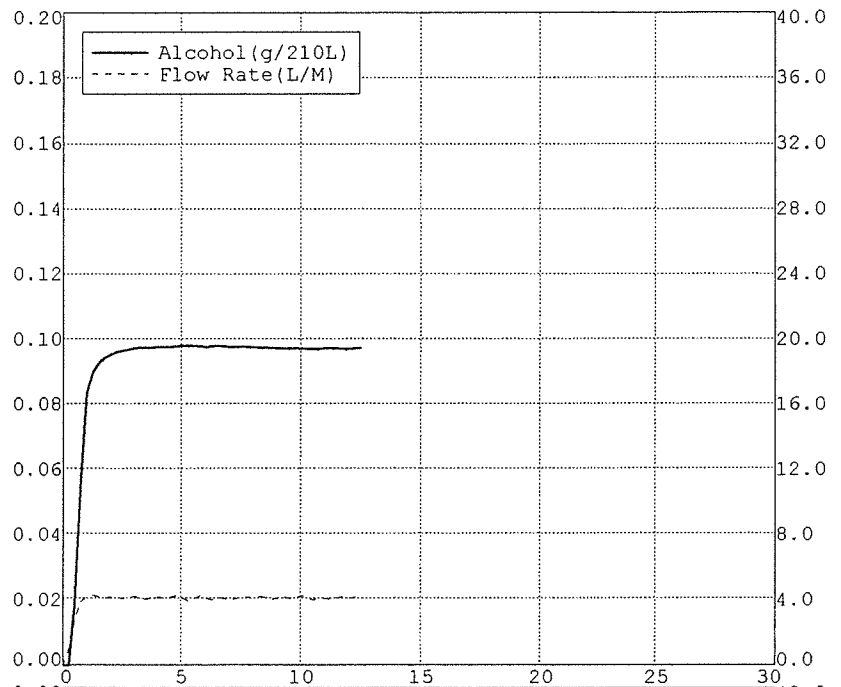

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/10/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:18
INTERNAL STANDARD	VERIFIED	09:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:19
BLANK TEST	0.00	09:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:20
BLANK TEST	0.00	09:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:21
BLANK TEST	0.00	09:22

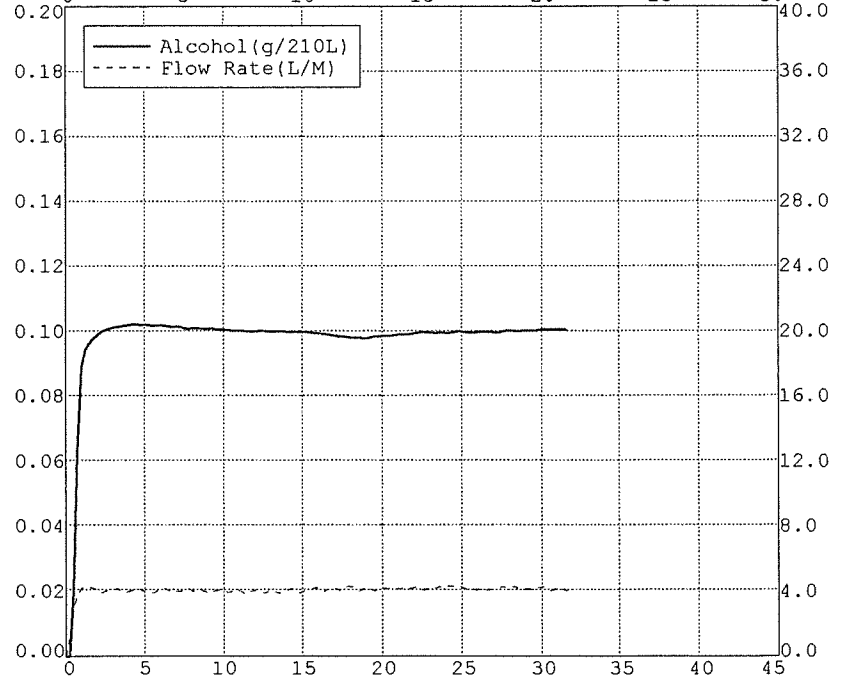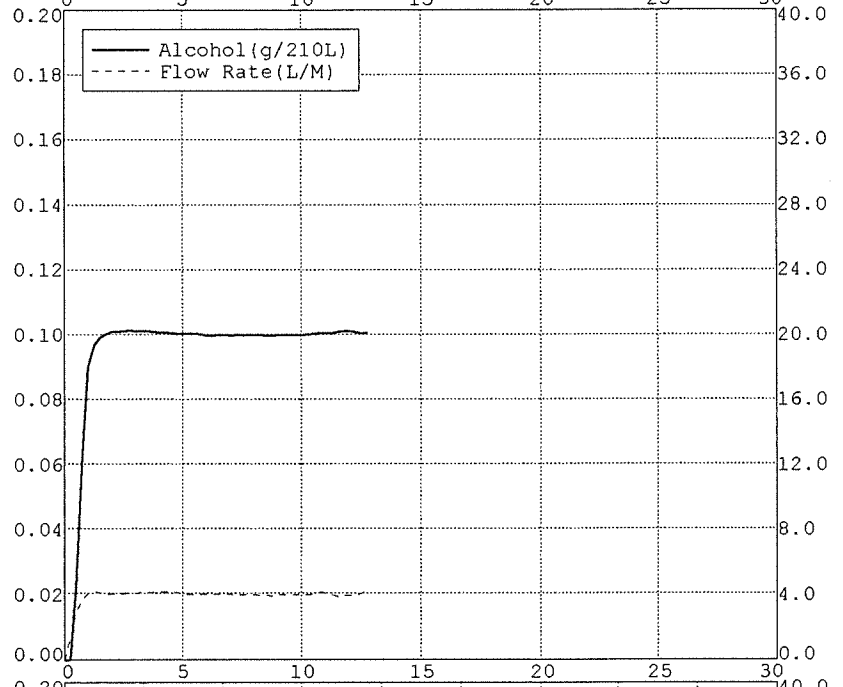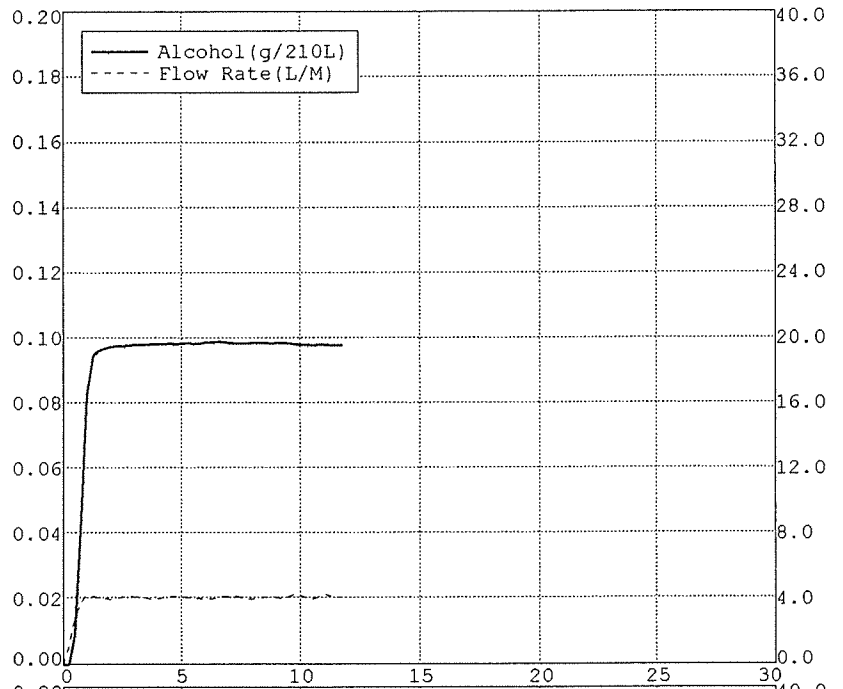

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/18/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:13
INTERNAL STANDARD	VERIFIED	10:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:13
BLANK TEST	0.00	10:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:14
BLANK TEST	0.00	10:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:15
BLANK TEST	0.00	10:16

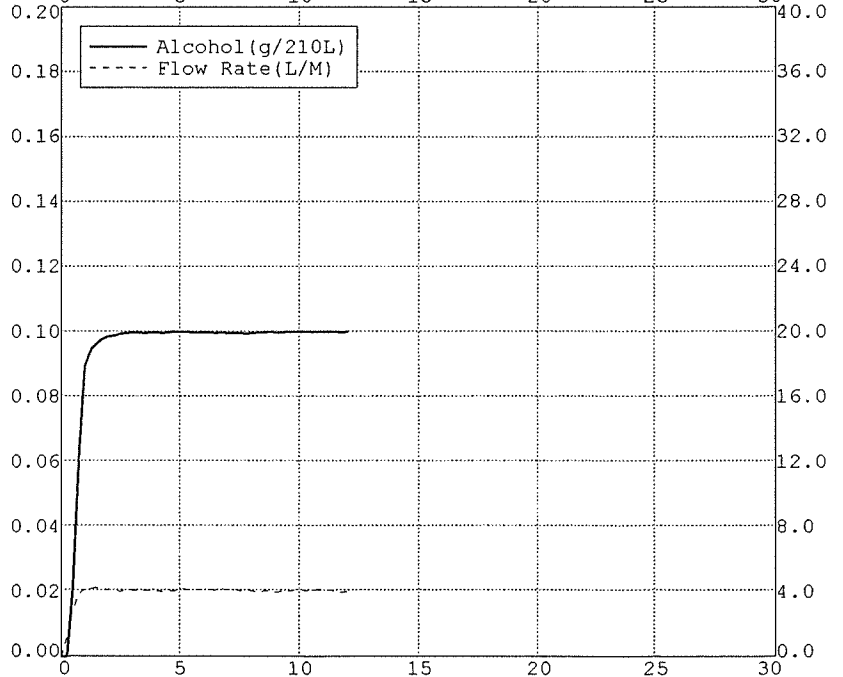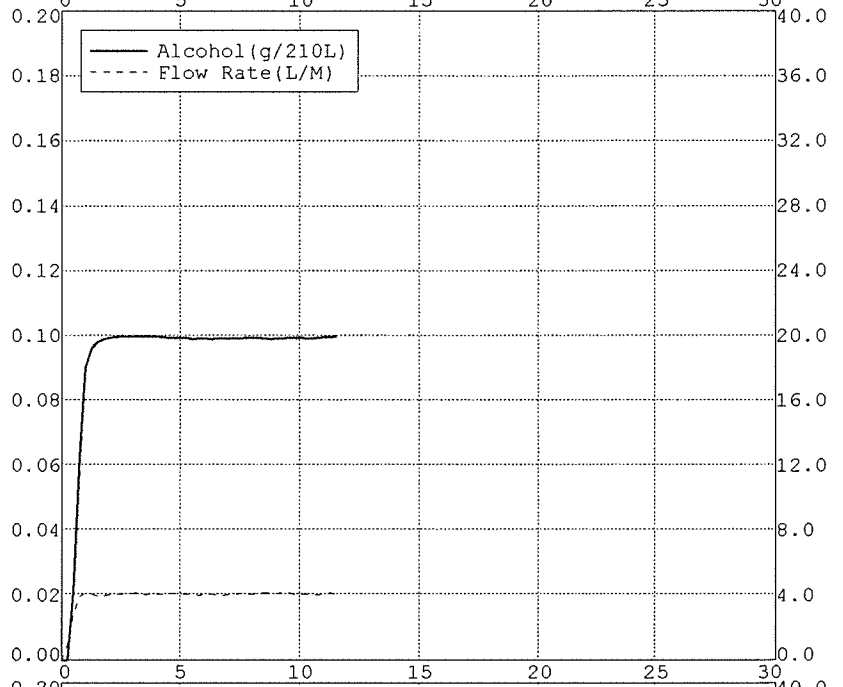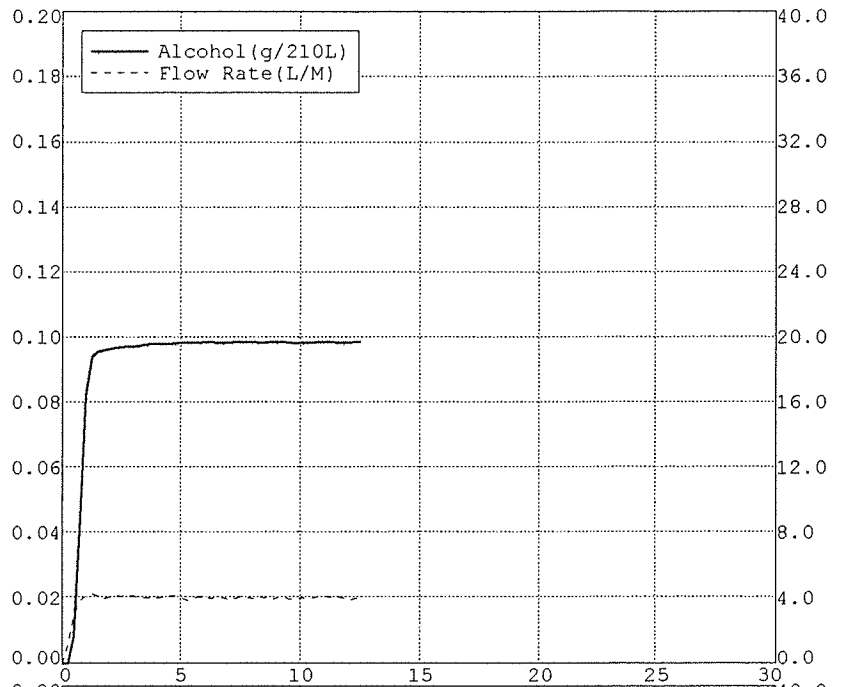

SUPERVISOR TEST

 LAKE PLACID VILLAGE
 POLICE DEPT.
 DATAMASTER dmt: 100290

Date: 01/24/2021

OPERATOR NAME:
 CHAD P BLINN
 Permit #: 33034
 Operator Agency/Dept: LAKE PLACID VILL. PD
 Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:44
INTERNAL STANDARD	VERIFIED	12:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:44
BLANK TEST	0.00	12:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:45
BLANK TEST	0.00	12:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:46
BLANK TEST	0.00	12:47

