

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/08/2024

OPERATOR NAME:
CATHERINE L VALENTINE
Permit #: 52253
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23350

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:23
INTERNAL STANDARD	VERIFIED	01:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:23
BLANK TEST	0.00	01:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:24
BLANK TEST	0.00	01:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:26
BLANK TEST	0.00	01:26

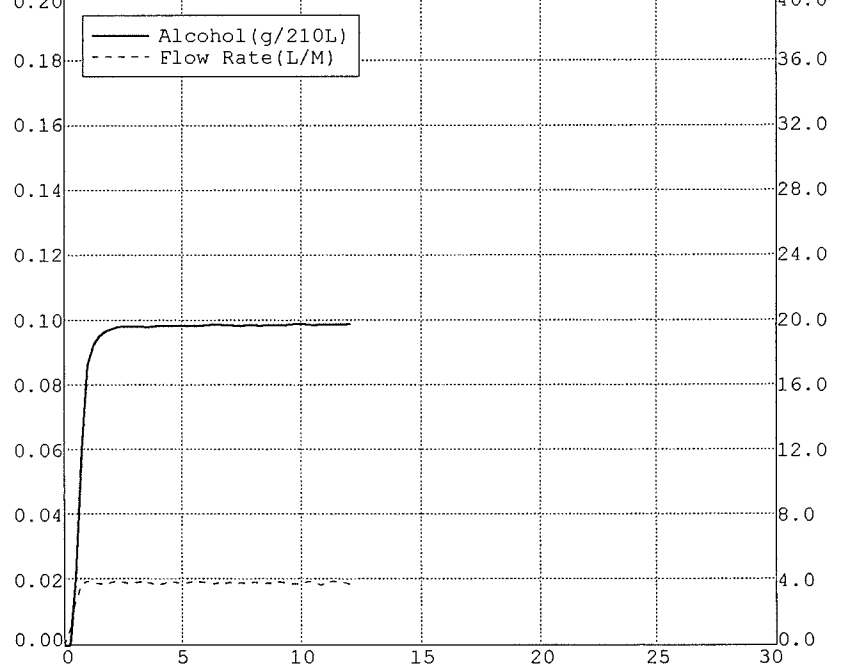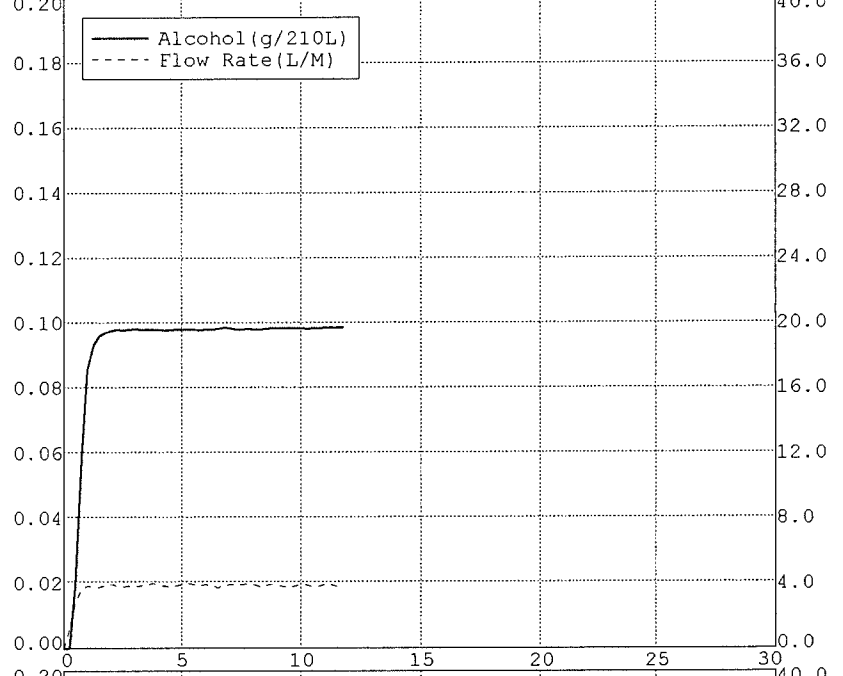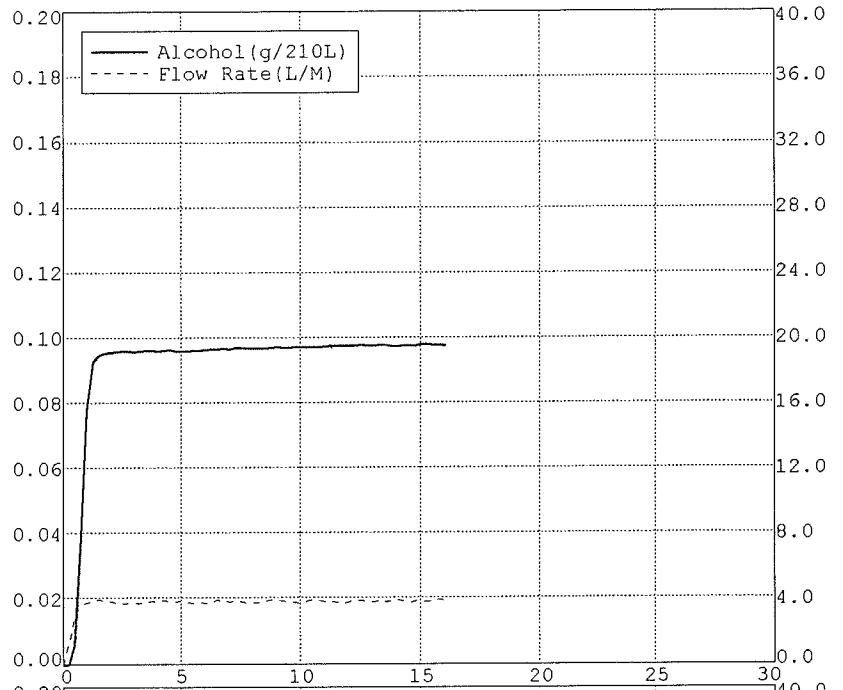

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/14/2024

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23350

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:20
INTERNAL STANDARD	VERIFIED	04:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:20
BLANK TEST	0.00	04:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:21
BLANK TEST	0.00	04:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:22
BLANK TEST	0.00	04:23

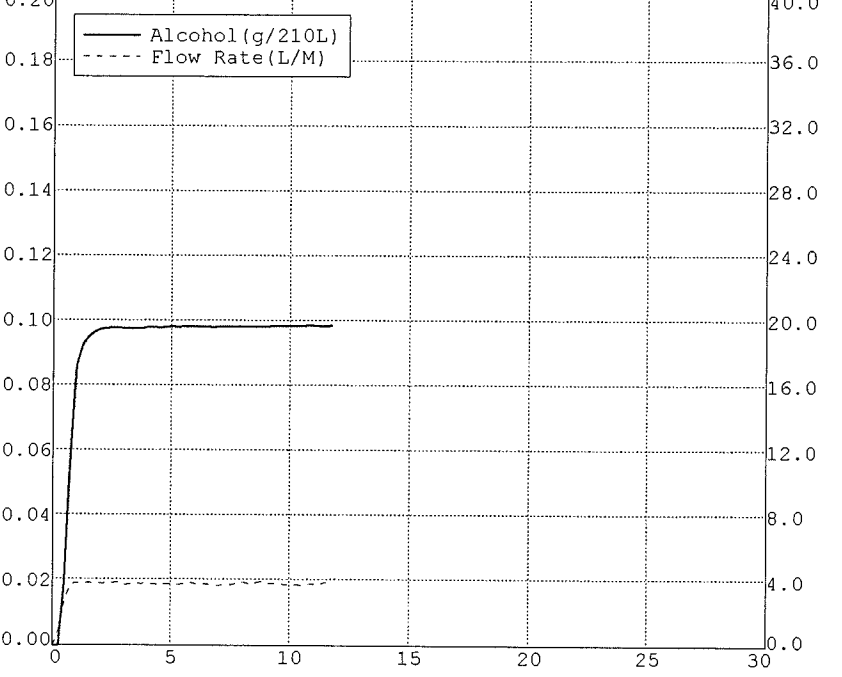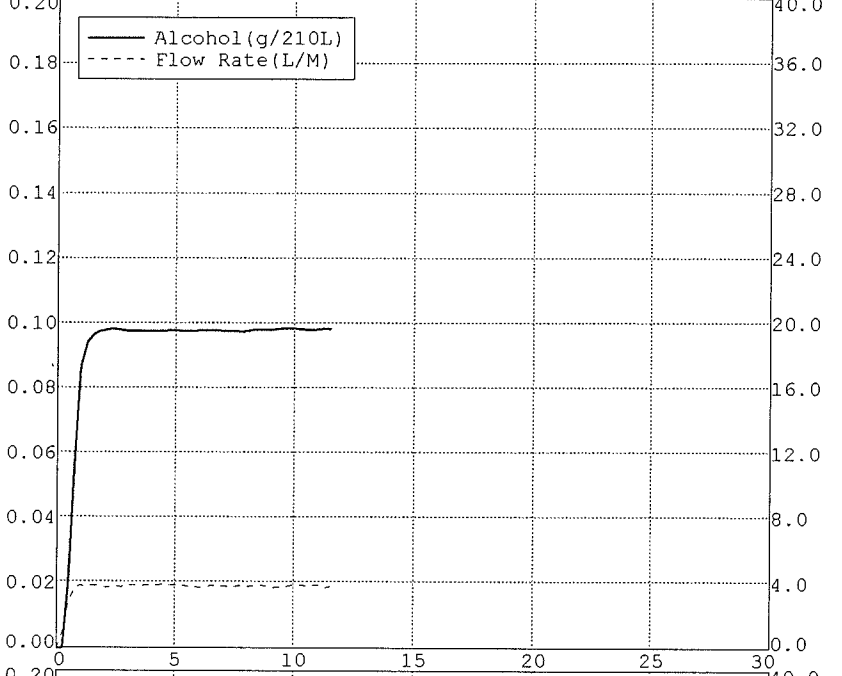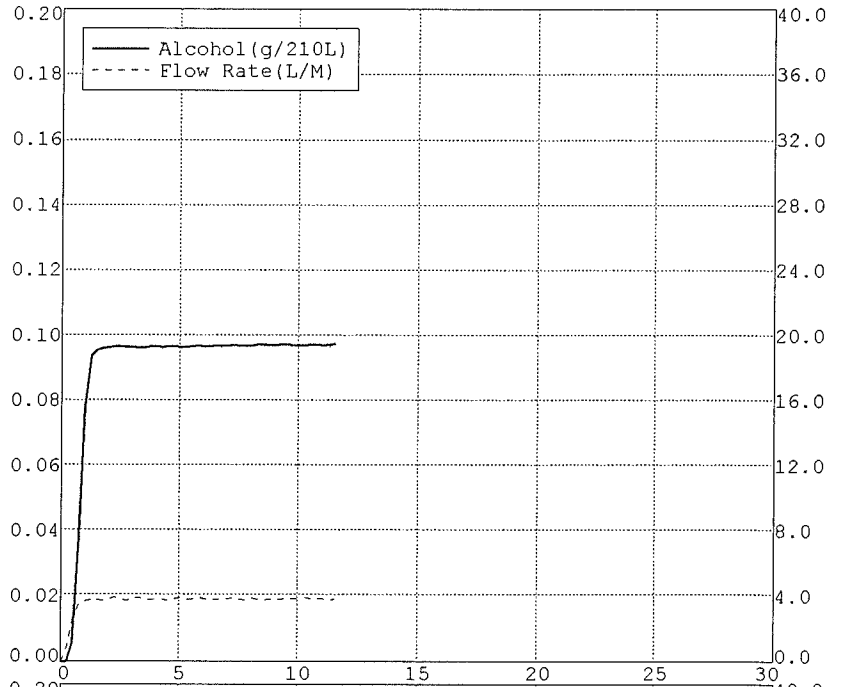

SUPERVISOR TEST




 LAKE PLACID VILLAGE
 POLICE DEPT.
 DATAMASTER dmt: 100290

Date: 01/22/2024

OPERATOR NAME:
 CATHERINE L VALENTINE
 Permit #: 52253
 Operator Agency/Dept: LAKE PLACID VILL. PD
 Reference Standard #: 23350

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:08
INTERNAL STANDARD	VERIFIED	03:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:09
BLANK TEST	0.00	03:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:10
BLANK TEST	0.00	03:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:11
BLANK TEST	0.00	03:12

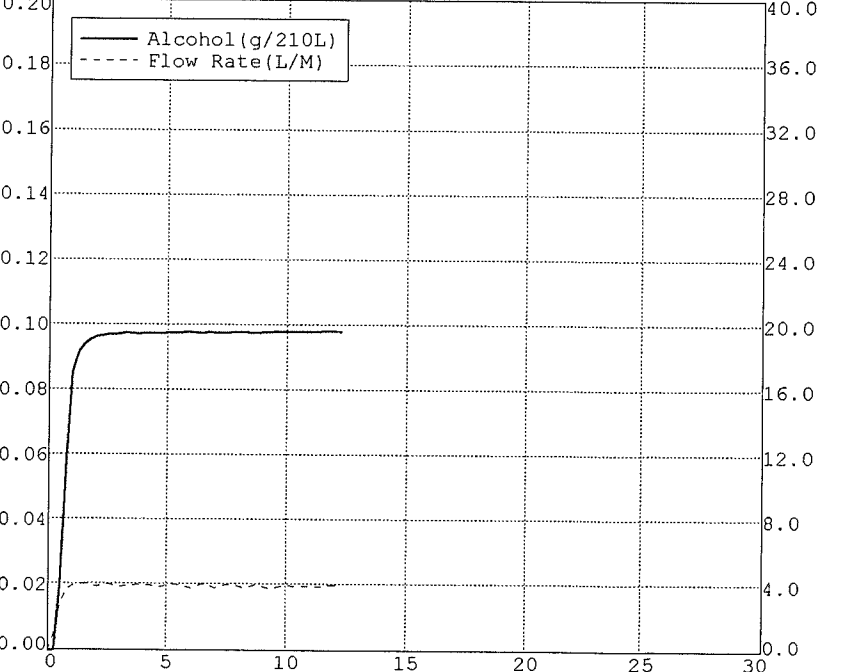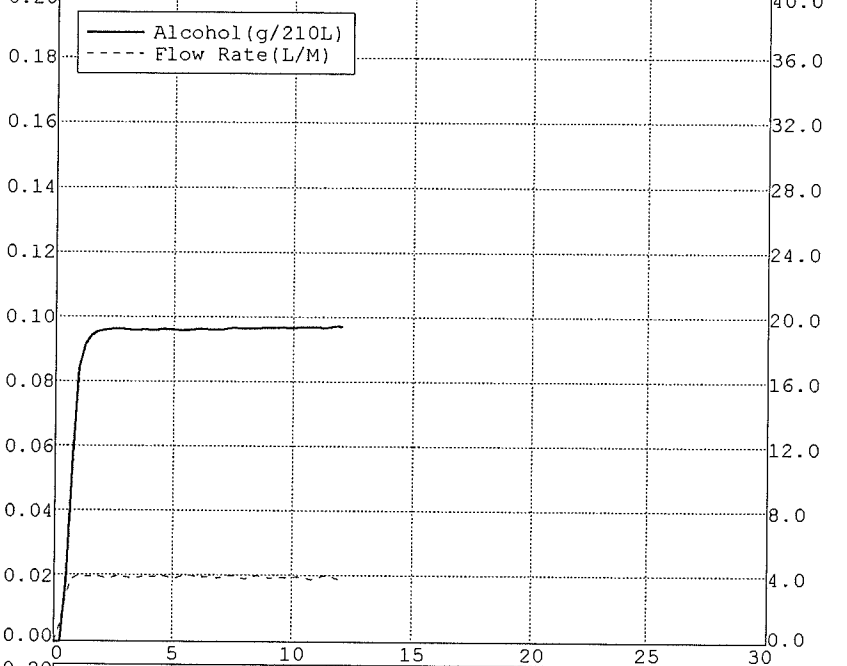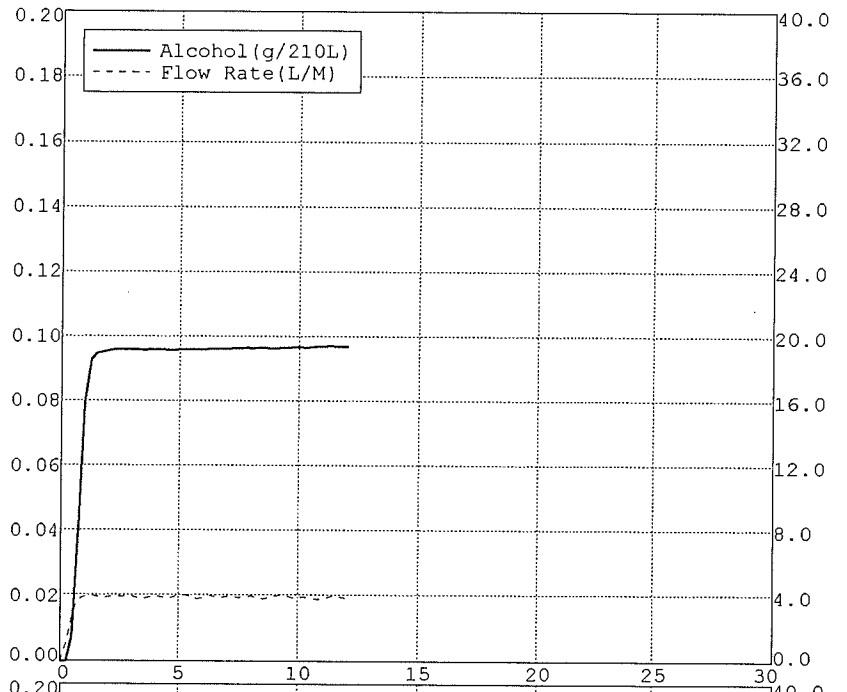

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/28/2024

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23430

Nominal = 0.10 g/210L

RFI Detected

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 01/28/2024

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23430

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:26
INTERNAL STANDARD	VERIFIED	18:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:26
BLANK TEST	0.00	18:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:27
BLANK TEST	0.00	18:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:28
BLANK TEST	0.00	18:29

