

SUPERVISOR TEST




LAKE PLACID VILLAGE  
 POLICE DEPT.  
 DATAMASTER dmt: 100290

Date: 02/03/2020

OPERATOR NAME:  
 CHAD P BLINN  
 Permit #: 33034  
 Operator Agency/Dept: LAKE PLACID VILL. PD  
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:04
INTERNAL STANDARD	VERIFIED	16:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:05
BLANK TEST	0.00	16:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:06
BLANK TEST	0.00	16:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:07
BLANK TEST	0.00	16:08

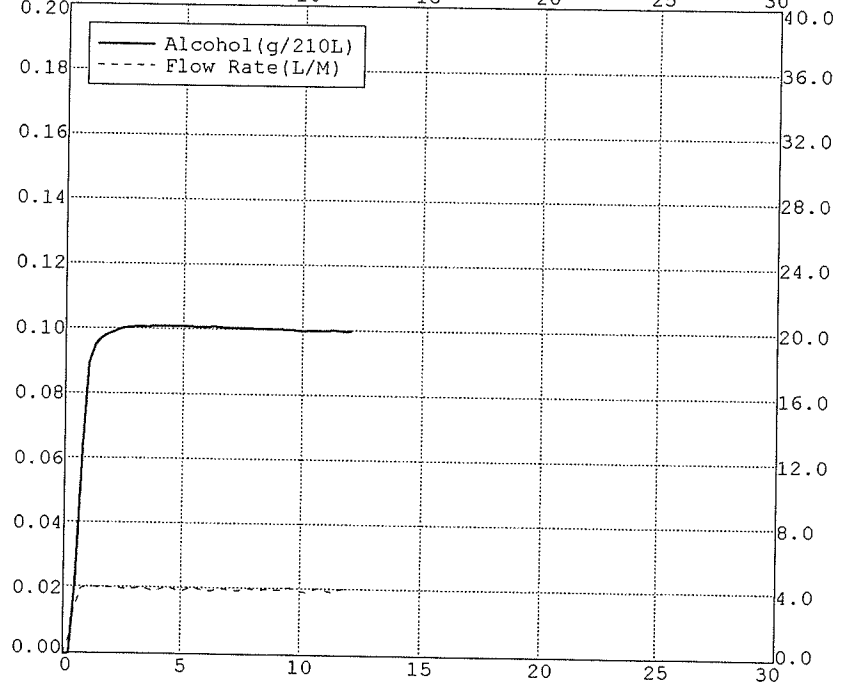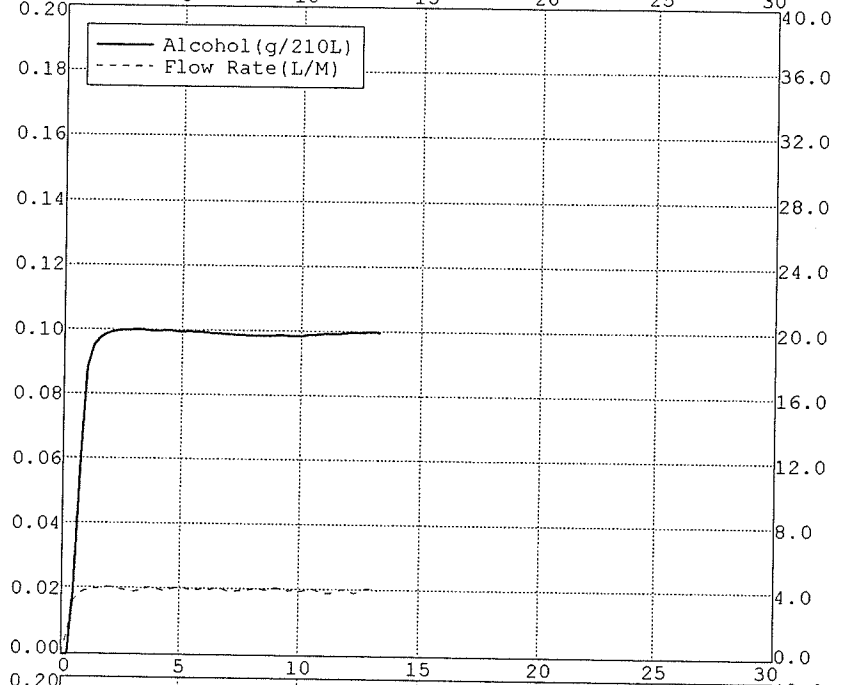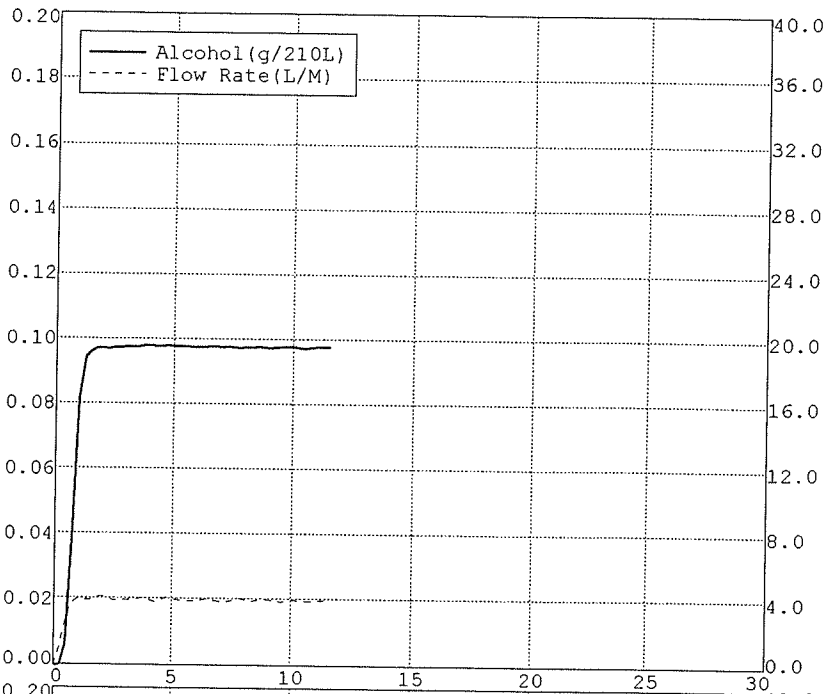

SUPERVISOR TEST

LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 02/09/2020

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:42
INTERNAL STANDARD	VERIFIED	07:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:43
BLANK TEST	0.00	07:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:44
BLANK TEST	0.00	07:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:45
BLANK TEST	0.00	07:46

