

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/14/2022

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:55
INTERNAL STANDARD	VERIFIED	18:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:55
BLANK TEST	0.00	18:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:57
BLANK TEST	0.00	18:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:58
BLANK TEST	0.00	18:59

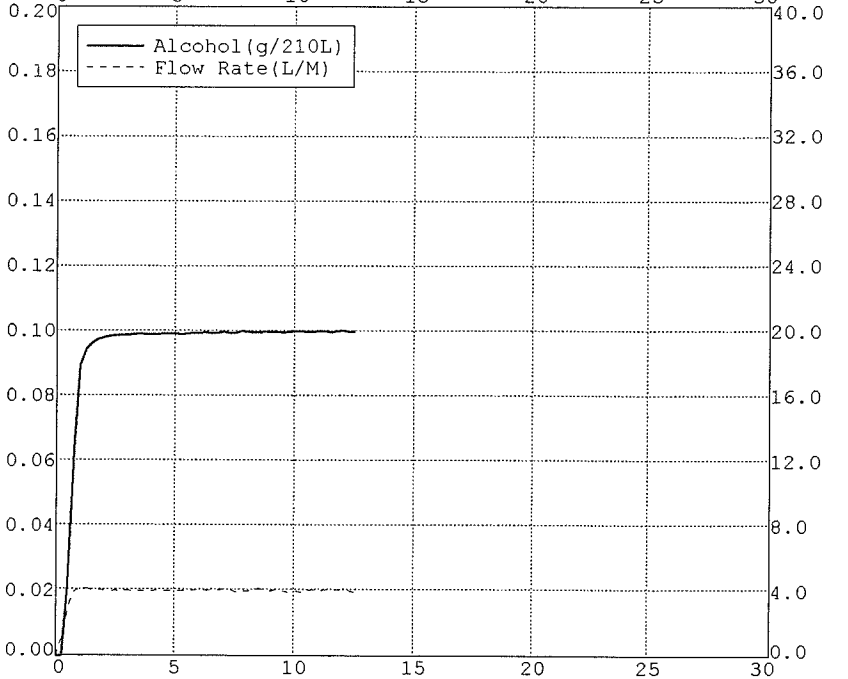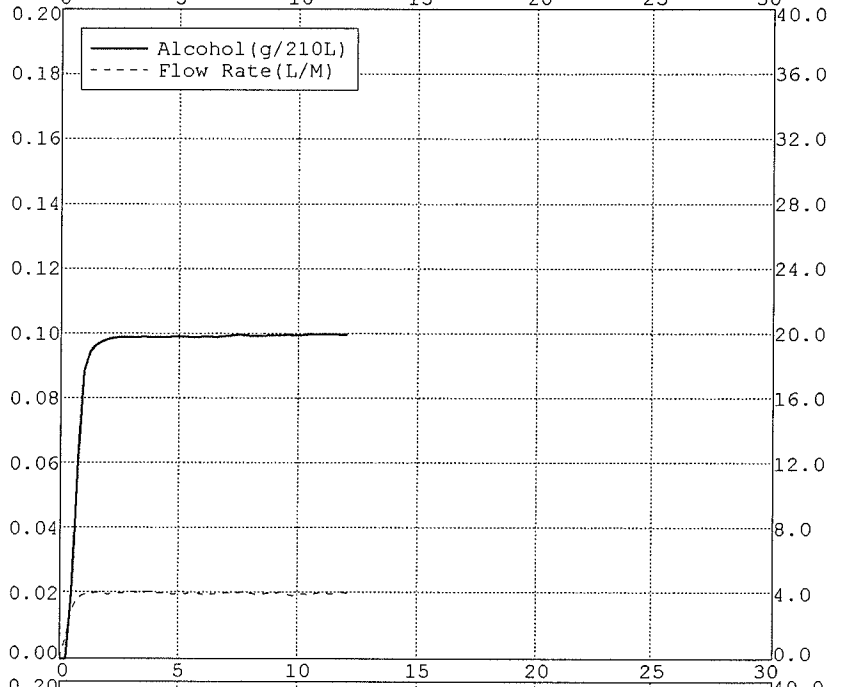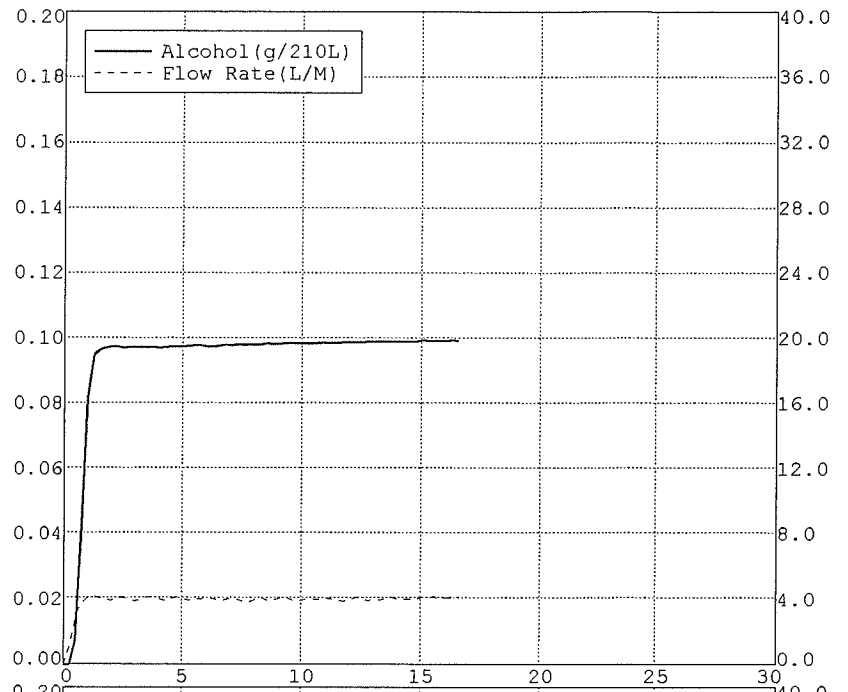

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/21/2022

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:28
INTERNAL STANDARD	VERIFIED	04:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:28
BLANK TEST	0.00	04:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:30
BLANK TEST	0.00	04:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:31
BLANK TEST	0.00	04:31

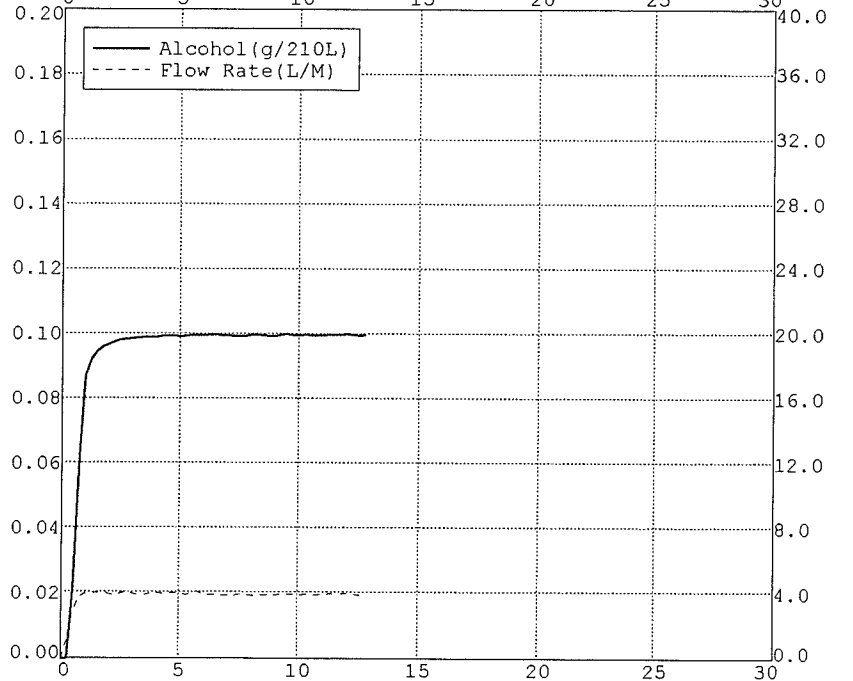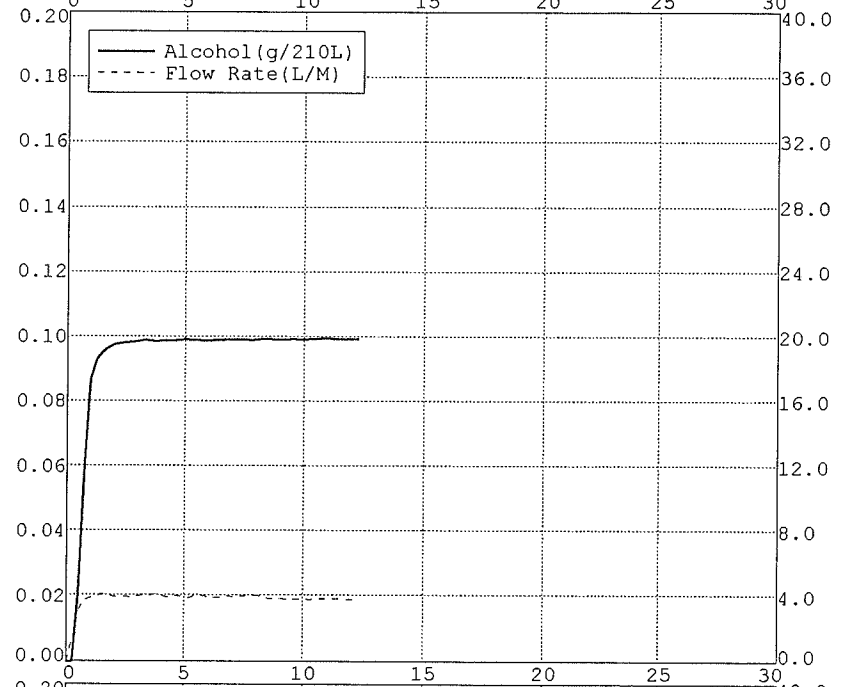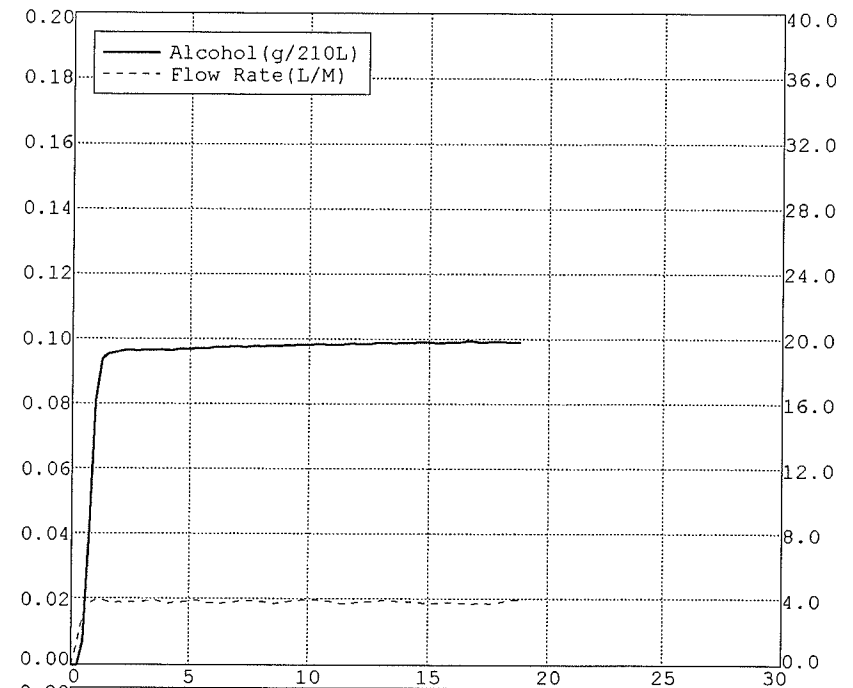

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/28/2022

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:56
INTERNAL STANDARD	VERIFIED	18:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:56
BLANK TEST	0.00	18:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:57
BLANK TEST	0.00	18:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:58
BLANK TEST	0.00	18:59

