

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 10/05/2019

OPERATOR NAME:  
FRANCIS P STRACK  
Permit #: 34240  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:29
INTERNAL STANDARD	VERIFIED	03:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:29
BLANK TEST	0.00	03:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:30
BLANK TEST	0.00	03:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:31
BLANK TEST	0.00	03:32

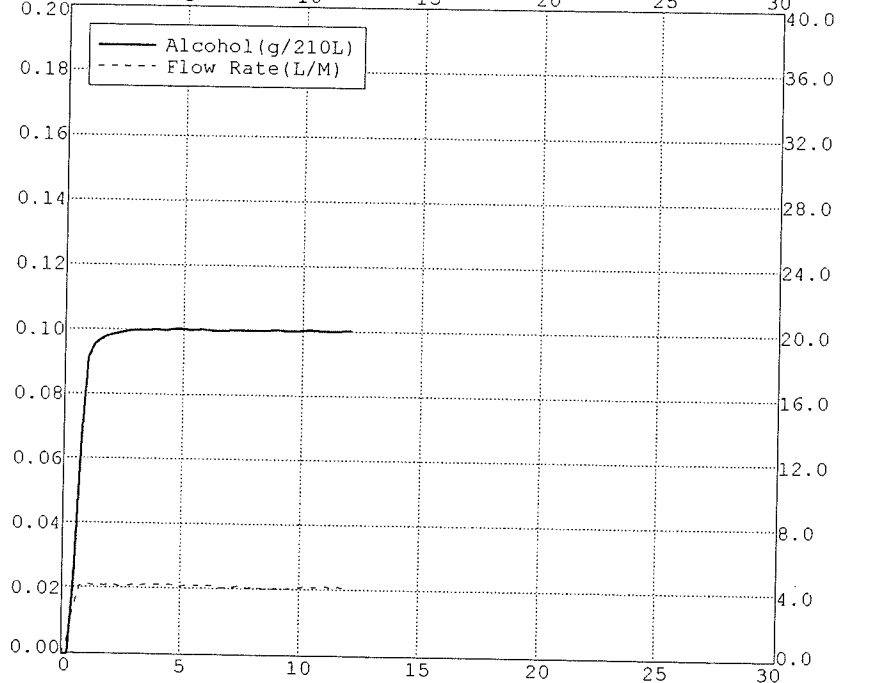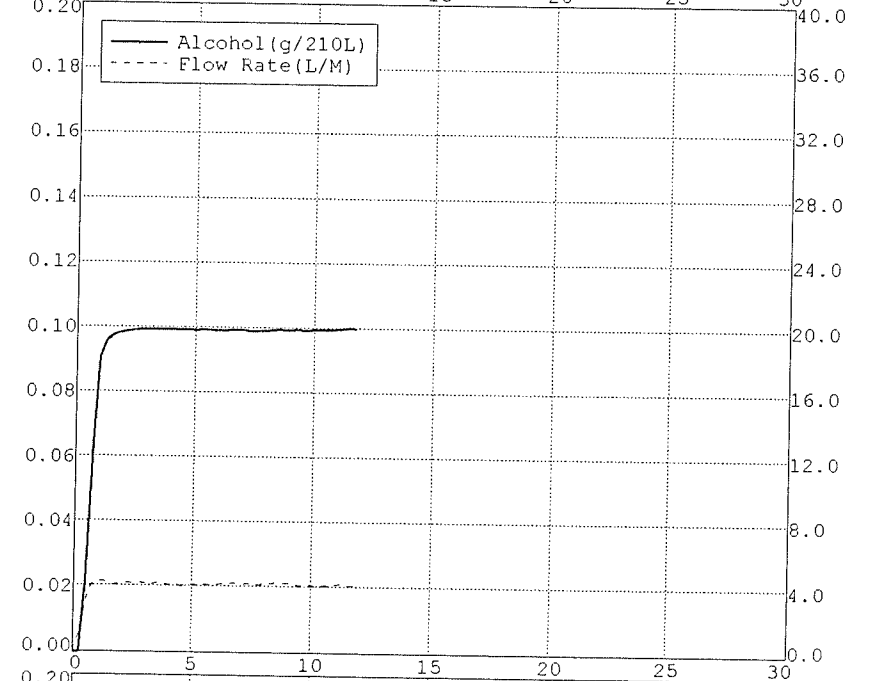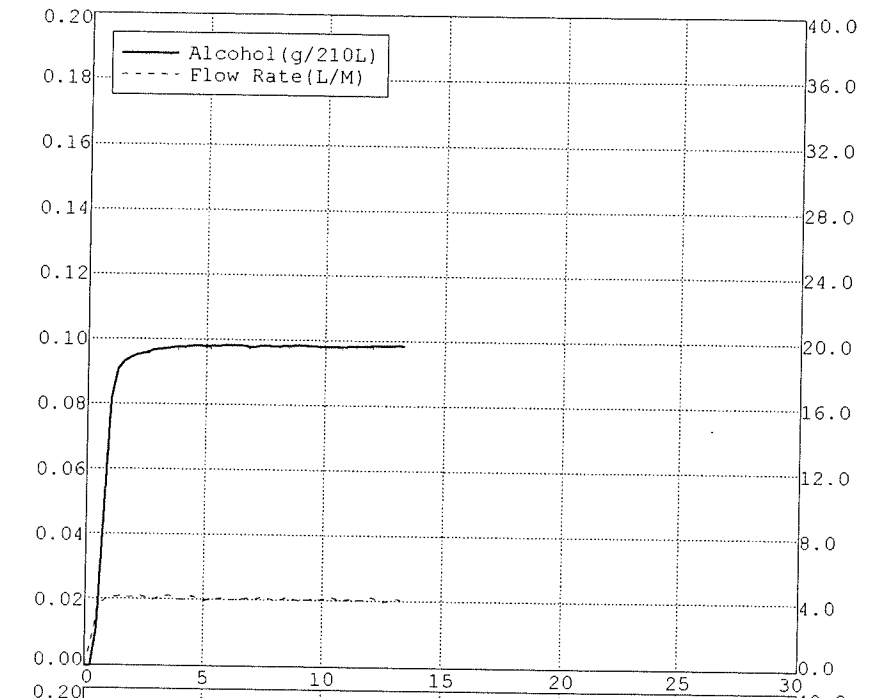

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 10/06/2019

OPERATOR NAME:  
CHAD P. LINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:38
INTERNAL STANDARD	VERIFIED	13:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:38
BLANK TEST	0.00	13:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:40
BLANK TEST	0.00	13:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:41
BLANK TEST	0.00	13:42

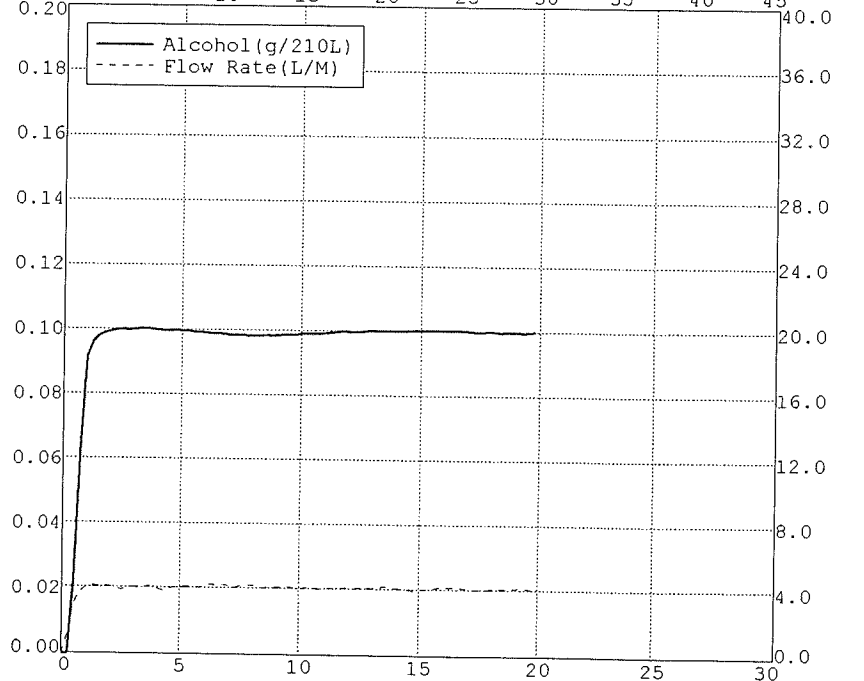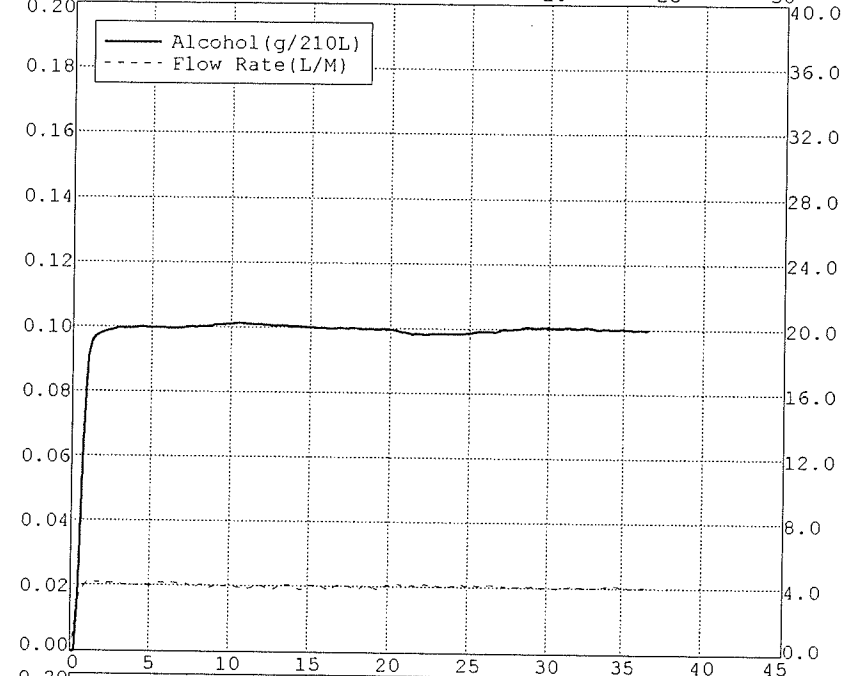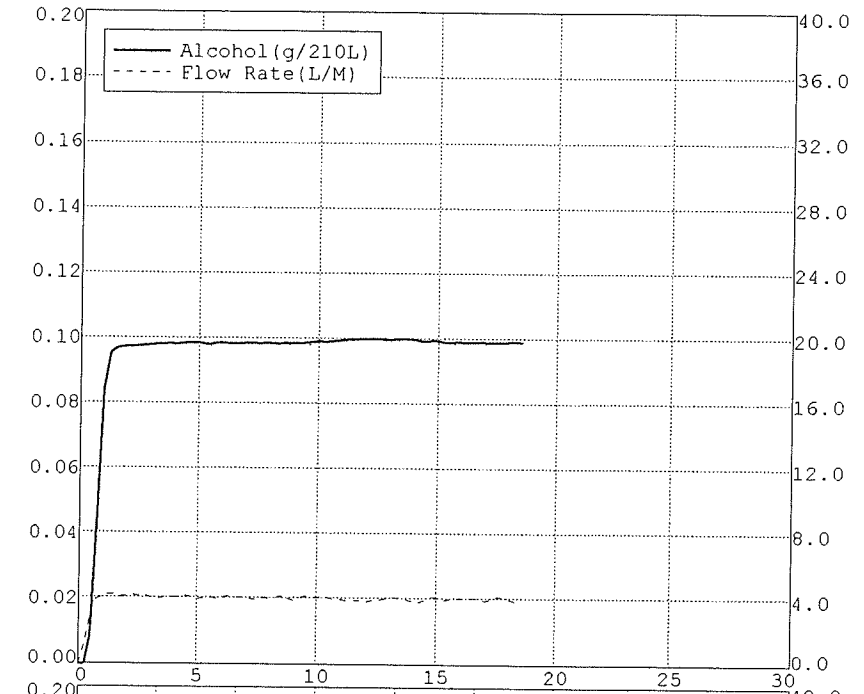

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 10/14/2019

OPERATOR NAME:  
DORAN H. SORRELL  
Permit #: 47507  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:35
INTERNAL STANDARD	VERIFIED	17:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:36
BLANK TEST	0.00	17:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:37
BLANK TEST	0.00	17:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:38
BLANK TEST	0.00	17:39

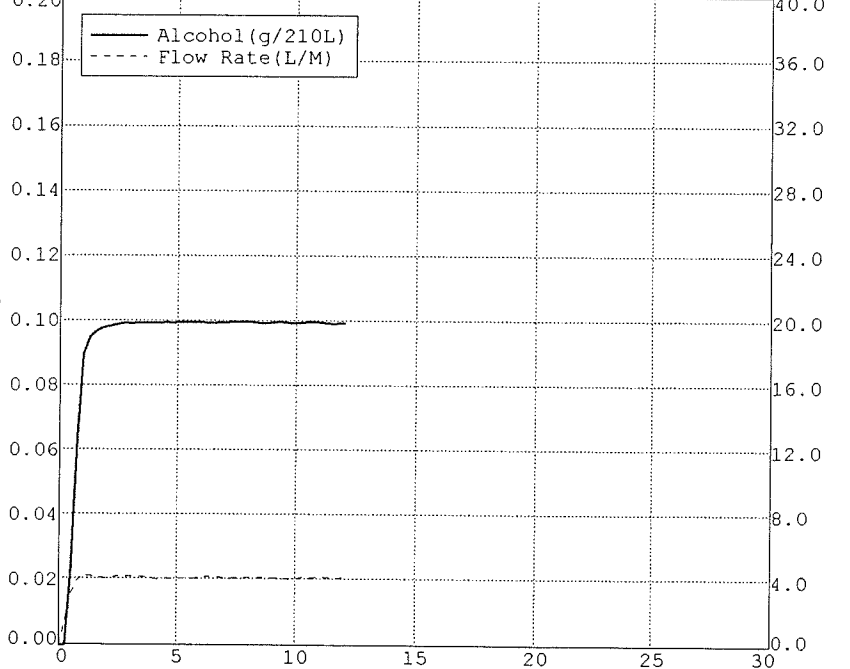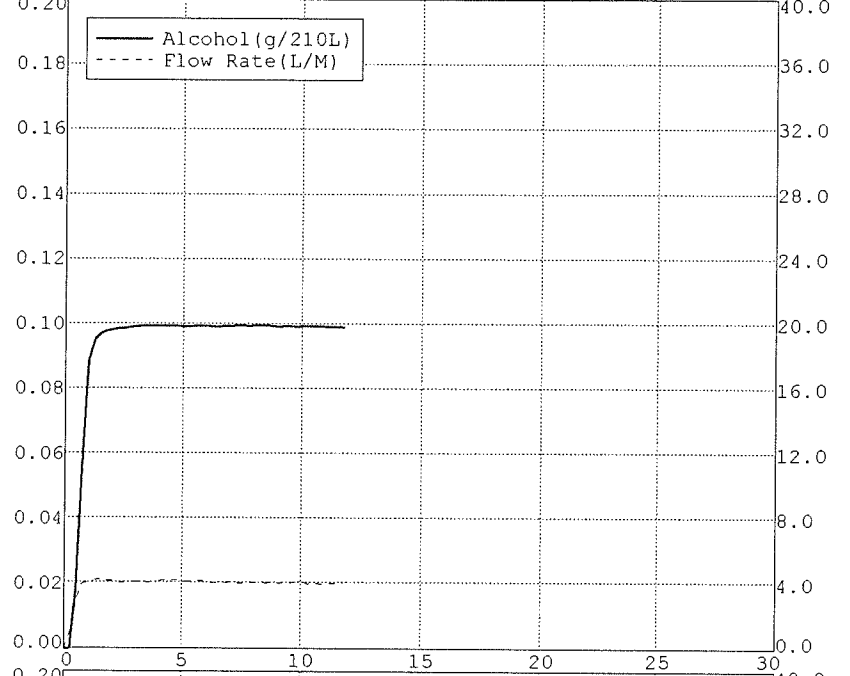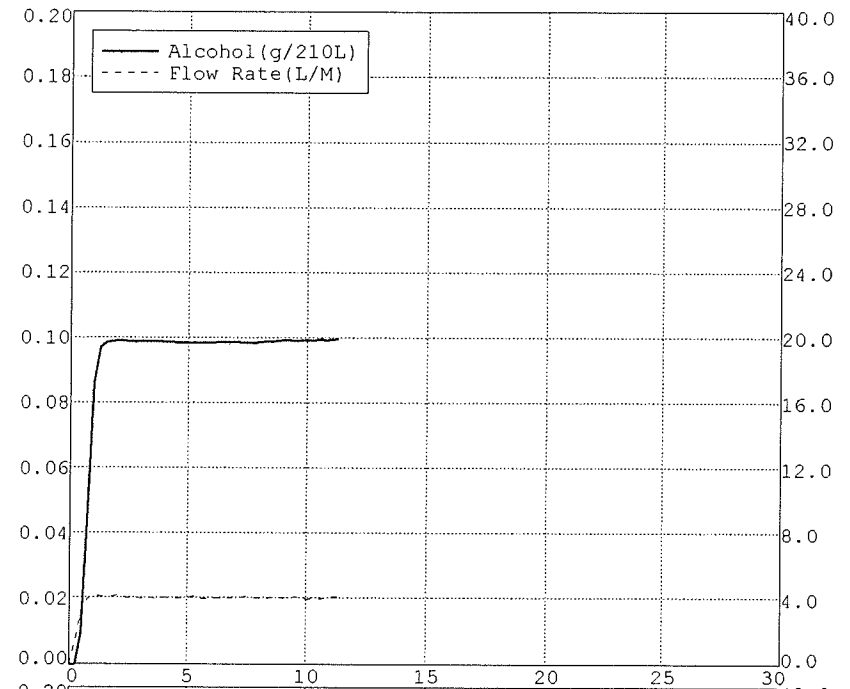

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 10/20/2019

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:59
INTERNAL STANDARD	VERIFIED	07:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:00
BLANK TEST	0.00	08:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:01
BLANK TEST	0.00	08:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:02
BLANK TEST	0.00	08:03

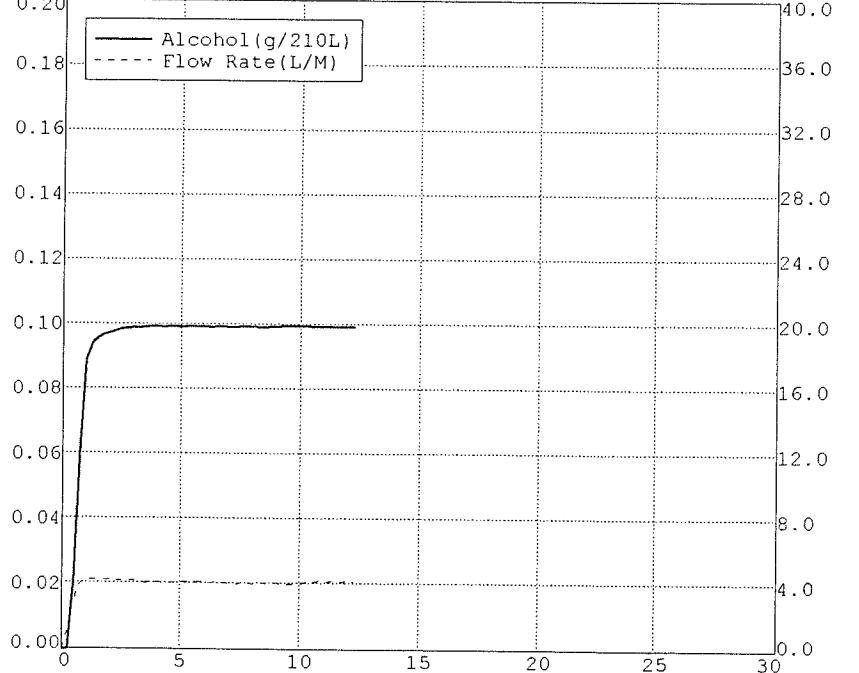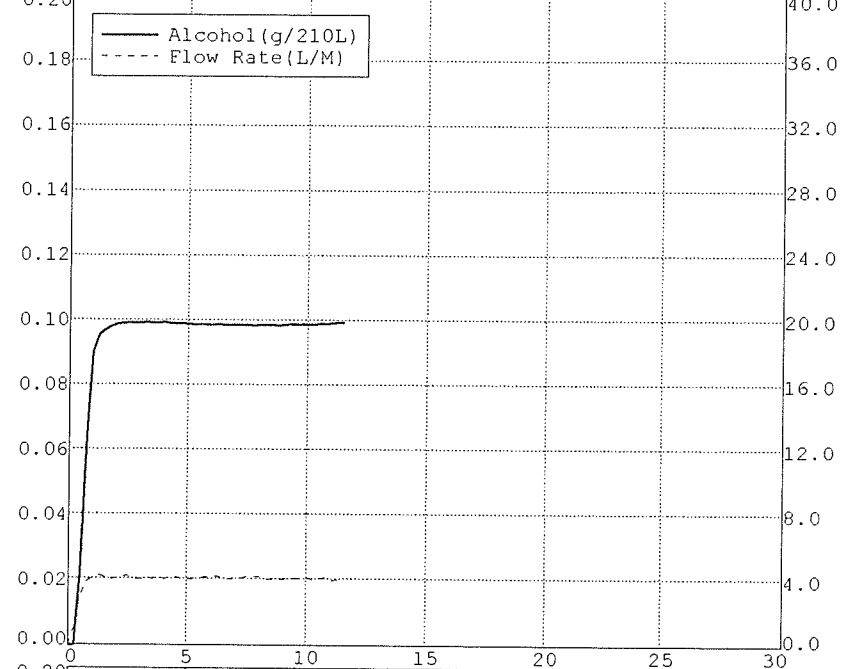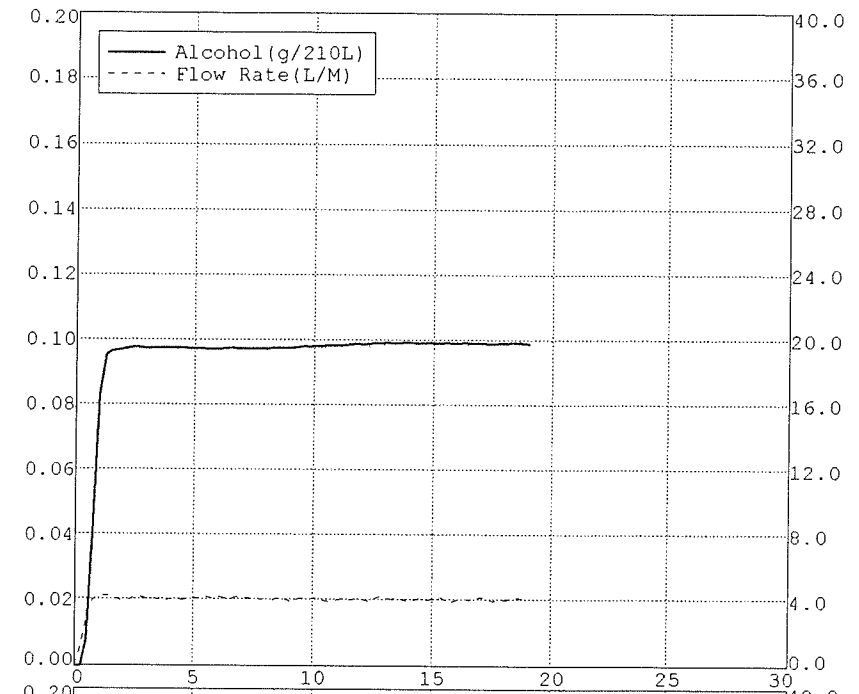

SU MISC TEST

LAKE PLACID VILLAGE  
 POLICE DEPT  
 DISTRICT: 100290

Date: 10/24/2019

OFFICER NAME:  
 DOUGLAS SCHELL  
 POLICE #: 07507  
 Officer Agency/Dept: LAKE PLACID VILL. PD  
 Reference Standard #: 19180

Net Weight = 1.10 g/210L

BEFORE TEST	0.00	10:32
INITIAL STANDARD	VERIFIED	10:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:32
BEFORE TEST	0.00	10:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:33
BEFORE TEST	0.00	10:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:35
BEFORE TEST	0.00	10:35

