

SUPERVISOR TEST



LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/04/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:54
INTERNAL STANDARD	VERIFIED	21:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:55
BLANK TEST	0.00	21:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:56
BLANK TEST	0.00	21:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:57
BLANK TEST	0.00	21:58

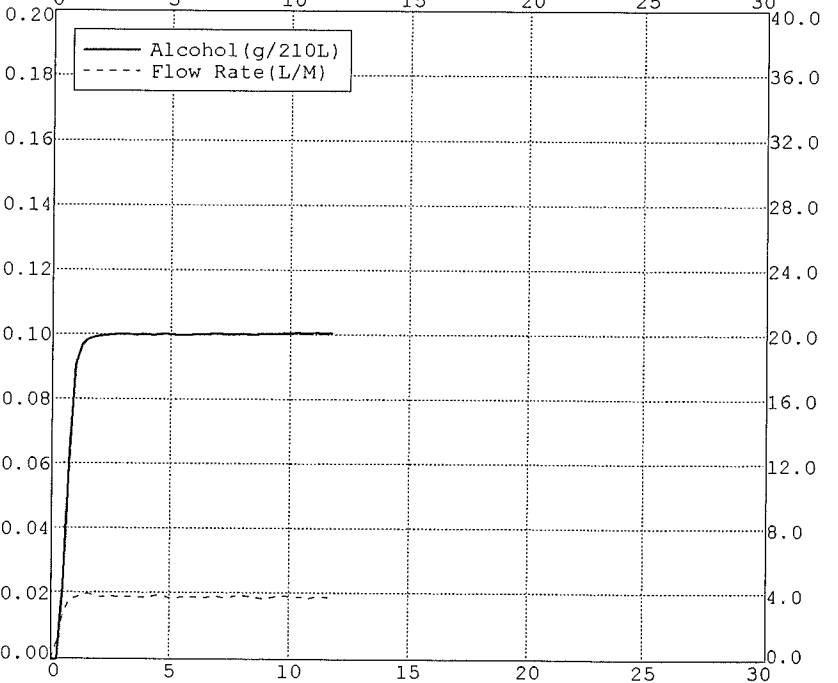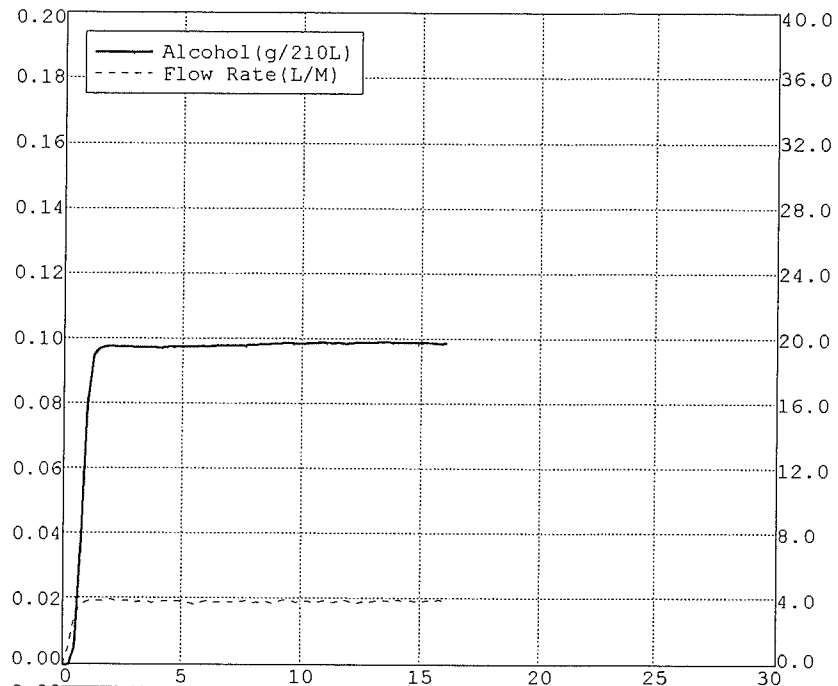

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/10/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:29
INTERNAL STANDARD	VERIFIED	21:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:29
BLANK TEST	0.00	21:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:31
BLANK TEST	0.00	21:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:32
BLANK TEST	0.00	21:33

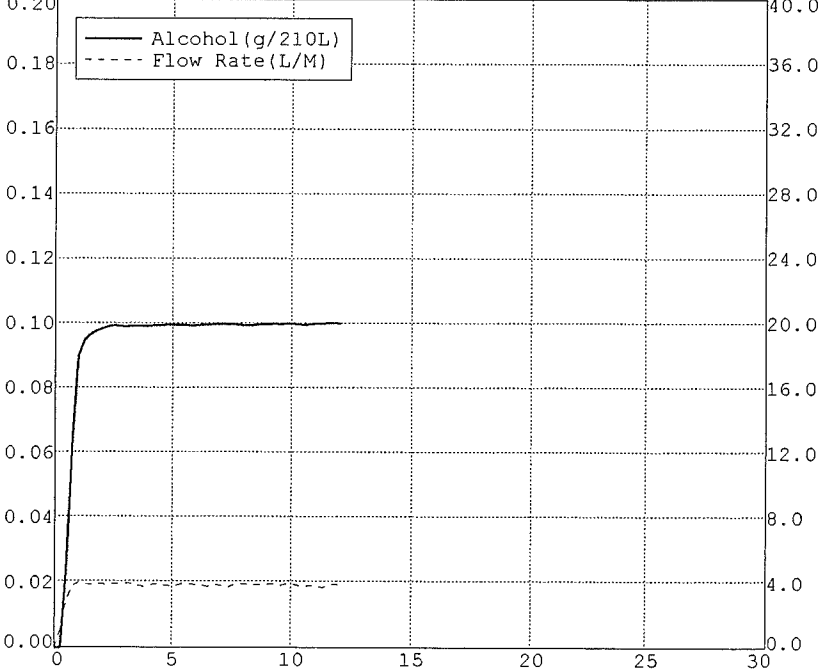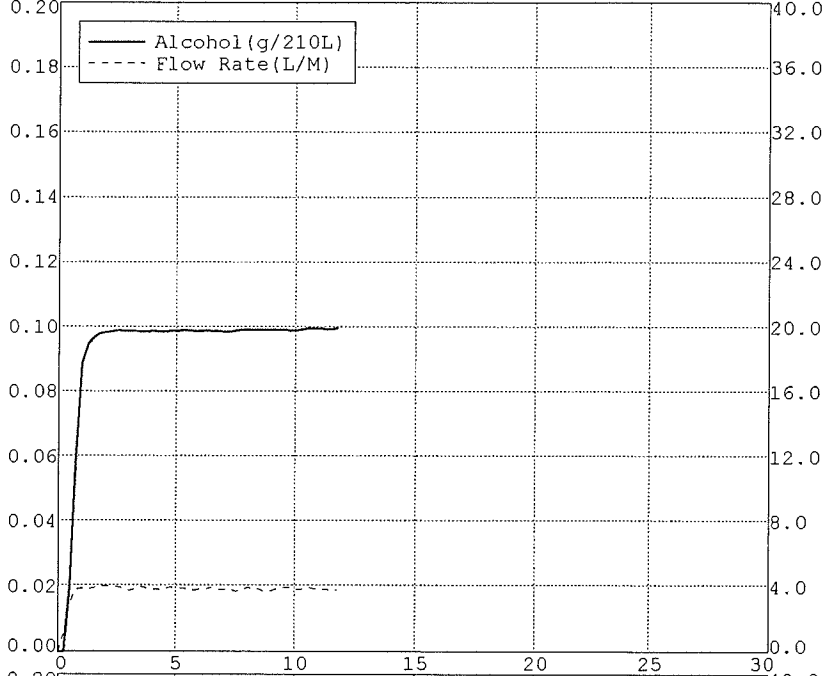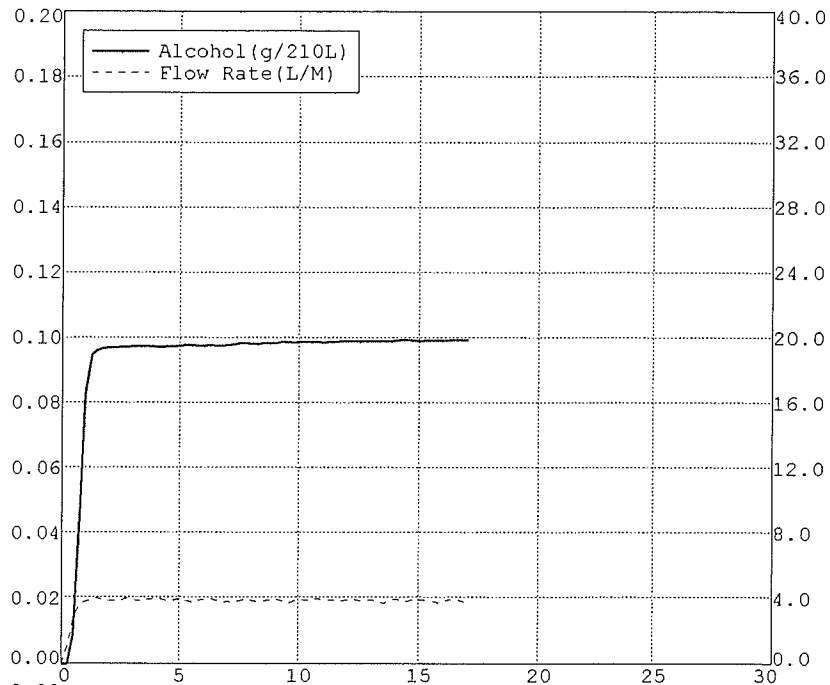

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/12/2023

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:20
INTERNAL STANDARD	VERIFIED	17:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:21
BLANK TEST	0.00	17:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:22
BLANK TEST	0.00	17:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:23
BLANK TEST	0.00	17:24

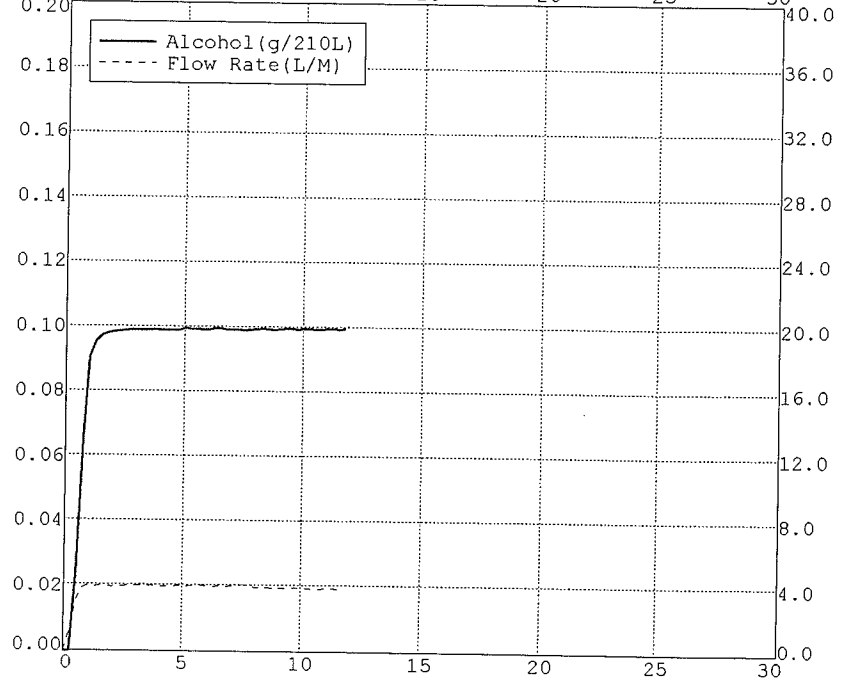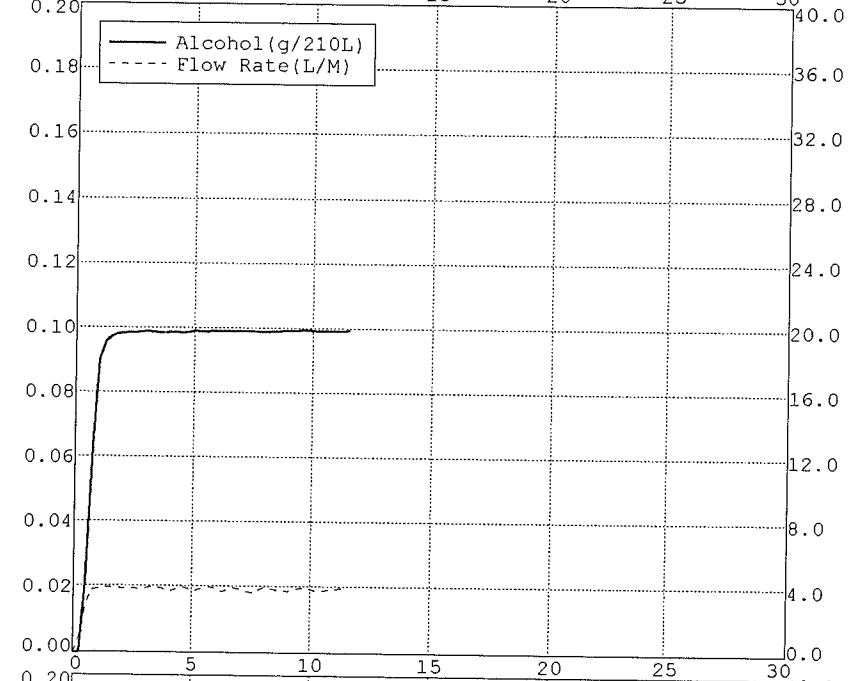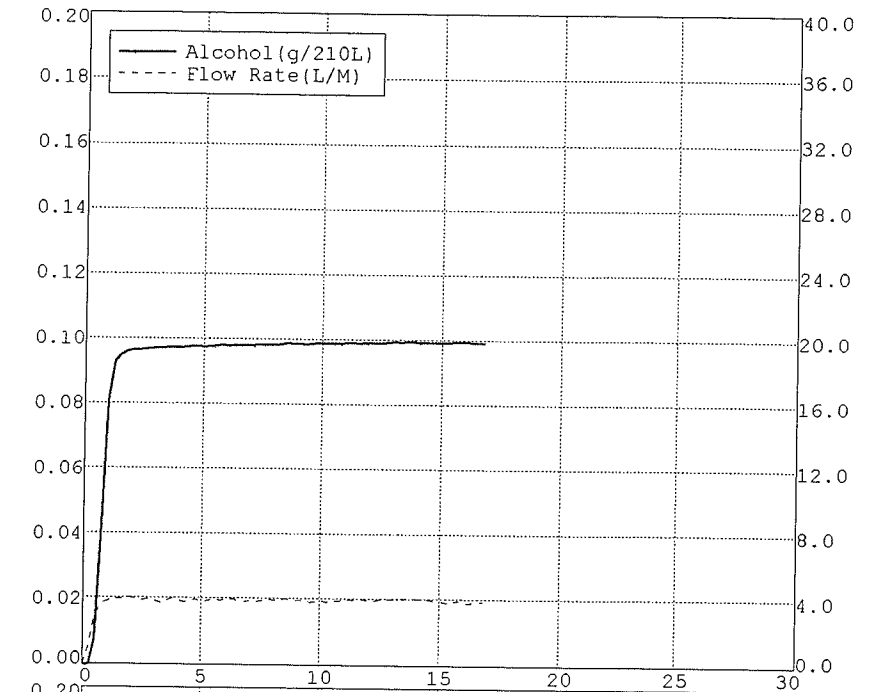

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/18/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:51
INTERNAL STANDARD	VERIFIED	17:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:51
BLANK TEST	0.00	17:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:53
BLANK TEST	0.00	17:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:54
BLANK TEST	0.00	17:55

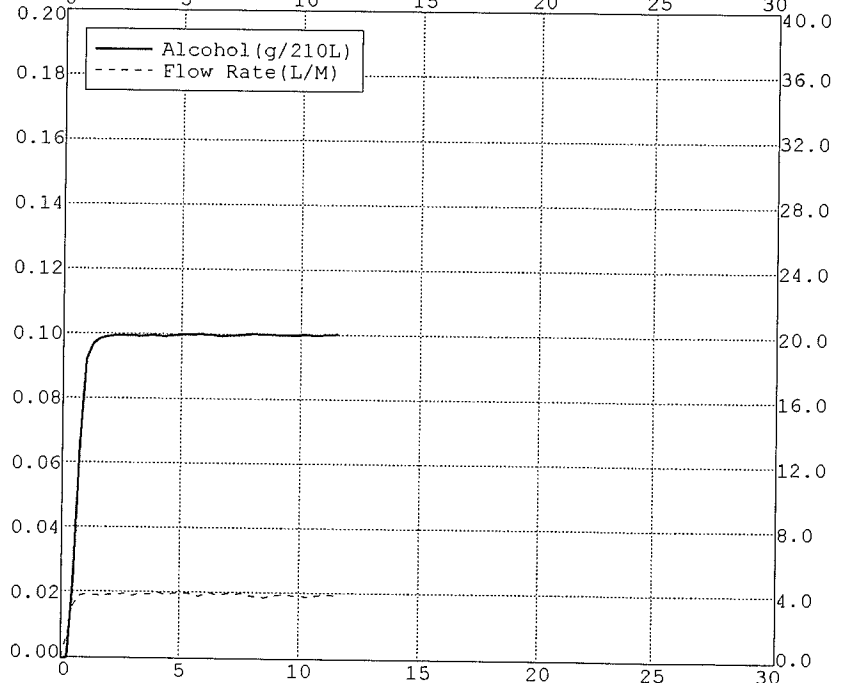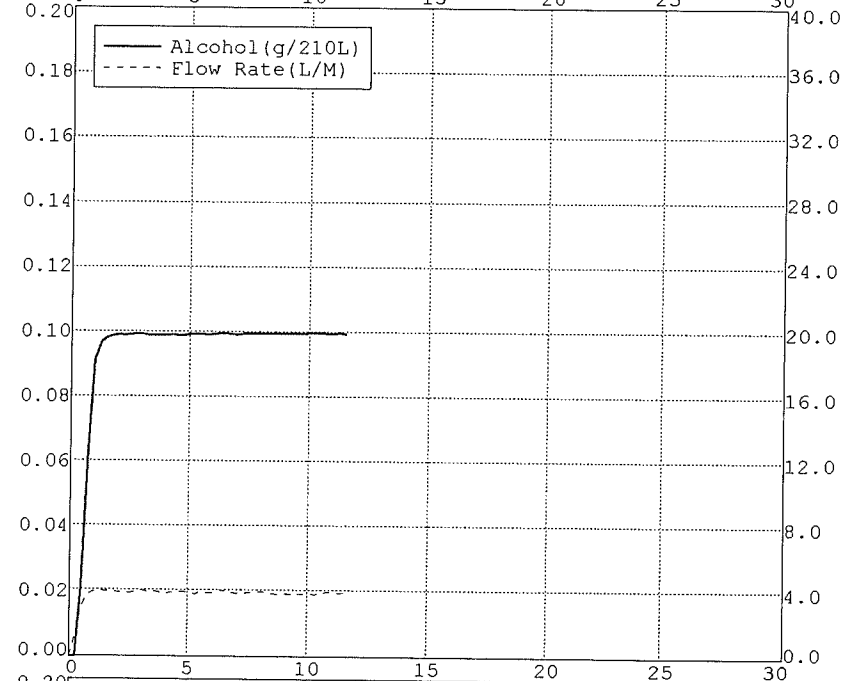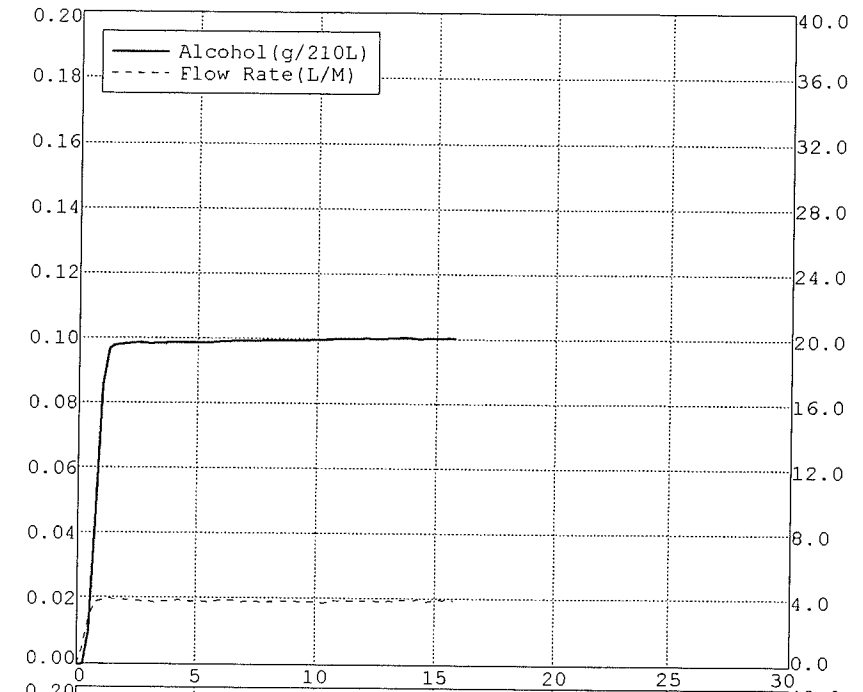

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 09/25/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:02
INTERNAL STANDARD	VERIFIED	03:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:03
BLANK TEST	0.00	03:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:04
BLANK TEST	0.00	03:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:05
BLANK TEST	0.00	03:06

