

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 10/05/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25250

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:42
INTERNAL STANDARD	VERIFIED	18:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:42
BLANK TEST	0.00	18:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:43
BLANK TEST	0.00	18:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:45
BLANK TEST	0.00	18:45

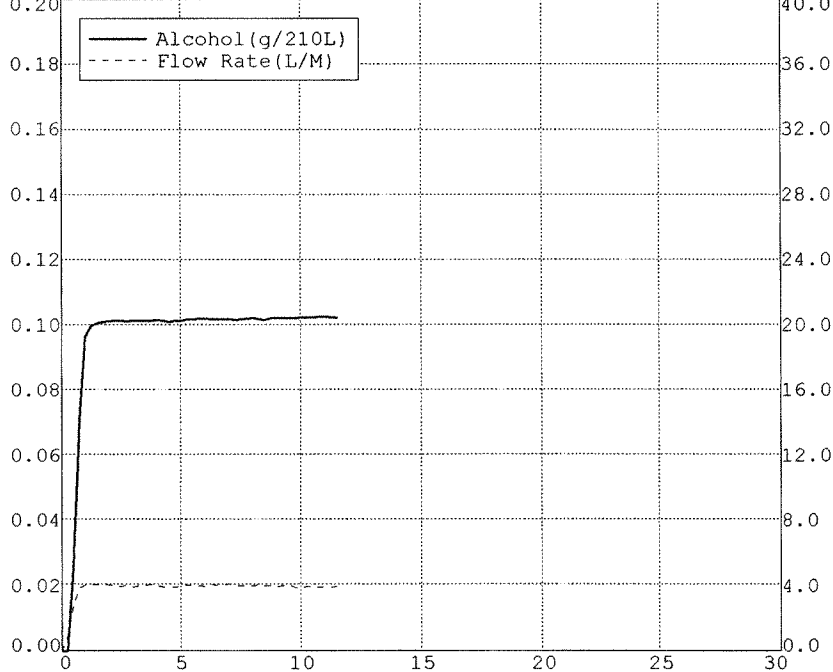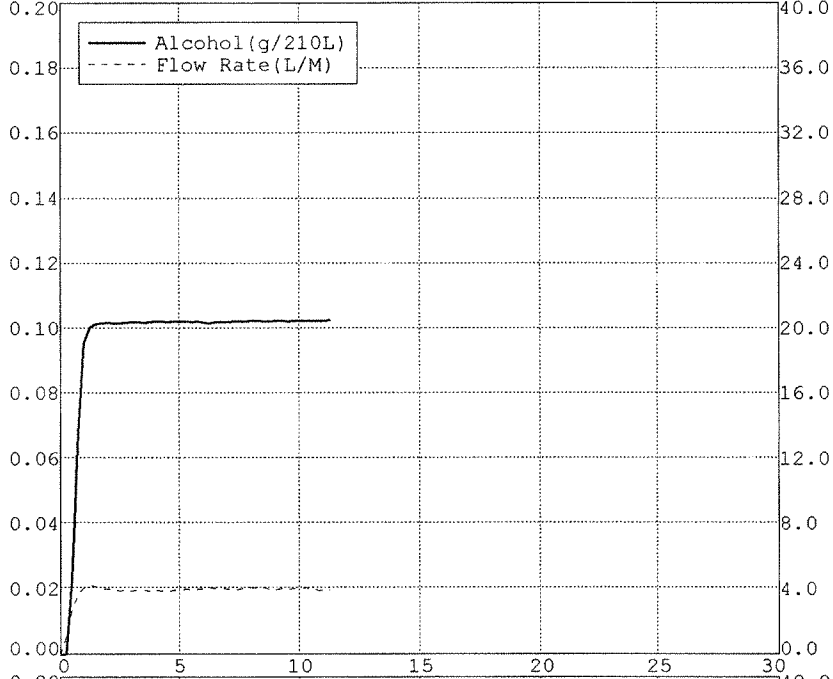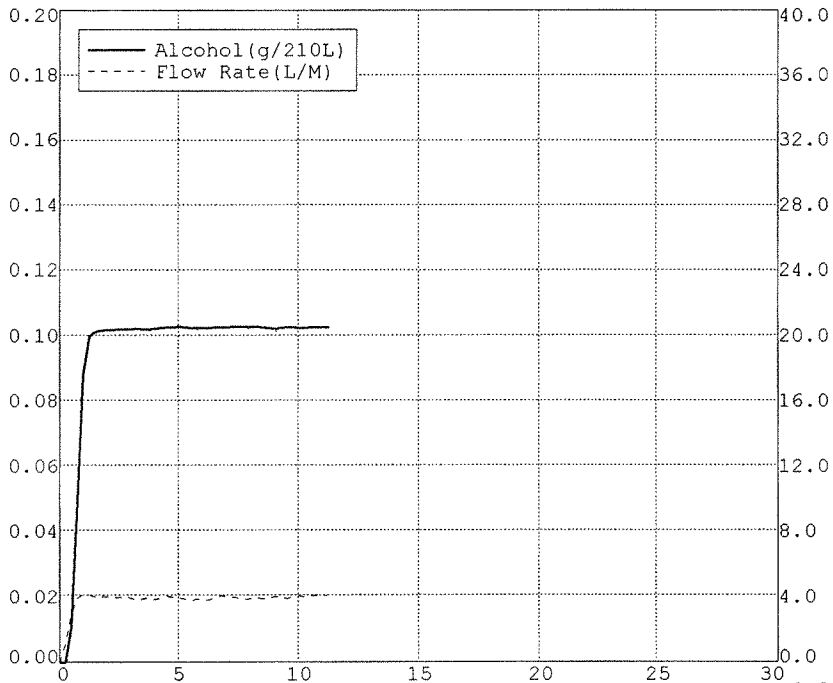

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 10/12/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25250

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:30
INTERNAL STANDARD	VERIFIED	18:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:31
BLANK TEST	0.00	18:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:32
BLANK TEST	0.00	18:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:33
BLANK TEST	0.00	18:34

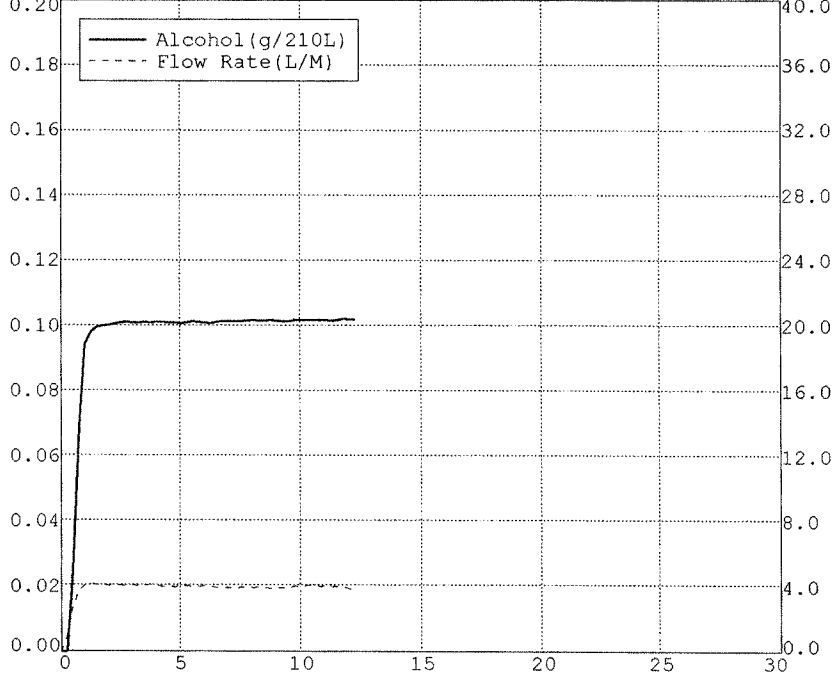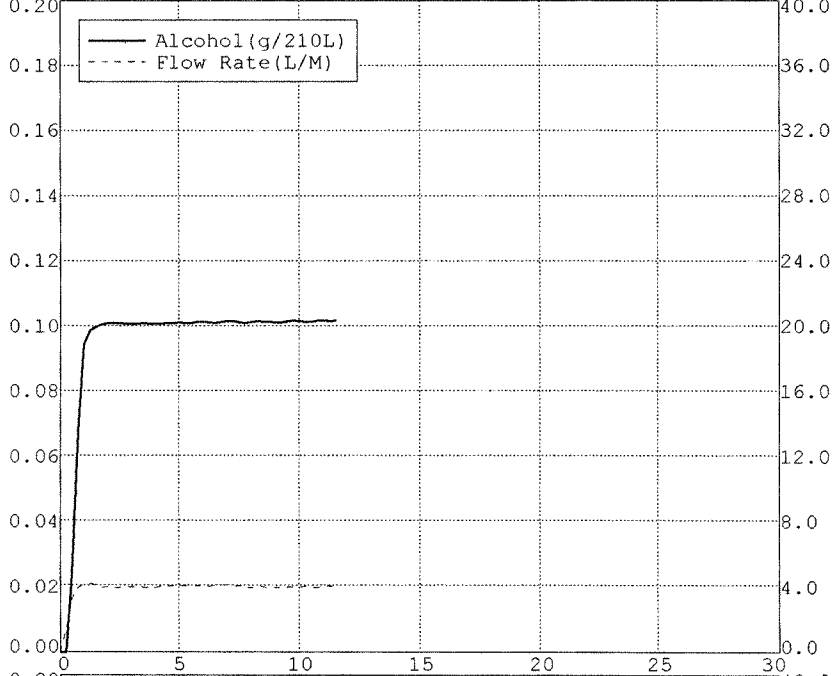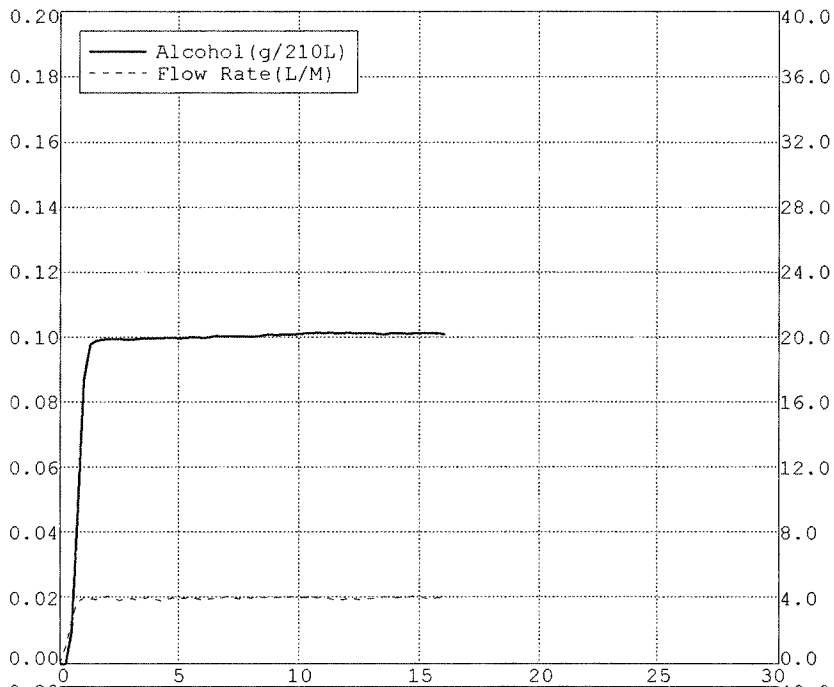

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 10/19/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25250

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:04
INTERNAL STANDARD	VERIFIED	22:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:05
BLANK TEST	0.00	22:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:06
BLANK TEST	0.00	22:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:07
BLANK TEST	0.00	22:08

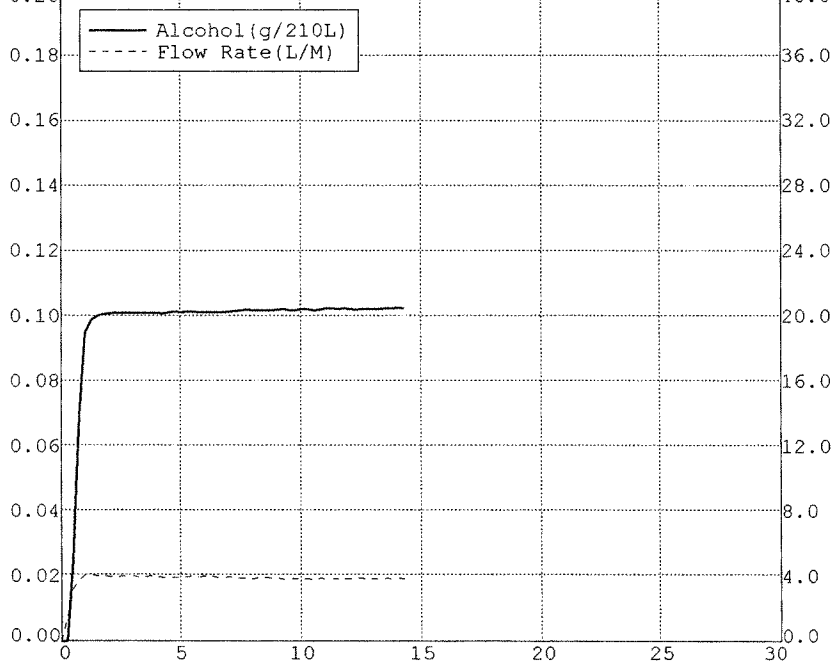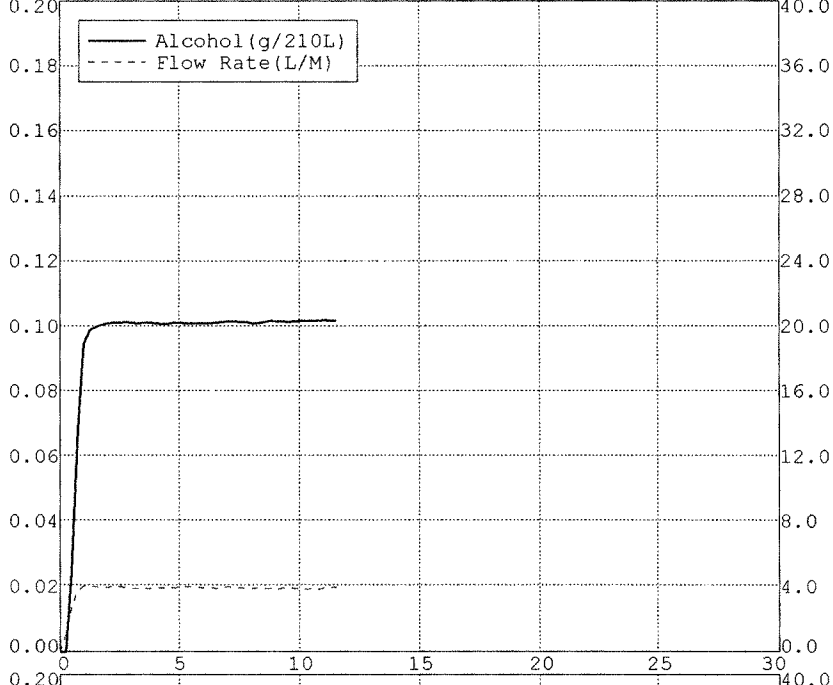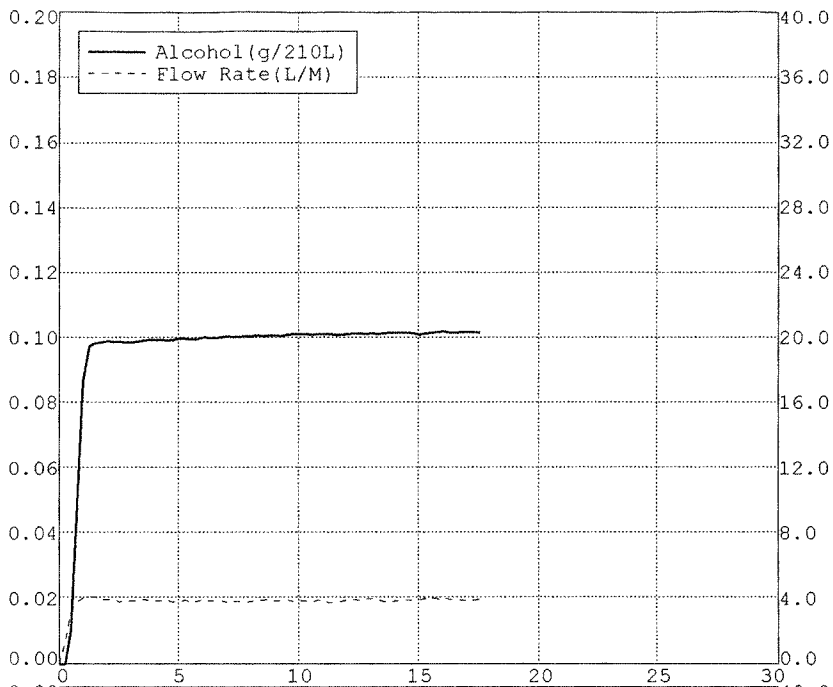

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 10/26/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25250

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:46
INTERNAL STANDARD	VERIFIED	15:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:47
BLANK TEST	0.00	15:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:48
BLANK TEST	0.00	15:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:49
BLANK TEST	0.00	15:50

