

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/03/2020

OPERATOR NAME:  
DORAN H SORRELL  
Permit #: 47507  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:53
INTERNAL STANDARD	VERIFIED	16:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:54
BLANK TEST	0.00	16:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:55
BLANK TEST	0.00	16:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:56
BLANK TEST	0.00	16:57

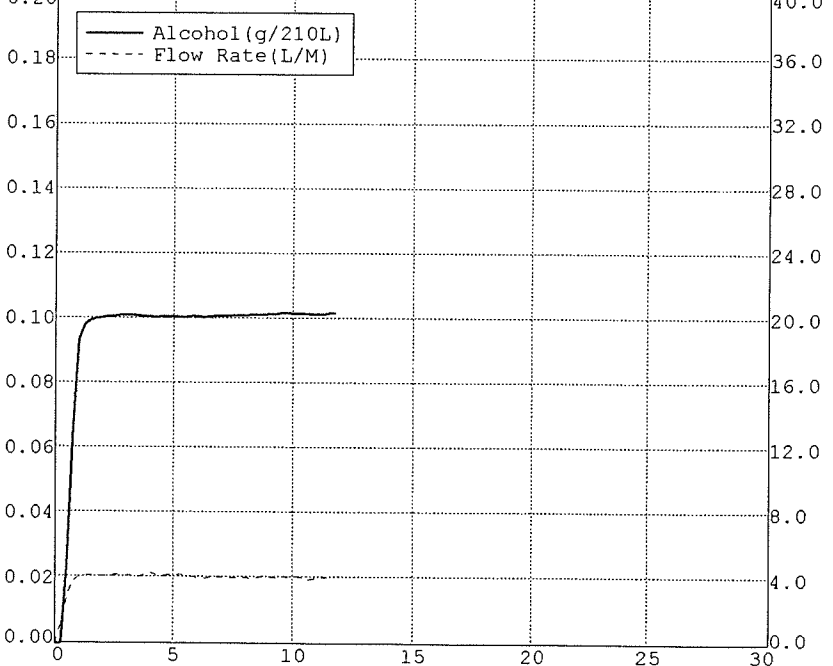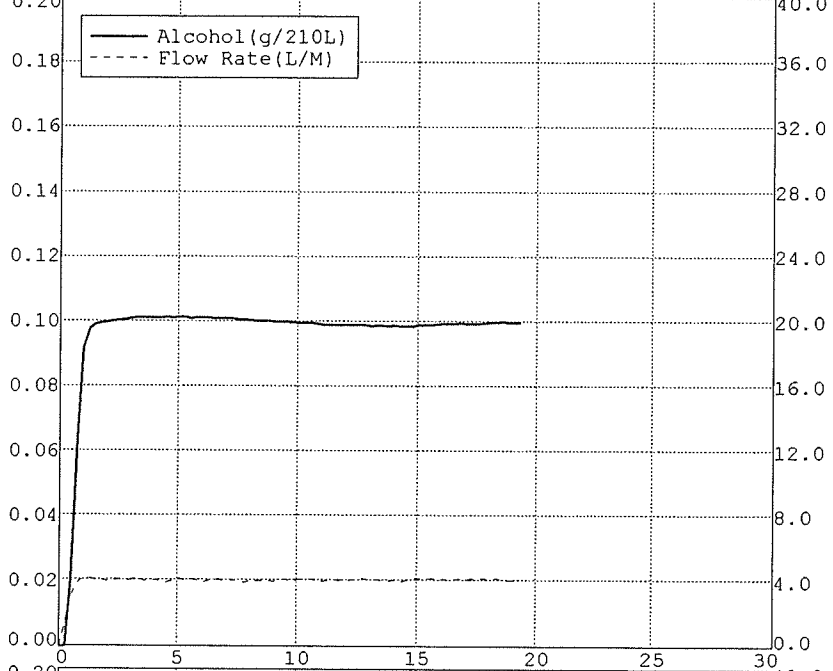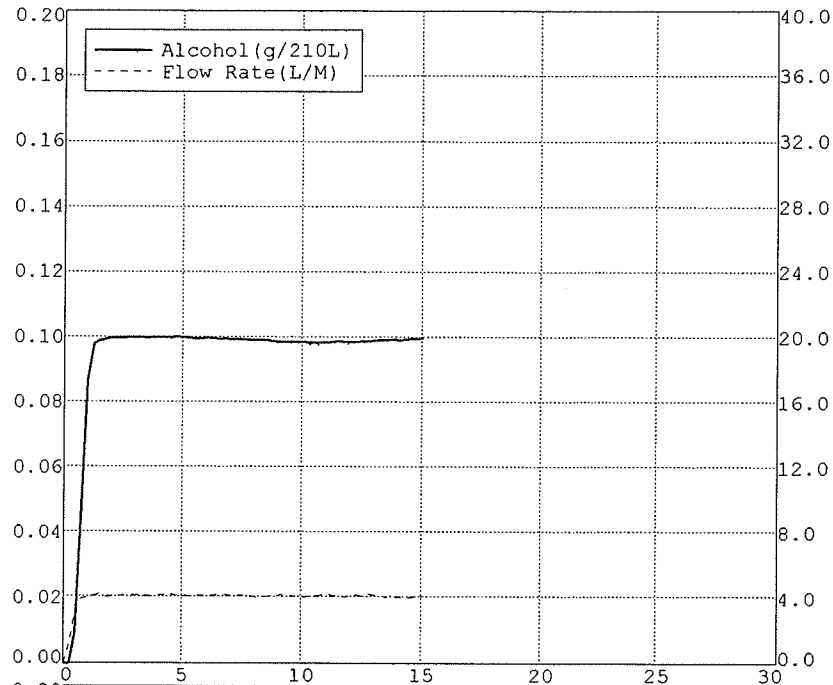

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/09/2020

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:27
INTERNAL STANDARD	VERIFIED	11:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:28
BLANK TEST	0.00	11:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:29
BLANK TEST	0.00	11:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:30
BLANK TEST	0.00	11:31

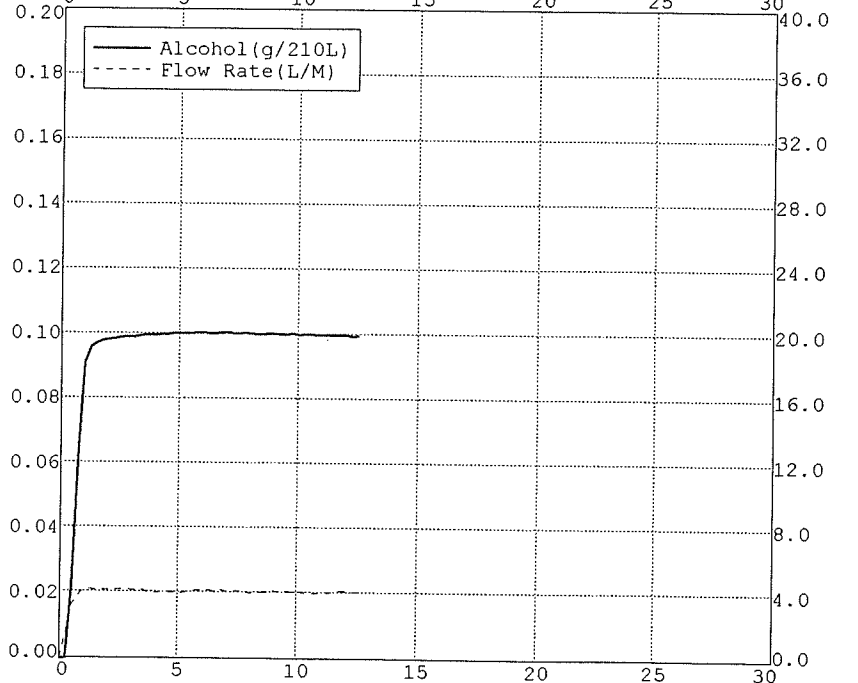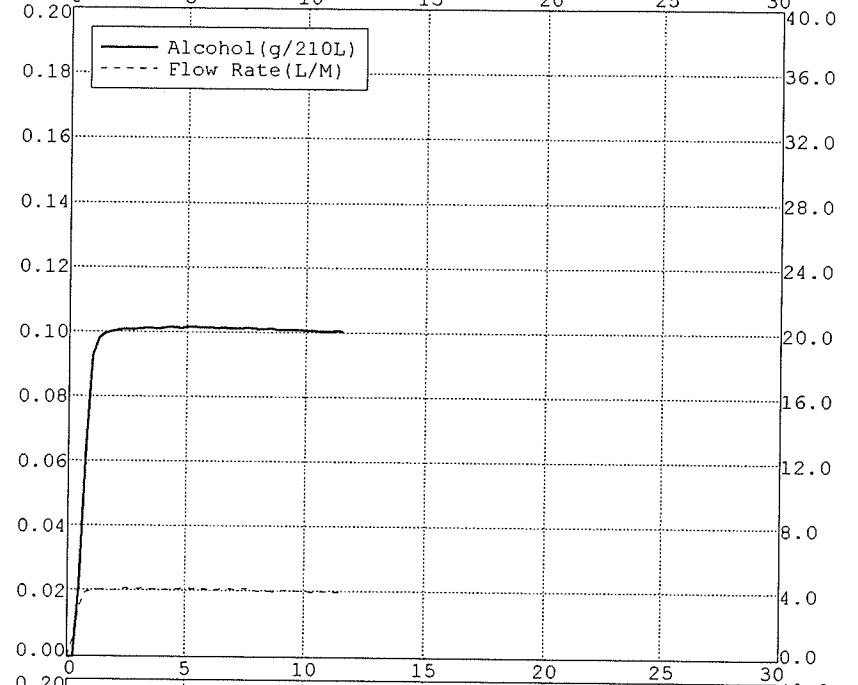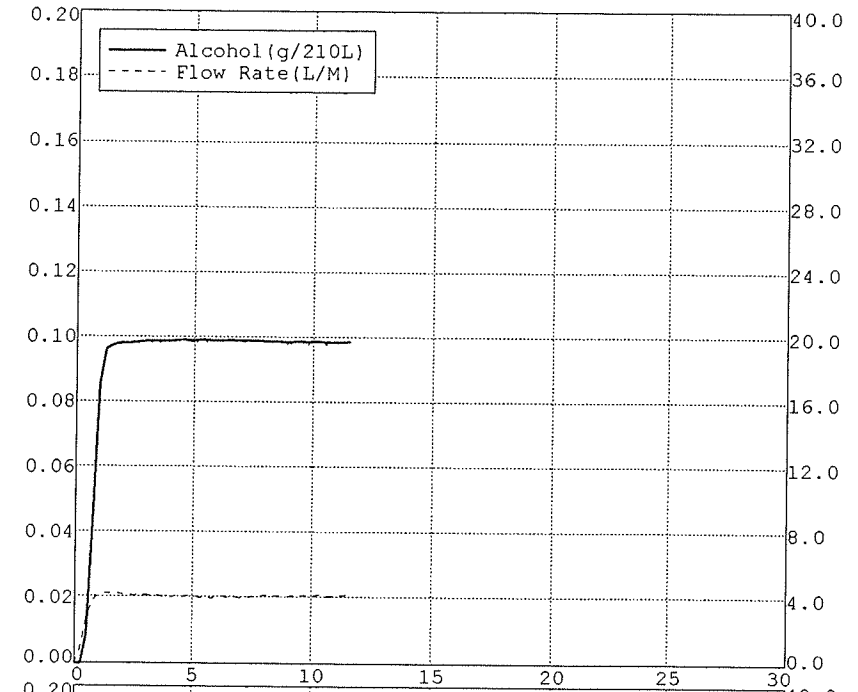

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/10/2020

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:11
INTERNAL STANDARD	VERIFIED	16:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:12
BLANK TEST	0.00	16:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:13
BLANK TEST	0.00	16:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:14
BLANK TEST	0.00	16:15

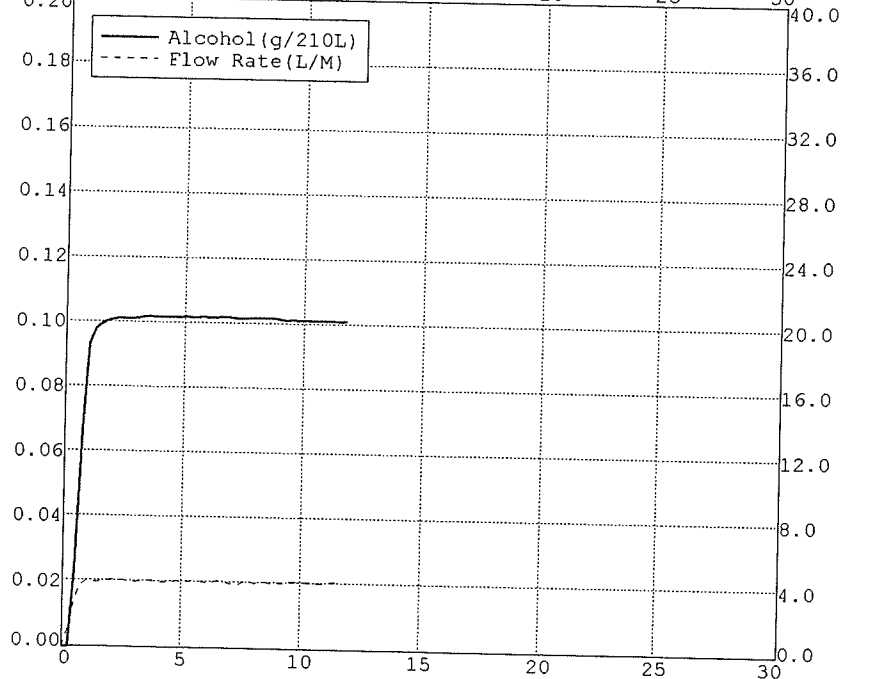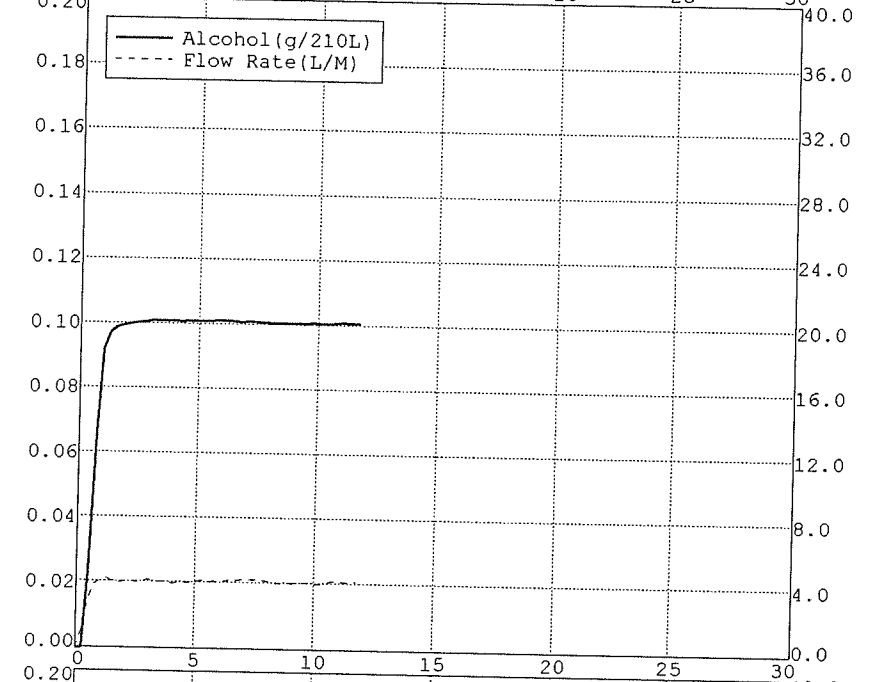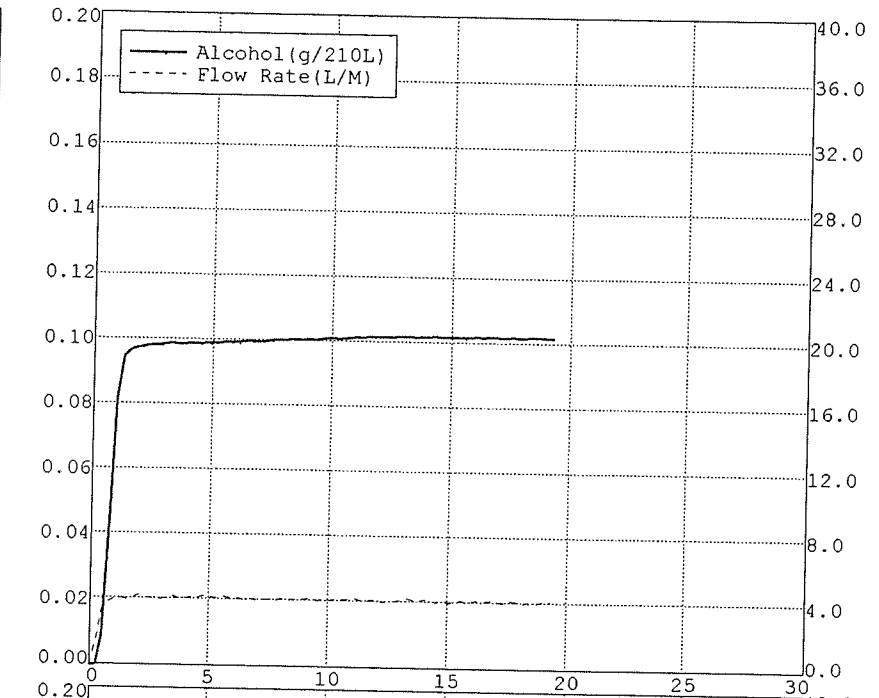

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/17/2020

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:48
INTERNAL STANDARD	VERIFIED	07:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:48
BLANK TEST	0.00	07:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:49
BLANK TEST	0.00	07:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:51
BLANK TEST	0.00	07:51

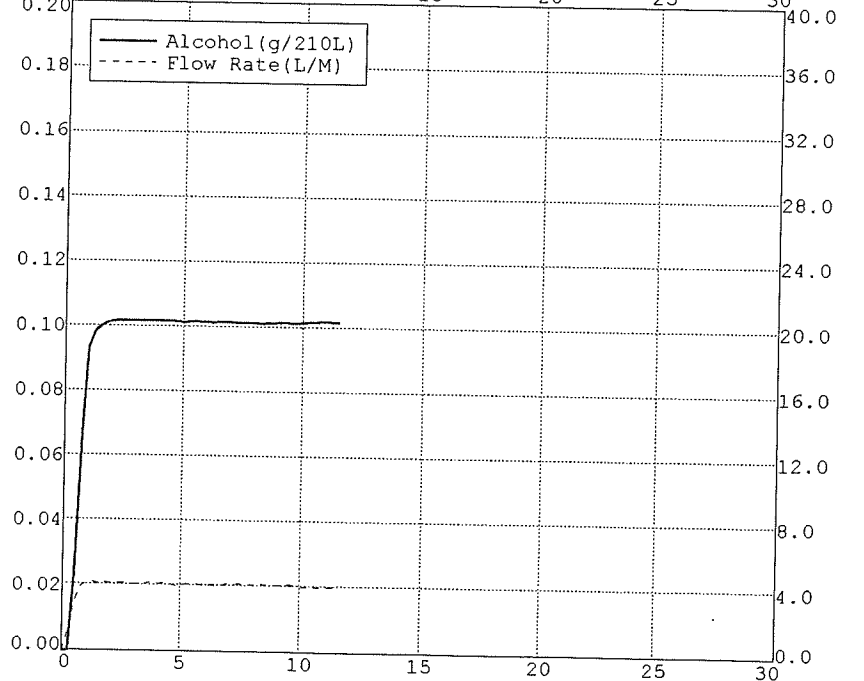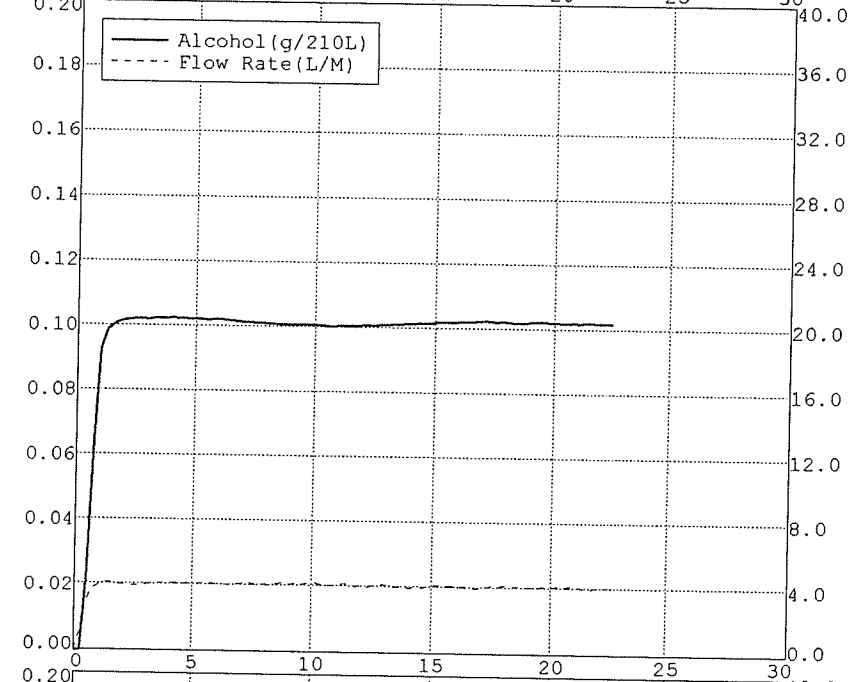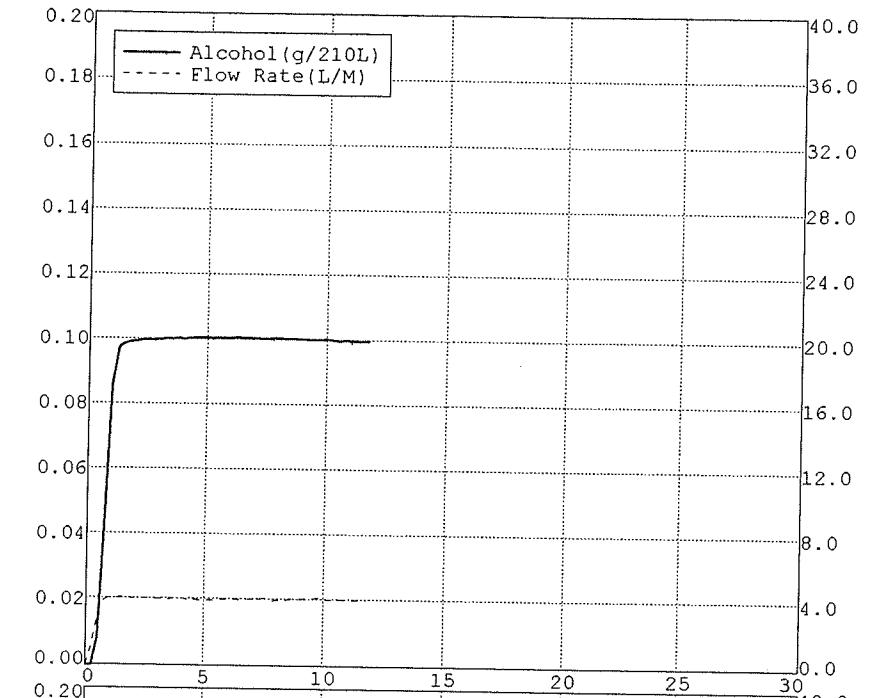

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/23/2020

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:53
INTERNAL STANDARD	VERIFIED	07:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:54
BLANK TEST	0.00	07:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:55
BLANK TEST	0.00	07:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:56
BLANK TEST	0.00	07:57

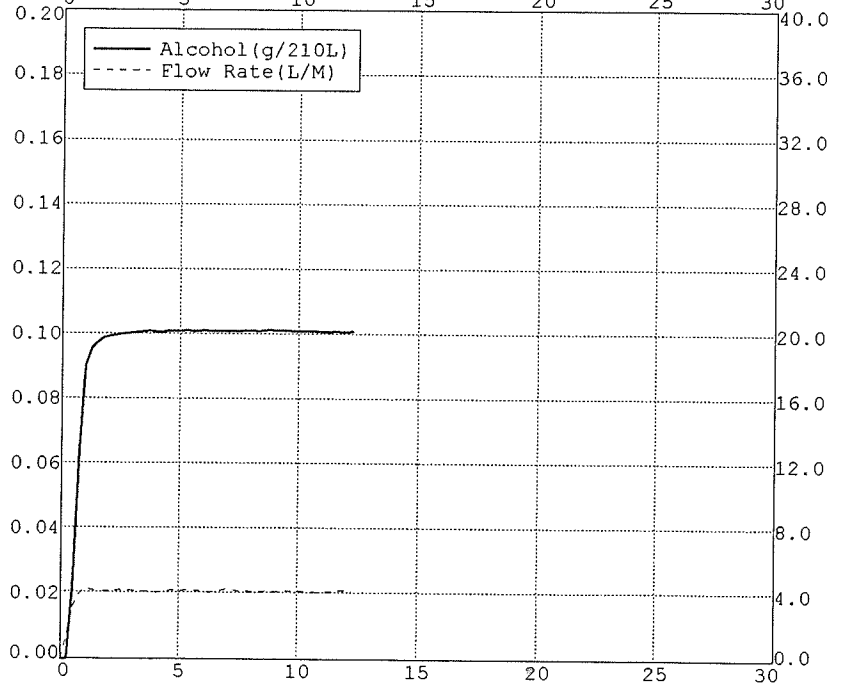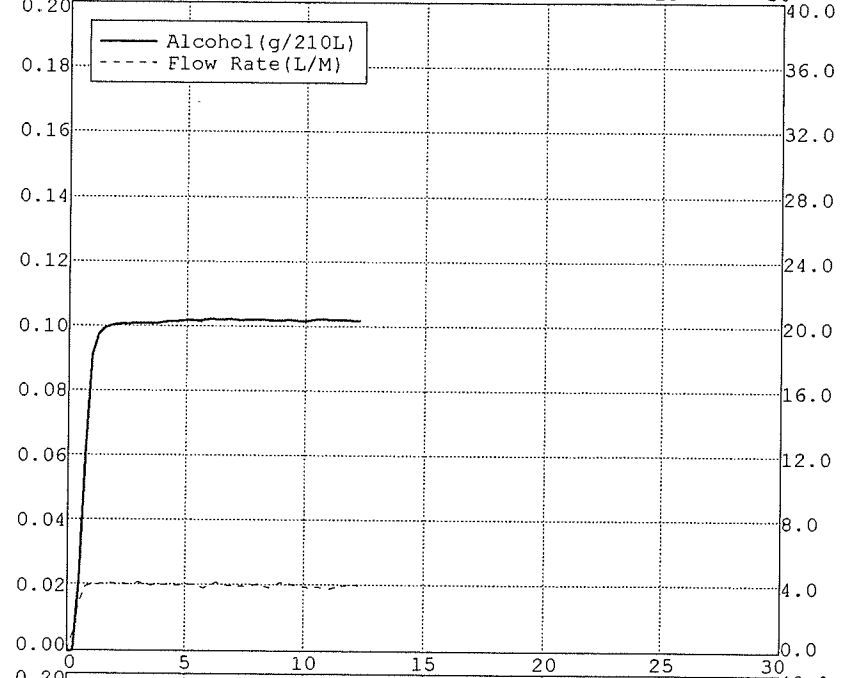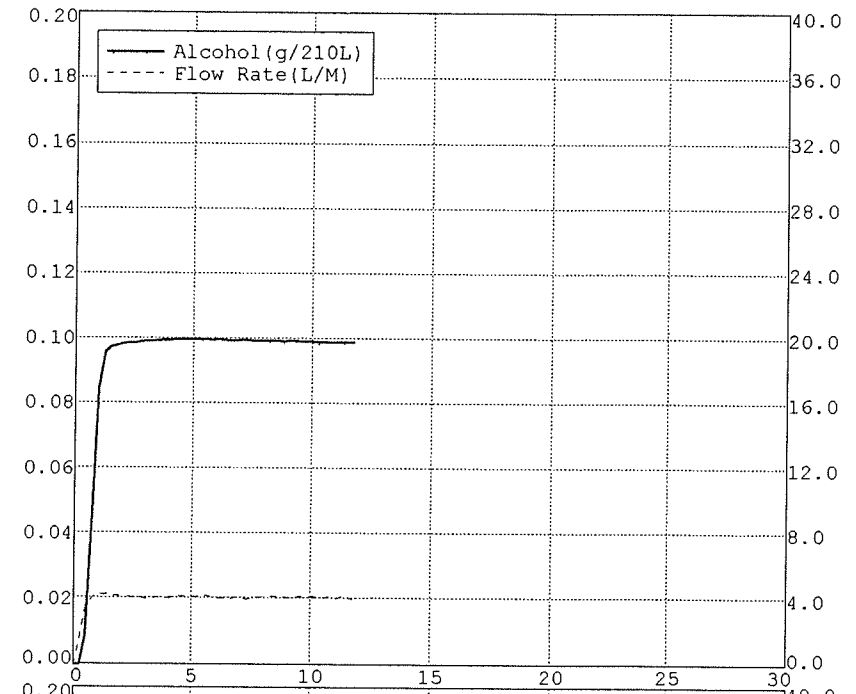

SUPERVISOR TEST

LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/31/2020

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:52
INTERNAL STANDARD	VERIFIED	08:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:52
BLANK TEST	0.00	08:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:53
BLANK TEST	0.00	08:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:54
BLANK TEST	0.00	08:55

