

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/07/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:54
INTERNAL STANDARD	VERIFIED	17:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:54
BLANK TEST	0.00	17:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:55
BLANK TEST	0.00	17:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:56
BLANK TEST	0.00	17:57

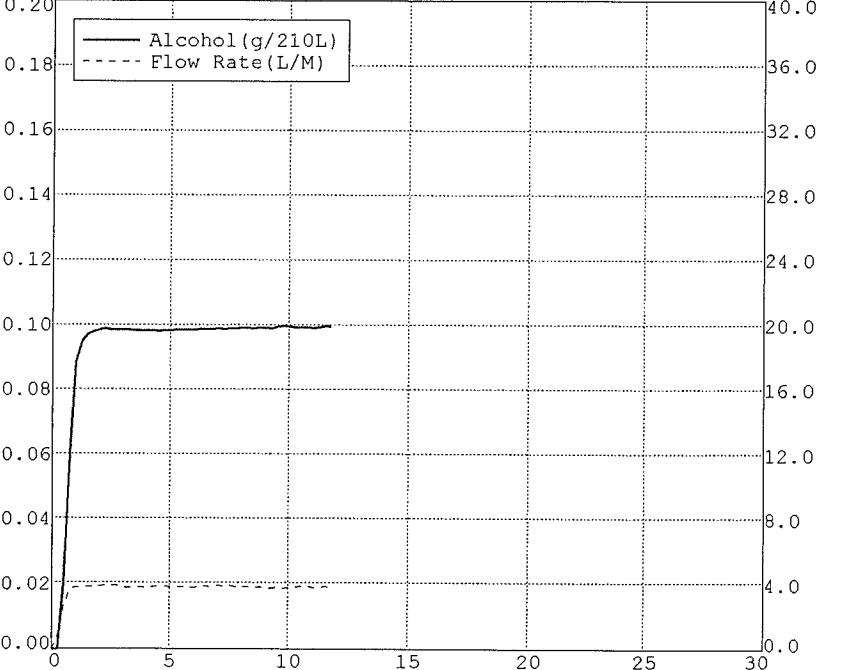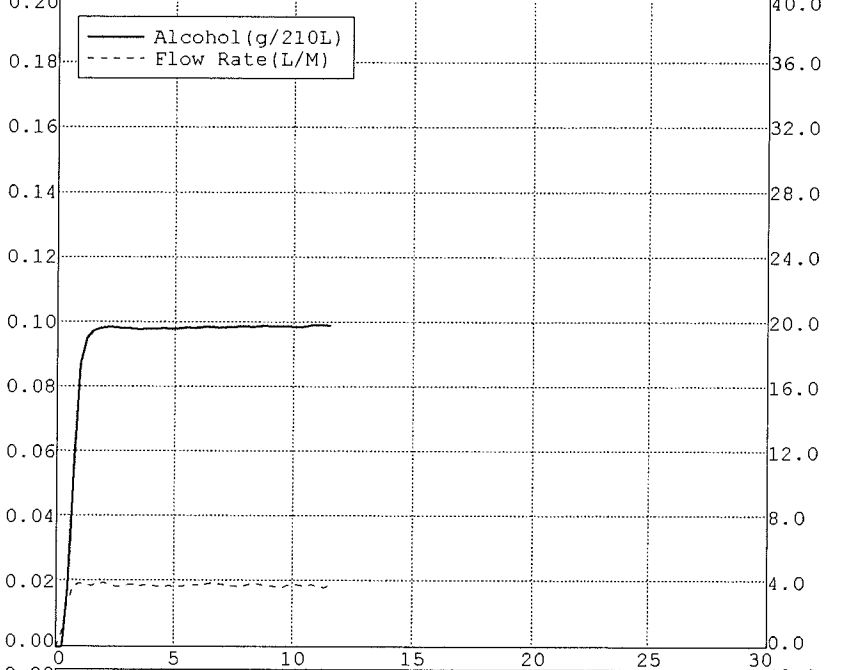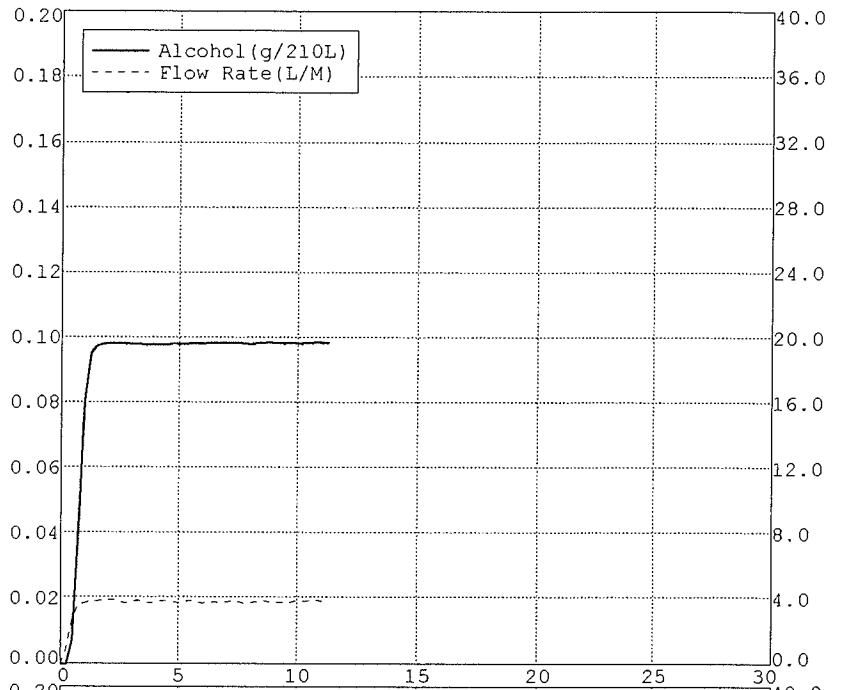

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/13/2023

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:24
INTERNAL STANDARD	VERIFIED	02:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:24
BLANK TEST	0.00	02:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:25
BLANK TEST	0.00	02:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:26
BLANK TEST	0.00	02:27

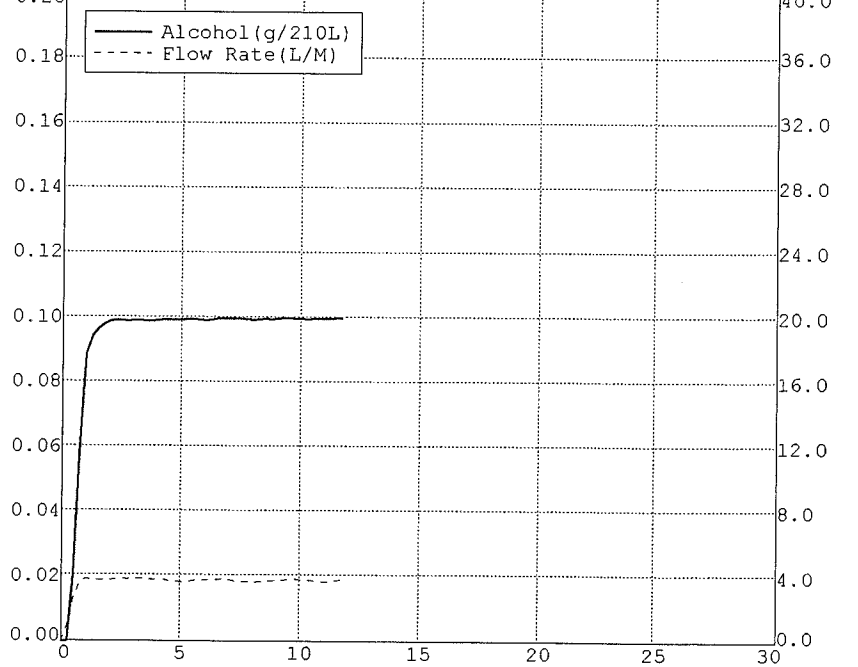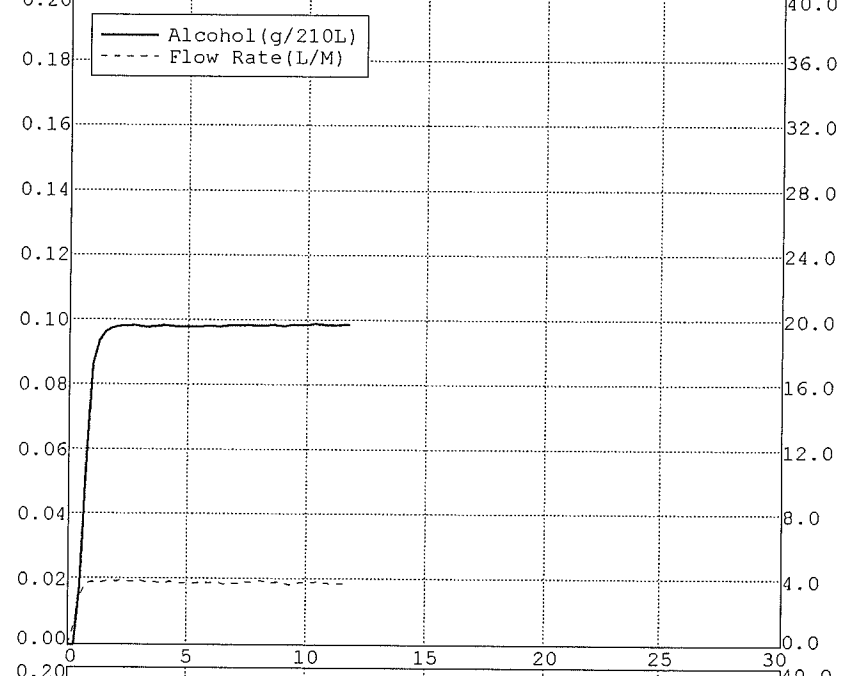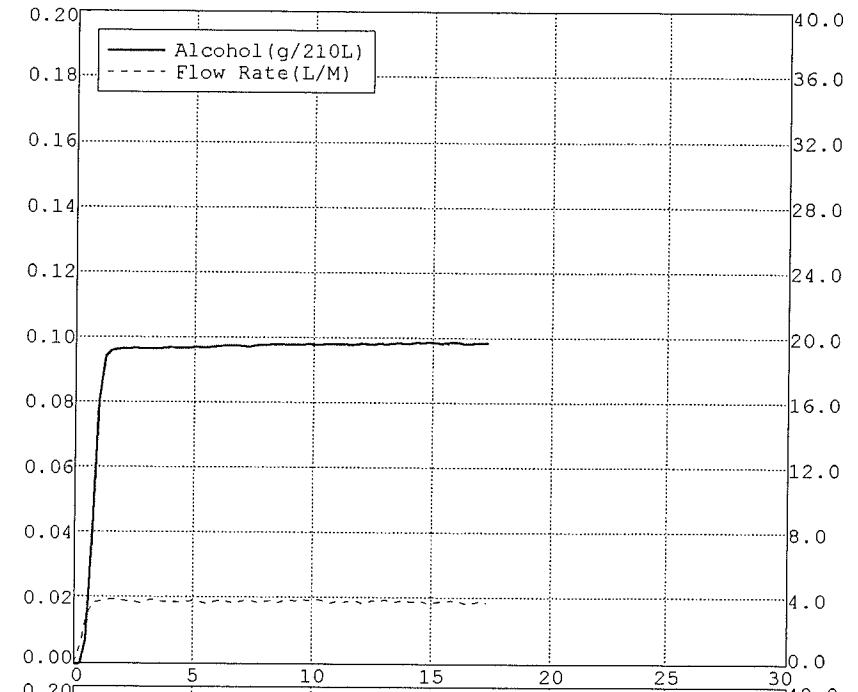

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/21/2023

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:54
INTERNAL STANDARD	VERIFIED	21:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:55
BLANK TEST	0.00	21:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:56
BLANK TEST	0.00	21:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:57
BLANK TEST	0.00	21:58

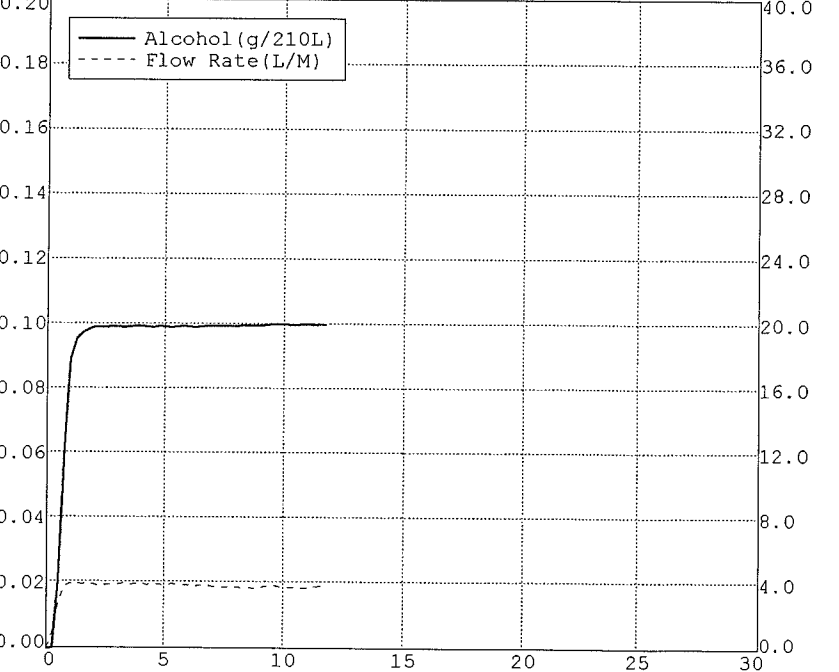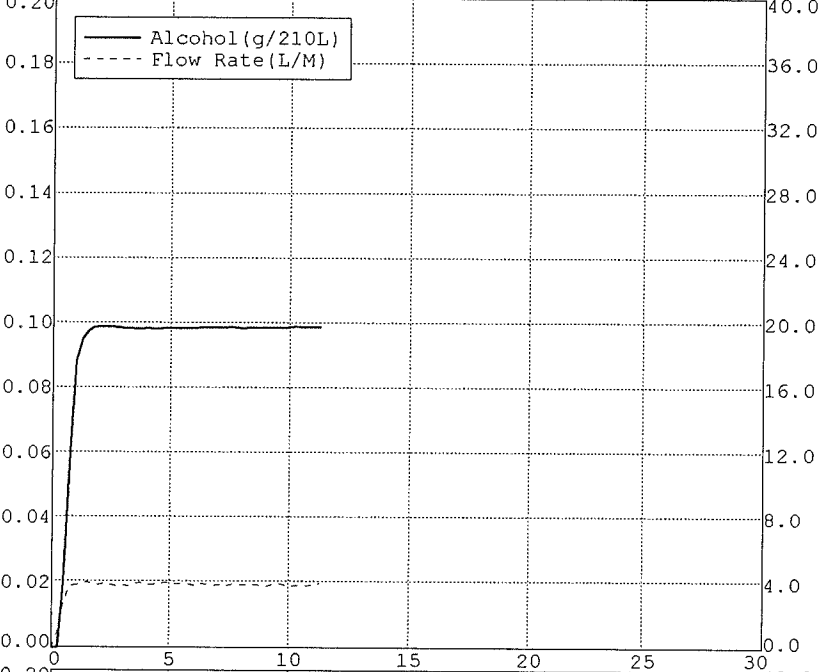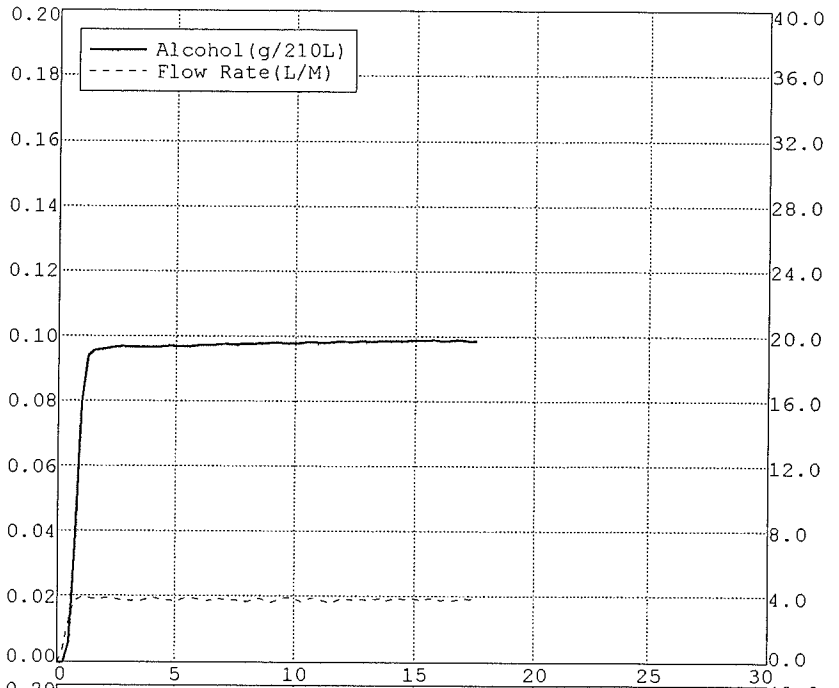

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 08/27/2023

OPERATOR NAME:
MAKENZIE A FULLER
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:44
INTERNAL STANDARD	VERIFIED	18:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:45
BLANK TEST	0.00	18:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:46
BLANK TEST	0.00	18:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:47
BLANK TEST	0.00	18:48

