

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/03/2019

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:24
INTERNAL STANDARD	VERIFIED	07:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:25
BLANK TEST	0.00	07:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:26
BLANK TEST	0.00	07:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:27
BLANK TEST	0.00	07:28

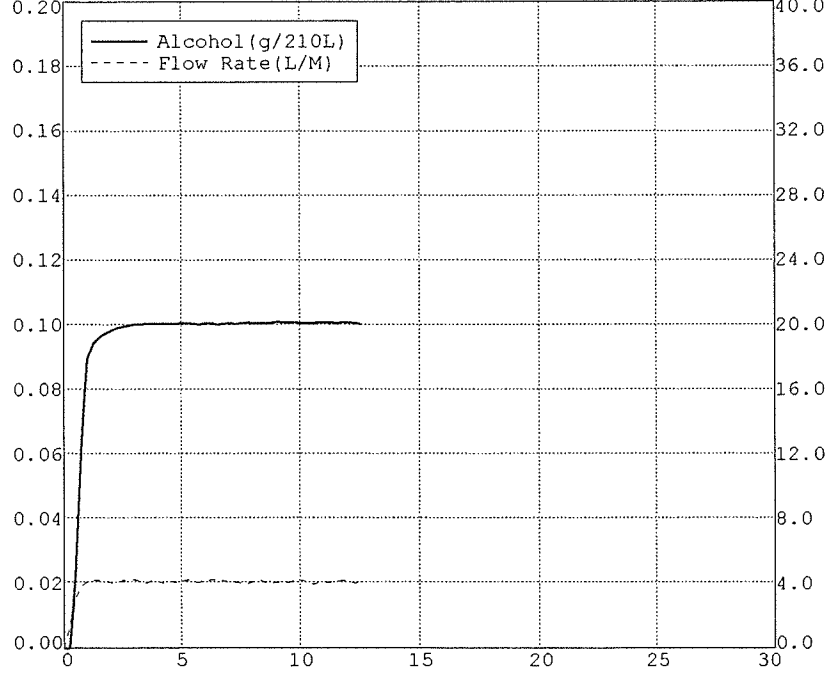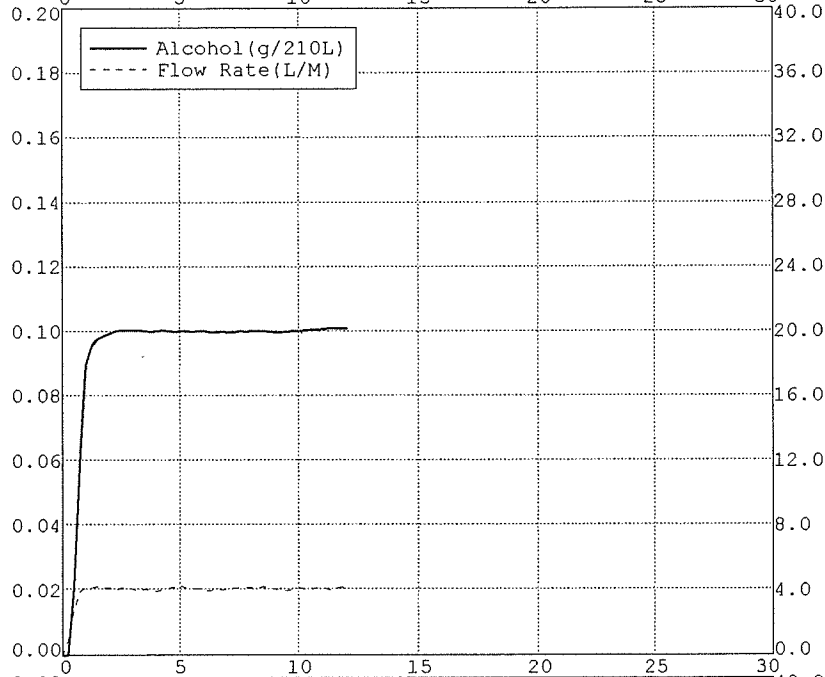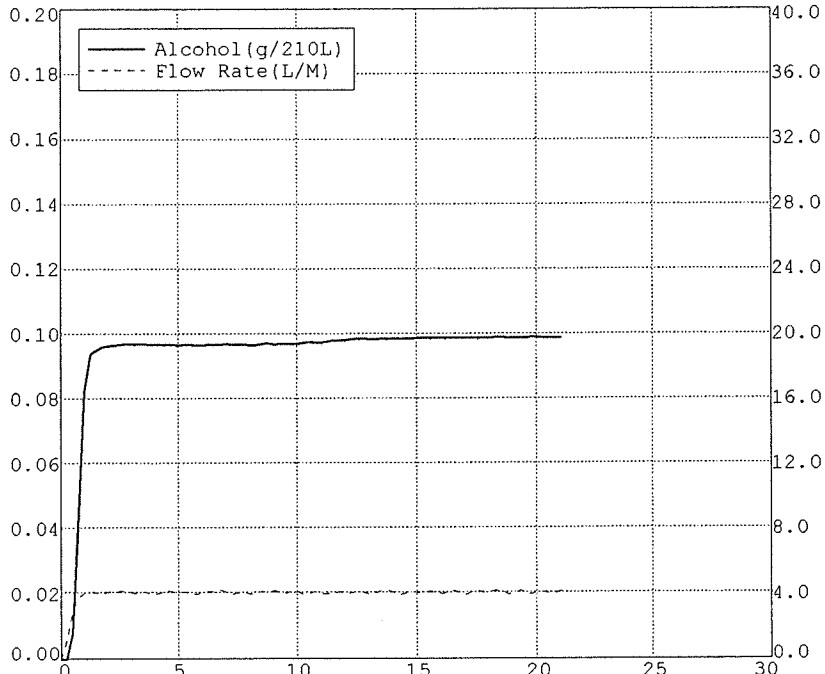

SUPERVISOR TEST




LAKE PLACID VILLAGE
 POLICE DEPT.
 DATAMASTER dmt: 100290

Date: 11/11/2019

OPERATOR NAME:
 DORAN H SORRELL
 Permit #: 47507
 Operator Agency/Dept: LAKE PLACID VILL. PD
 Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:34
INTERNAL STANDARD	VERIFIED	14:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:35
BLANK TEST	0.00	14:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:36
BLANK TEST	0.00	14:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:37
BLANK TEST	0.00	14:38

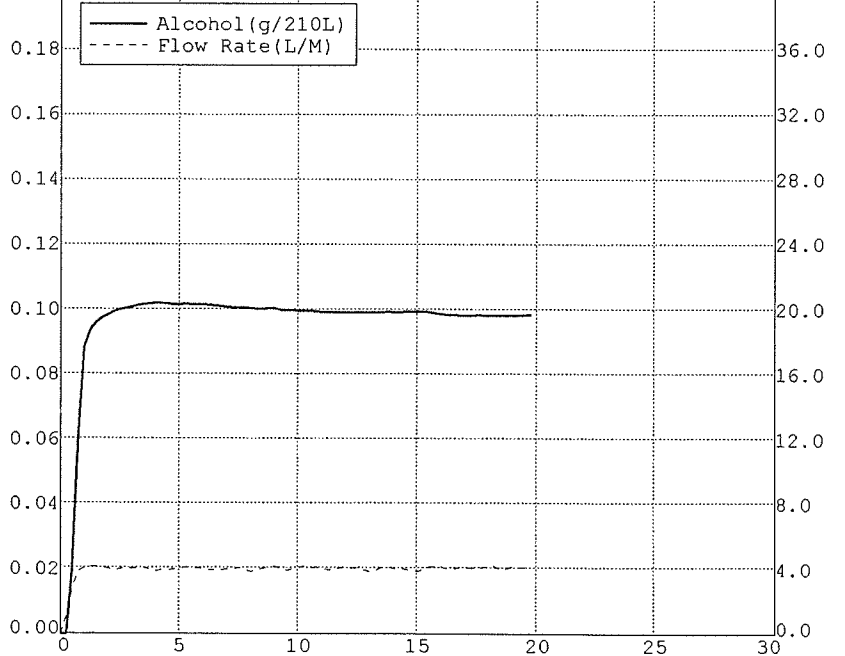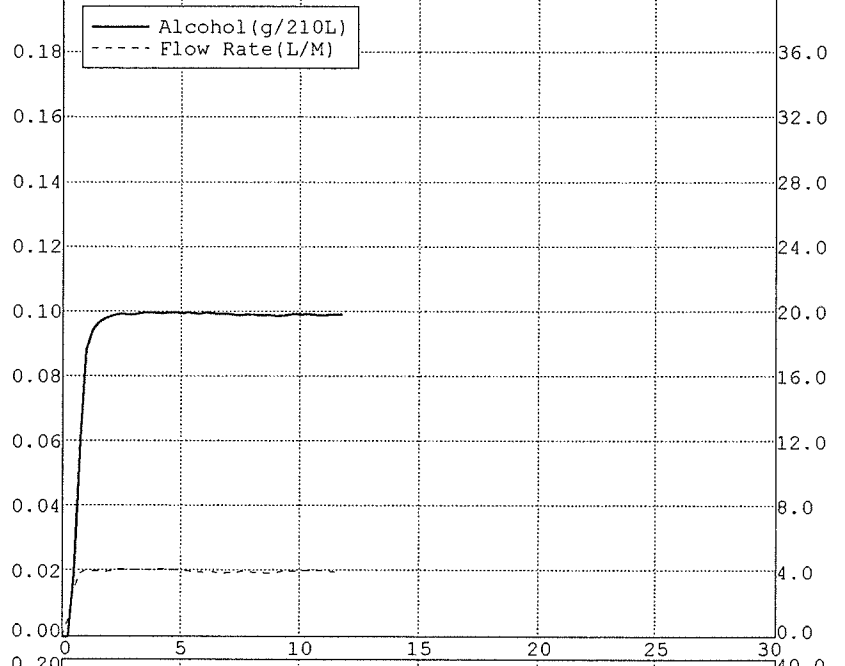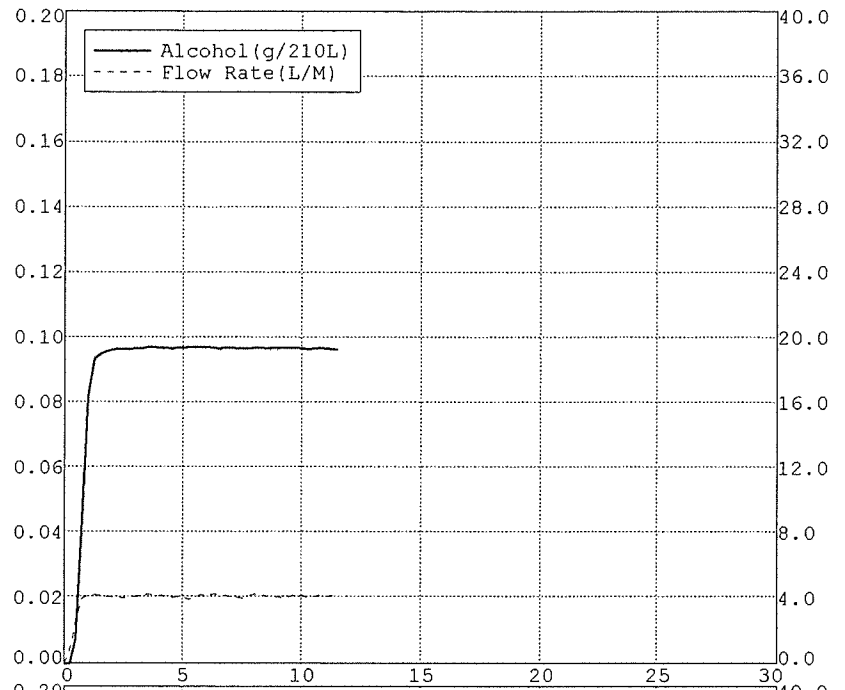

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/17/2019

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:10
INTERNAL STANDARD	VERIFIED	20:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:10
BLANK TEST	0.00	20:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:11
BLANK TEST	0.00	20:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:13
BLANK TEST	0.00	20:13

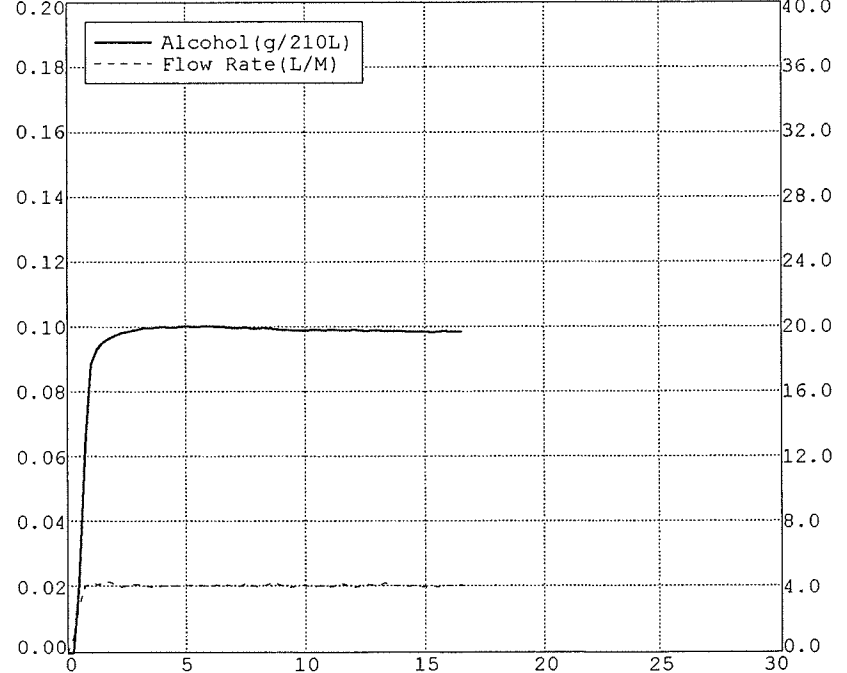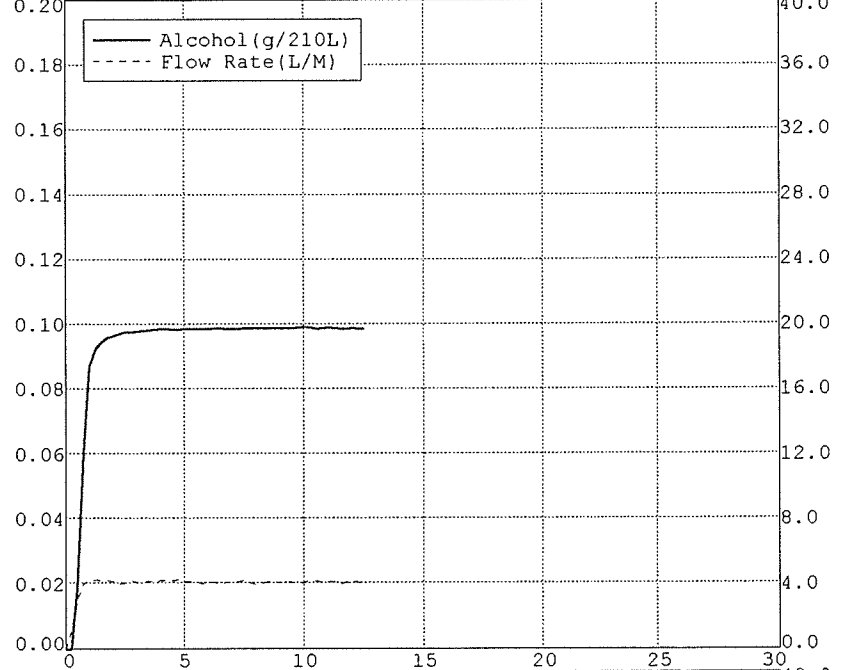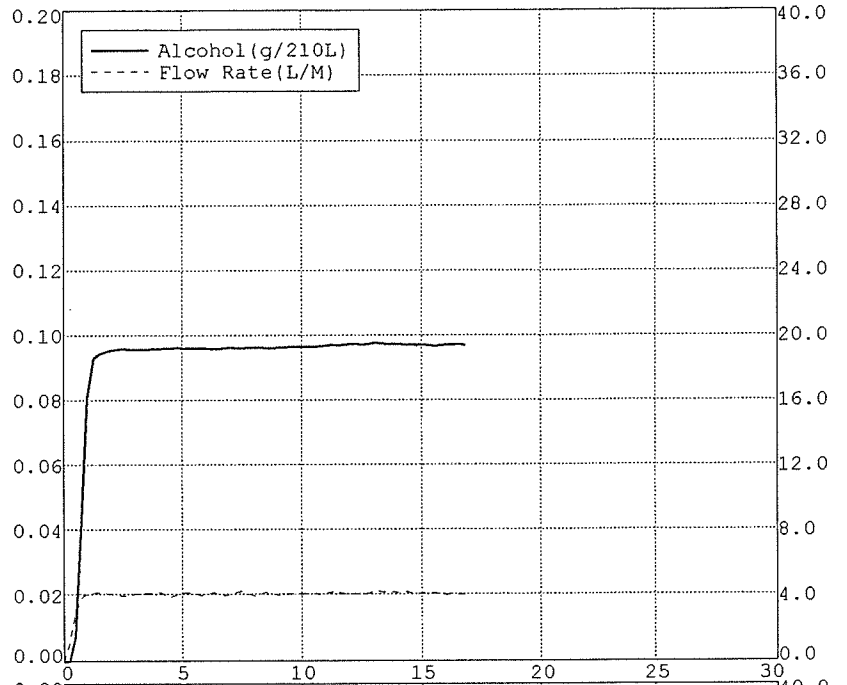

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 11/25/2019

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:10
INTERNAL STANDARD	VERIFIED	08:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:10
BLANK TEST	0.00	08:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:11
BLANK TEST	0.00	08:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:13
BLANK TEST	0.00	08:13

