

SOLUTION CHANGE




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/01/2021

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:07
INTERNAL STANDARD	VERIFIED	16:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:08
BLANK TEST	0.00	16:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:09
BLANK TEST	0.00	16:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:10
BLANK TEST	0.00	16:11

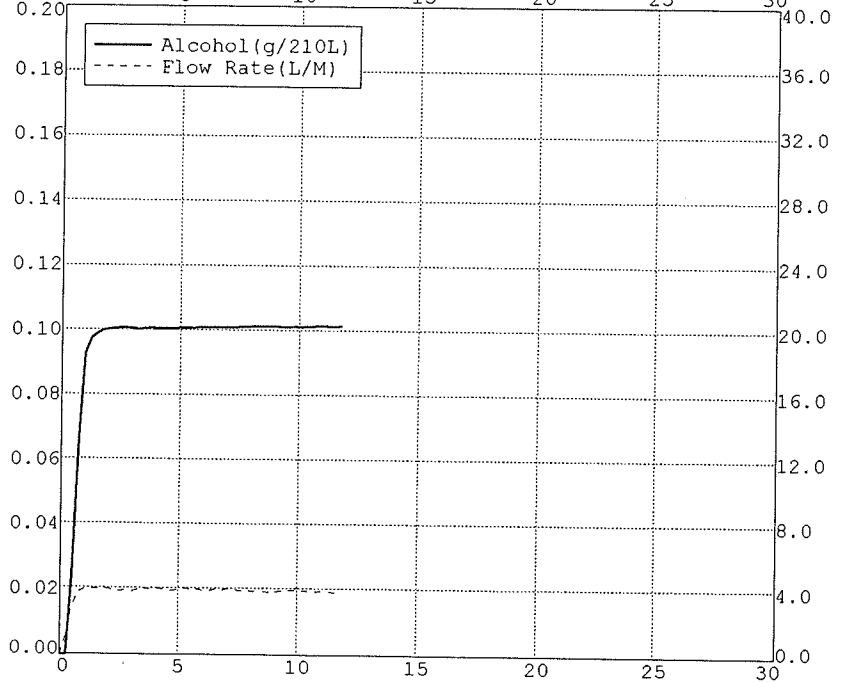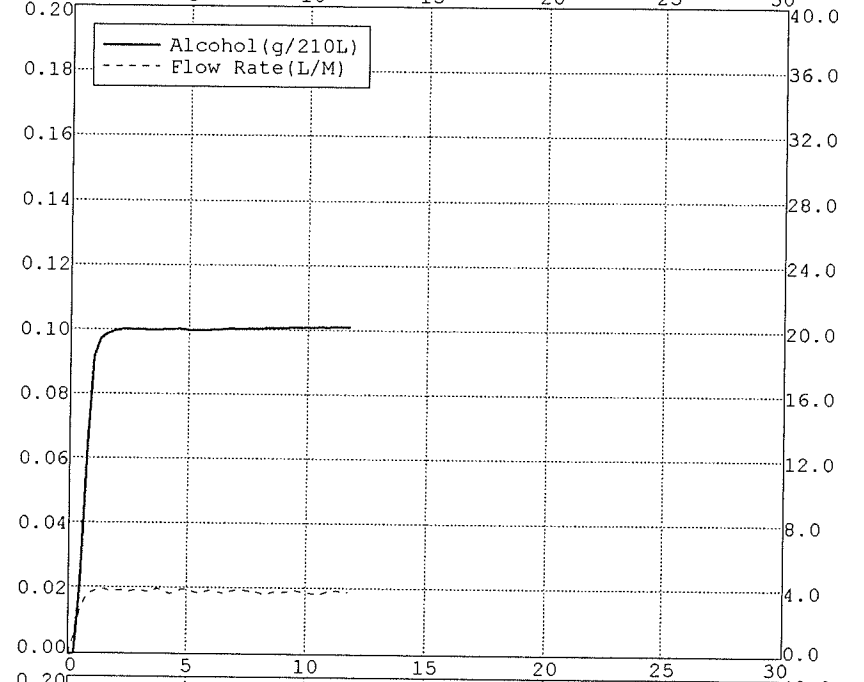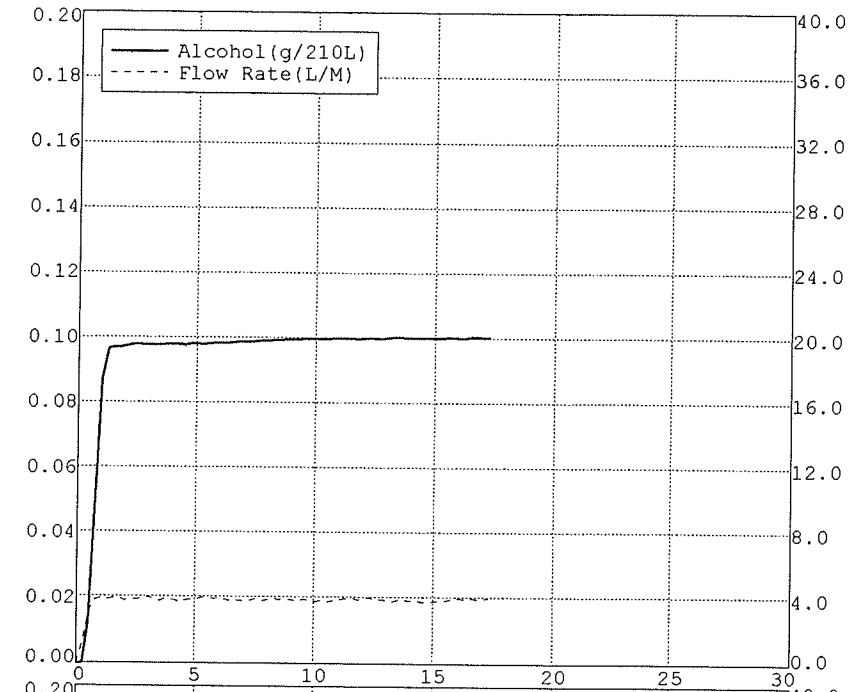

TECHNICIAN TEST


LAKE PLACID VILLAGE  
 POLICE DEPT.  
 DATAMASTER dmt: 100290

Date: 08/02/2021

Nominal = 0.100 g/210L

BLANK TEST	0.000	09:25
INTERNAL STANDARD	VERIFIED	09:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.096	09:26
BLANK TEST	0.000	09:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.096	09:27
BLANK TEST	0.000	09:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.098	09:28
BLANK TEST	0.000	09:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.098	09:29
BLANK TEST	0.000	09:30

Average = 0.0970  
 Std Dev = 0.0012

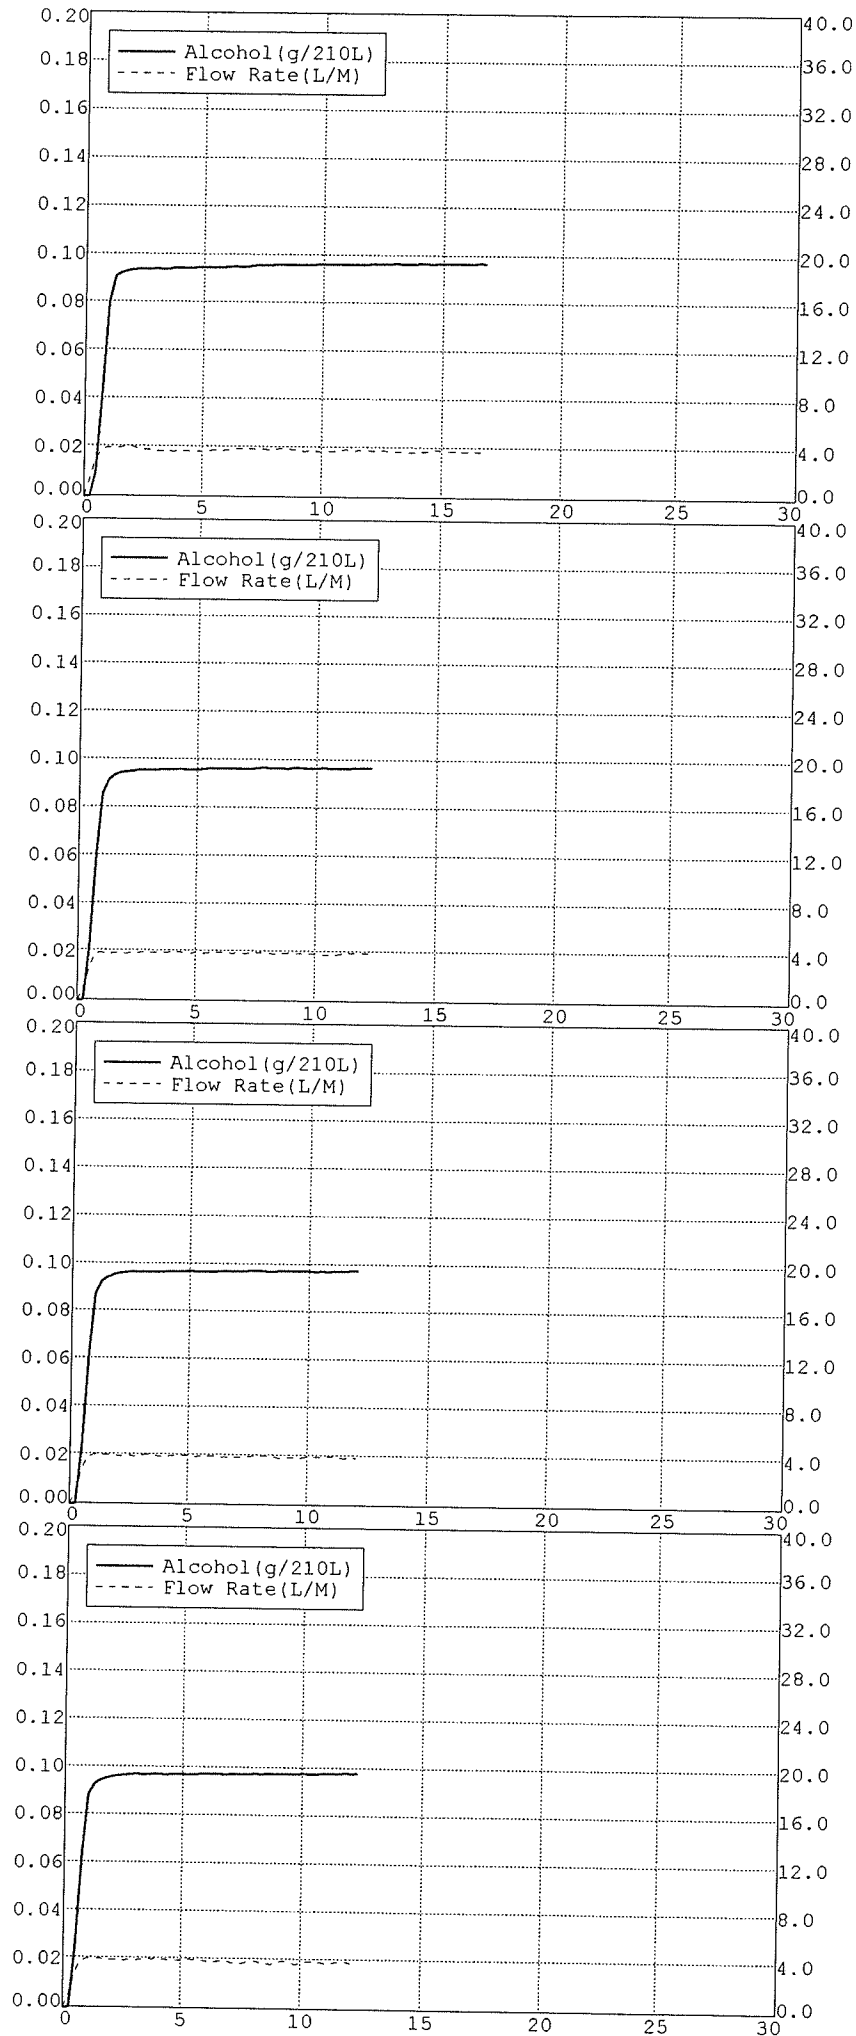

SUPERVISOR TEST




-----  
LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290  
-----

Date: 08/08/2021

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:45
INTERNAL STANDARD	VERIFIED	12:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:46
BLANK TEST	0.00	12:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:47
BLANK TEST	0.00	12:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:48
BLANK TEST	0.00	12:49

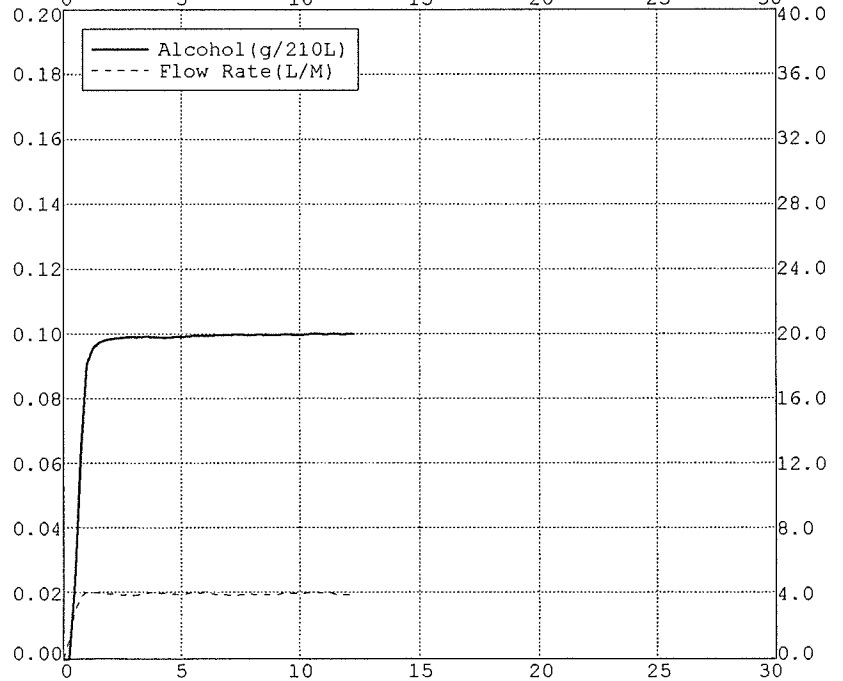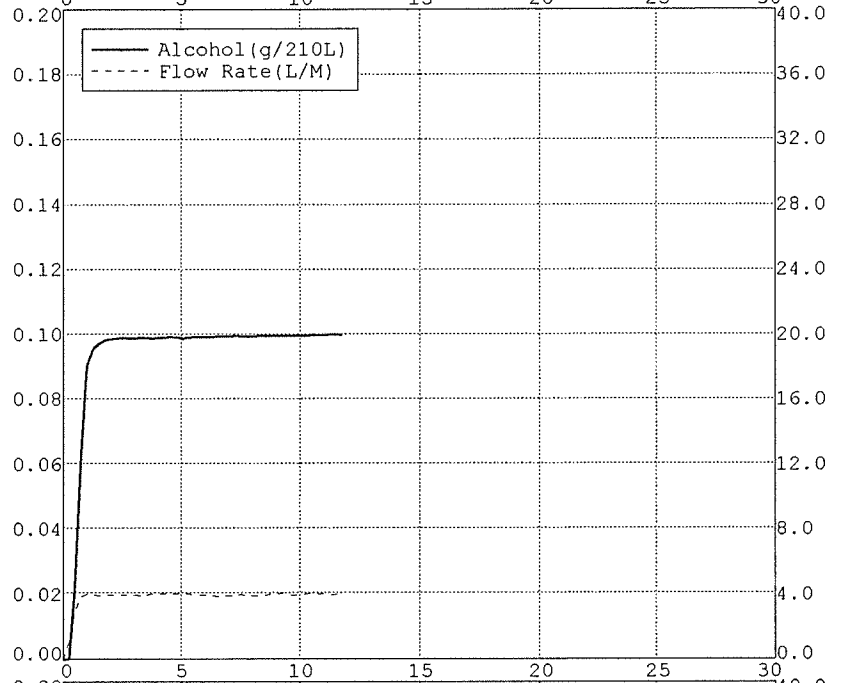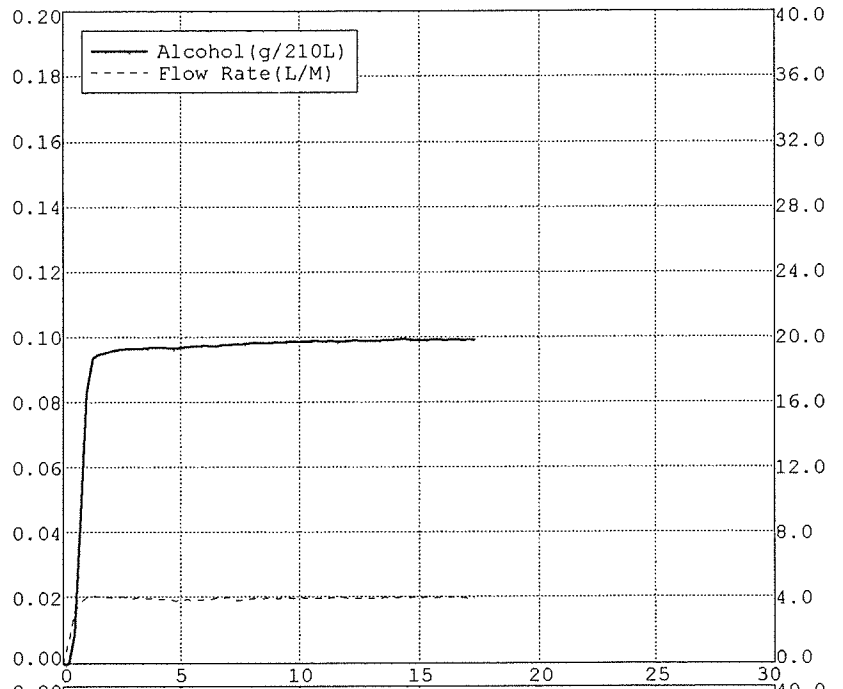

SUPERVISOR TEST




LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/16/2021

OPERATOR NAME:  
DORAN H SORRELL  
Permit #: 47507  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:02
INTERNAL STANDARD	VERIFIED	06:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:03
BLANK TEST	0.00	06:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:04
BLANK TEST	0.00	06:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:05
BLANK TEST	0.00	06:06

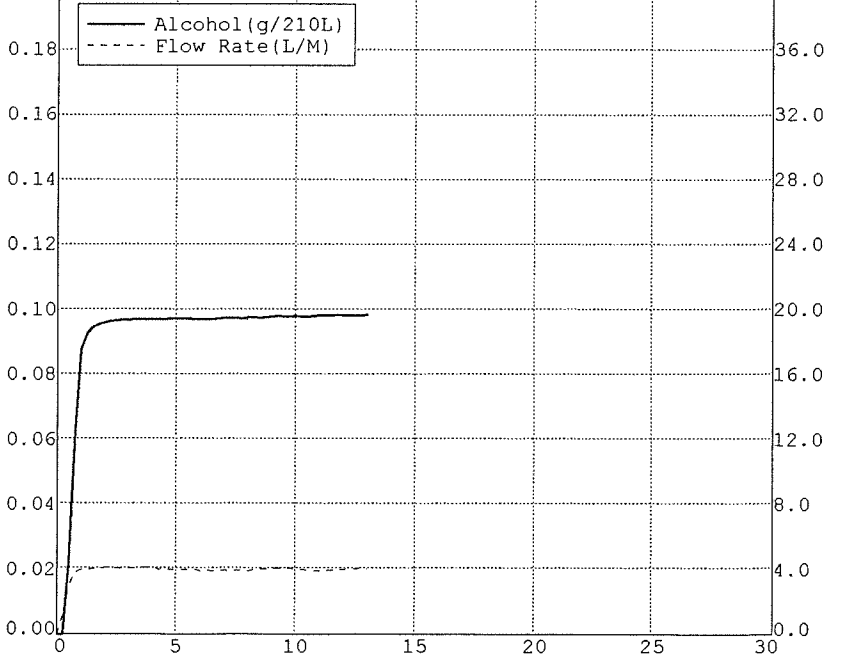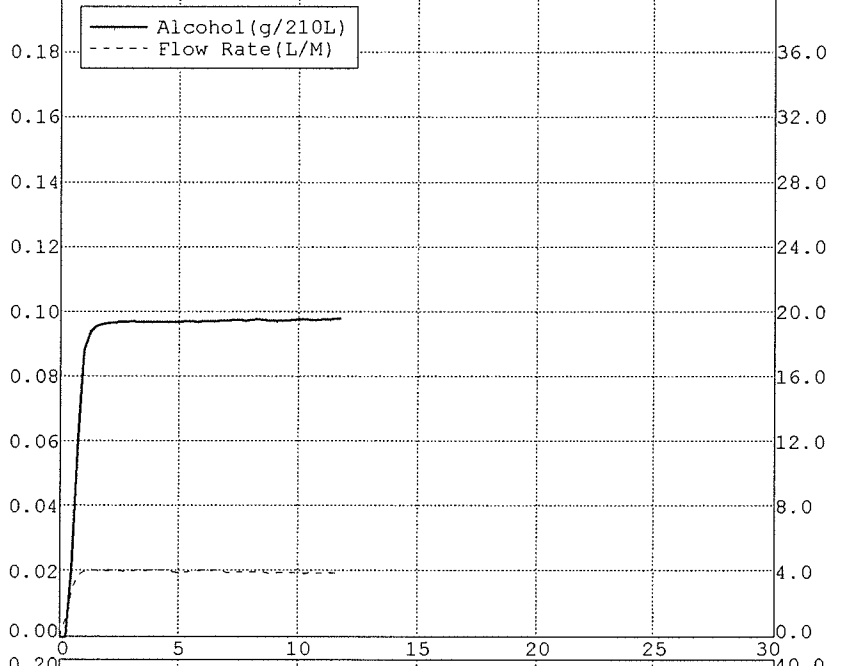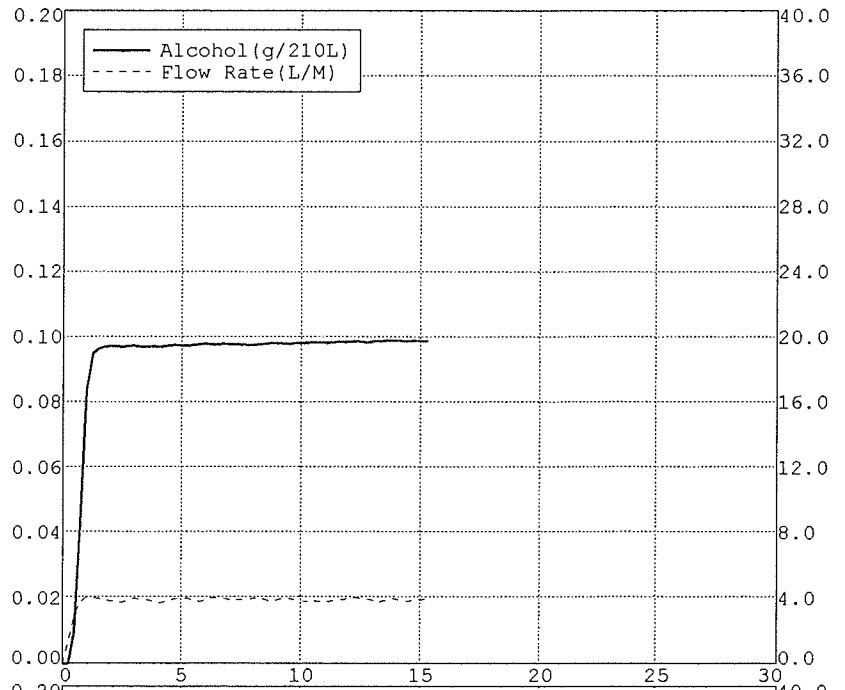

SUPERVISOR TEST



LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290

Date: 08/22/2021

OPERATOR NAME:  
CHAD P BLINN  
Permit #: 33034  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:32
INTERNAL STANDARD	VERIFIED	06:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:32
BLANK TEST	0.00	06:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:33
BLANK TEST	0.00	06:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:35
BLANK TEST	0.00	06:35

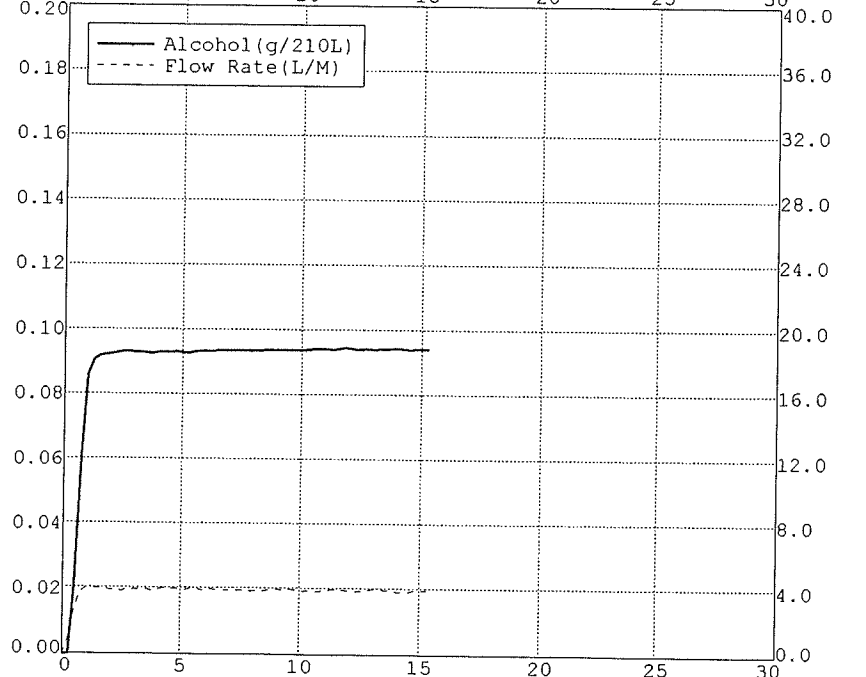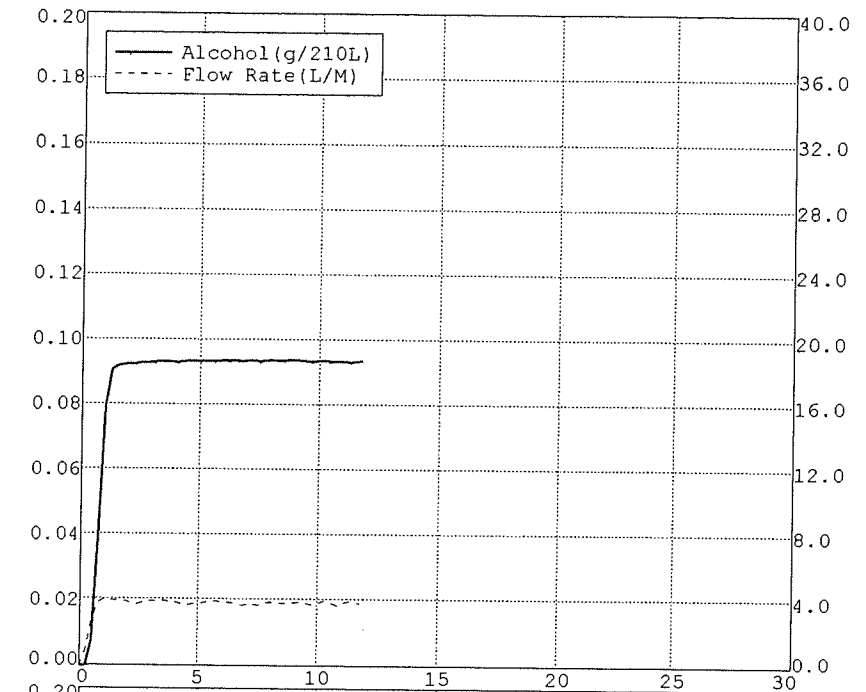

SUPERVISOR TEST

-----  
LAKE PLACID VILLAGE  
POLICE DEPT.  
DATAMASTER dmt: 100290  
-----

Date: 08/30/2021

OPERATOR NAME:  
DORAN H SORRELL  
Permit #: 47507  
Operator Agency/Dept: LAKE PLACID VILL. PD  
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:13
INTERNAL STANDARD	VERIFIED	18:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:13
BLANK TEST	0.00	18:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:15
BLANK TEST	0.00	18:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:16
BLANK TEST	0.00	18:17

