

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/03/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23030

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 18:09 |
| INTERNAL STANDARD | VERIFIED | 18:09 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:09 |
| BLANK TEST | 0.00 | 18:10 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:11 |
| BLANK TEST | 0.00 | 18:11 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 18:12 |
| BLANK TEST | 0.00 | 18:12 |

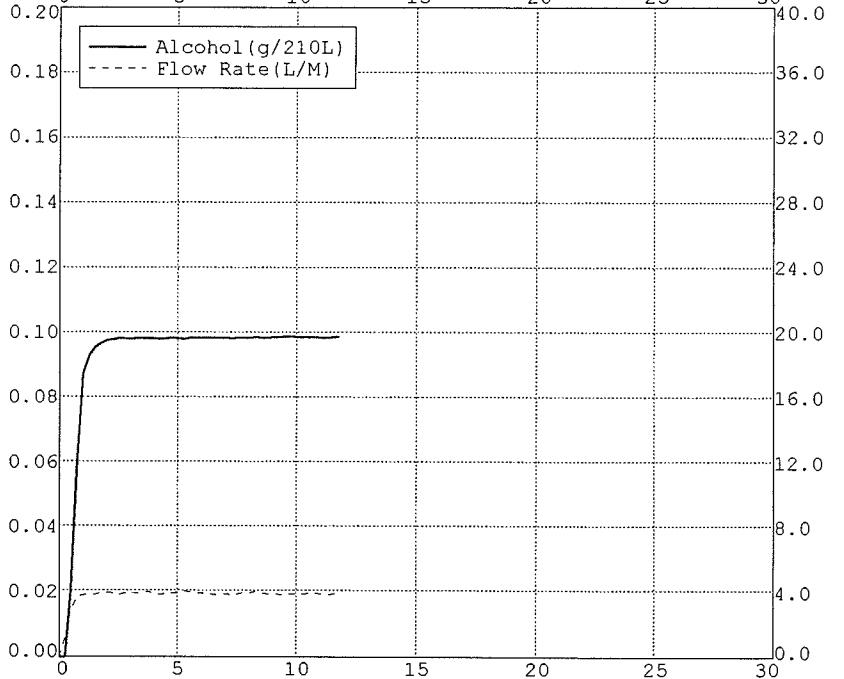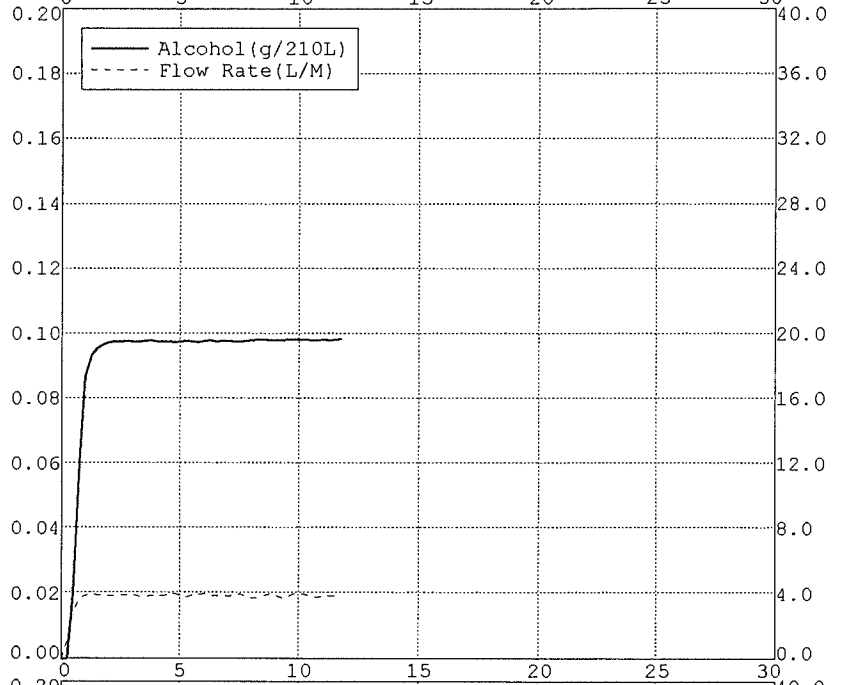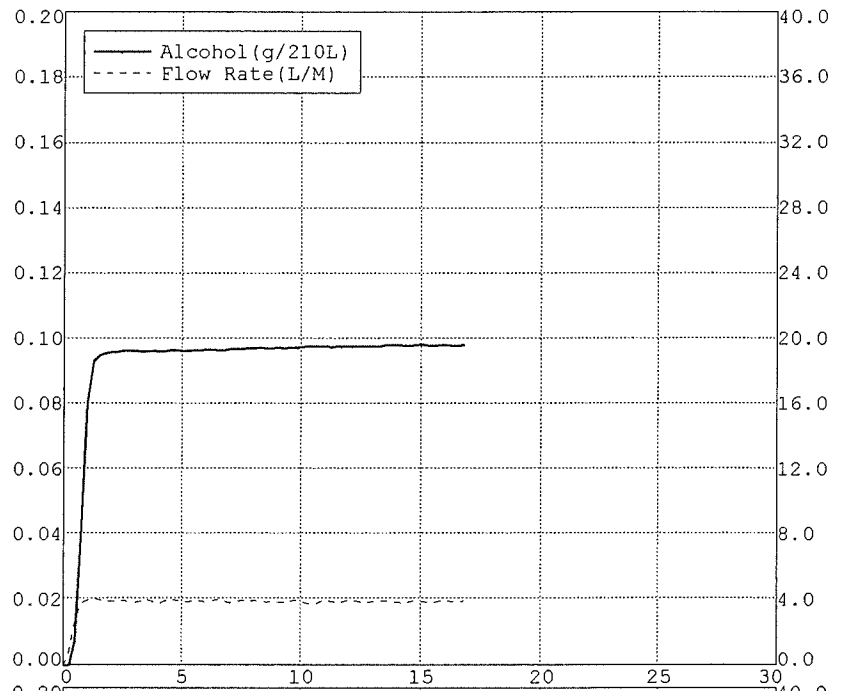

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/09/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23030

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 18:05 |
| INTERNAL STANDARD | VERIFIED | 18:05 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:06 |
| BLANK TEST | 0.00 | 18:07 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 18:07 |
| BLANK TEST | 0.00 | 18:08 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 18:08 |
| BLANK TEST | 0.00 | 18:09 |

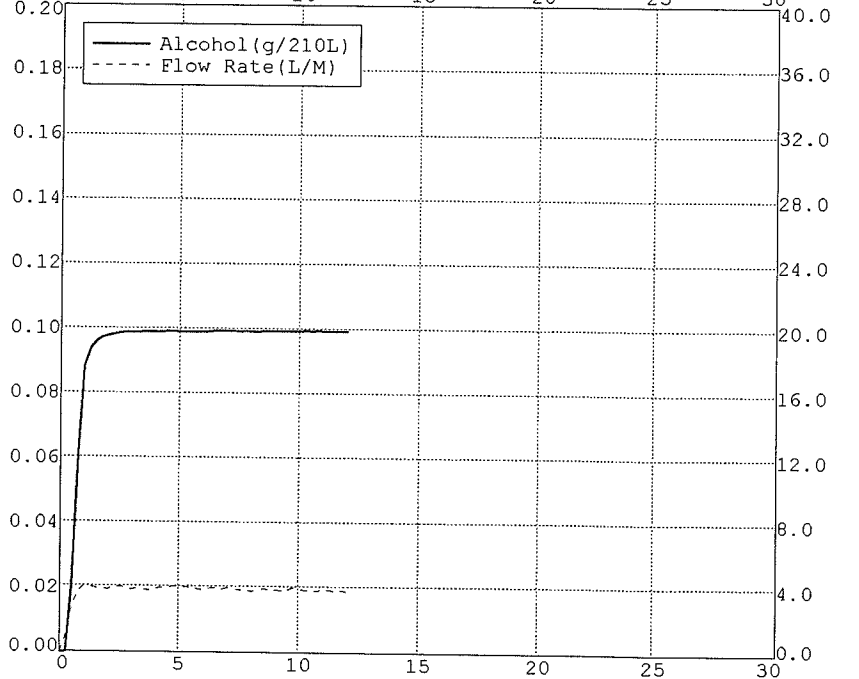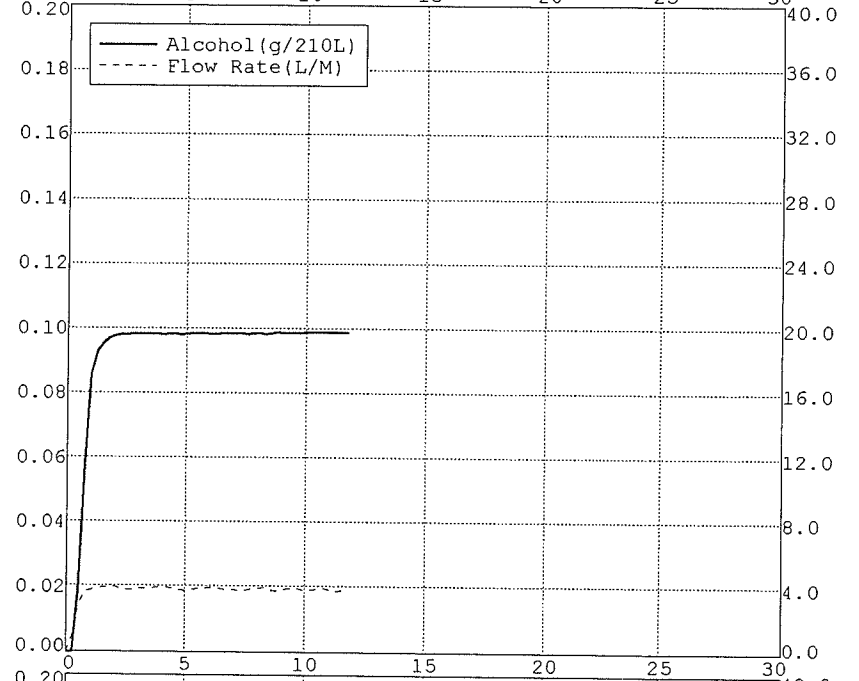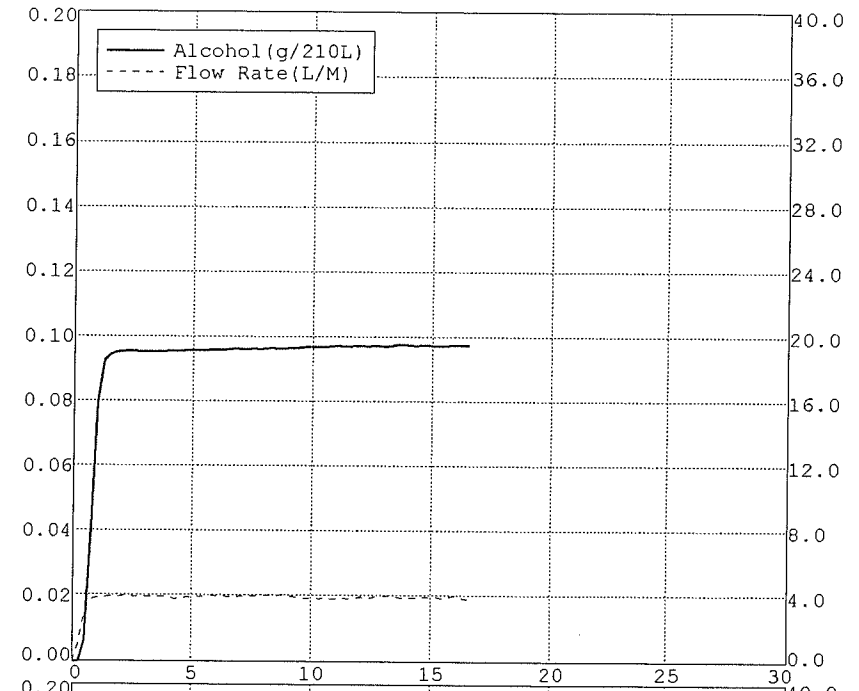

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/17/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23030

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 18:05 |
| INTERNAL STANDARD | VERIFIED | 18:05 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:06 |
| BLANK TEST | 0.00 | 18:06 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:07 |
| BLANK TEST | 0.00 | 18:08 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:08 |
| BLANK TEST | 0.00 | 18:09 |

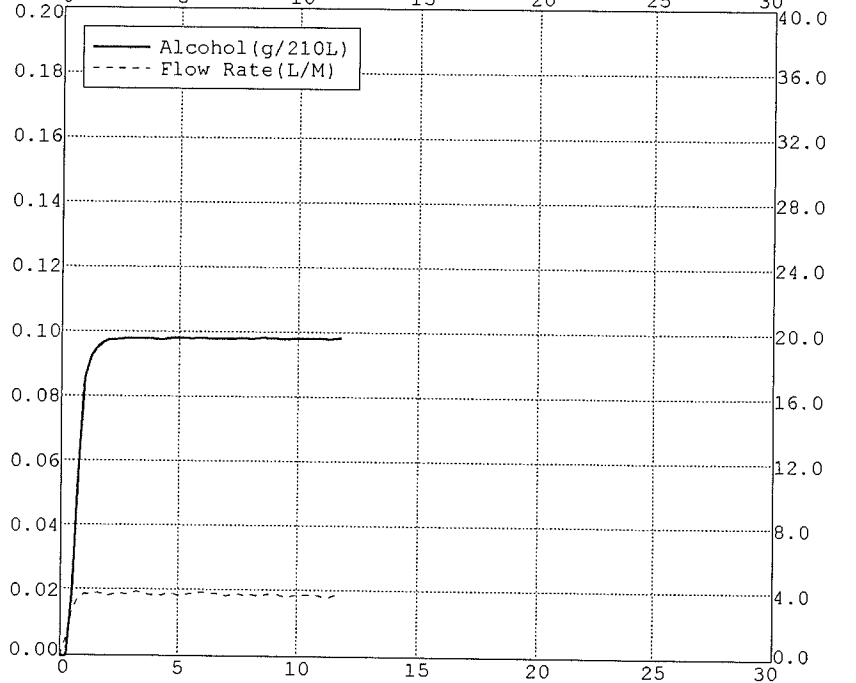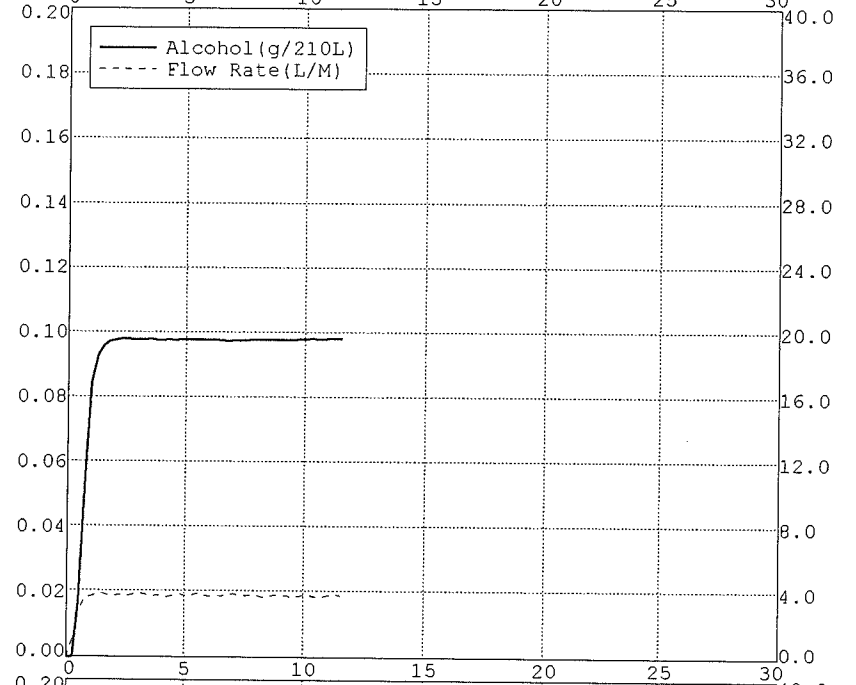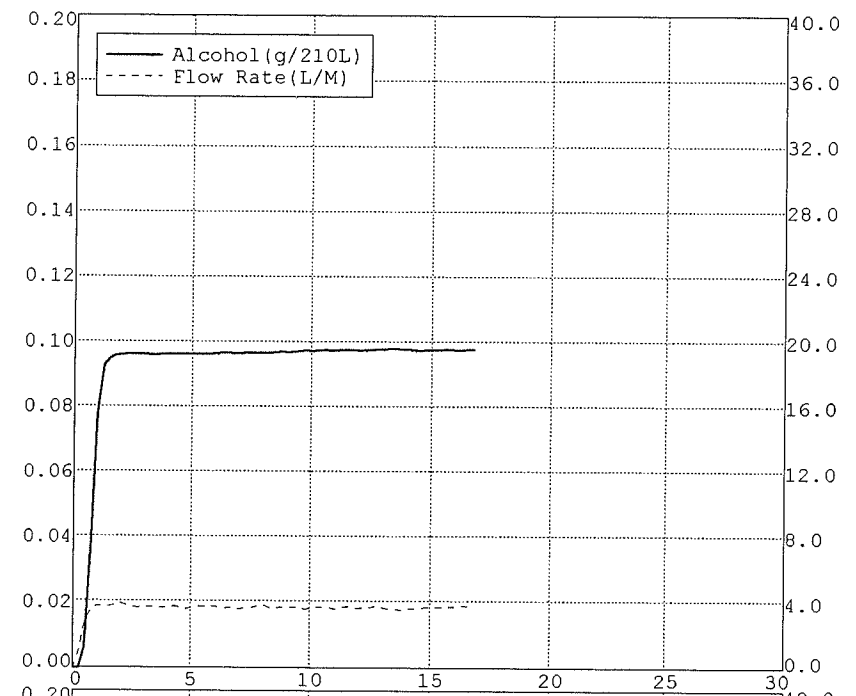

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/23/2023

OPERATOR NAME:
IAN O GORDON
Permit #: 50784
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 23030

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 15:05 |
| INTERNAL STANDARD | VERIFIED | 15:05 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 15:05 |
| BLANK TEST | 0.00 | 15:06 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 15:06 |
| BLANK TEST | 0.00 | 15:07 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 15:07 |
| BLANK TEST | 0.00 | 15:08 |

