

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/02/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:18
INTERNAL STANDARD	VERIFIED	10:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:18
BLANK TEST	0.00	10:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:20
BLANK TEST	0.00	10:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:21
BLANK TEST	0.00	10:22

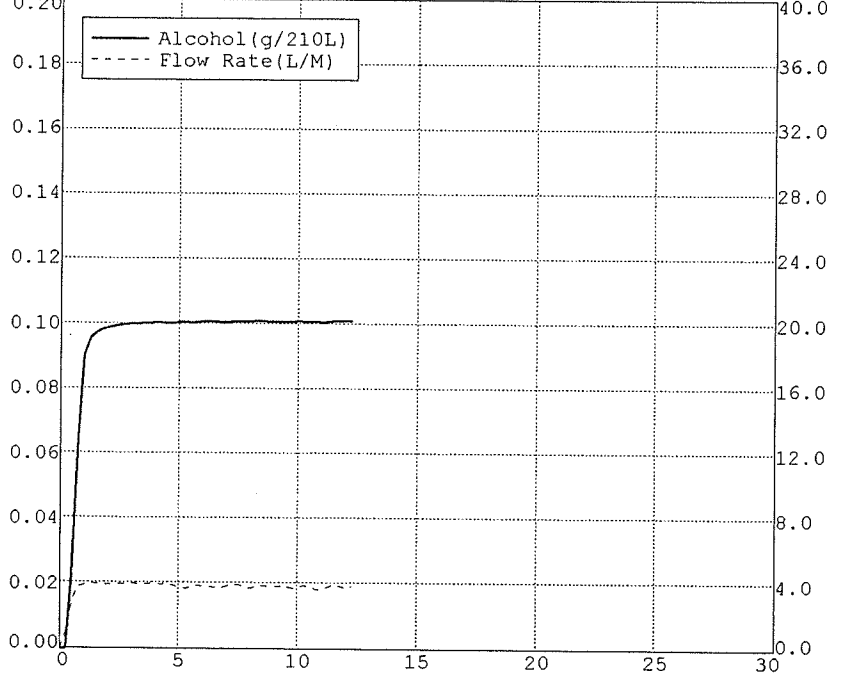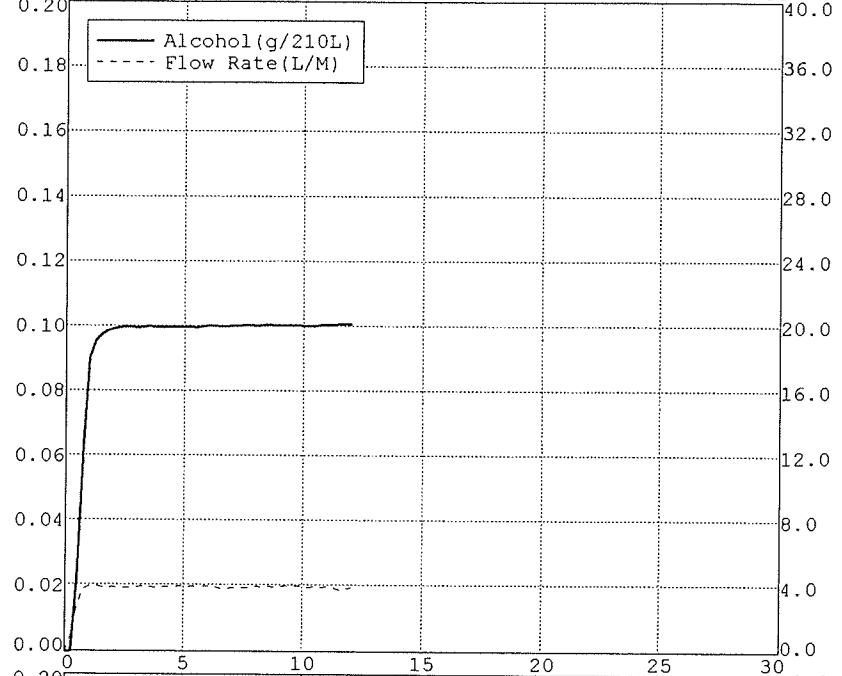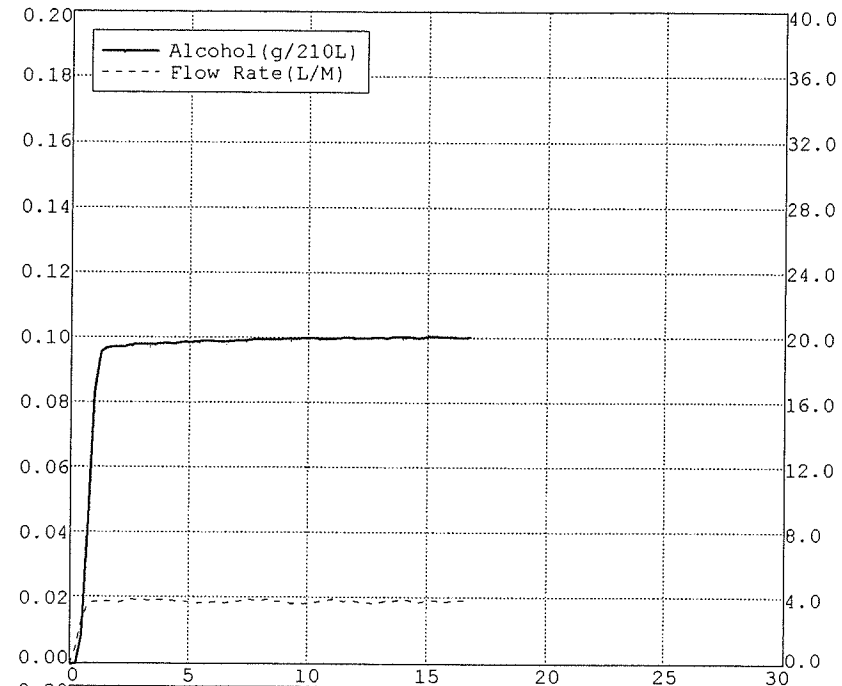

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290


Date: 05/10/2021

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:32
INTERNAL STANDARD	VERIFIED	06:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	INTERFERENCE	06:32

Interference Detected

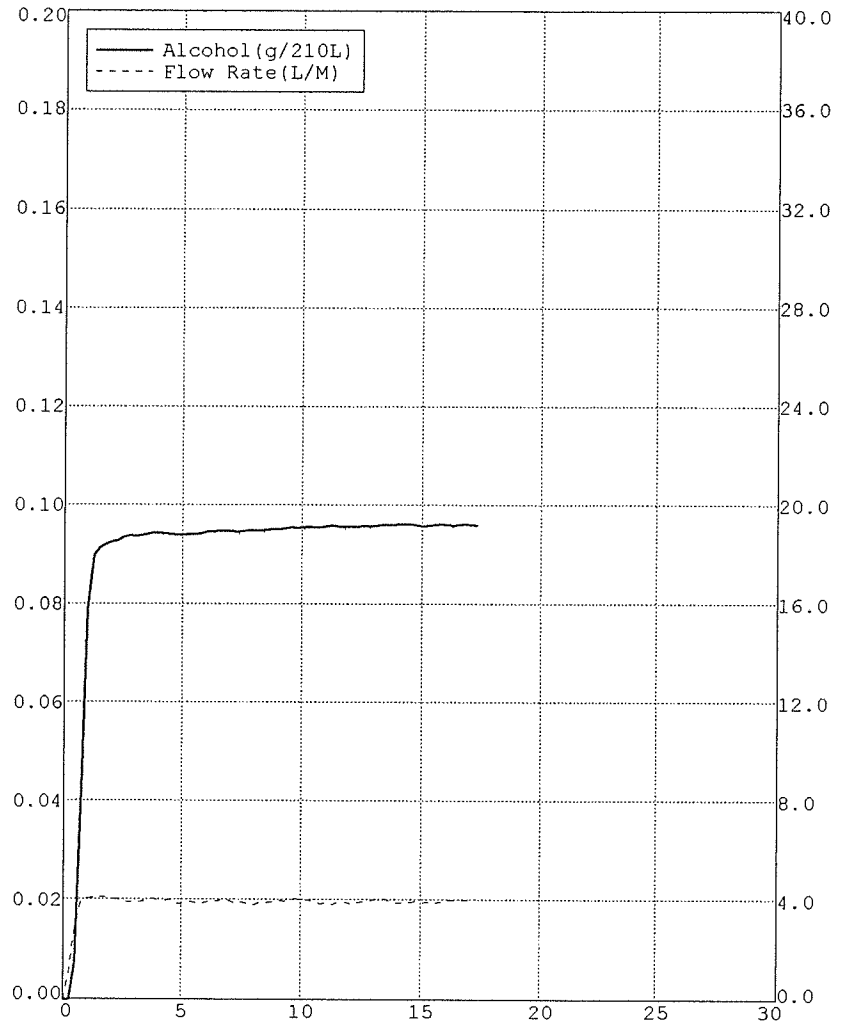

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290


Date: 05/10/2021

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:40
INTERNAL STANDARD	VERIFIED	06:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	INTERFERENCE	06:40

Interference Detected

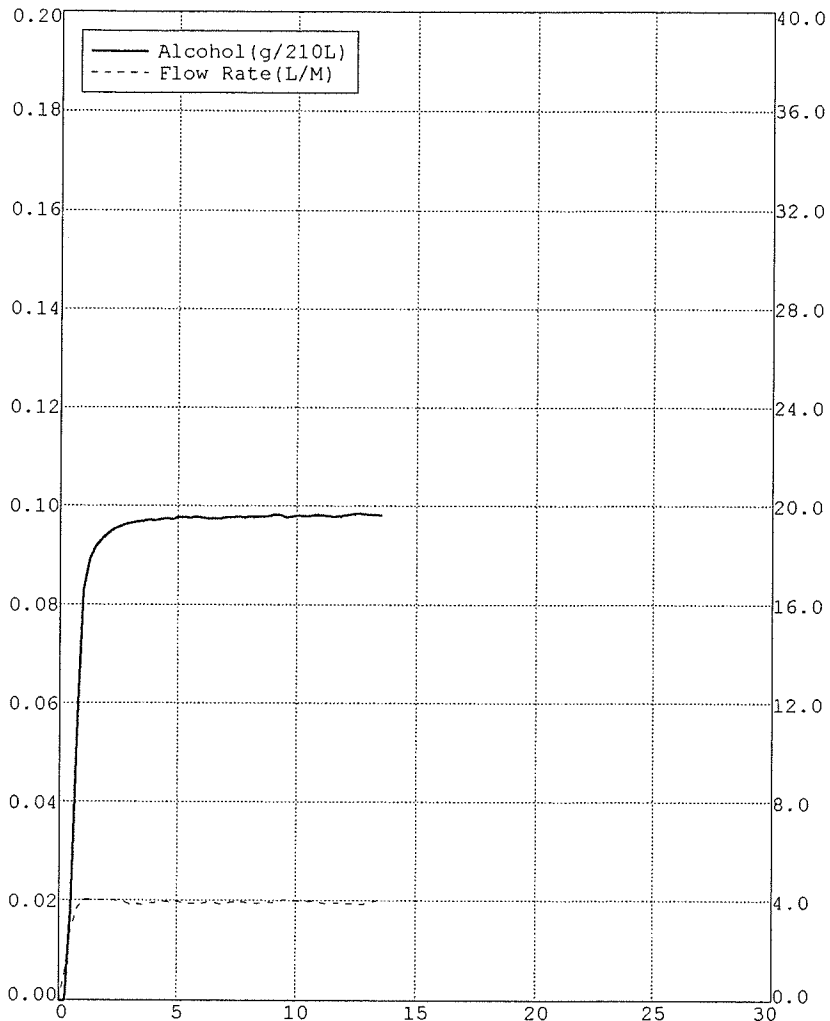

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290


Date: 05/10/2021

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:35
INTERNAL STANDARD	VERIFIED	06:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	INTERFERENCE	06:36

Interference Detected

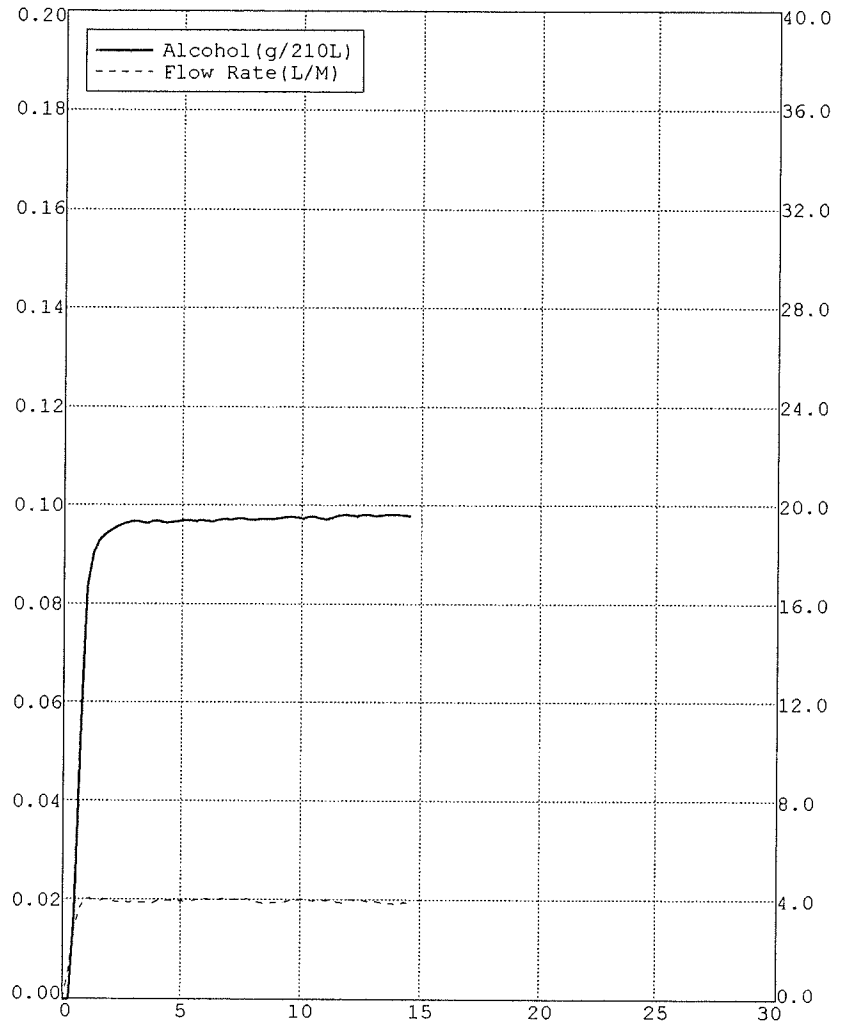

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/10/2021

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:24
INTERNAL STANDARD	VERIFIED	07:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:24
BLANK TEST	0.00	07:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:25
BLANK TEST	0.00	07:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:26
BLANK TEST	0.00	07:27

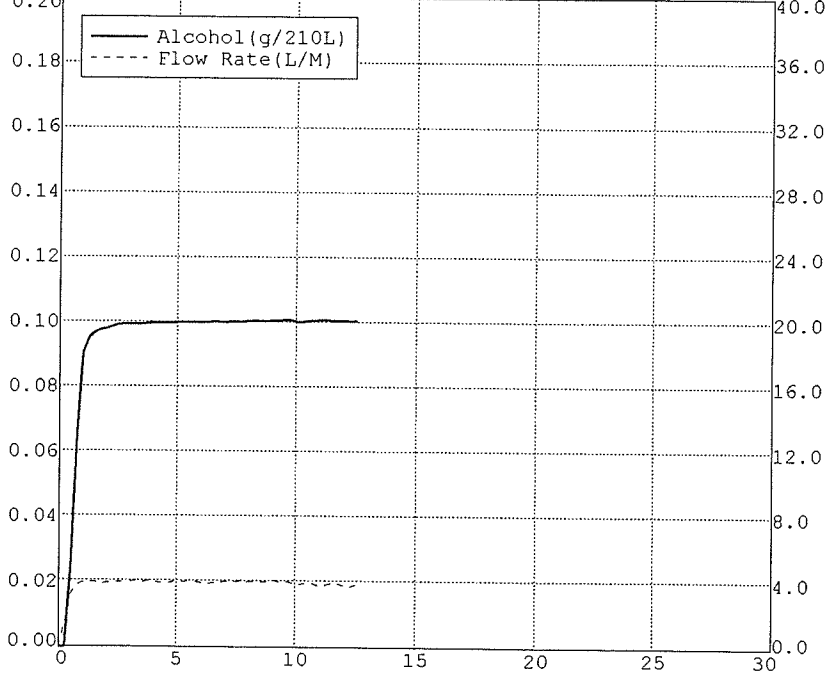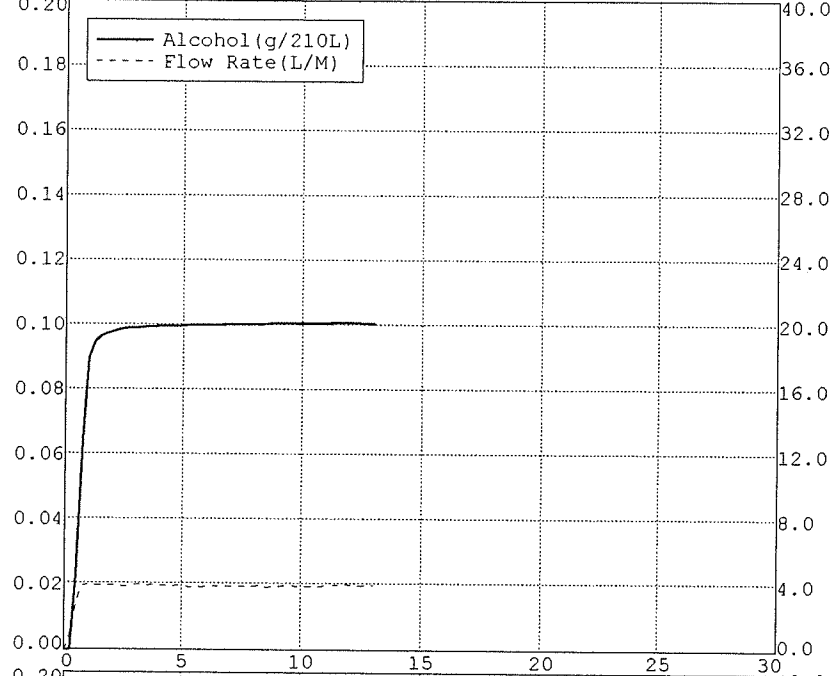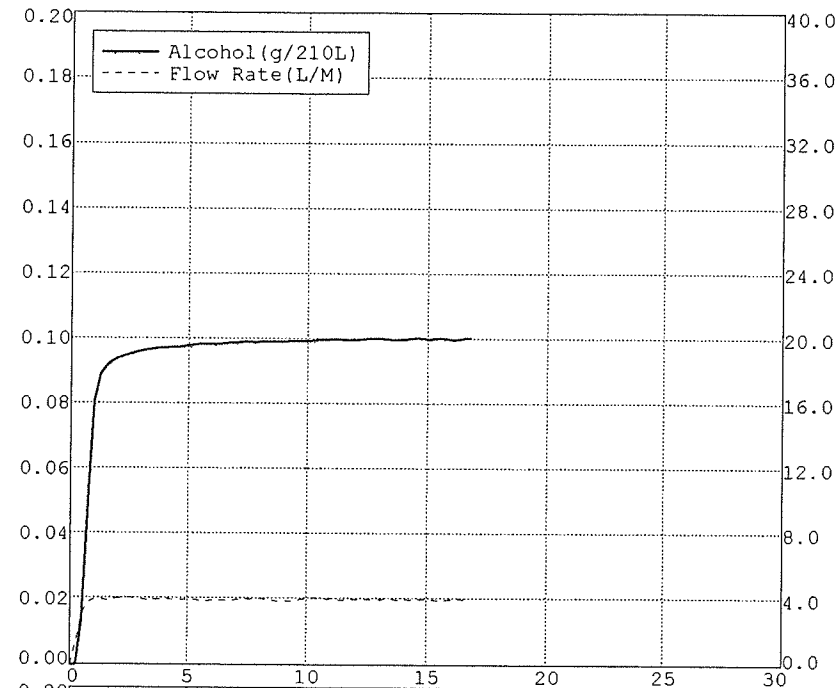

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/16/2021

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:22
INTERNAL STANDARD	VERIFIED	18:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:22
BLANK TEST	0.00	18:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:24
BLANK TEST	0.00	18:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:25
BLANK TEST	0.00	18:25

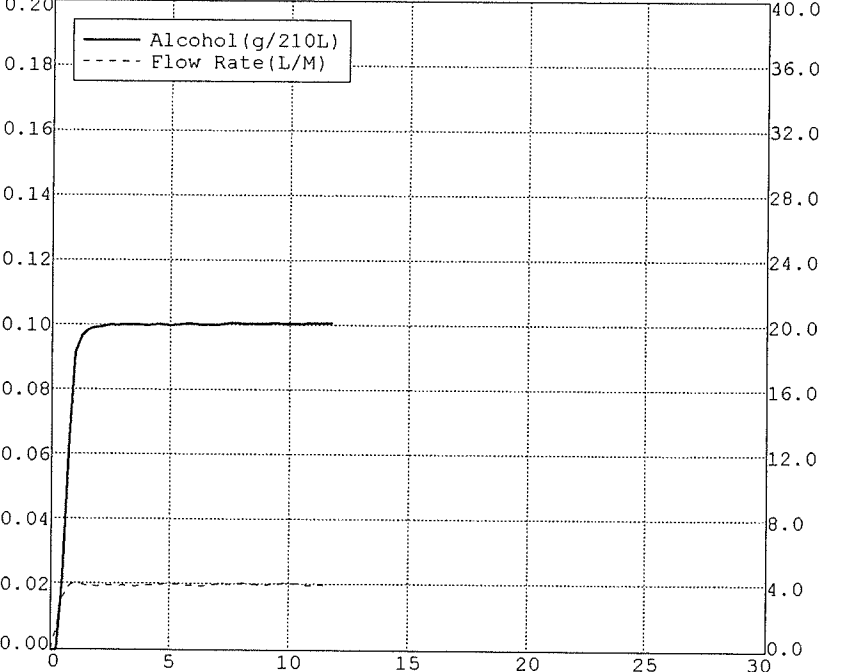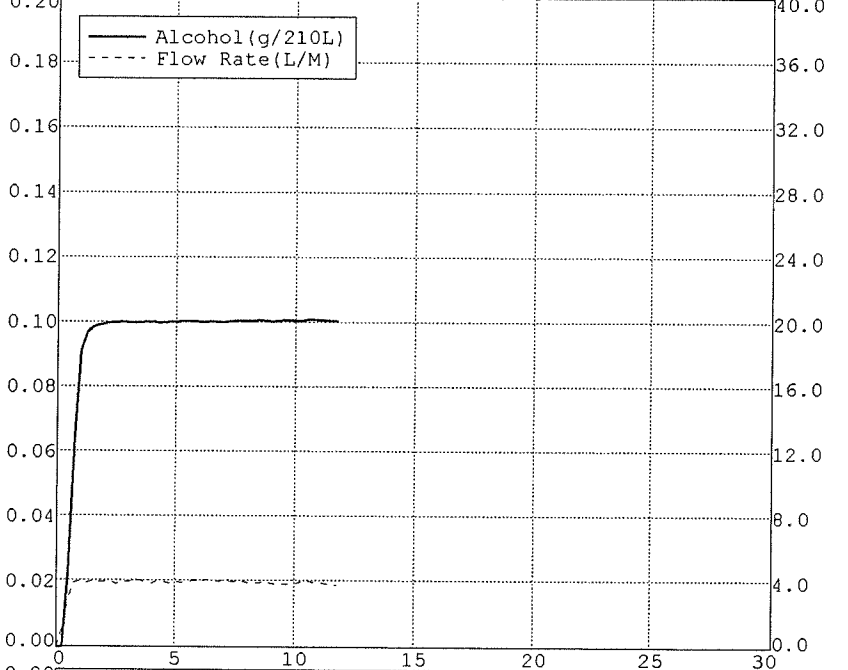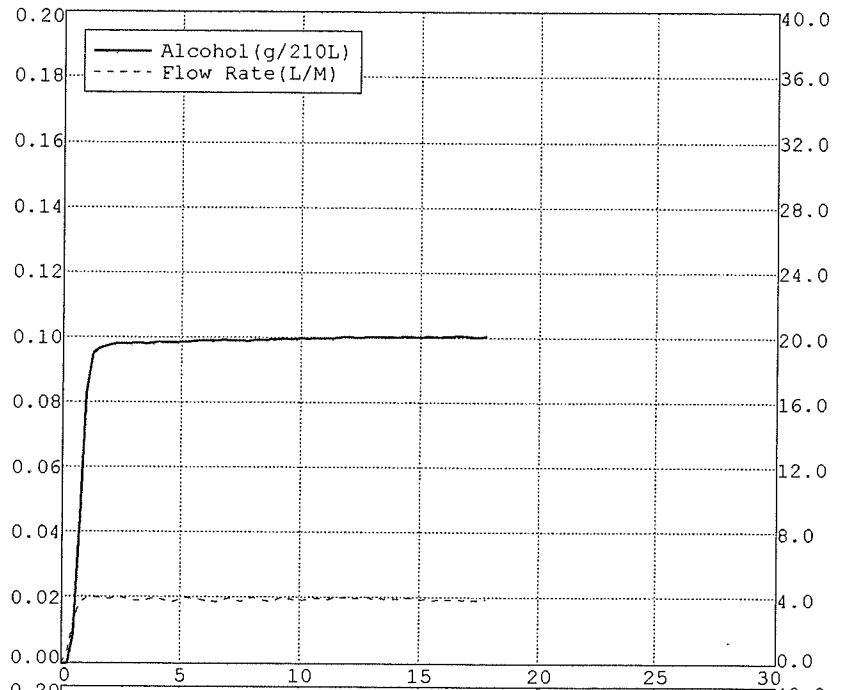

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 05/24/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:48
INTERNAL STANDARD	VERIFIED	16:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:49
BLANK TEST	0.00	16:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:50
BLANK TEST	0.00	16:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:51
BLANK TEST	0.00	16:52

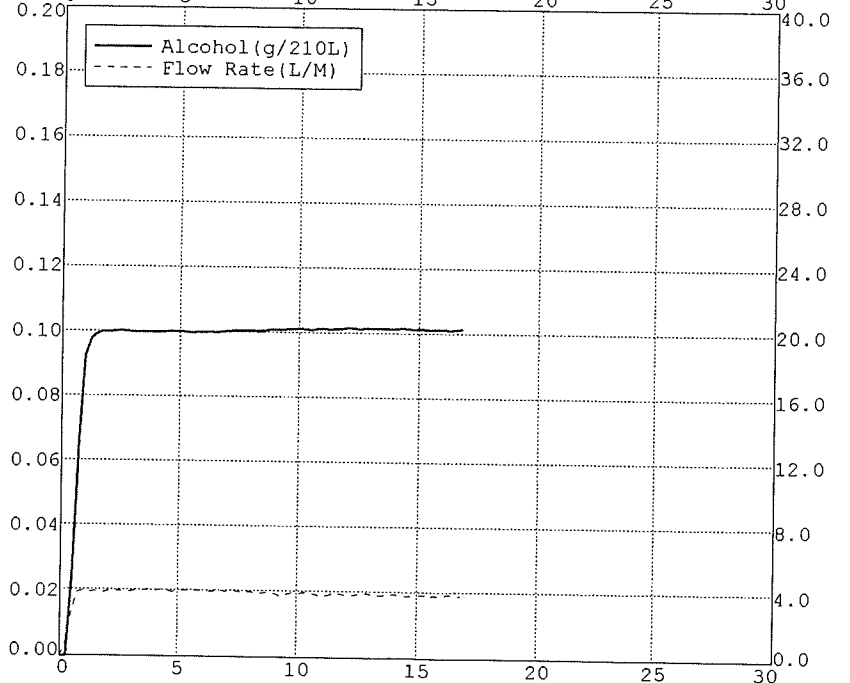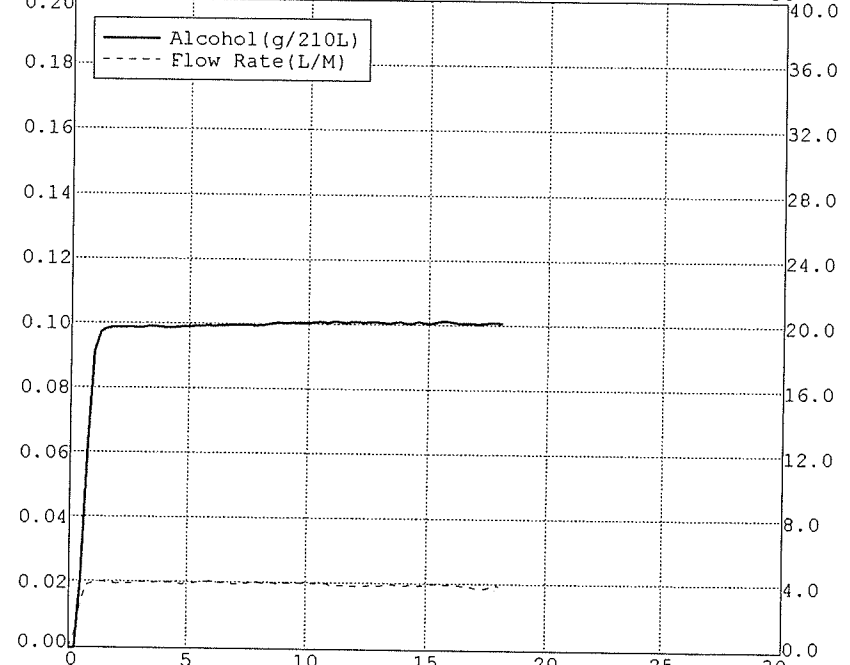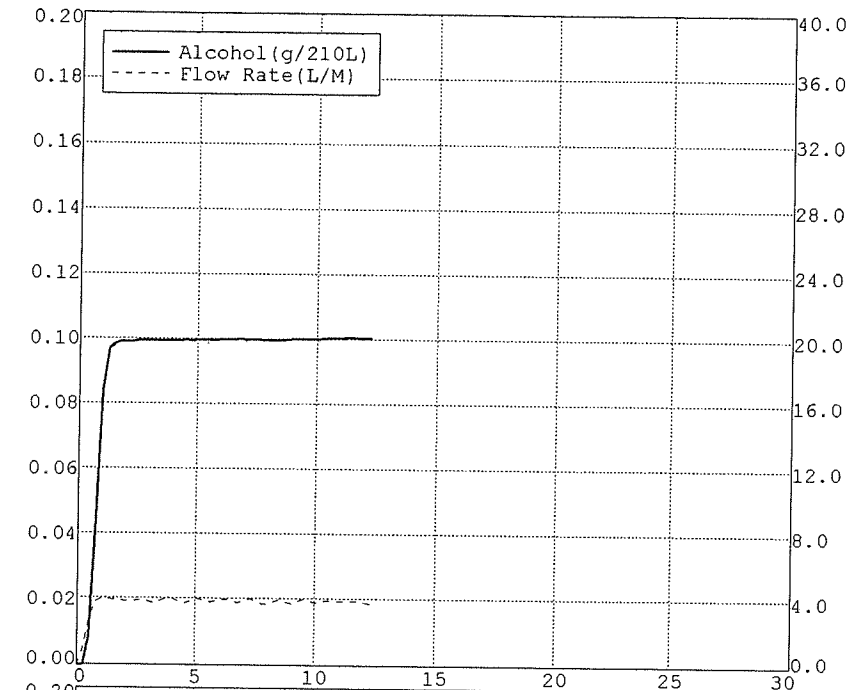

SOLUTION CHANGE

LAKE PLACID VILLAGE
 POLICE DEPT.
 DATAMASTER dmt: 100290

Date: 05/30/2021

OPERATOR NAME:
 DORAN H SORRELL
 Permit #: 47507
 Operator Agency/Dept: LAKE PLACID VILL. PD
 Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:46
INTERNAL STANDARD	VERIFIED	06:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:47
BLANK TEST	0.00	06:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:48
BLANK TEST	0.00	06:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:49
BLANK TEST	0.00	06:50

