

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/01/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:36
INTERNAL STANDARD	VERIFIED	12:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:37
BLANK TEST	0.00	12:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:38
BLANK TEST	0.00	12:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:39
BLANK TEST	0.00	12:40

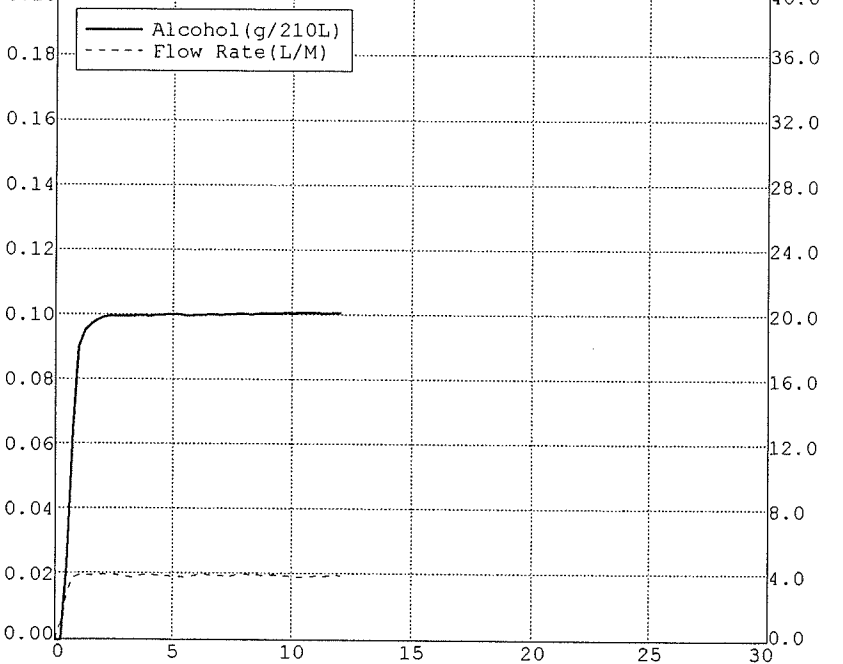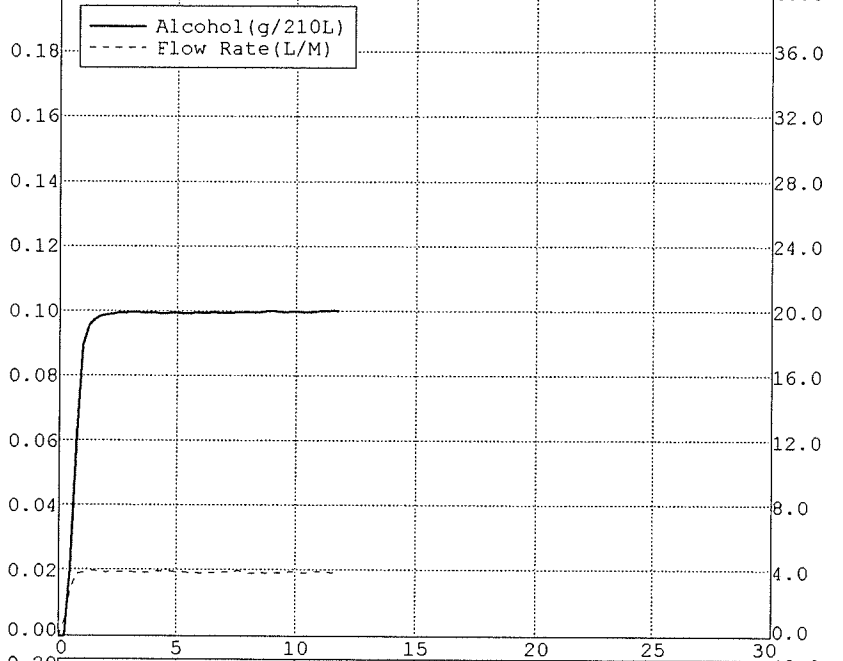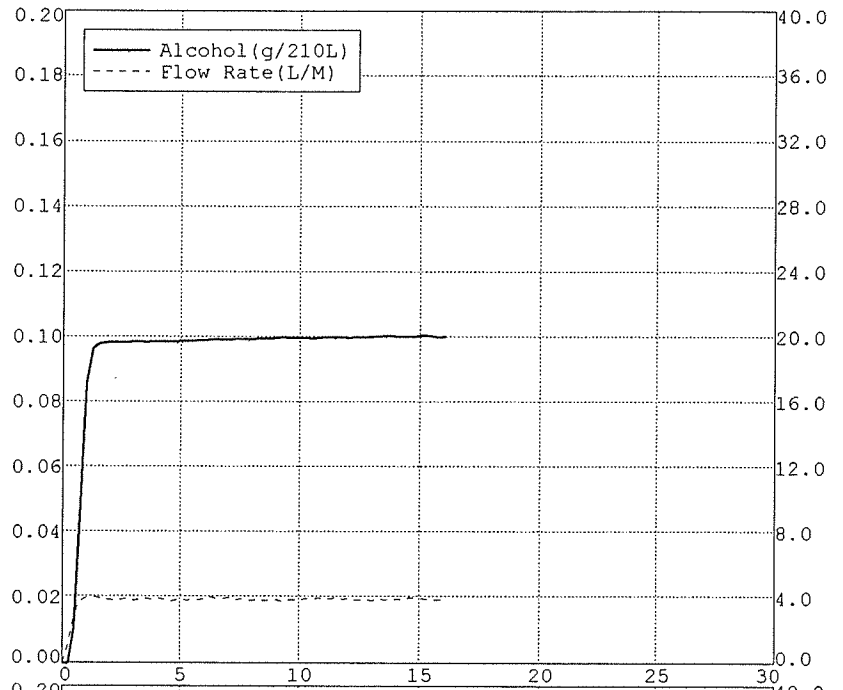

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/07/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:57
INTERNAL STANDARD	VERIFIED	12:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:58
BLANK TEST	0.00	12:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:59
BLANK TEST	0.00	13:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:00
BLANK TEST	0.00	13:01

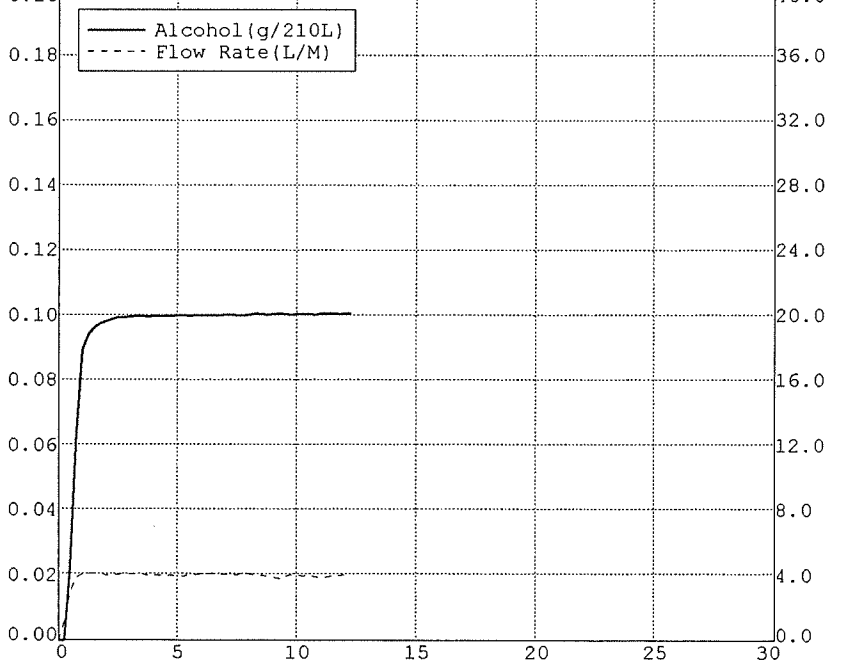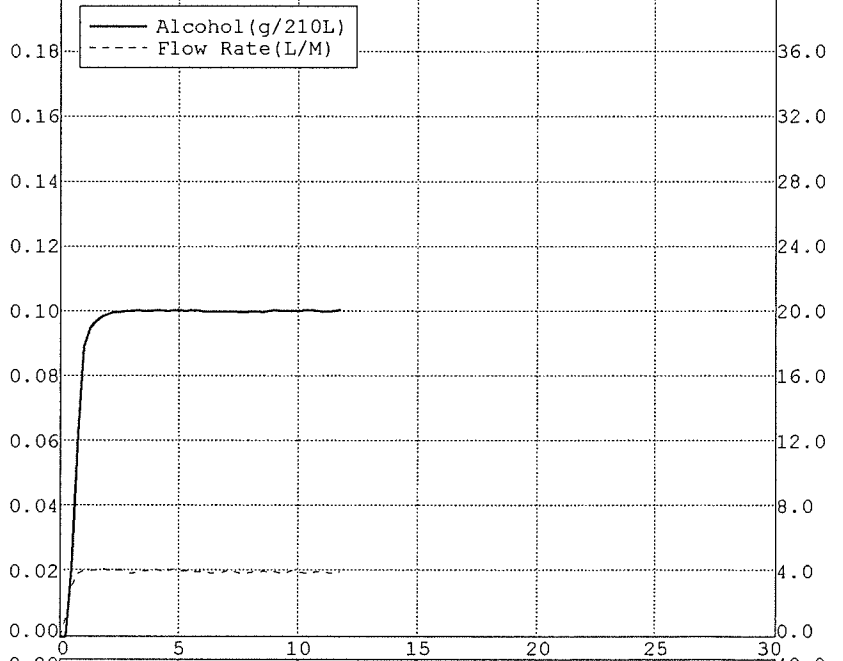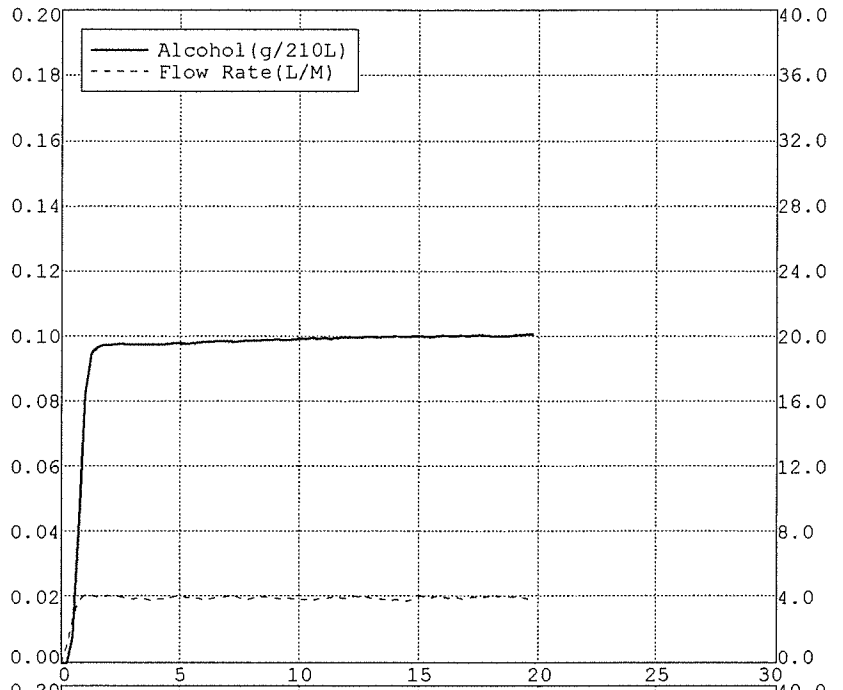

SUPERVISOR TEST




LAKE PLACID VILLAGE
 POLICE DEPT.
 DATAMASTER dmt: 100290

Date: 03/15/2021

OPERATOR NAME:
 CHAD P BLINN
 Permit #: 33034
 Operator Agency/Dept: LAKE PLACID VILL. PD
 Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:17
INTERNAL STANDARD	VERIFIED	15:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:17
BLANK TEST	0.00	15:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:19
BLANK TEST	0.00	15:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:20
BLANK TEST	0.00	15:20

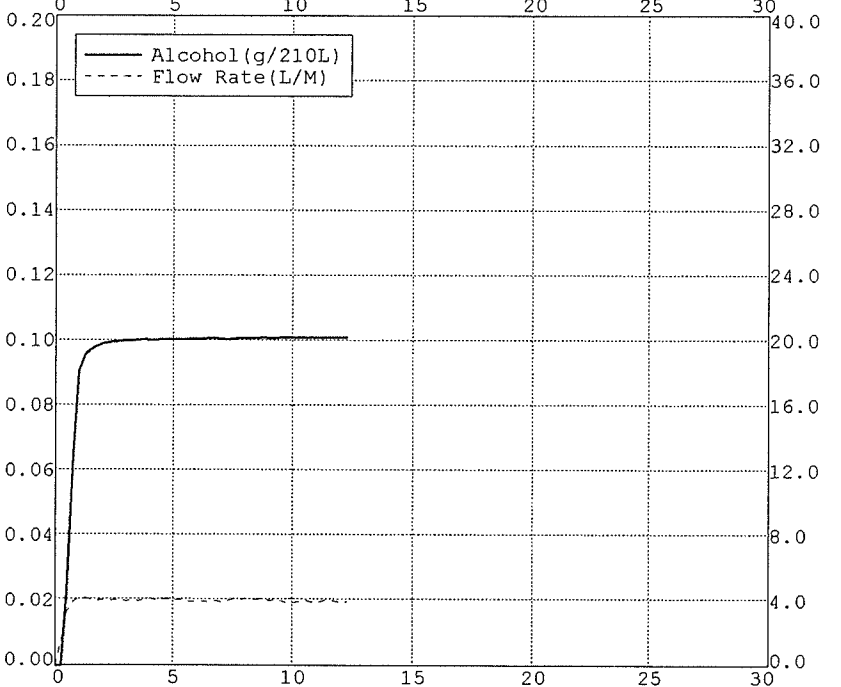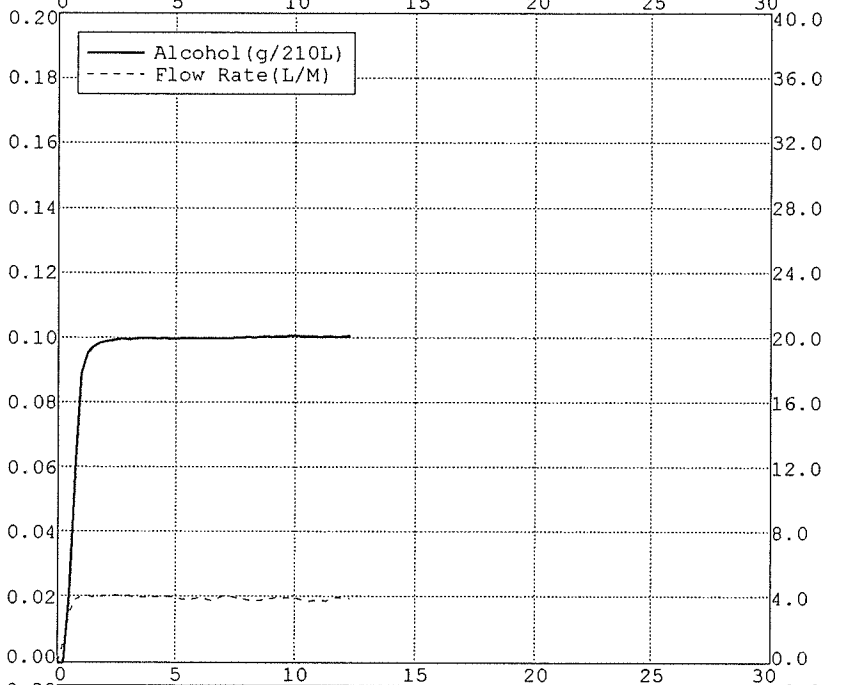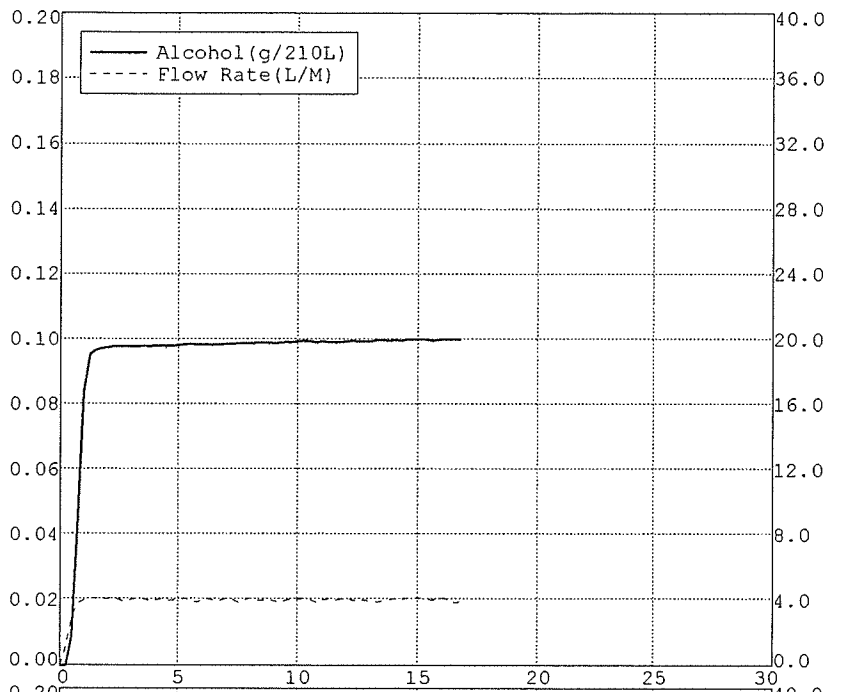

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/21/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:00
INTERNAL STANDARD	VERIFIED	13:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:00
BLANK TEST	0.00	13:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:01
BLANK TEST	0.00	13:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:02
BLANK TEST	0.00	13:03

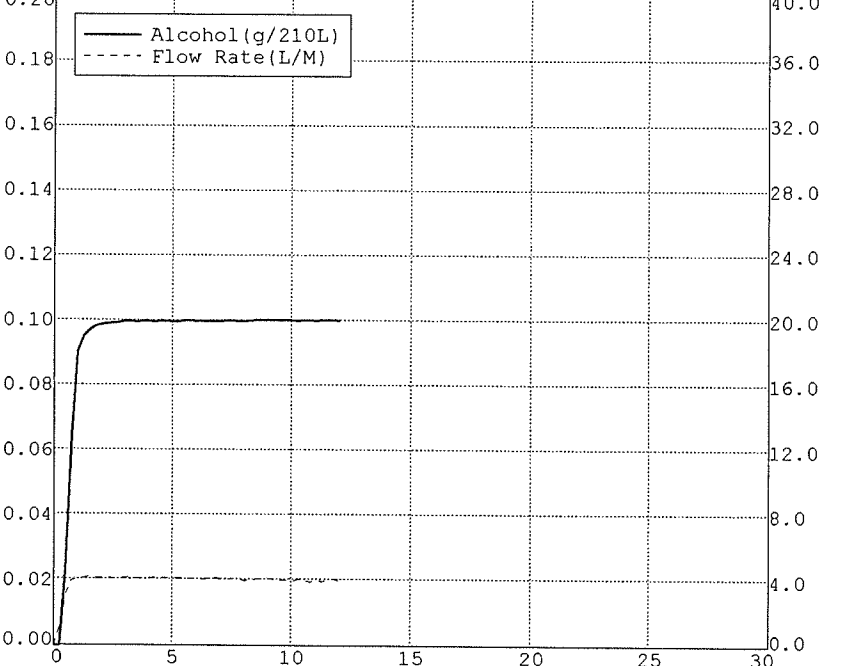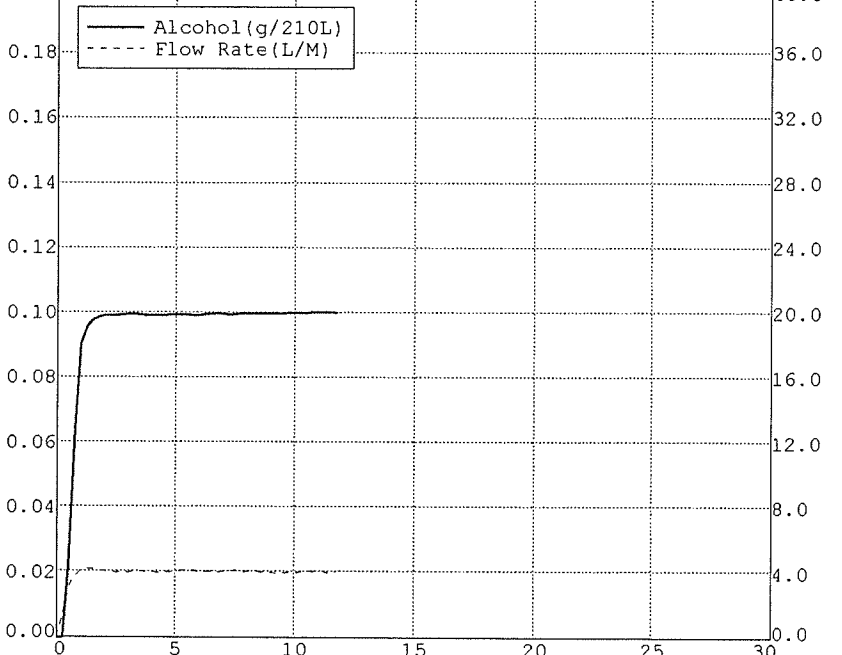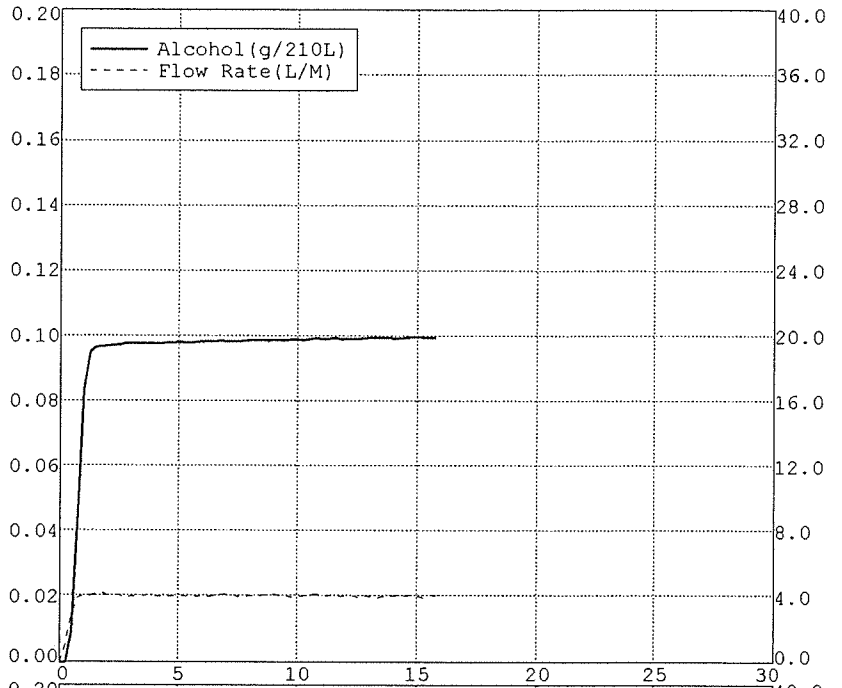

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/29/2021

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:59
INTERNAL STANDARD	VERIFIED	12:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:59
BLANK TEST	0.00	13:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:00
BLANK TEST	0.00	13:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:02
BLANK TEST	0.00	13:02

