

SUPERVISOR TEST



LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/05/2020

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:05
INTERNAL STANDARD	VERIFIED	18:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:05
BLANK TEST	0.00	18:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:07
BLANK TEST	0.00	18:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:08
BLANK TEST	0.00	18:09

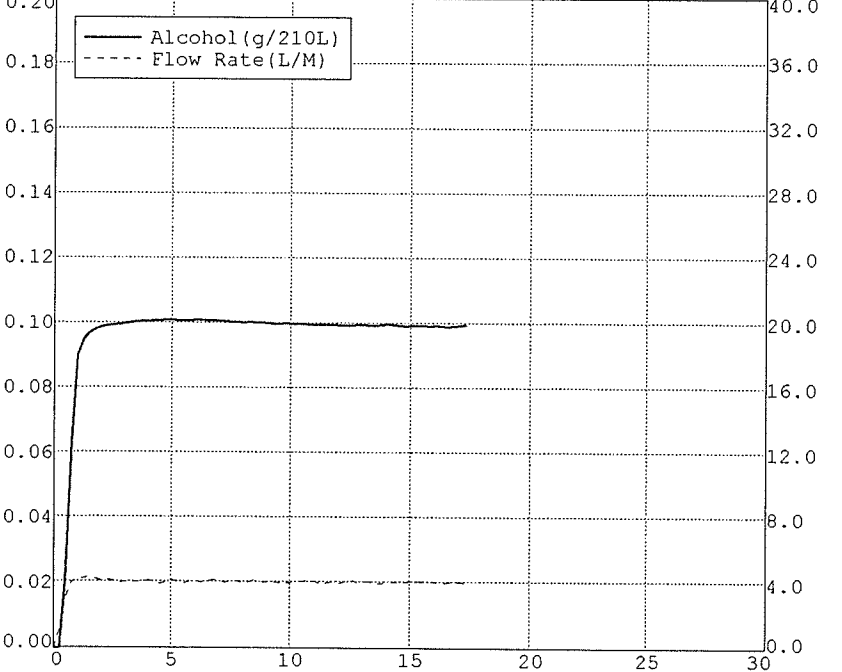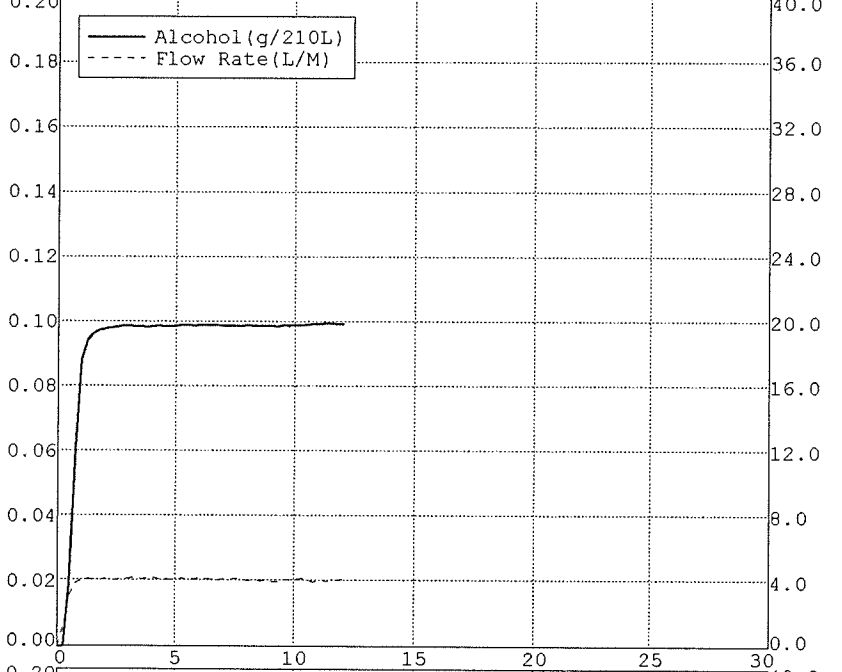

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/12/2020

OPERATOR NAME:
THOMAS J THERRIEN
Permit #: 44459
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:17
INTERNAL STANDARD	VERIFIED	20:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:17
BLANK TEST	0.00	20:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:19
BLANK TEST	0.00	20:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:20
BLANK TEST	0.00	20:20

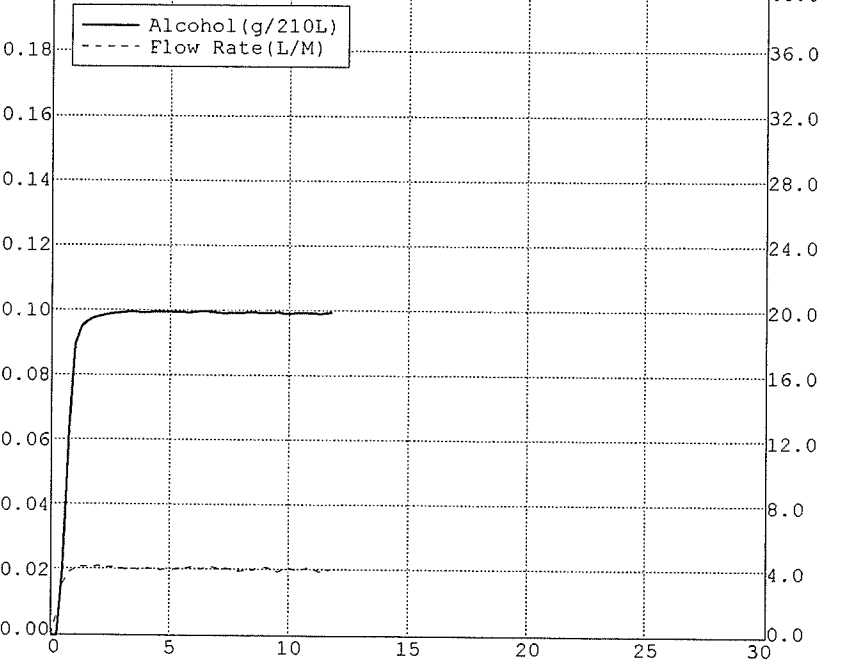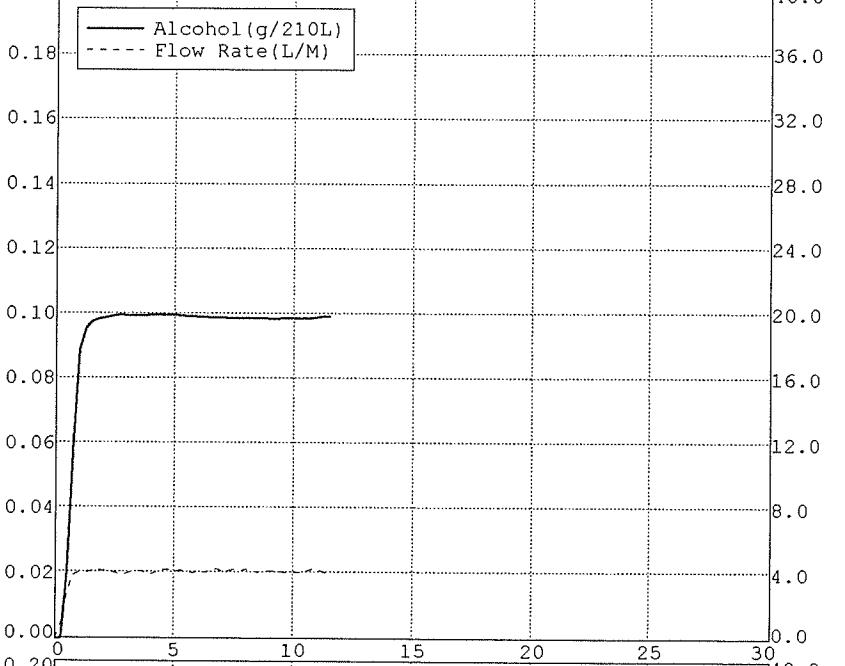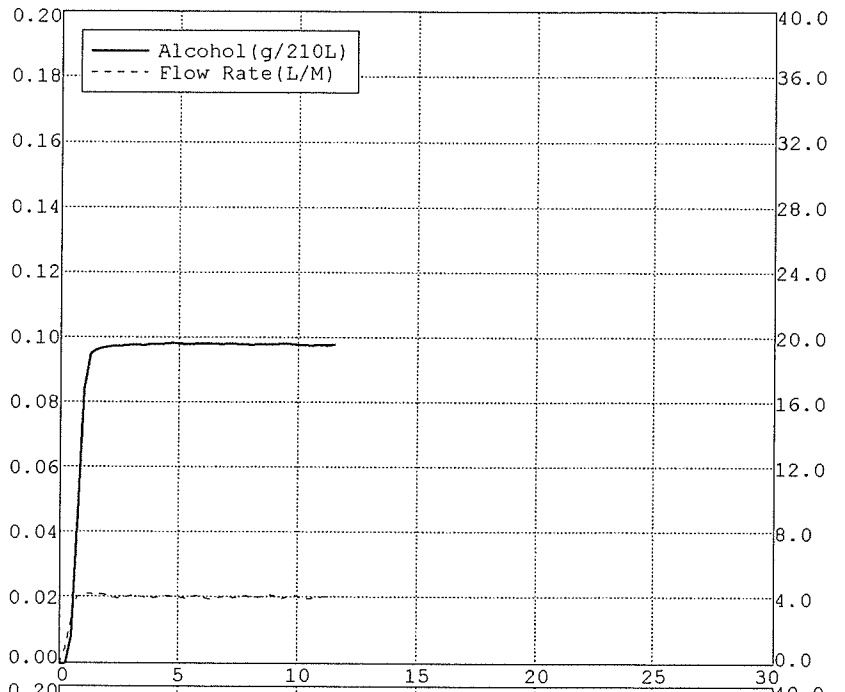

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/19/2020

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:35
INTERNAL STANDARD	VERIFIED	18:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:36
BLANK TEST	0.00	18:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:37
BLANK TEST	0.00	18:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:38
BLANK TEST	0.00	18:39

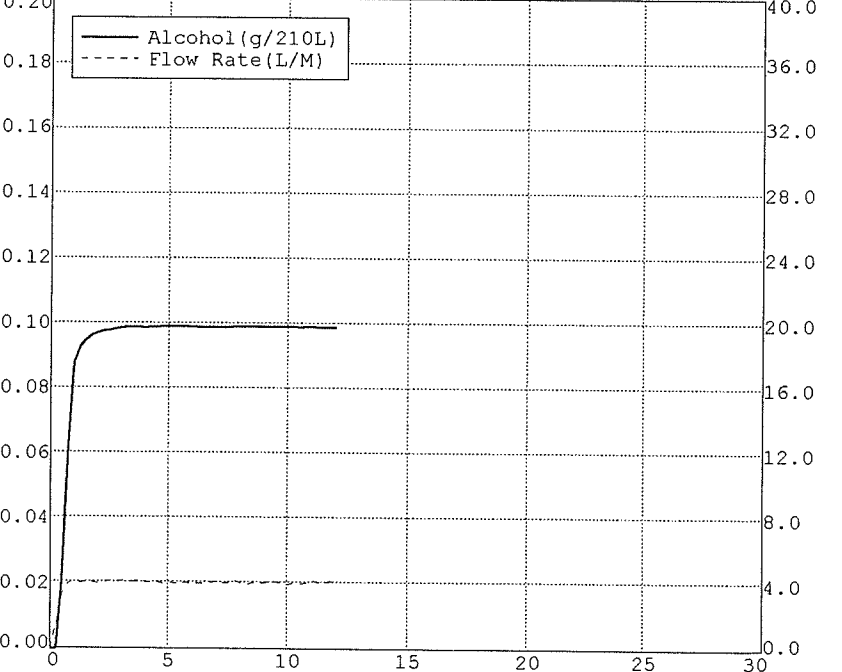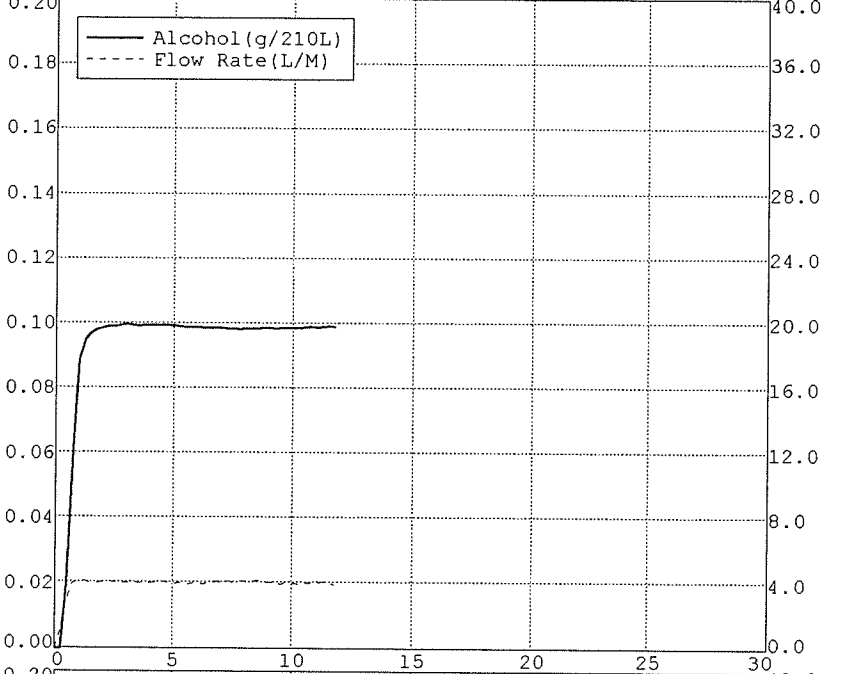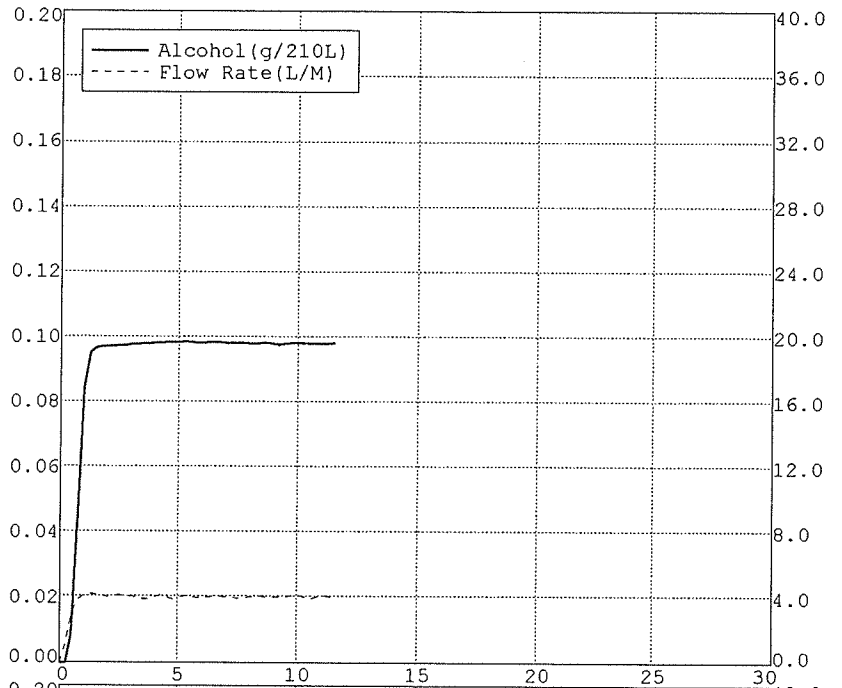

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/27/2020

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:53
INTERNAL STANDARD	VERIFIED	17:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:53
BLANK TEST	0.00	17:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:54
BLANK TEST	0.00	17:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:55
BLANK TEST	0.00	17:56

