

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/02/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24410

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:50
INTERNAL STANDARD	VERIFIED	14:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:50
BLANK TEST	0.00	14:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:51
BLANK TEST	0.00	14:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:52
BLANK TEST	0.00	14:53

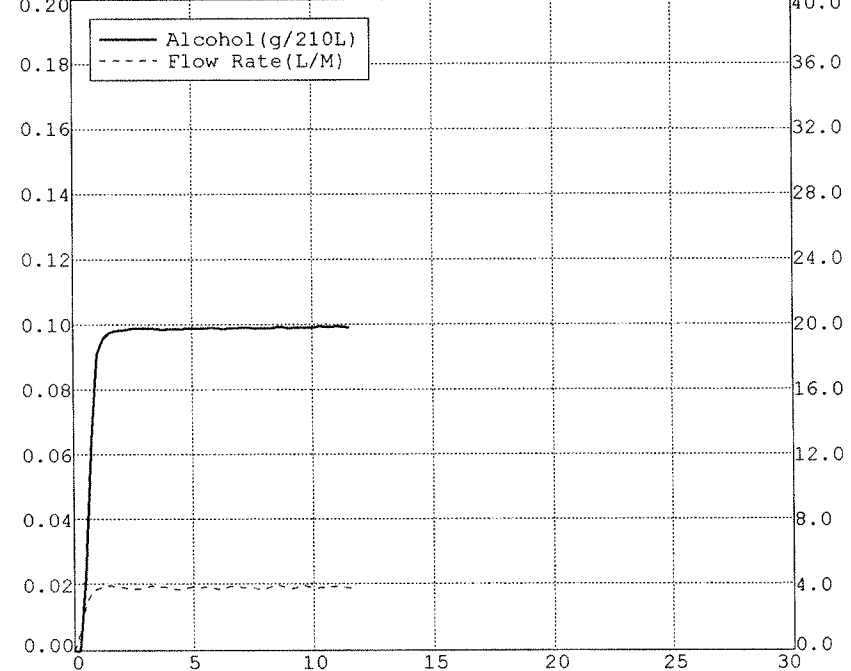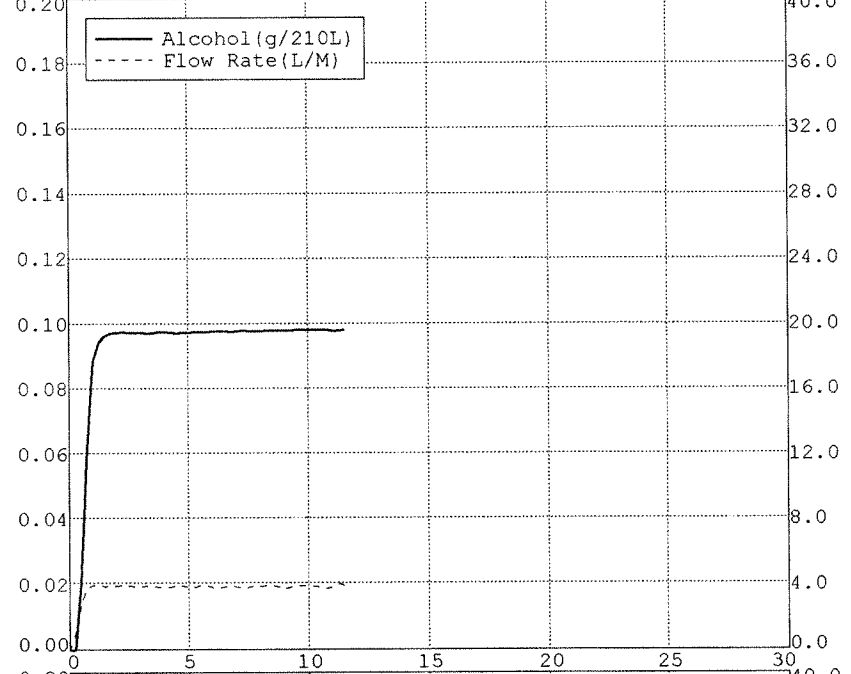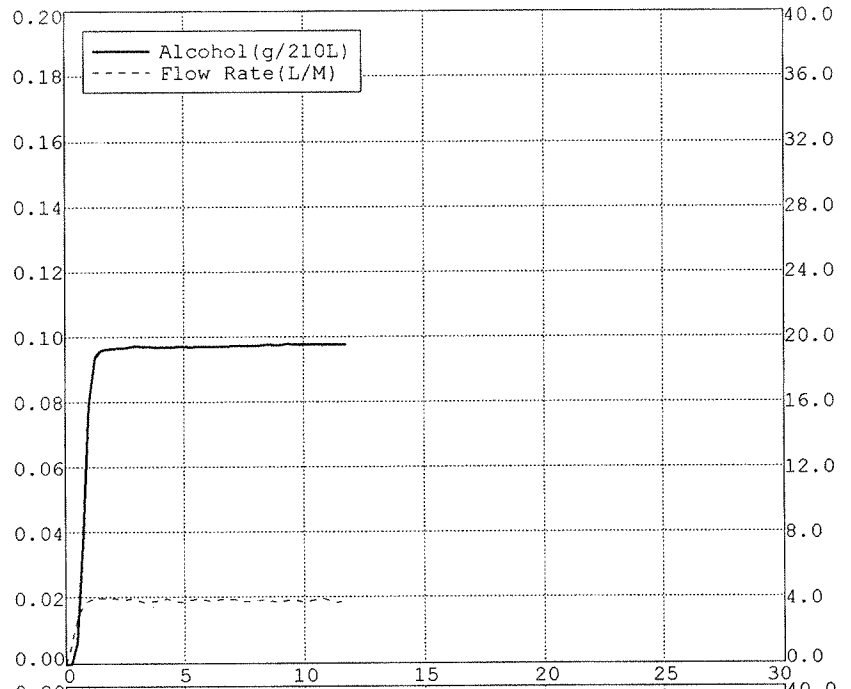

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/09/2025

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24410

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:19
INTERNAL STANDARD	VERIFIED	09:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:19
BLANK TEST	0.00	09:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:20
BLANK TEST	0.00	09:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:21
BLANK TEST	0.00	09:22

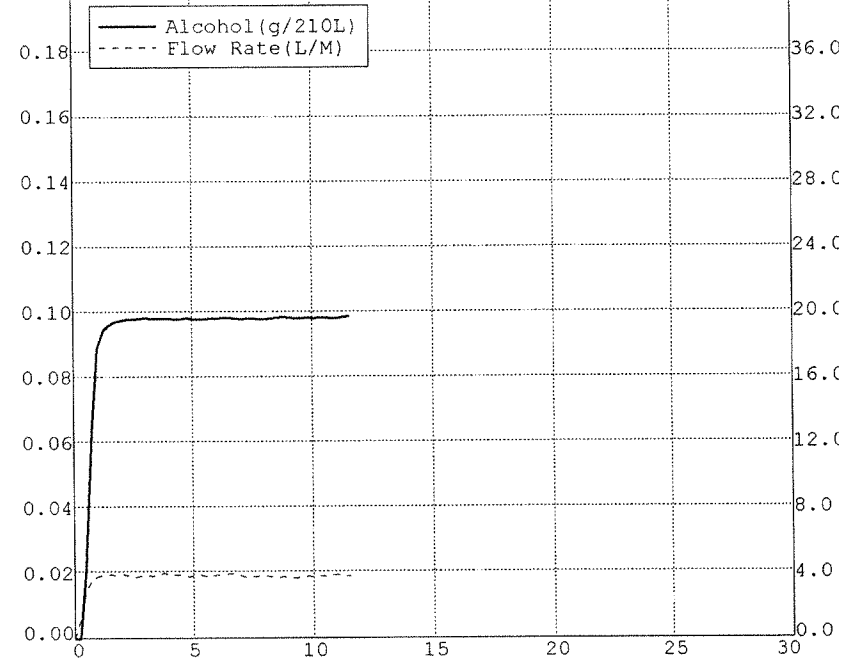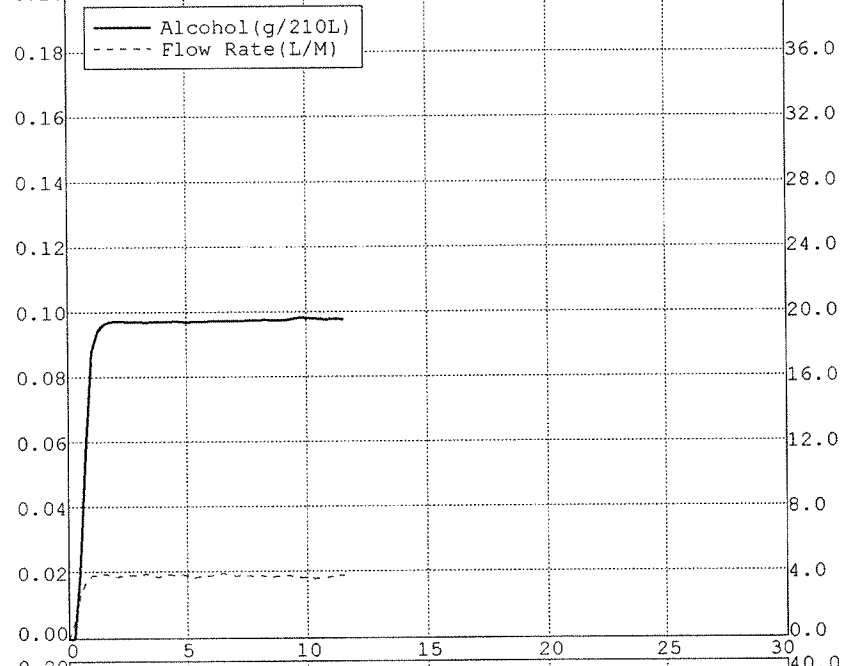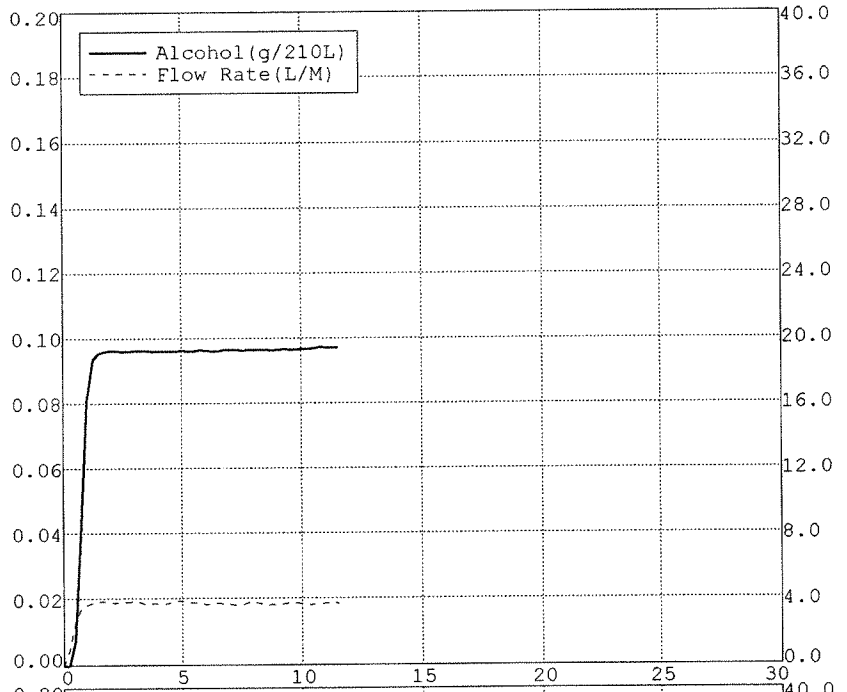

SUPERVISOR TEST



LAKE PLACID VILLAGE
 POLICE DEPT.
 DATAMASTER dmt: 100290

Date: 03/16/2025

OPERATOR NAME:
 CHAD P BLINN
 Permit #: 33034
 Operator Agency/Dept: LAKE PLACID VILL. PD
 Reference Standard #: 24410

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:38
INTERNAL STANDARD	VERIFIED	04:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:38
BLANK TEST	0.00	04:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:39
BLANK TEST	0.00	04:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:41
BLANK TEST	0.00	04:41

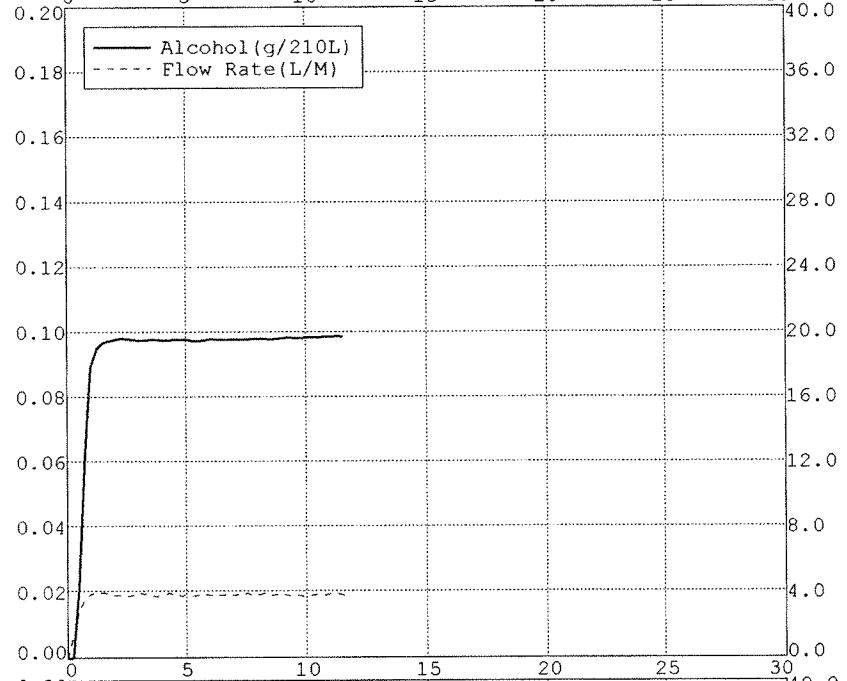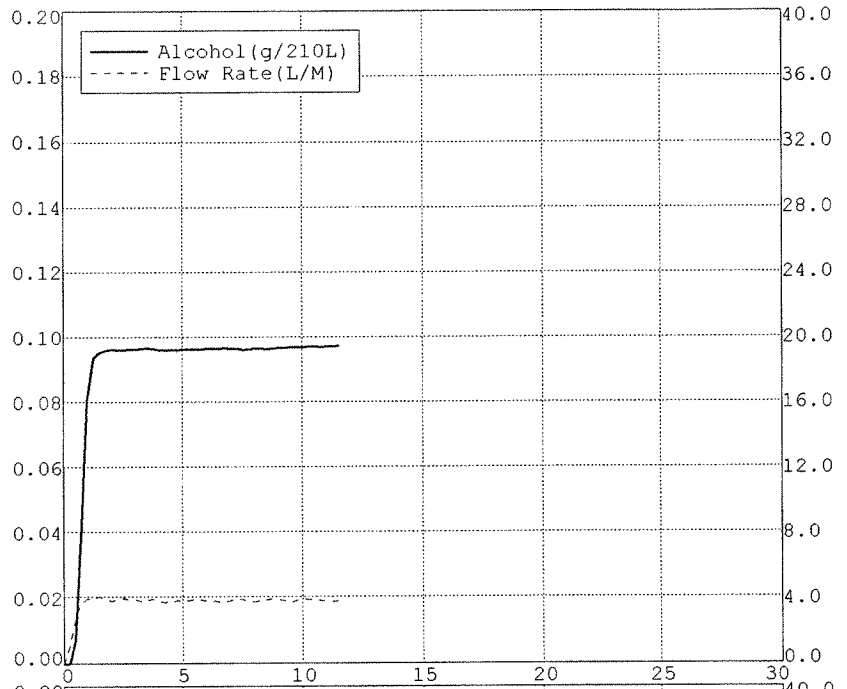

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/23/2025

OPERATOR NAME:
MAKENZIE A HAYES
Permit #: 49532
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 24410

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:58
INTERNAL STANDARD	VERIFIED	09:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:58
BLANK TEST	0.00	09:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:59
BLANK TEST	0.00	10:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:00
BLANK TEST	0.00	10:01

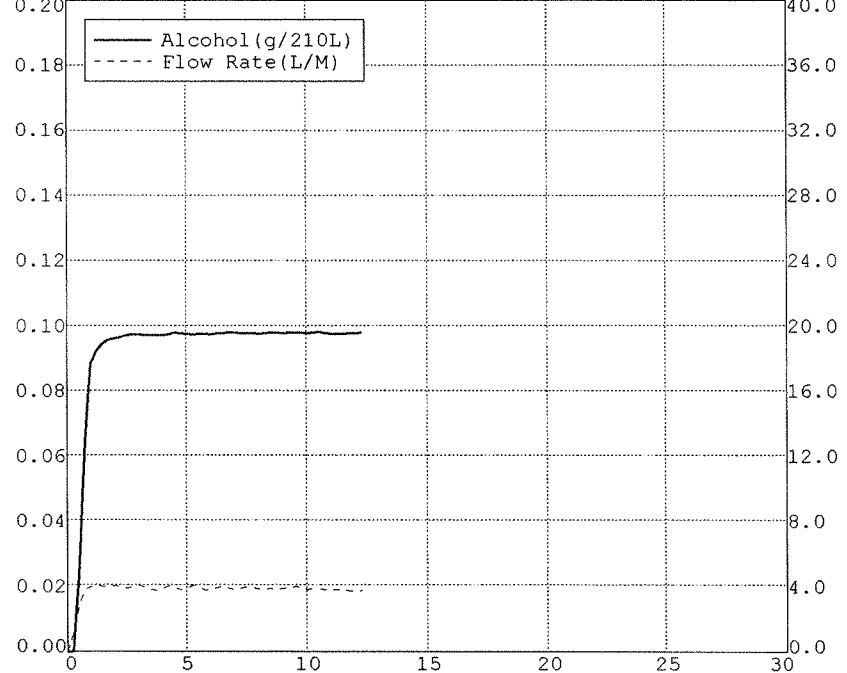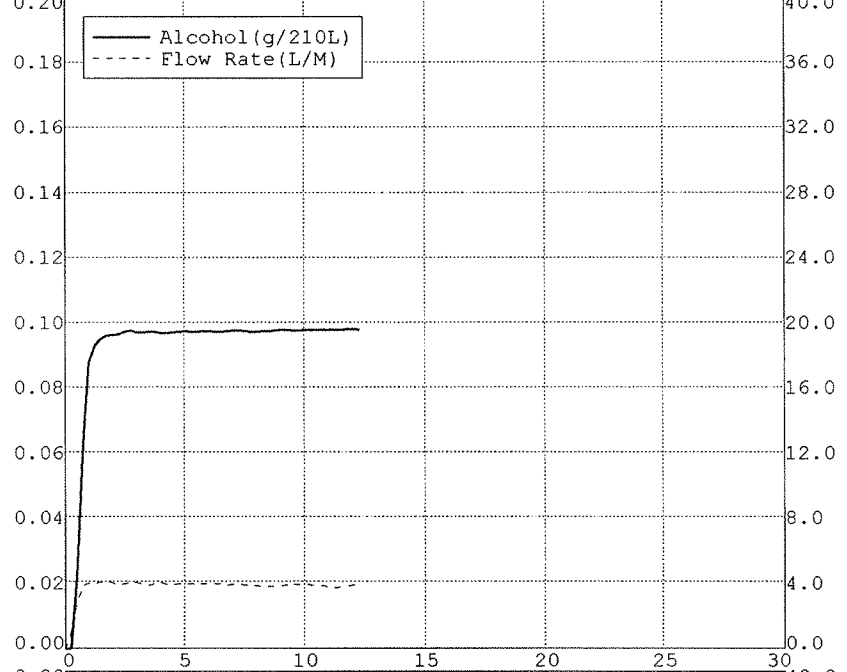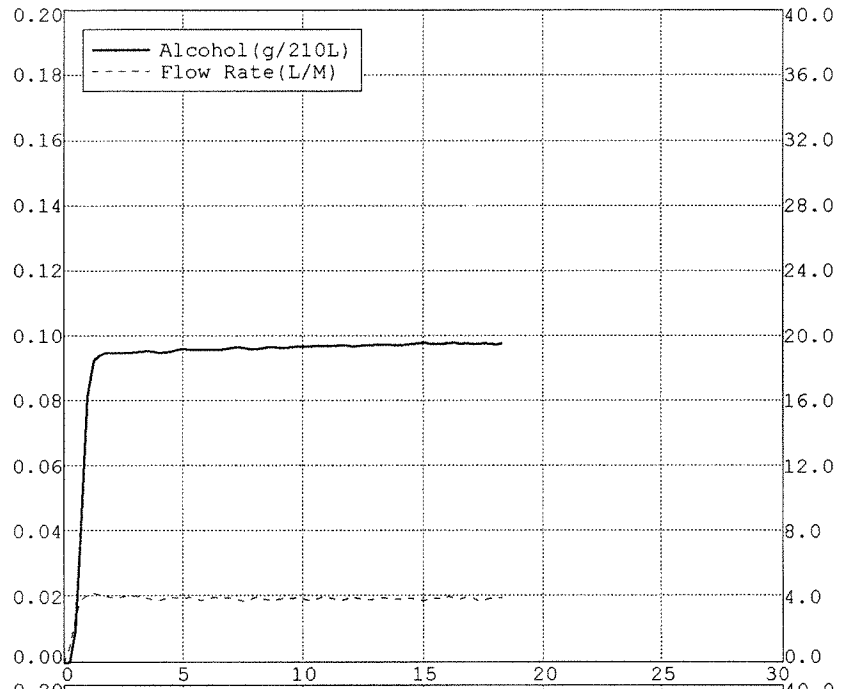

SOLUTION CHANGE




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/30/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25040

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:11
INTERNAL STANDARD	VERIFIED	05:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:12
BLANK TEST	0.00	05:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:13
BLANK TEST	0.00	05:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:14
BLANK TEST	0.00	05:15

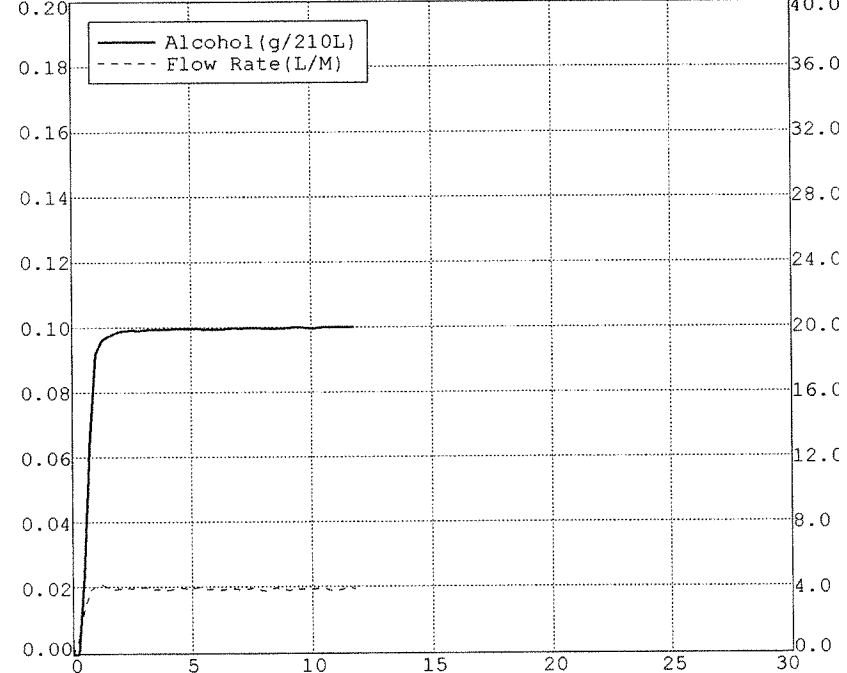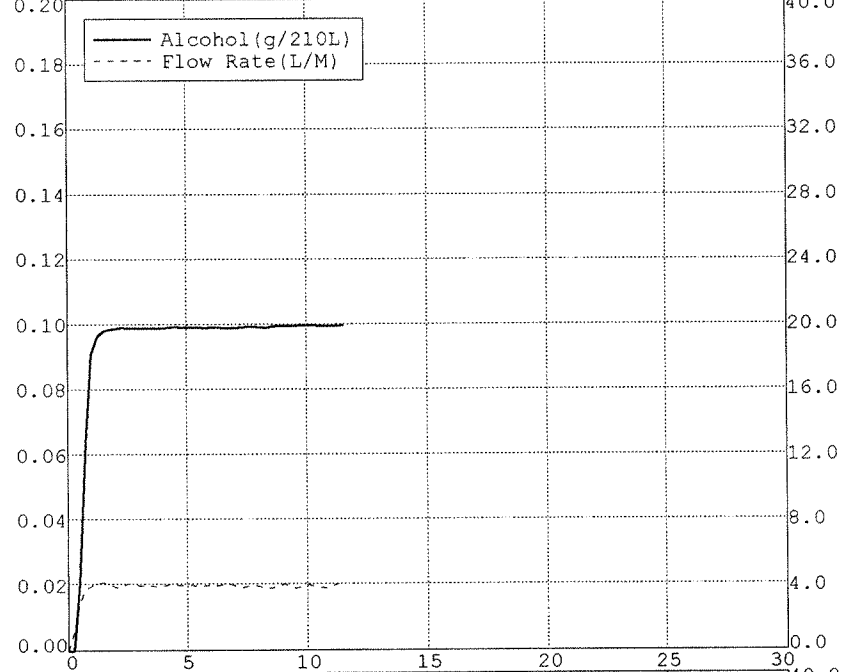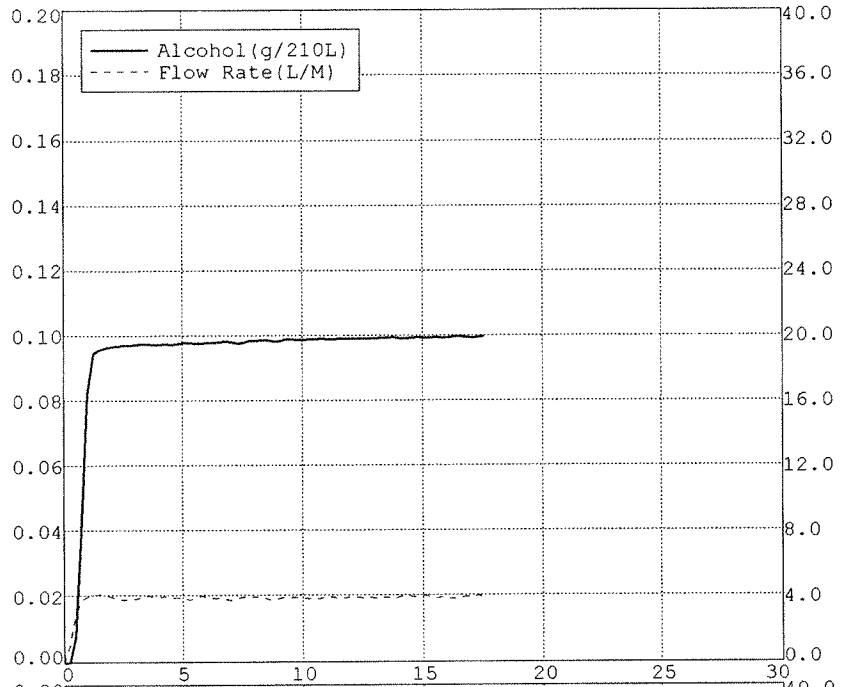

SOLUTION CHANGE

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 03/30/2025

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 25040

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:11
INTERNAL STANDARD	VERIFIED	05:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:12
BLANK TEST	0.00	05:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:13
BLANK TEST	0.00	05:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:14
BLANK TEST	0.00	05:15

