

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/03/2022

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:14
INTERNAL STANDARD	VERIFIED	12:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:14
BLANK TEST	0.00	12:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:15
BLANK TEST	0.00	12:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:17
BLANK TEST	0.00	12:17

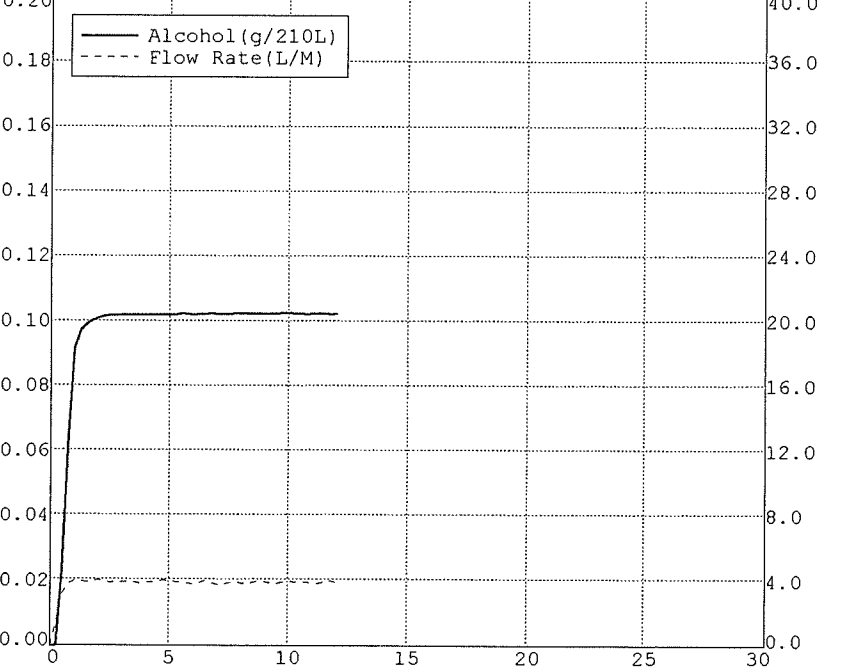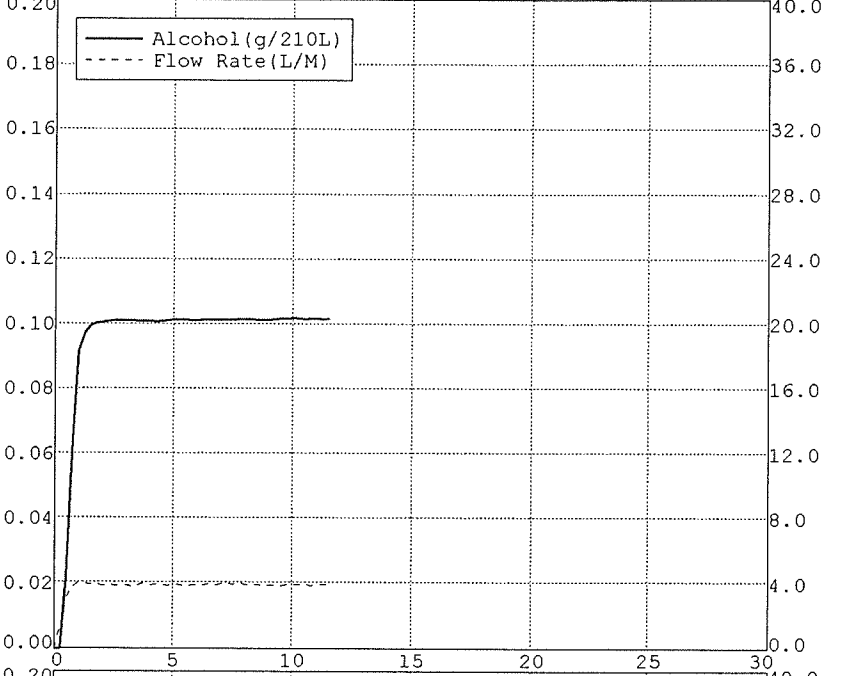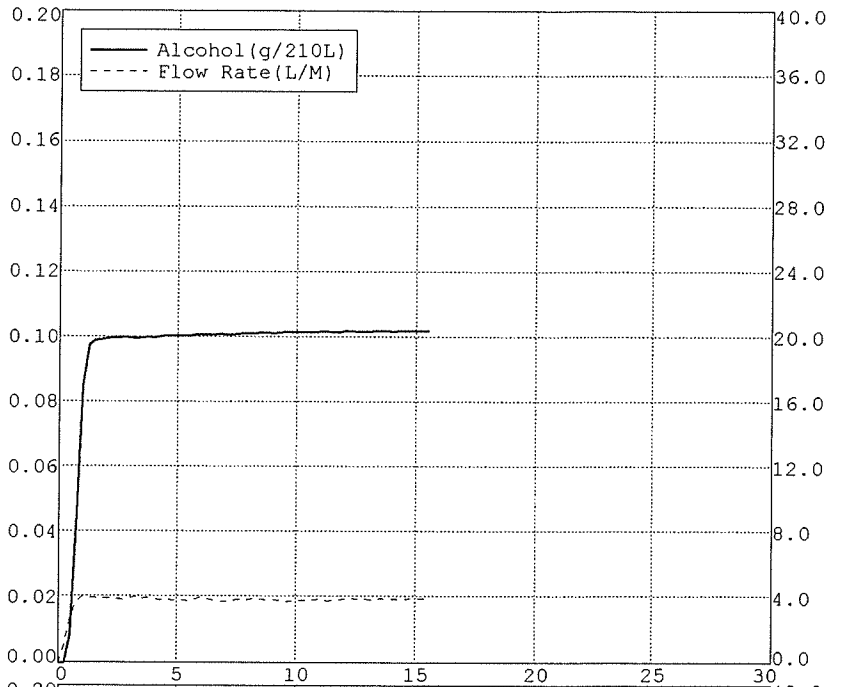

SUPERVISOR TEST




LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/11/2022

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:40
INTERNAL STANDARD	VERIFIED	12:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:41
BLANK TEST	0.00	12:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:42
BLANK TEST	0.00	12:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:43
BLANK TEST	0.00	12:44

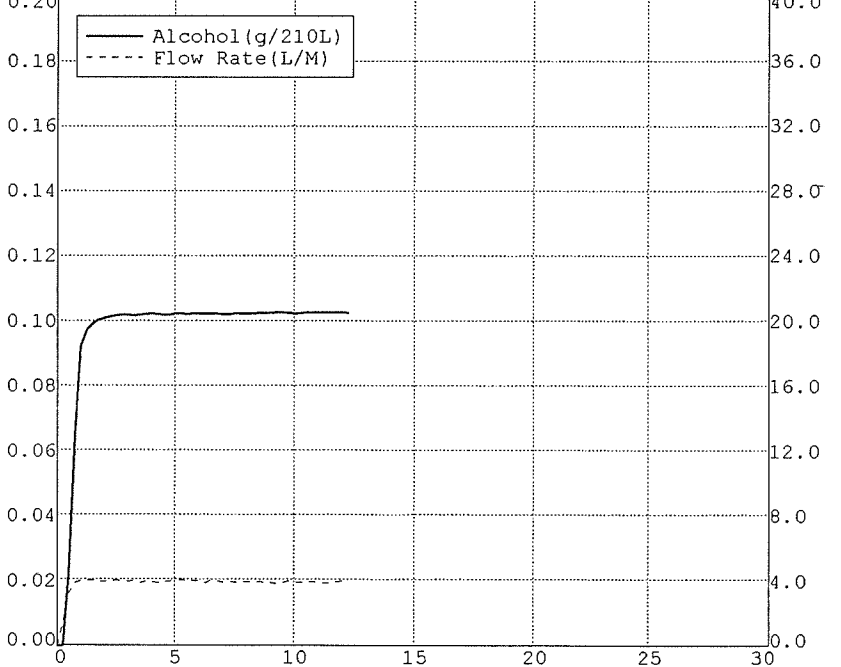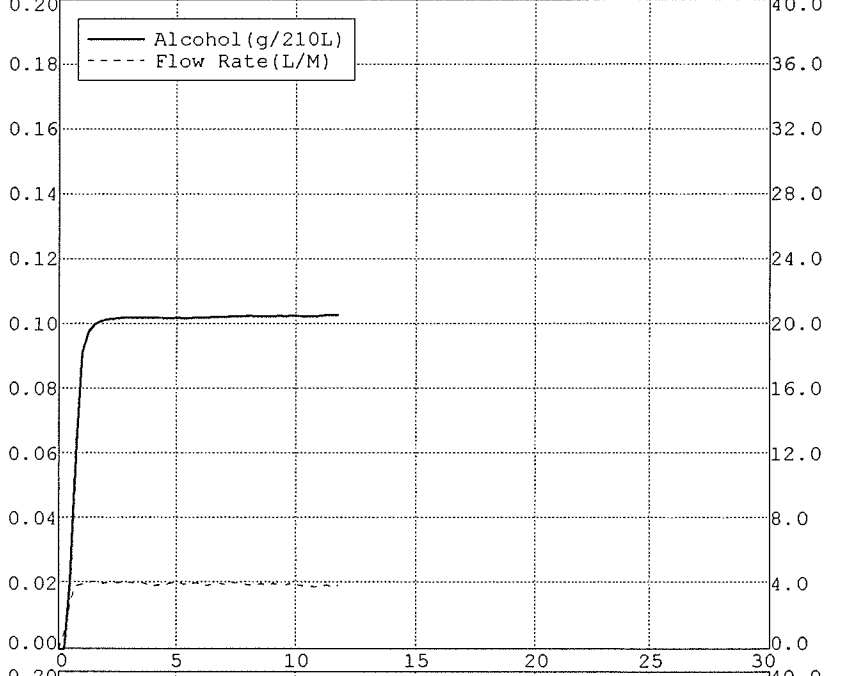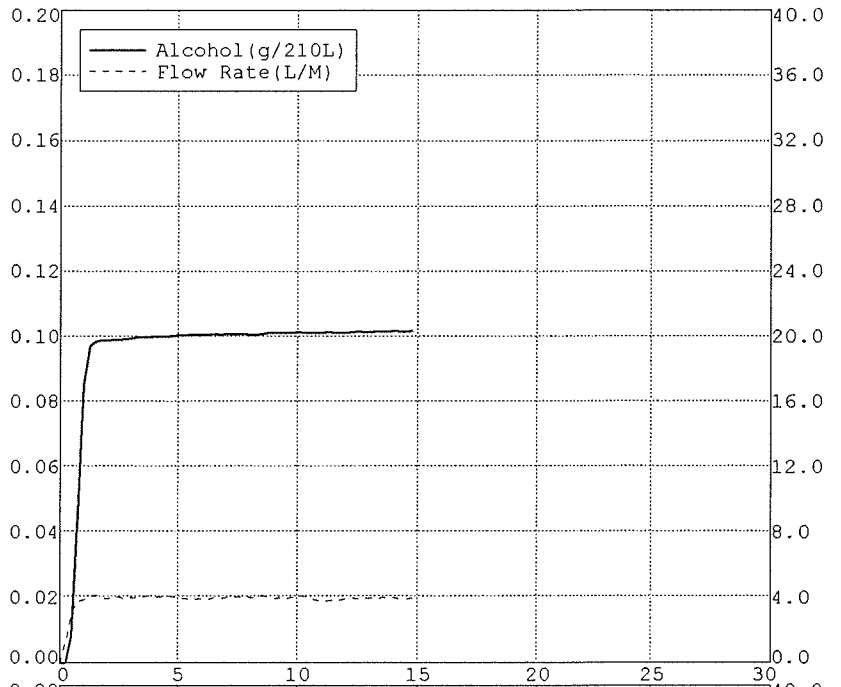

SUPERVISOR TEST


LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/17/2022

OPERATOR NAME:
DORAN H SORRELL
Permit #: 47507
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:07
INTERNAL STANDARD	VERIFIED	18:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:08
BLANK TEST	0.00	18:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:09
BLANK TEST	0.00	18:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:10
BLANK TEST	0.00	18:11

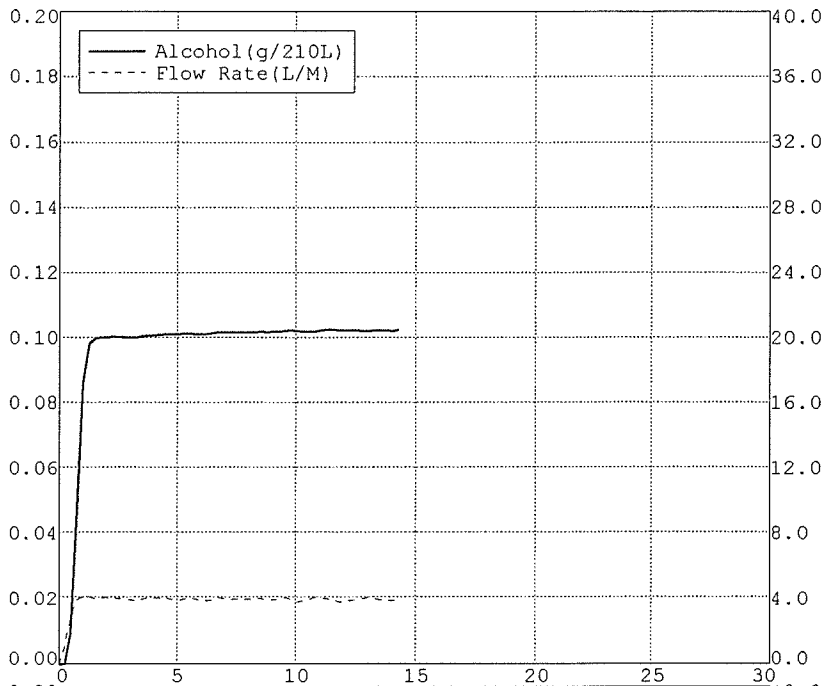

SUPERVISOR TEST

LAKE PLACID VILLAGE
POLICE DEPT.
DATAMASTER dmt: 100290

Date: 04/25/2022

OPERATOR NAME:
CHAD P BLINN
Permit #: 33034
Operator Agency/Dept: LAKE PLACID VILL. PD
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:44
INTERNAL STANDARD	VERIFIED	06:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:45
BLANK TEST	0.00	06:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:46
BLANK TEST	0.00	06:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	06:47
BLANK TEST	0.00	06:48

